
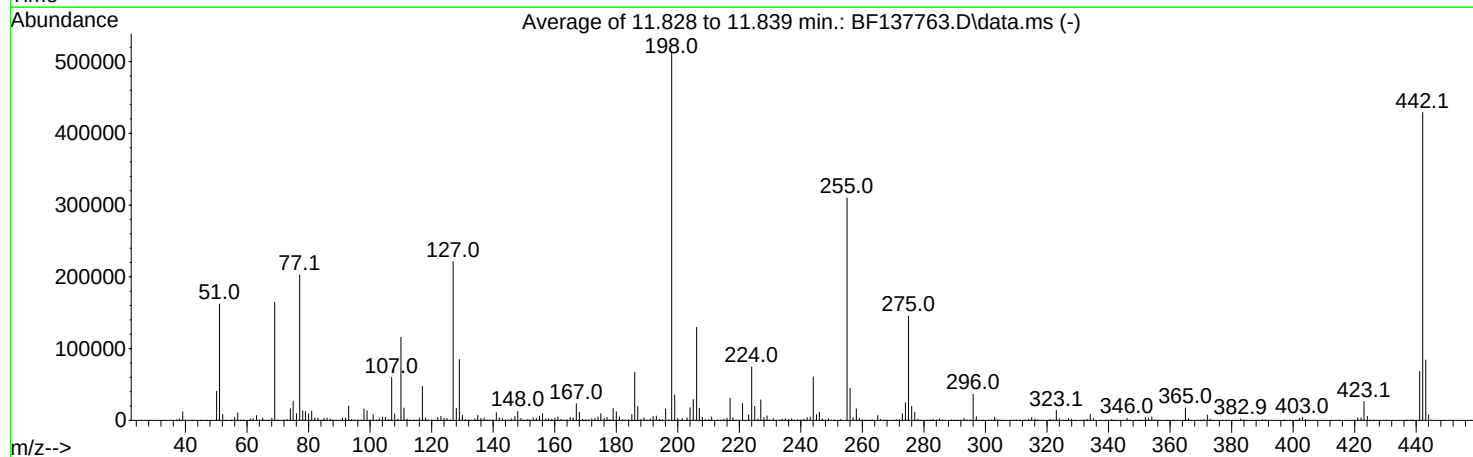


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043024\
Data File : BF137763.D
Acq On : 30 Apr 2024 10:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 03:25:08 2024

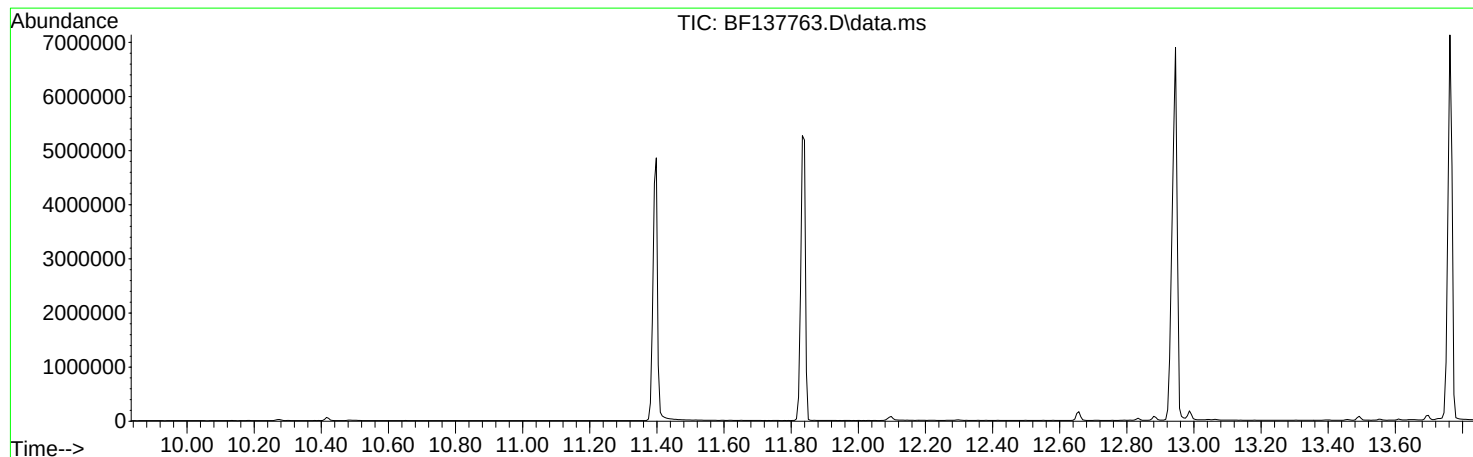




AutoFind: Scans 1656, 1657, 1658; Background Corrected with Scan 1650

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	31.6	162105	PASS
68	69	0.00	2	1.8	3013	PASS
69	198	0.00	100	32.1	164547	PASS
70	69	0.00	2	0.5	794	PASS
127	198	10	80	43.1	221141	PASS
197	198	0.00	2	0.1	699	PASS
198	198	100	100	100.0	512619	PASS
199	198	5	9	6.9	35227	PASS
275	198	10	60	28.4	145448	PASS
365	198	1	100	3.4	17344	PASS
441	198	0.01	100	13.3	68291	PASS
442	442	50	100	100.0	428949	PASS
443	442	15	24	19.6	84072	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043024\
Data File : BF137763.D
Acq On : 30 Apr 2024 10:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 02 19:57:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

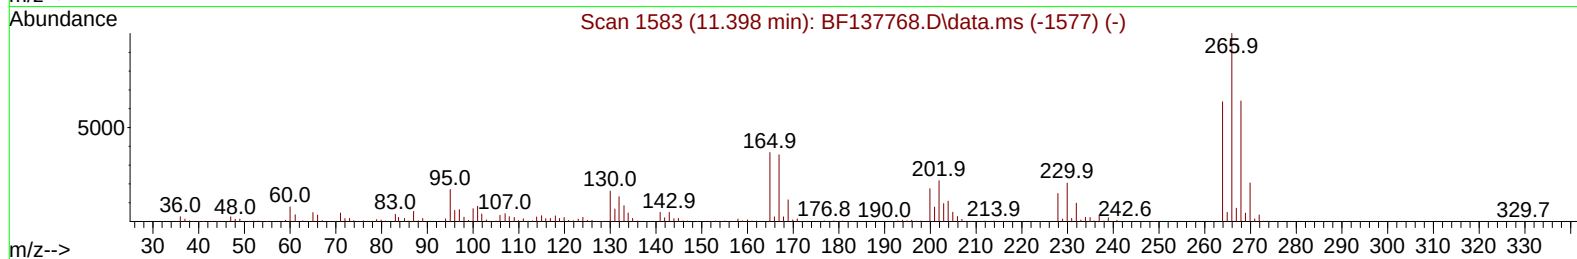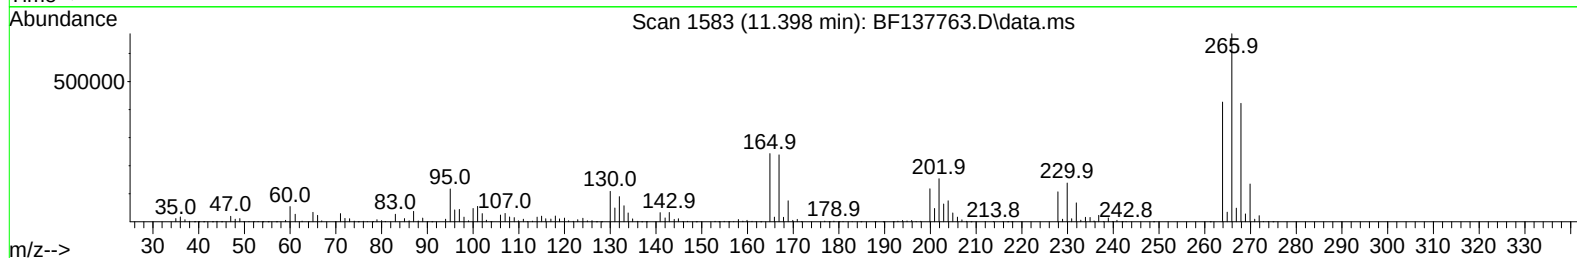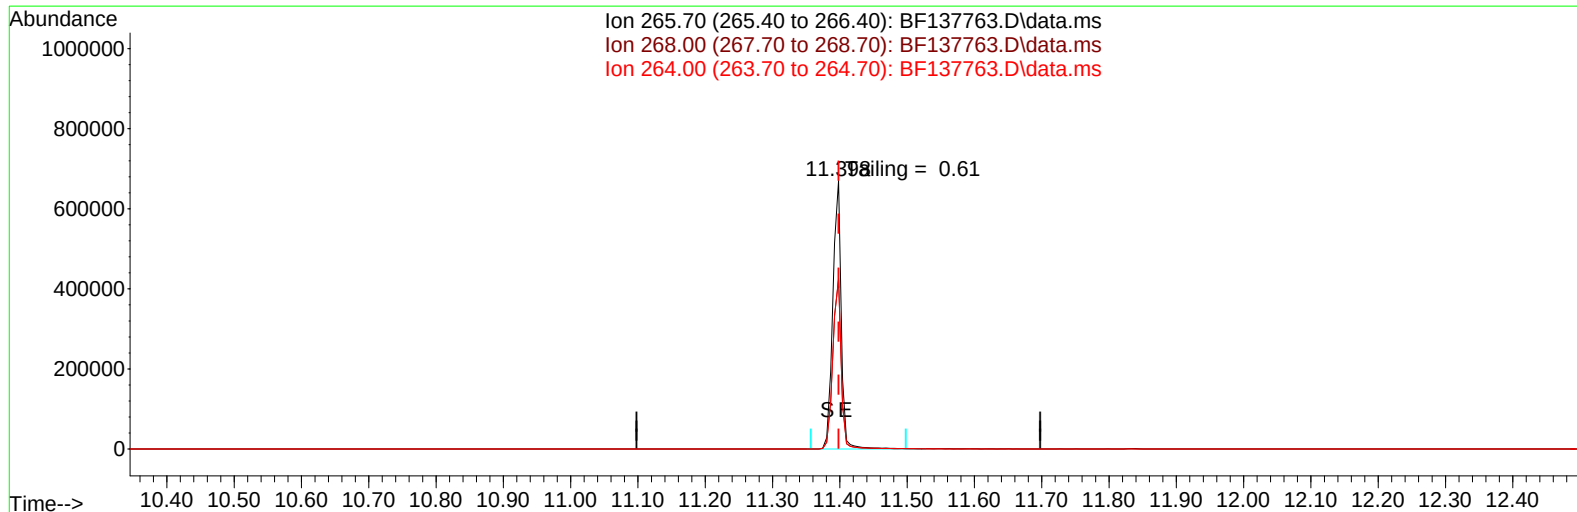

TIC: BF137763.D\data.ms

(70) Pentachlorophenol (C)

11.398min (+ 0.000) 455467.36 ng




response 585142

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	62.95
264.00	63.70	63.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043024\
Data File : BF137763.D
Acq On : 30 Apr 2024 10:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 02 19:57:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

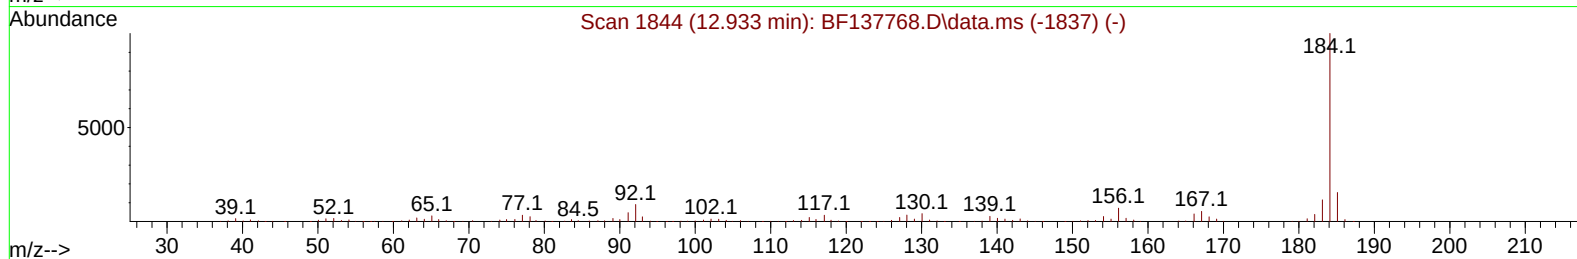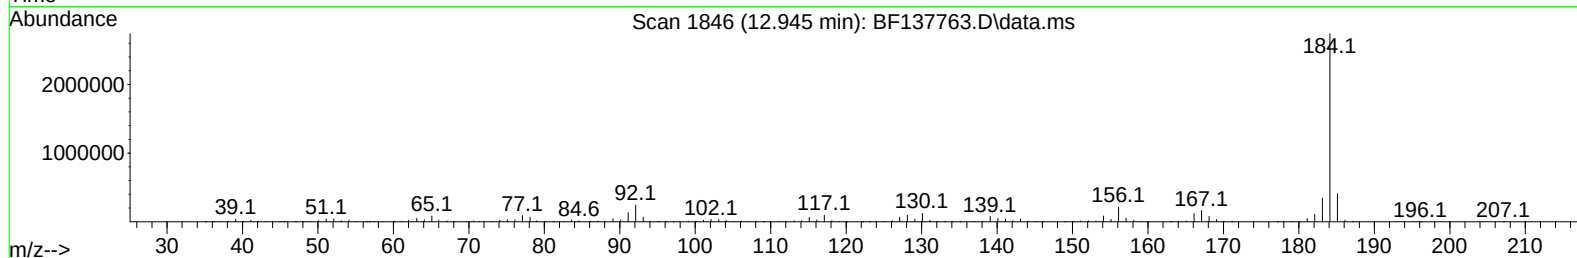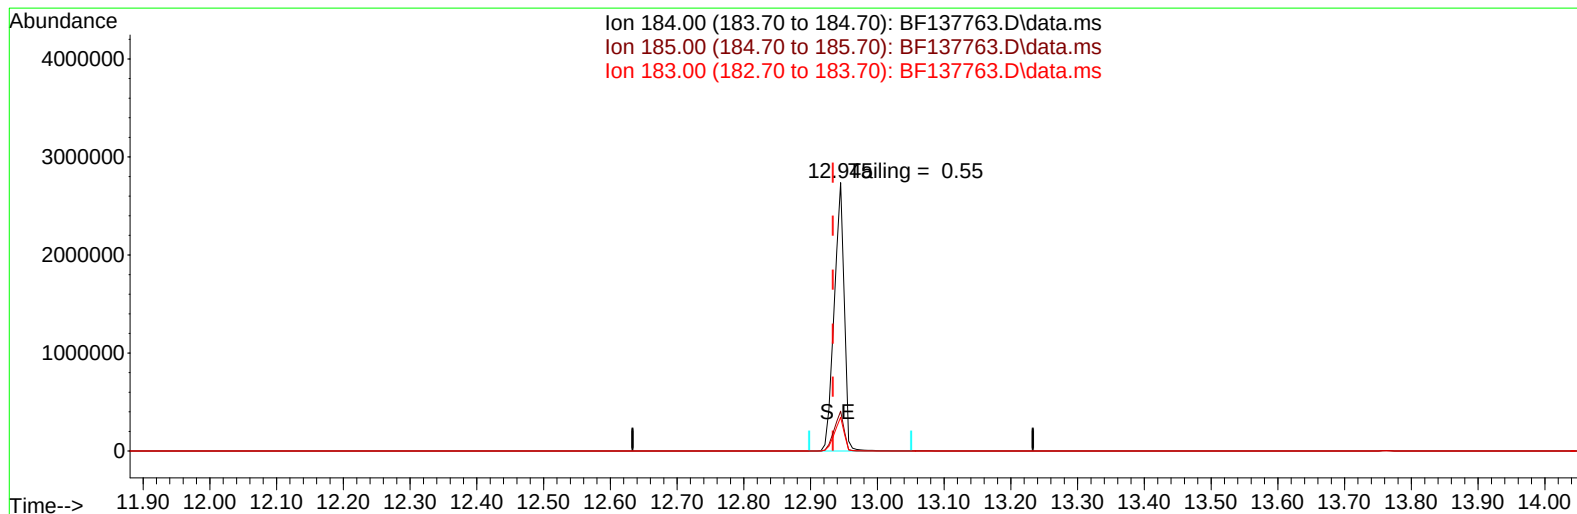

TIC: BF137763.D\data.ms

(77) Benzidine

12.945min (+ 0.012) 515509.87 ng

response 2873337

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.87
183.00	11.50	12.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/1/2024	BNA_F	<u>BF137763.D</u>
Compound Name	Response	Retention Time
DDT	1228976	13.763
DDD	12382	13.492
DDE	289	13.122
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12671	1241647	1.02

Instrument :
BNA_F
ClientSampleId :
DFTPP