
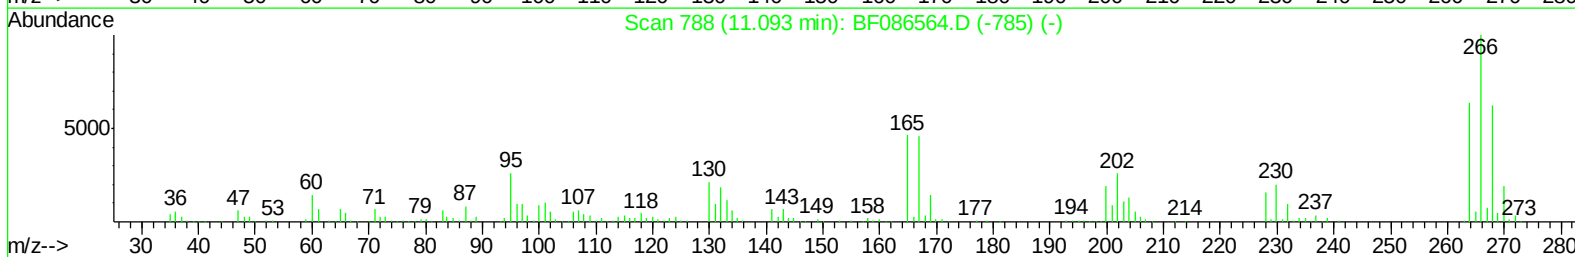
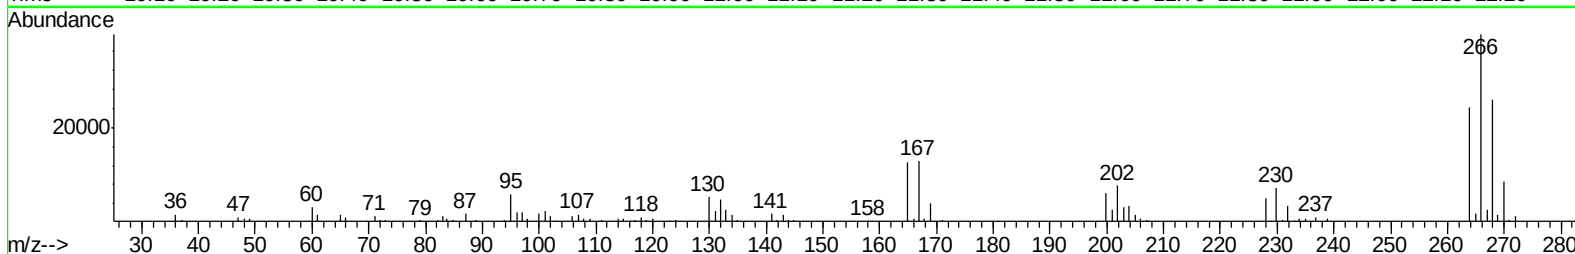


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050116\
Data File : BF086563.D
Acq On : 1 May 2016 11:51
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 05:43:43 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 02 04:16:52 2016
Response via : Initial Calibration

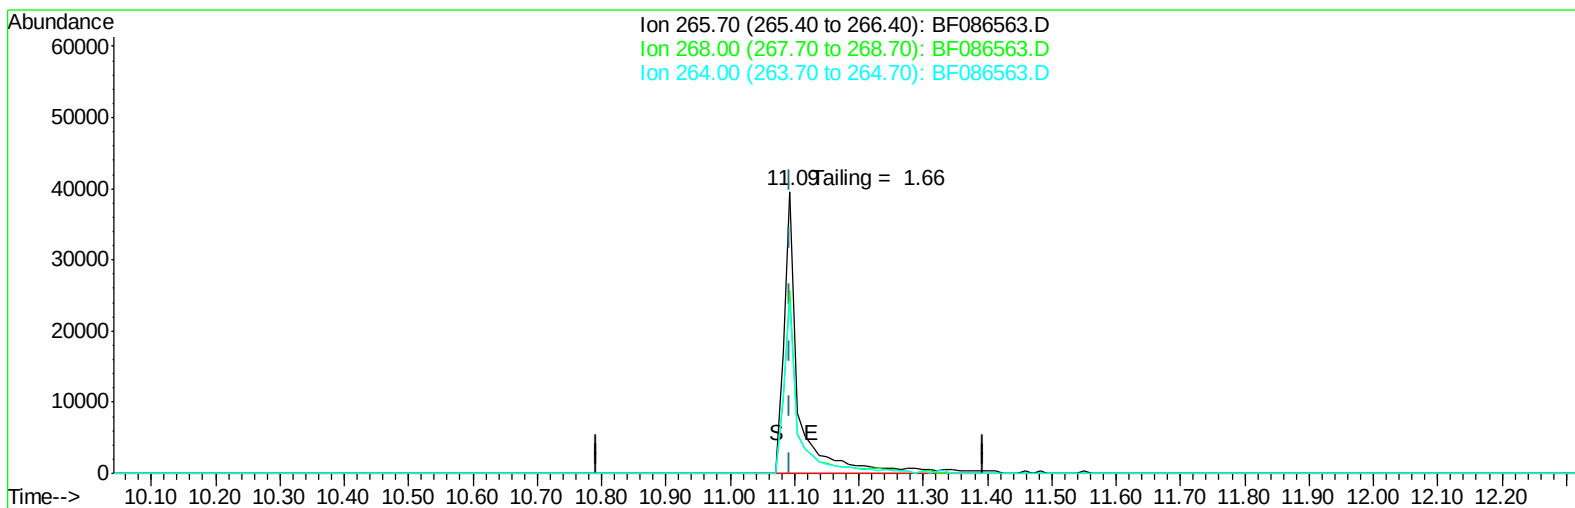

TIC: BF086563.D

(69) Pentachlorophenol (C)




11.093min (+0.000) 0.00ng

response 63345

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	65.16
264.00	66.10	61.10
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050116\
Data File : BF086563.D
Acq On : 1 May 2016 11:51
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 05:43:43 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 02 04:16:52 2016
Response via : Initial Calibration

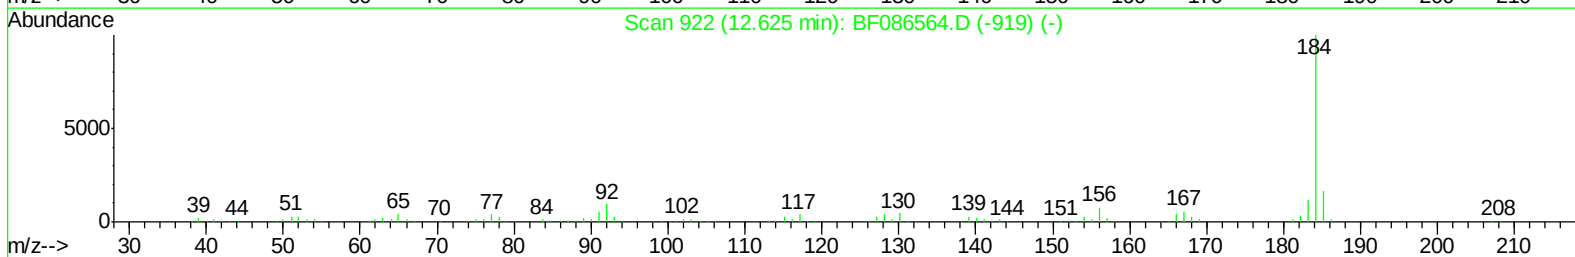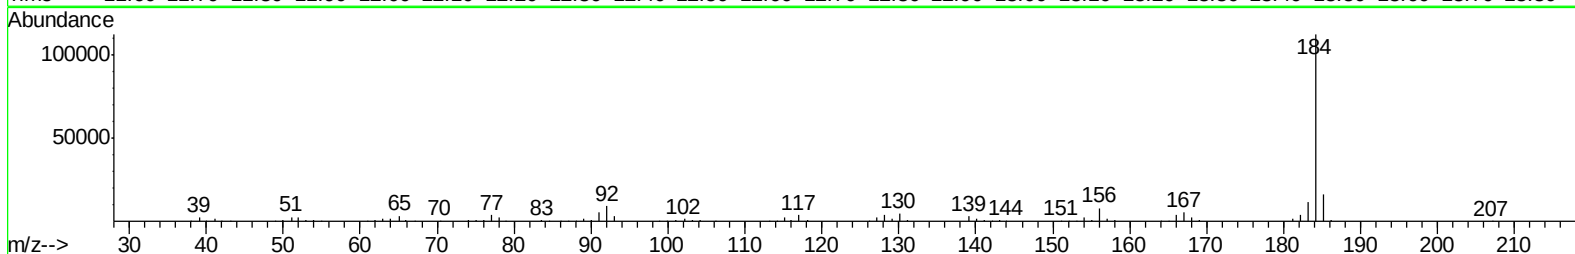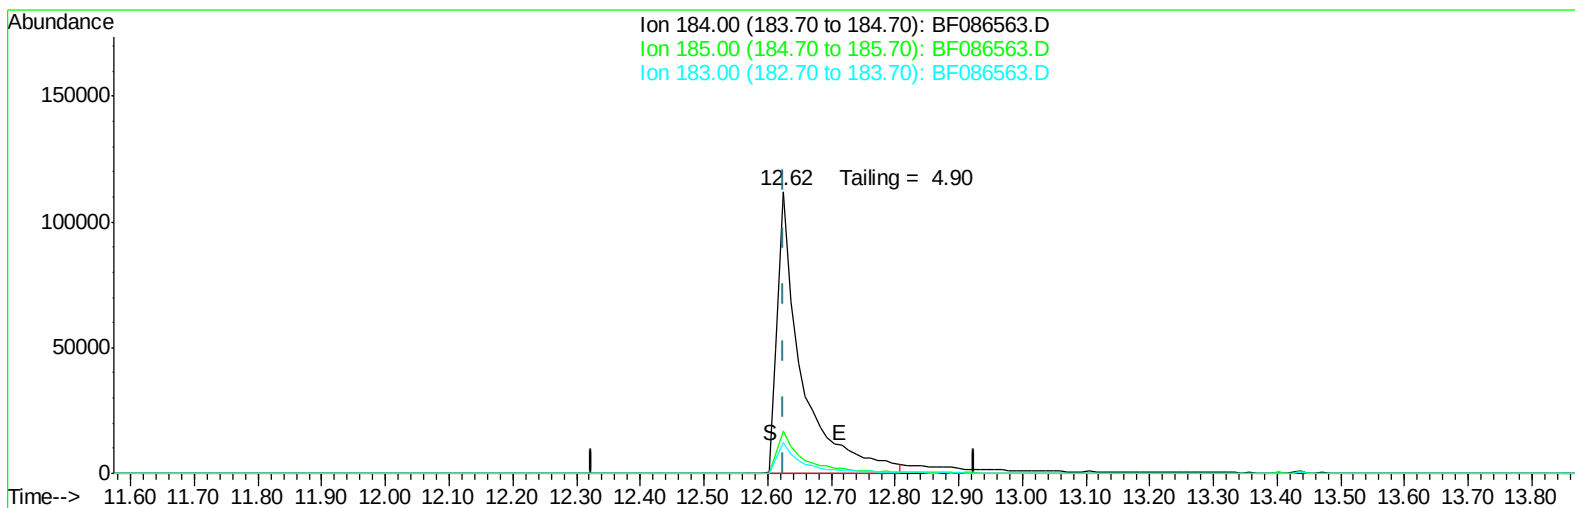

TIC: BF086563.D

(76) Benzidine

12.625min (+0.000) 0.00ng m

response 295876

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.89
183.00	12.20	10.83
0.00	0.00	0.00