
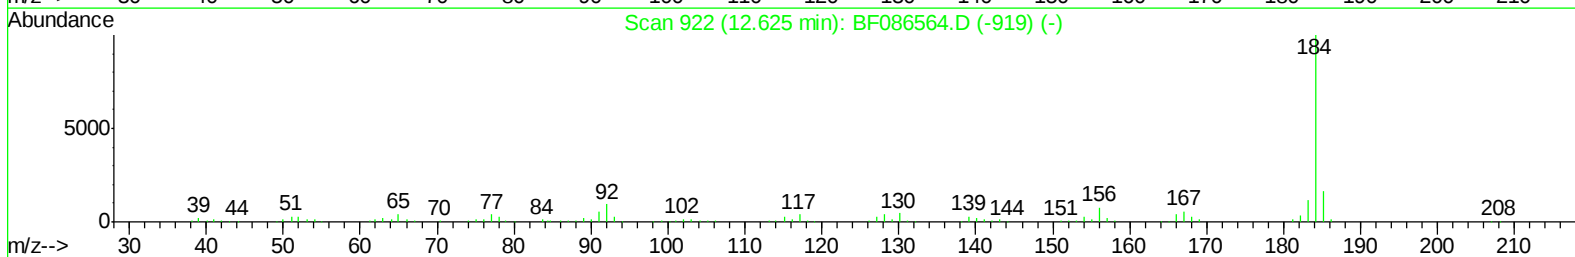
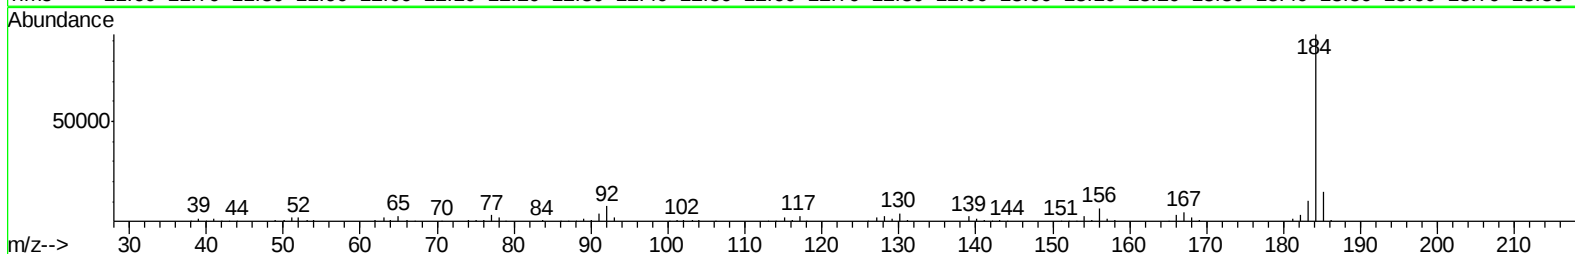


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050116\
Data File : BF086589.D
Acq On : 2 May 2016 00:57
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 05:44:56 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 02 04:16:52 2016
Response via : Initial Calibration

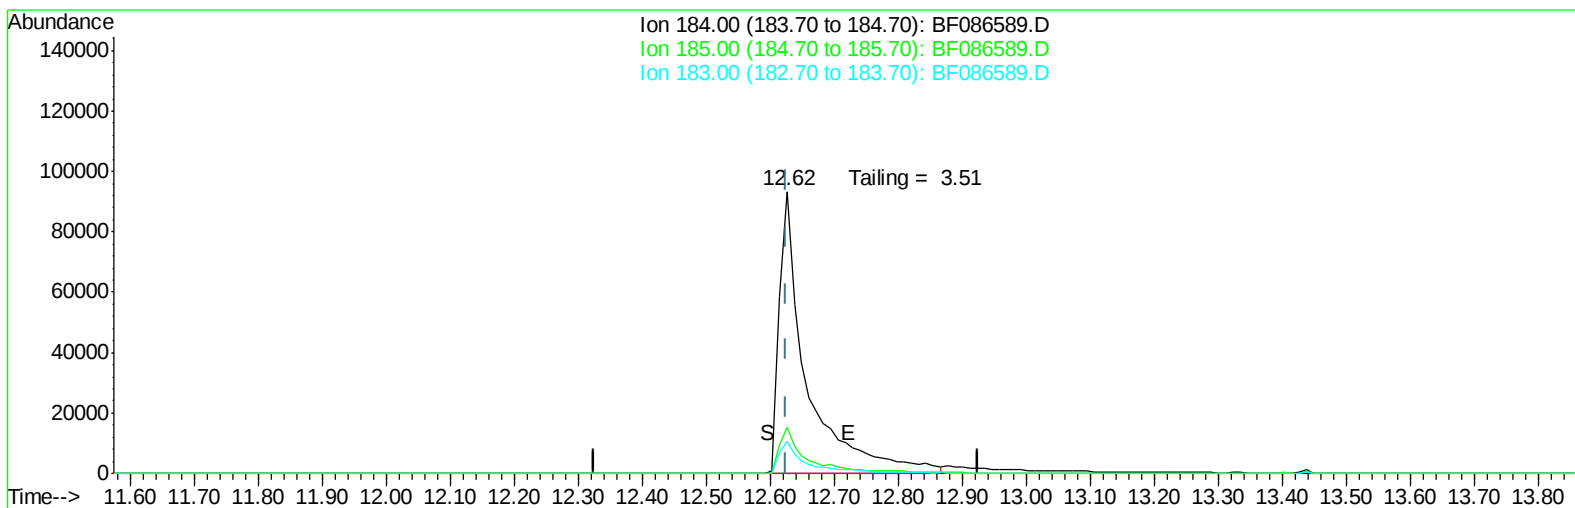

TIC: BF086589.D

(76) Benzidine




12.625min (+0.000) 0.00ng m

response 277175

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	16.20
183.00	12.20	11.51
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050116\
Data File : BF086589.D
Acq On : 2 May 2016 00:57
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 05:44:56 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 02 04:16:52 2016
Response via : Initial Calibration

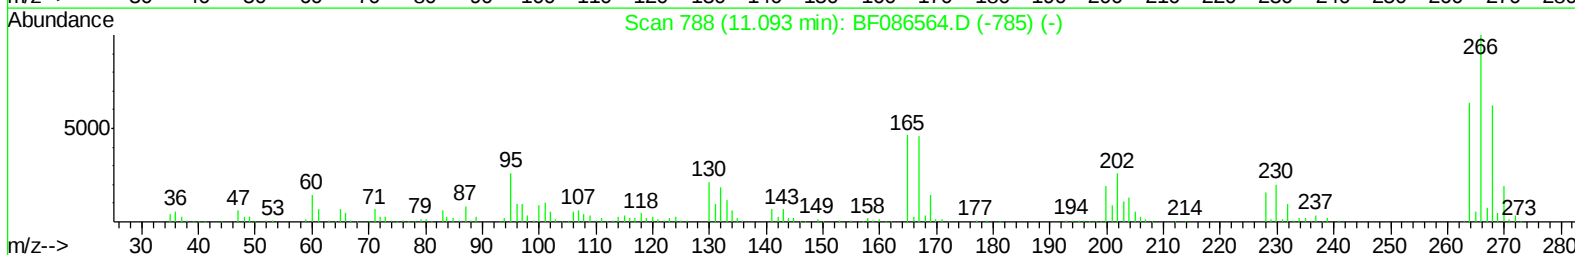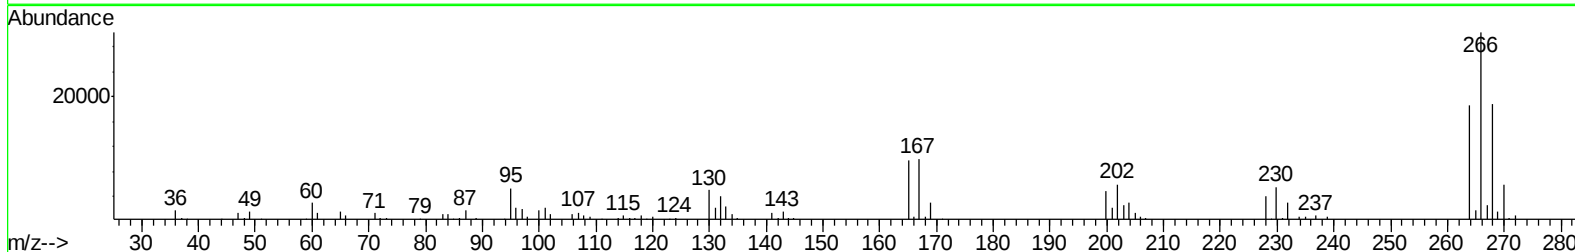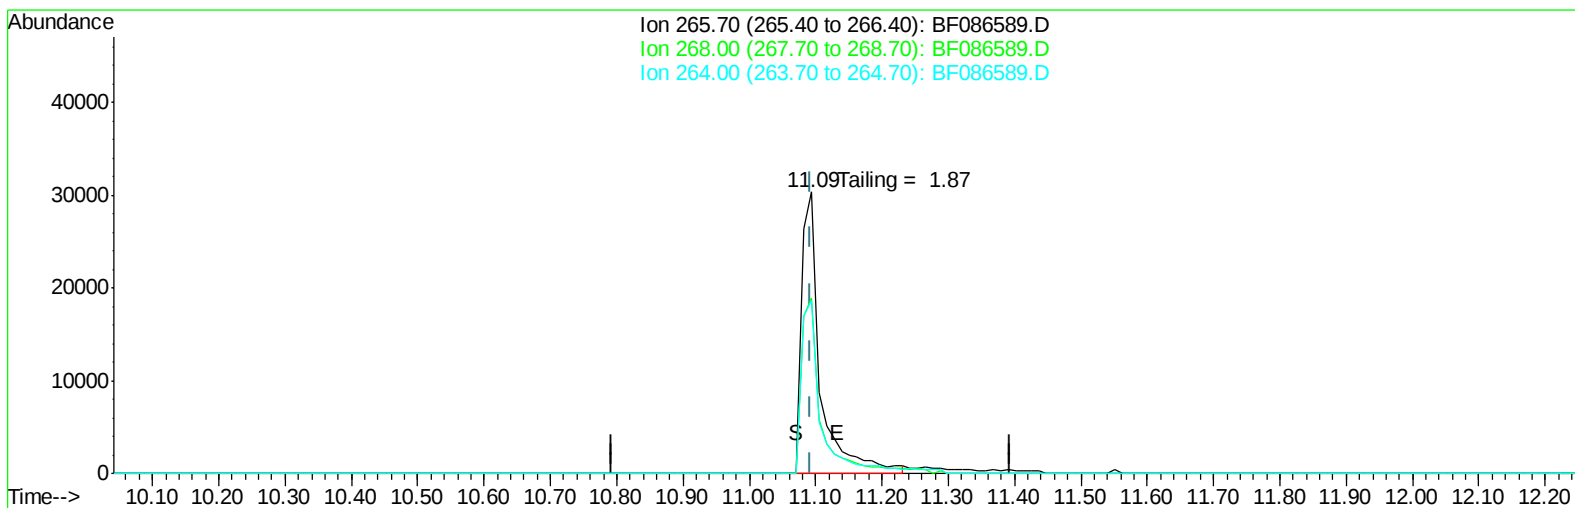

TIC: BF086589.D

(69) Pentachlorophenol (C)

11.093min (+0.000) 22601.46ng

response 60262

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.28
264.00	66.10	61.60
0.00	0.00	0.00