

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050116\
 Data File : BF086603.D
 Acq On : 2 May 2016 7:28
 Operator : UM/SJ
 Sample : H2686-07
 Misc :
 ALS Vial : 86 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 26WARD-2B-CS-4(0-10FTBGS)

Quant Time: May 02 07:51:23 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 27 14:20:52 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.76	152	135142	20.00	ng	-0.05
21) Naphthalene-d8	8.05	136	568641	20.00	ng	-0.05
38) Acenaphthene-d10	9.80	164	275066	20.00	ng	-0.05
63) Phenanthrene-d10	11.28	188	516623	20.00	ng	-0.05
75) Chrysene-d12	13.91	240	362257	20.00	ng	-0.06
86) Perylene-d12	15.30	264	324193	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	1062782	135.65	ng	-0.02
7) Phenol-d6	6.41	99	1291041	118.06	ng	-0.03
23) Nitrobenzene-d5	7.33	82	987907	93.64	ng	-0.05
41) 2,4,6-Tribromophenol	10.59	330	387534	133.60	ng	-0.05
44) 2-Fluorobiphenyl	9.13	172	1449816	94.42	ng	-0.05
78) Terphenyl-d14	12.86	244	1373941	83.56	ng	-0.05
Target Compounds						
31) Naphthalene	8.06	128	130010	4.49	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050116\
Data File : BF086603.D
Acq On : 2 May 2016 7:28
Operator : UM/SJ
Sample : H2686-07
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
26WARD-2B-CS-4(0-10FTBGS)

Quant Time: May 02 07:51:23 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 14:20:52 2016
Response via : Initial Calibration

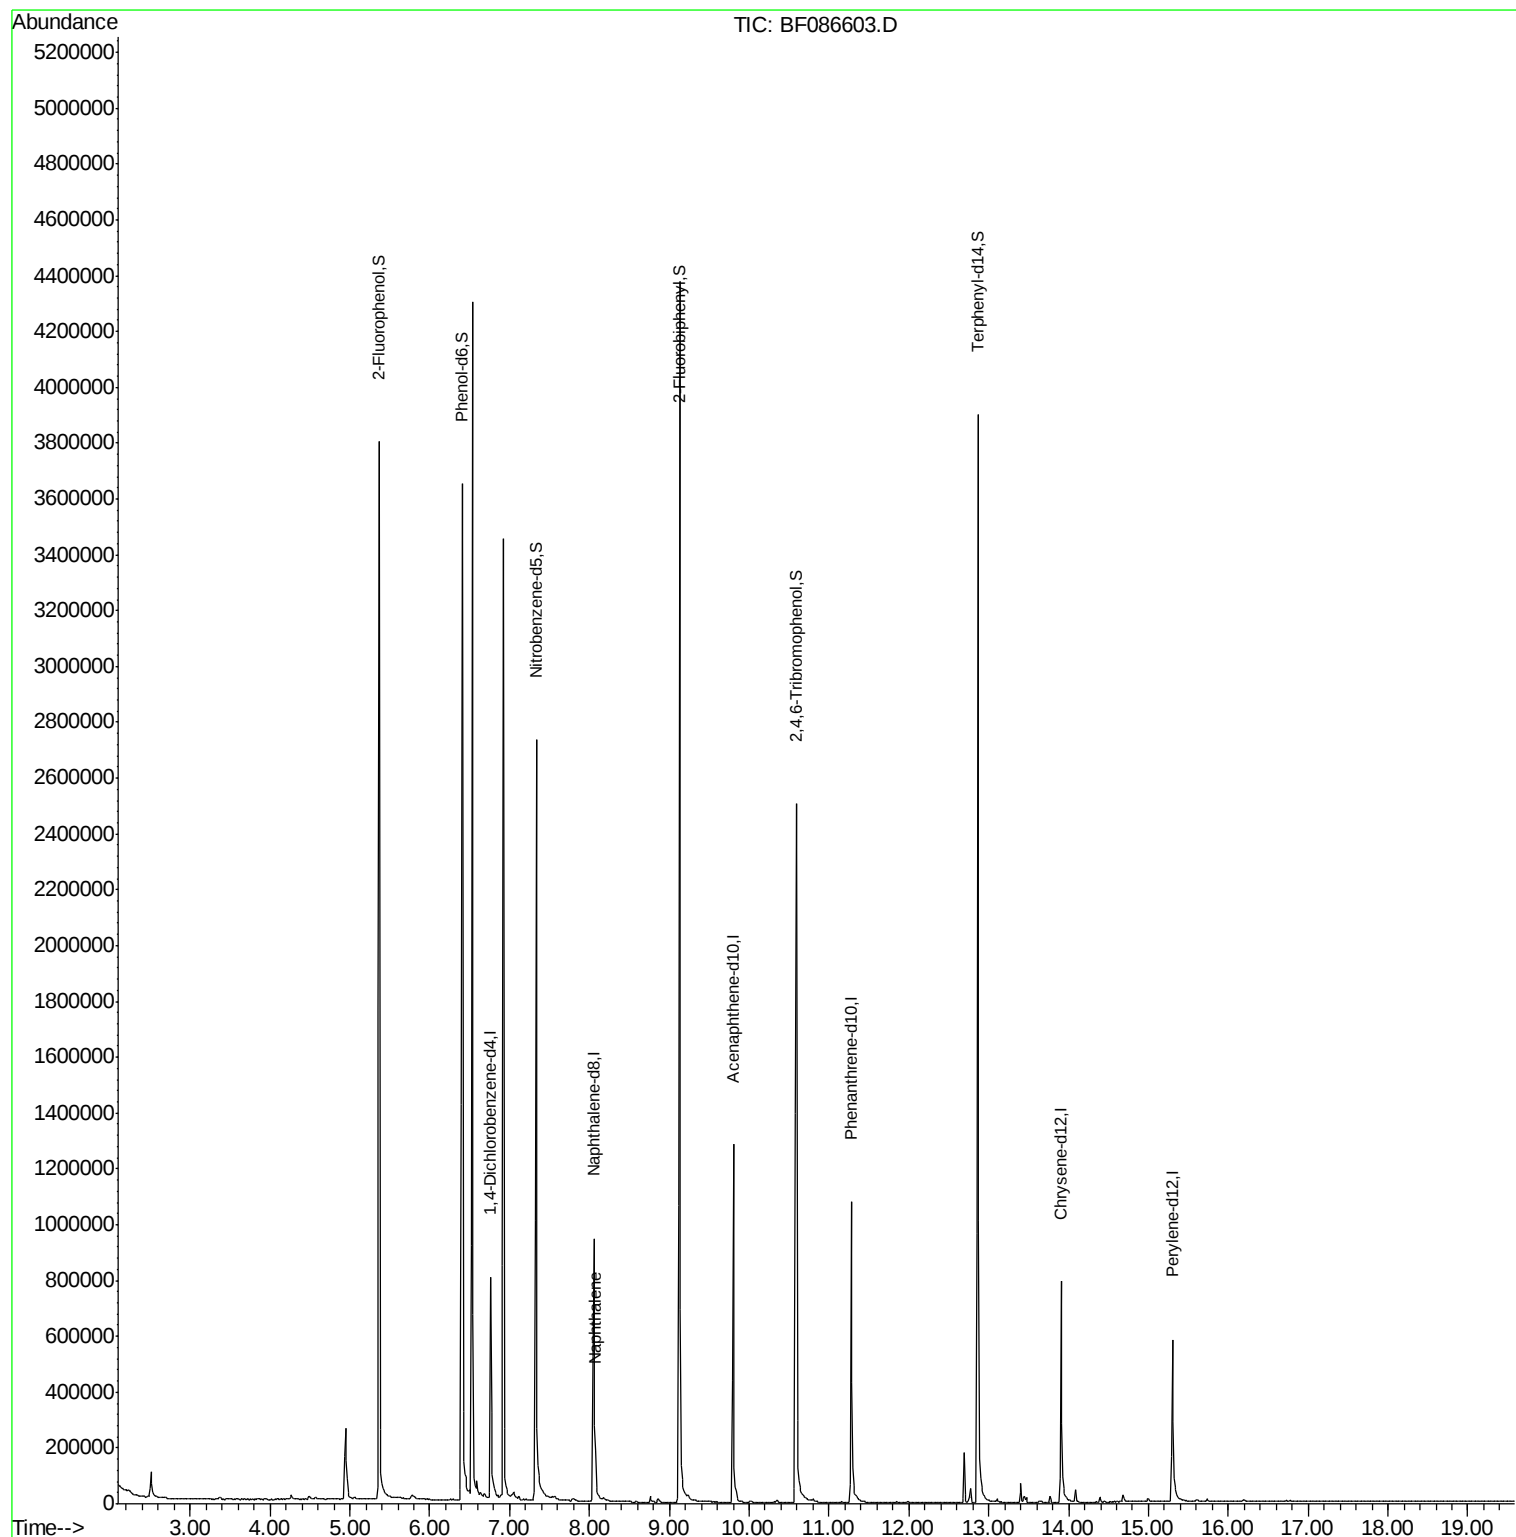

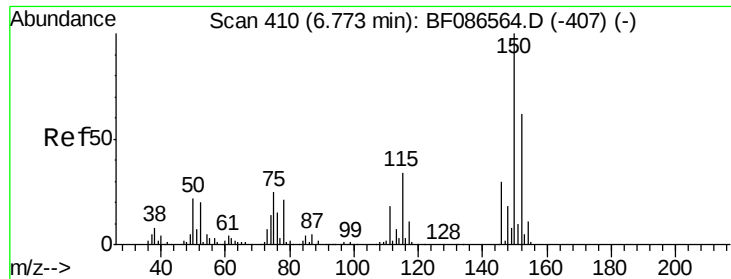

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.76 min Scan# 409

Delta R.T. -0.05 min

Lab File: BF086603.D

Acq: 2 May 2016 7:28

Instrument :

BNA_F

ClientSampleId :

26WARD-2B-CS-4(0-10FTBGS)


Tgt Ion:152 Resp: 135142

Ion Ratio Lower Upper

152 100

150 161.0 125.8 188.6




115 70.6 51.5 77.3

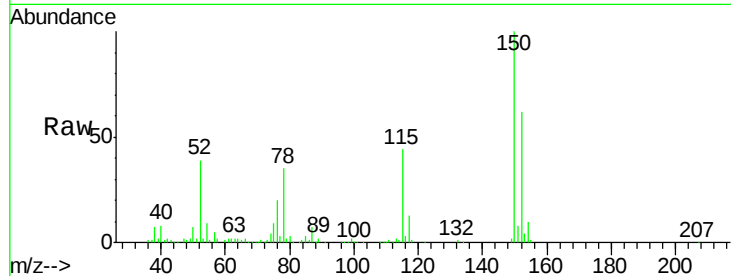

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

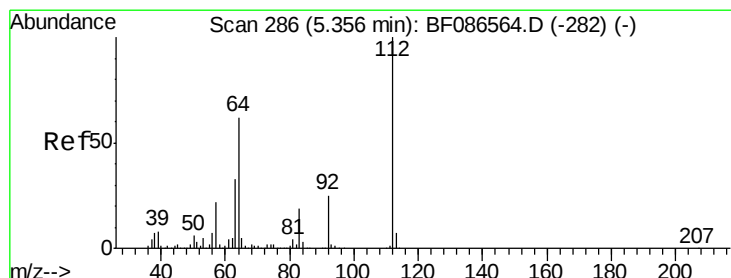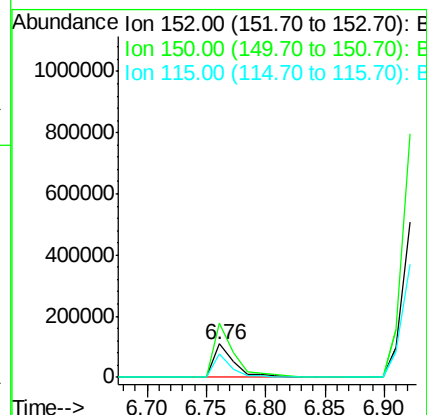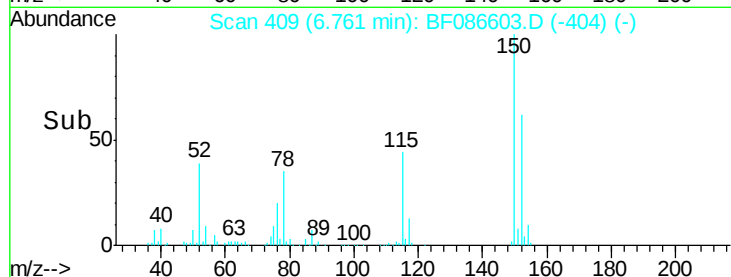

#5

2-Fluorophenol

Concen: 135.65 ng

RT: 5.37 min Scan# 287

Delta R.T. -0.02 min

Lab File: BF086603.D

Acq: 2 May 2016 7:28


Tgt Ion:112 Resp: 1062782

Ion Ratio Lower Upper

112 100

64 67.2 52.1 78.1



63 36.3 25.7 38.5

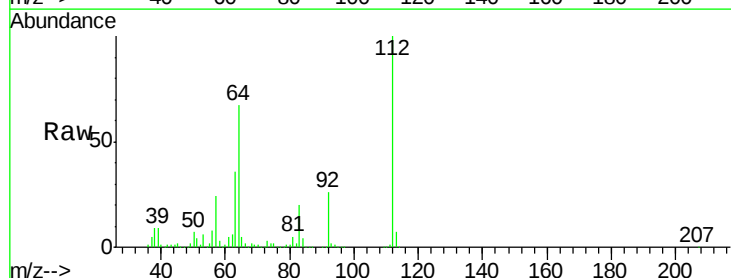


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

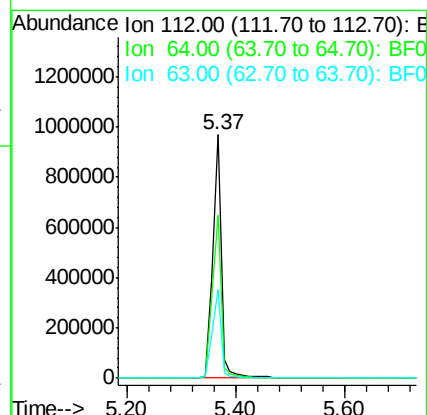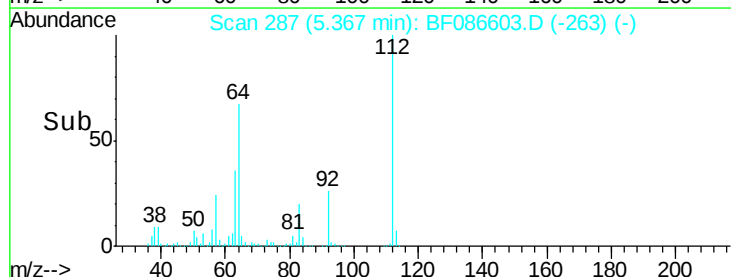

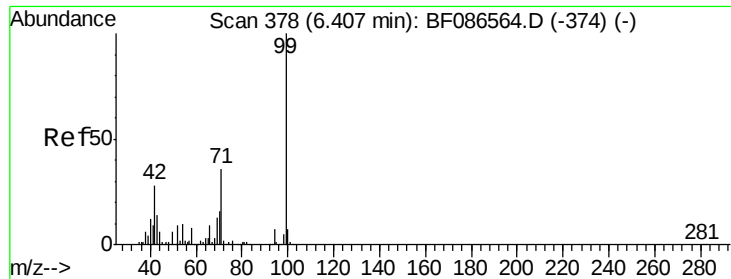

#7

Phenol-d6

Concen: 118.06 ng

RT: 6.41 min Scan# 378

Delta R.T. -0.03 min

Lab File: BF086603.D

Acq: 2 May 2016 7:28

Instrument :

BNA_F

ClientSampleId :

26WARD-2B-CS-4(0-10FTBGS)





Tgt Ion: 99 Resp: 1291041

Ion Ratio Lower Upper

99 100

42 27.7 13.6 20.4#

71 37.6 24.6 36.8#

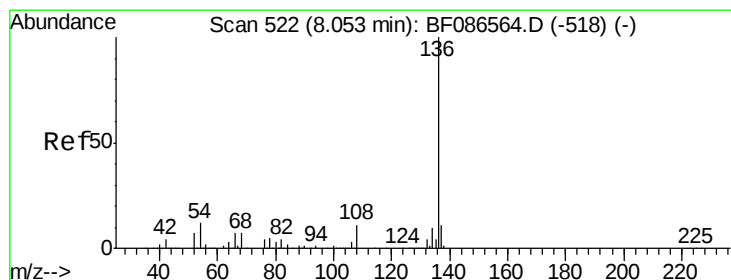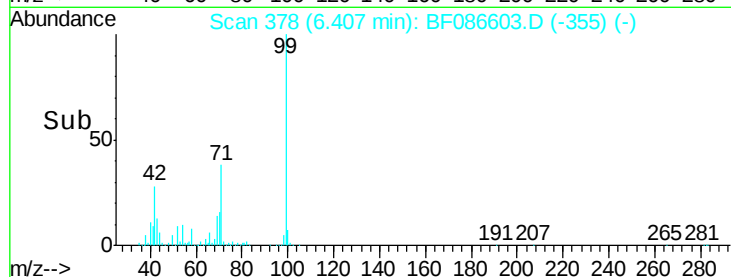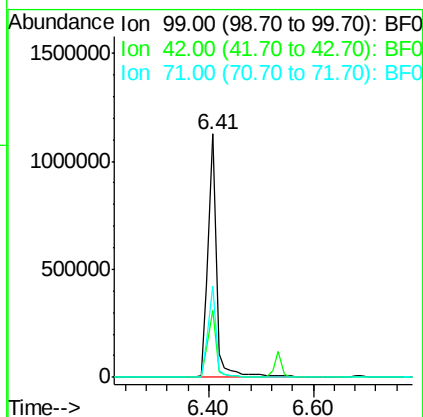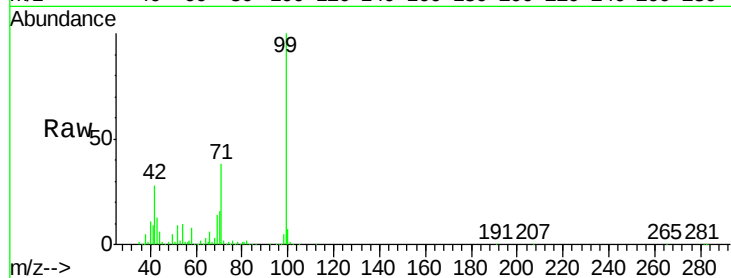

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.05 min Scan# 522

Delta R.T. -0.05 min

Lab File: BF086603.D

Acq: 2 May 2016 7:28

Tgt Ion: 136 Resp: 568641




Ion Ratio Lower Upper

136 100

137 10.8 8.8 13.2

54 9.1 5.0 7.4#

68 5.9 4.4 6.6


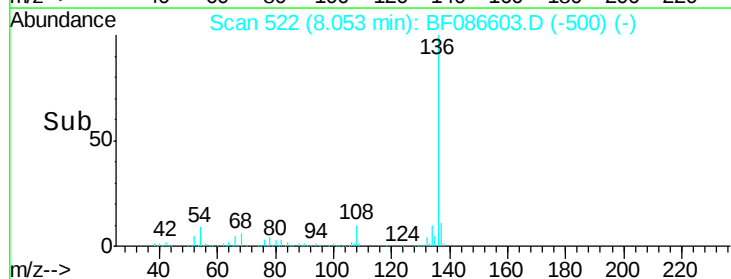
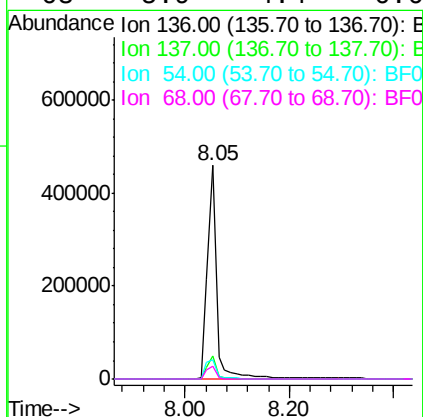
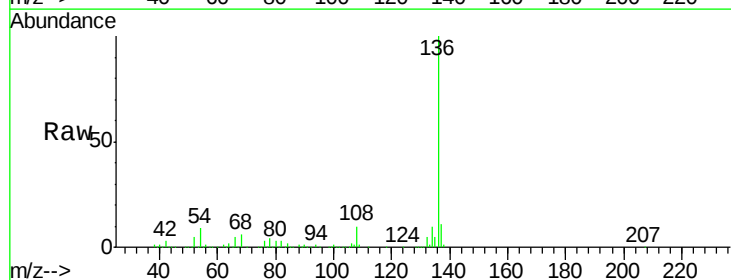




#23
 Nitrobenzene-d5
 Concen: 93.64 ng
 RT: 7.33 min Scan# 459
 Delta R.T. -0.05 min
 Lab File: BF086603.D
 Acq: 2 May 2016 7:28




Instrument :
 BNA_F
 ClientSampleId :
 26WARD-2B-CS-4(0-10FTBGS)


Tgt Ion: 82 Resp: 987907
 Ion Ratio Lower Upper
 82 100
 128 41.5 40.6 61.0
 54 66.8 38.1 57.1#

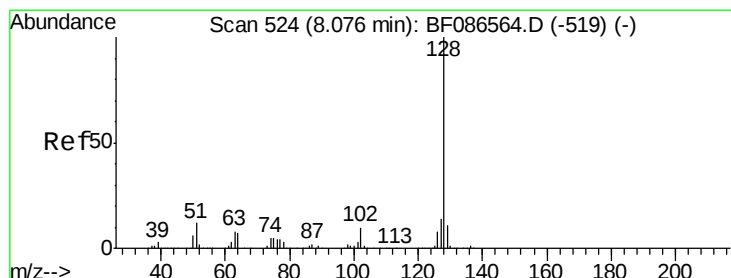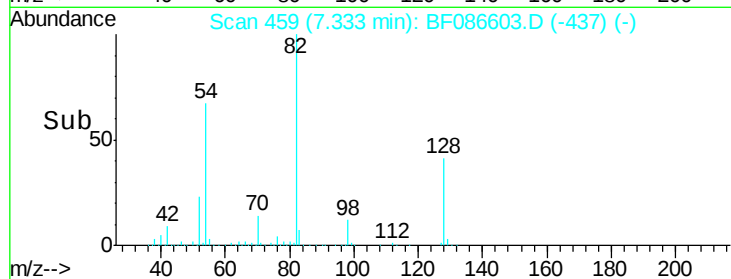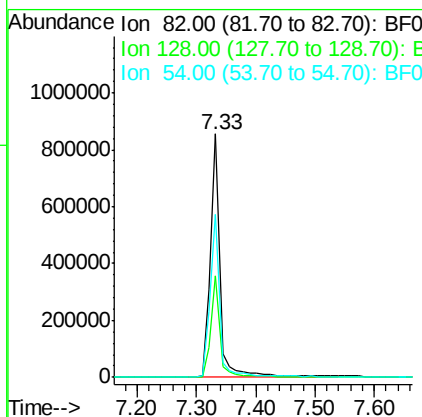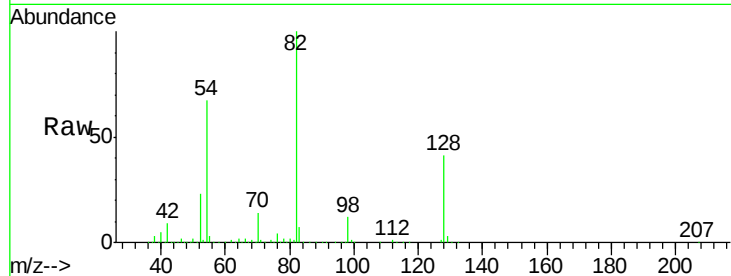

#31
 Naphthalene
 Concen: 4.49 ng
 RT: 8.06 min Scan# 523
 Delta R.T. -0.05 min
 Lab File: BF086603.D
 Acq: 2 May 2016 7:28

Tgt Ion: 128 Resp: 130010
 Ion Ratio Lower Upper
 128 100
 129 11.0 8.6 13.0
 127 13.1 10.8 16.2

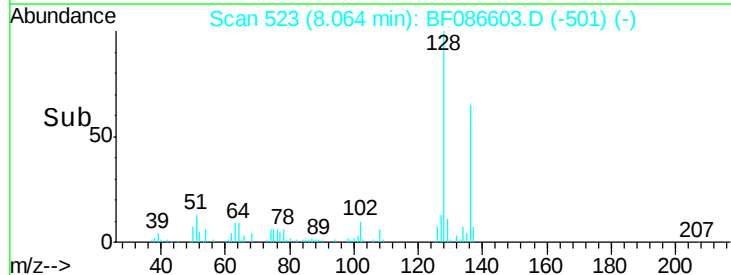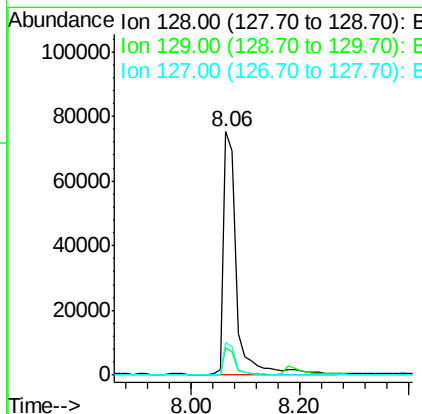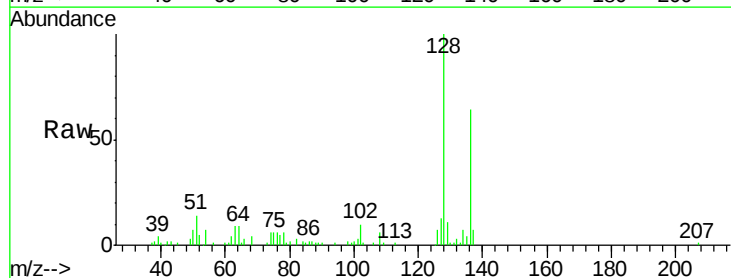


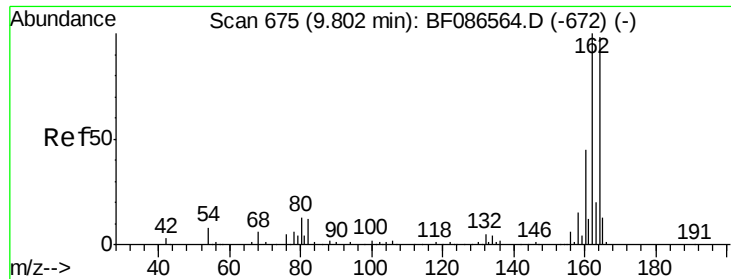




#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.80 min Scan# 675
Delta R.T. -0.05 min
Lab File: BF086603.D
Acq: 2 May 2016 7:28

Instrument :
BNA_F
ClientSampleId :
26WARD-2B-CS-4(0-10FTBGS)

Tgt Ion	Ratio	Lower	Upper
164	100		
162	105.2	82.8	124.2
160	47.3	36.9	55.3

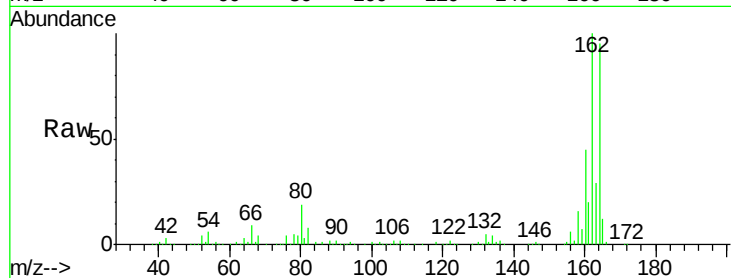


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

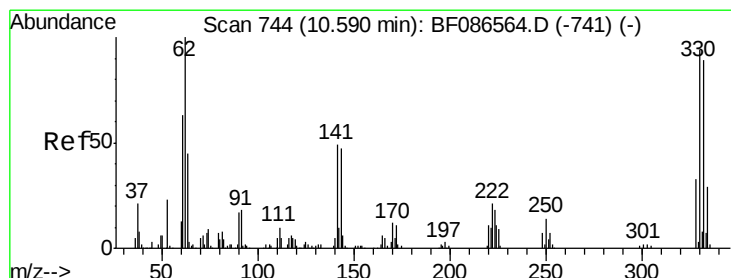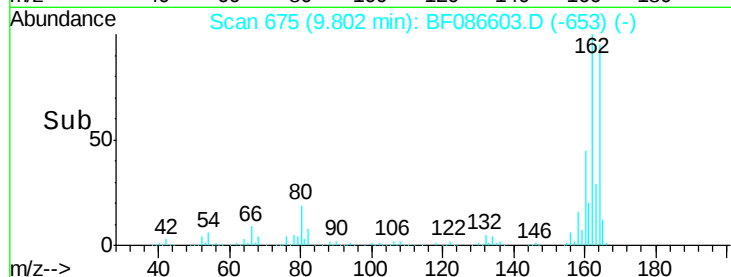
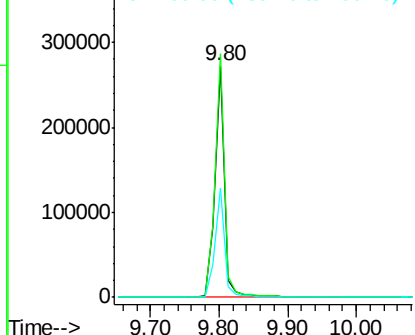



#41
2,4,6-Tribromophenol
Concen: 133.60 ng
RT: 10.59 min Scan# 744
Delta R.T. -0.05 min
Lab File: BF086603.D
Acq: 2 May 2016 7:28

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.6	79.0	118.4
141	36.2	31.2	46.8

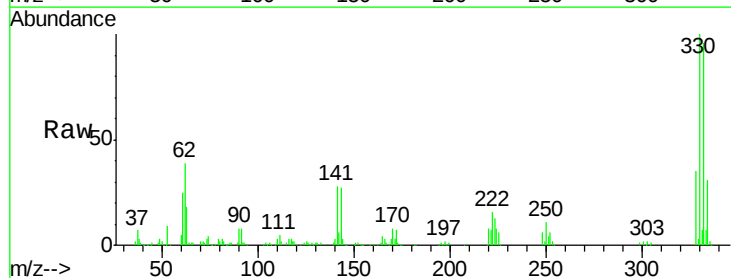

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

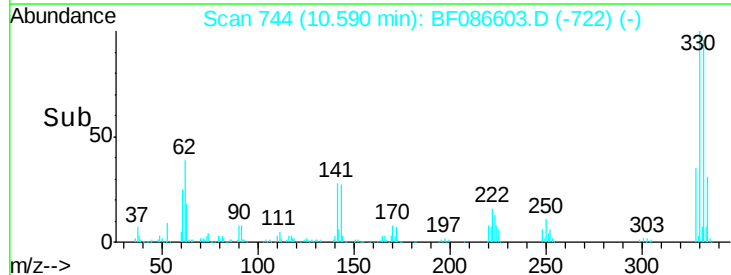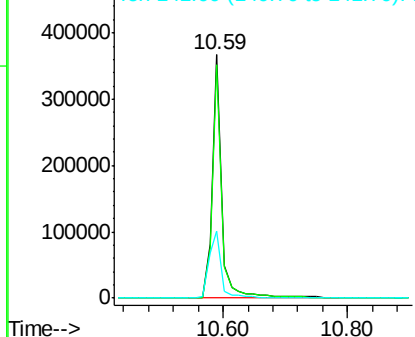


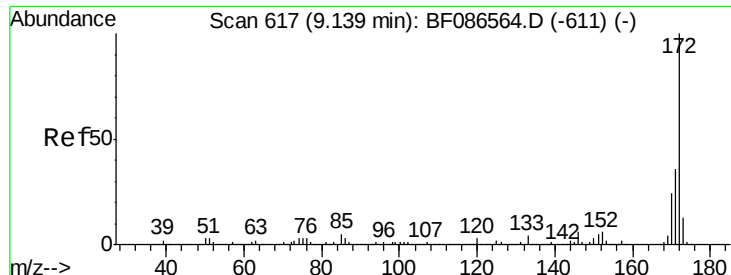




#44
 2-Fluorobiphenyl
 Concen: 94.42 ng
 RT: 9.13 min Scan# 616
 Delta R.T. -0.05 min
 Lab File: BF086603.D
 Acq: 2 May 2016 7:28

Instrument :
 BNA_F
 ClientSampleId :
 26WARD-2B-CS-4(0-10FTBGS)

Tgt Ion:172 Resp: 1449816
 Ion Ratio Lower Upper
 172 100
 171 36.4 29.0 43.6
 170 24.7 19.8 29.8

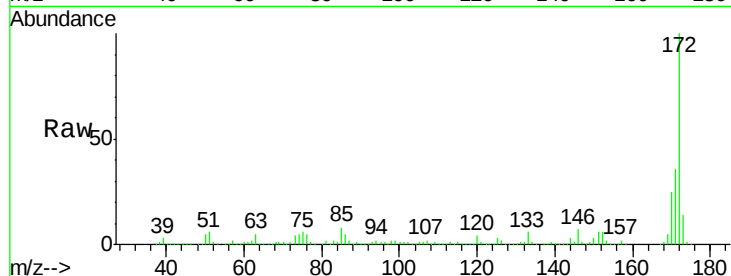


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

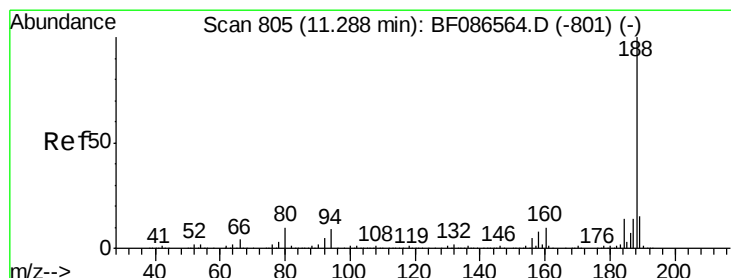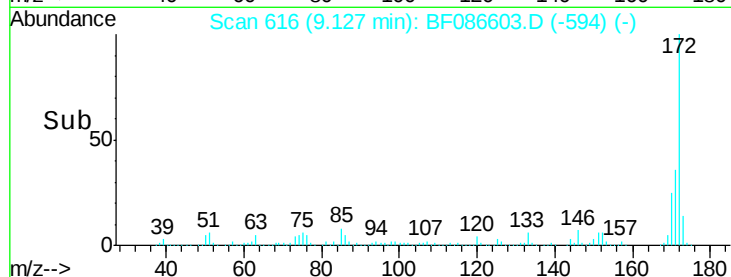
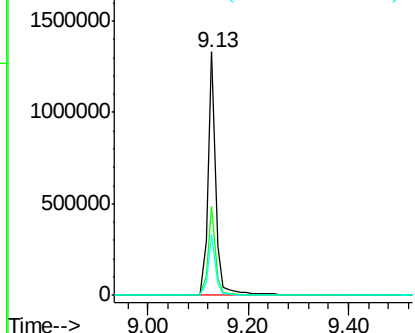



#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.28 min Scan# 804
 Delta R.T. -0.05 min
 Lab File: BF086603.D
 Acq: 2 May 2016 7:28

Tgt Ion:188 Resp: 516623
 Ion Ratio Lower Upper
 188 100
 94 12.7 6.8 10.2#
 80 13.7 7.1 10.7#

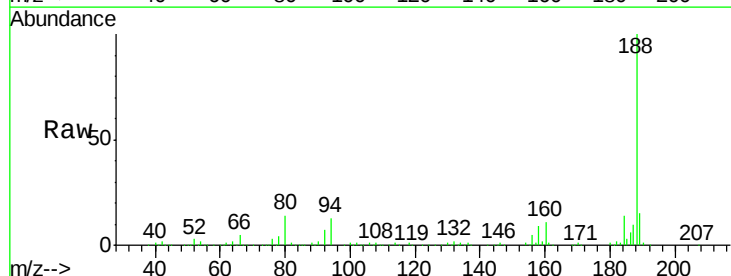

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

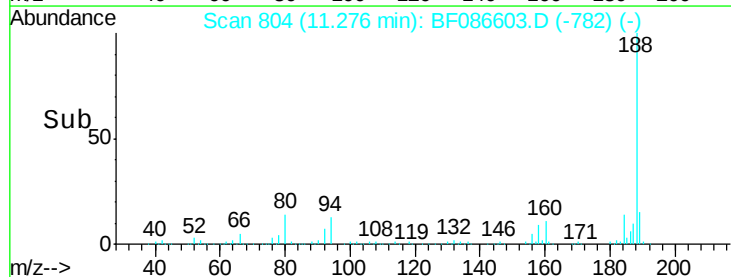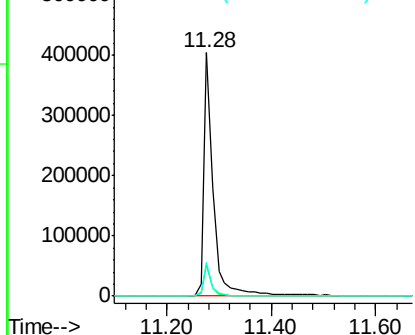

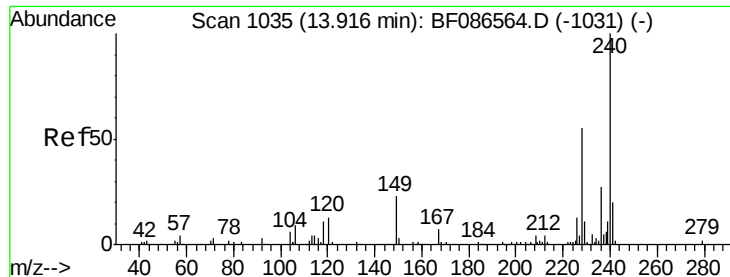

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.91 min Scan# 1034

Delta R.T. -0.06 min

Lab File: BF086603.D

Acq: 2 May 2016 7:28

Instrument :

BNA_F

ClientSampleId :

26WARD-2B-CS-4(0-10FTBGS)


Tgt Ion:240 Resp: 362257

Ion Ratio Lower Upper

240 100

120 14.4 11.2 16.8




236 26.9 21.2 31.8

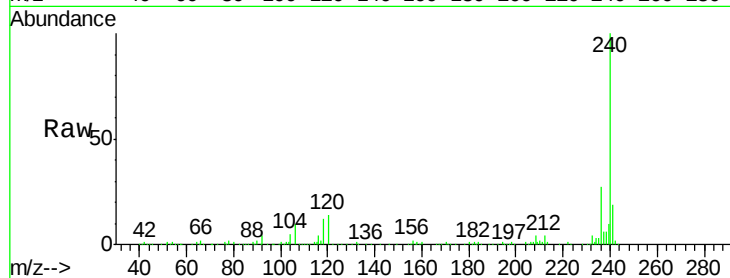

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

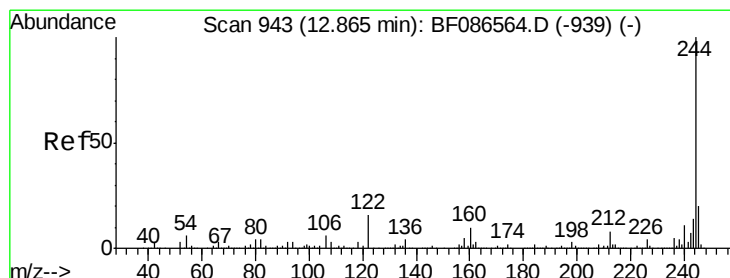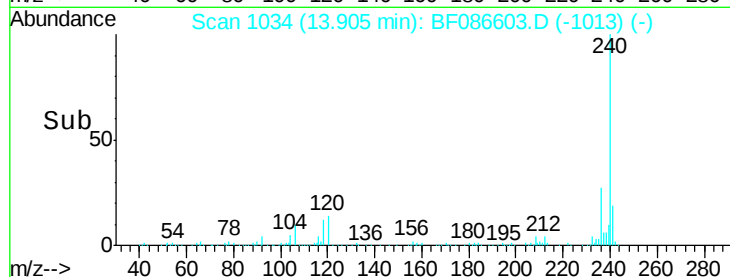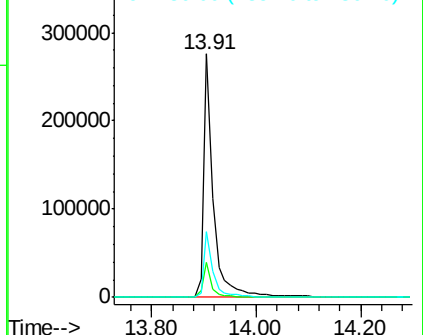

#78

Terphenyl-d14

Concen: 83.56 ng

RT: 12.86 min Scan# 943

Delta R.T. -0.05 min

Lab File: BF086603.D

Acq: 2 May 2016 7:28


Tgt Ion:244 Resp: 1373941

Ion Ratio Lower Upper

244 100

212 7.8 6.2 9.2



122 14.4 12.0 18.0



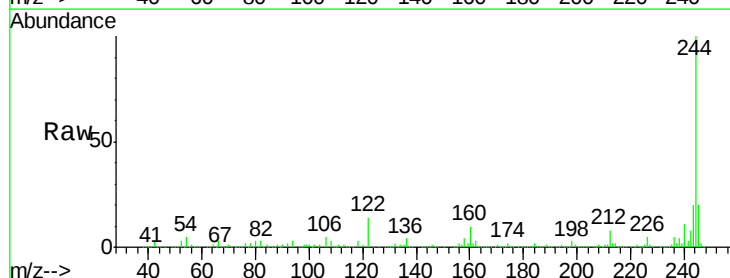


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

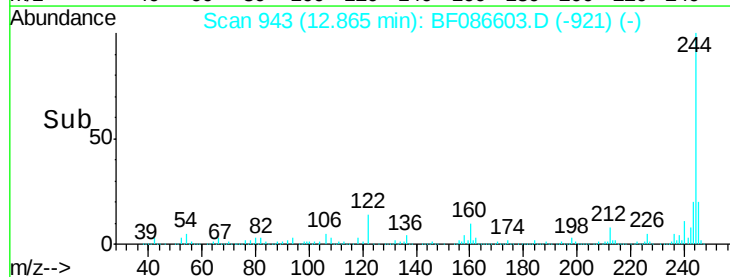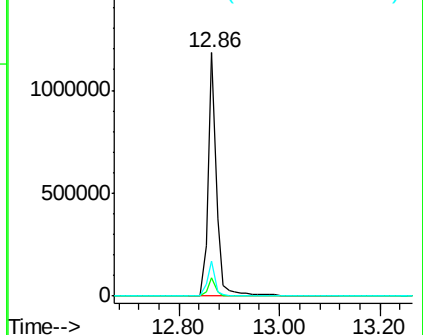

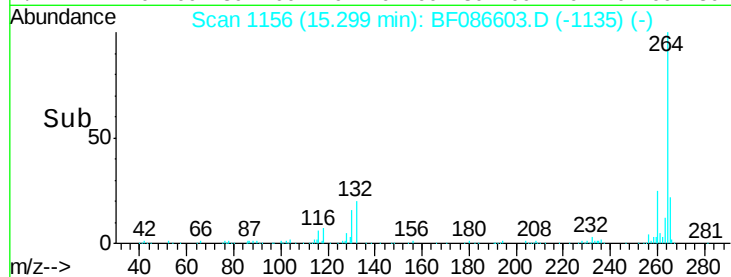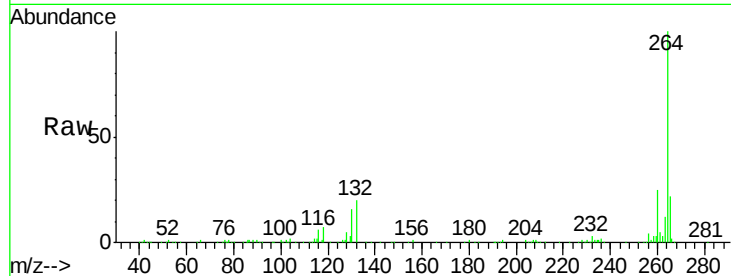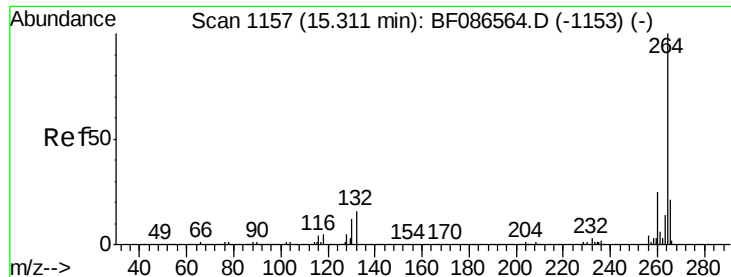

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.30 min Scan# 1156

Delta R.T. -0.06 min

Lab File: BF086603.D

Acq: 2 May 2016 7:28

Instrument :

BNA_F

ClientSampleId :

26WARD-2B-CS-4(0-10FTBGS)

Tgt Ion: 264 Resp: 324193

Ion Ratio Lower Upper

264 100

260 25.3 19.5 29.3

265 21.7 17.3 25.9

