


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050116\
 Data File : BF086563.D
 Acq On : 1 May 2016 10:54
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 27 14:20:52 2016

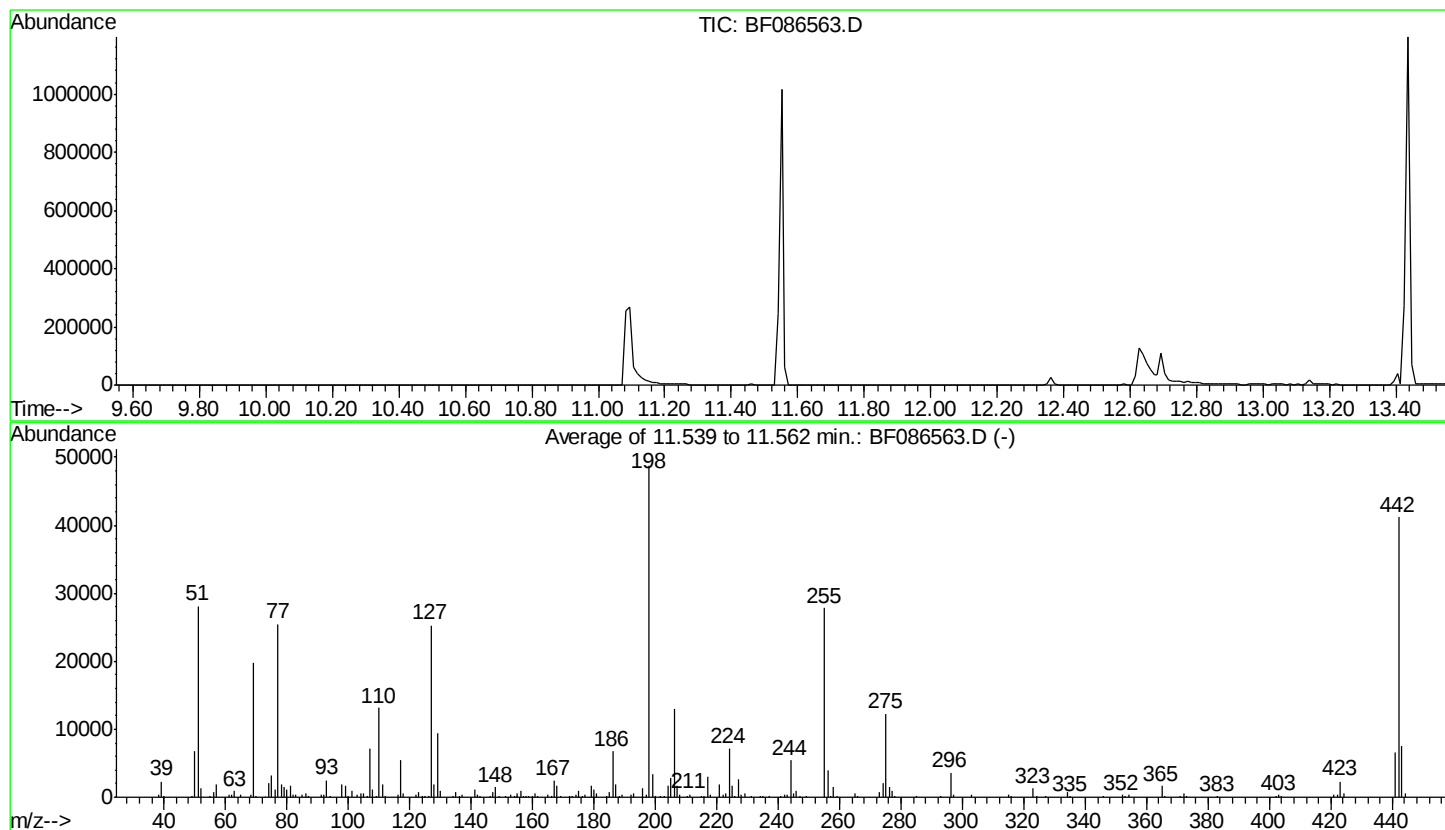

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.6	28090	PASS
68	69	0.00	2	1.7	331	PASS
69	198	0.00	100	40.4	19688	PASS
70	69	0.00	2	0.6	114	PASS
127	198	10	80	51.8	25242	PASS
197	198	0.00	2	0.7	346	PASS
198	198	100	100	100.0	48775	PASS
199	198	5	9	6.8	3320	PASS
275	198	10	60	25.1	12263	PASS
365	198	1	100	3.3	1622	PASS
441	442	0.01	24	15.9	6568	PASS
442	198	50	100	84.5	41216	PASS
443	442	15	24	18.4	7572	PASS