


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050116\
Data File : BF086589.D
Acq On : 2 May 2016 00:57
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 27 14:20:52 2016

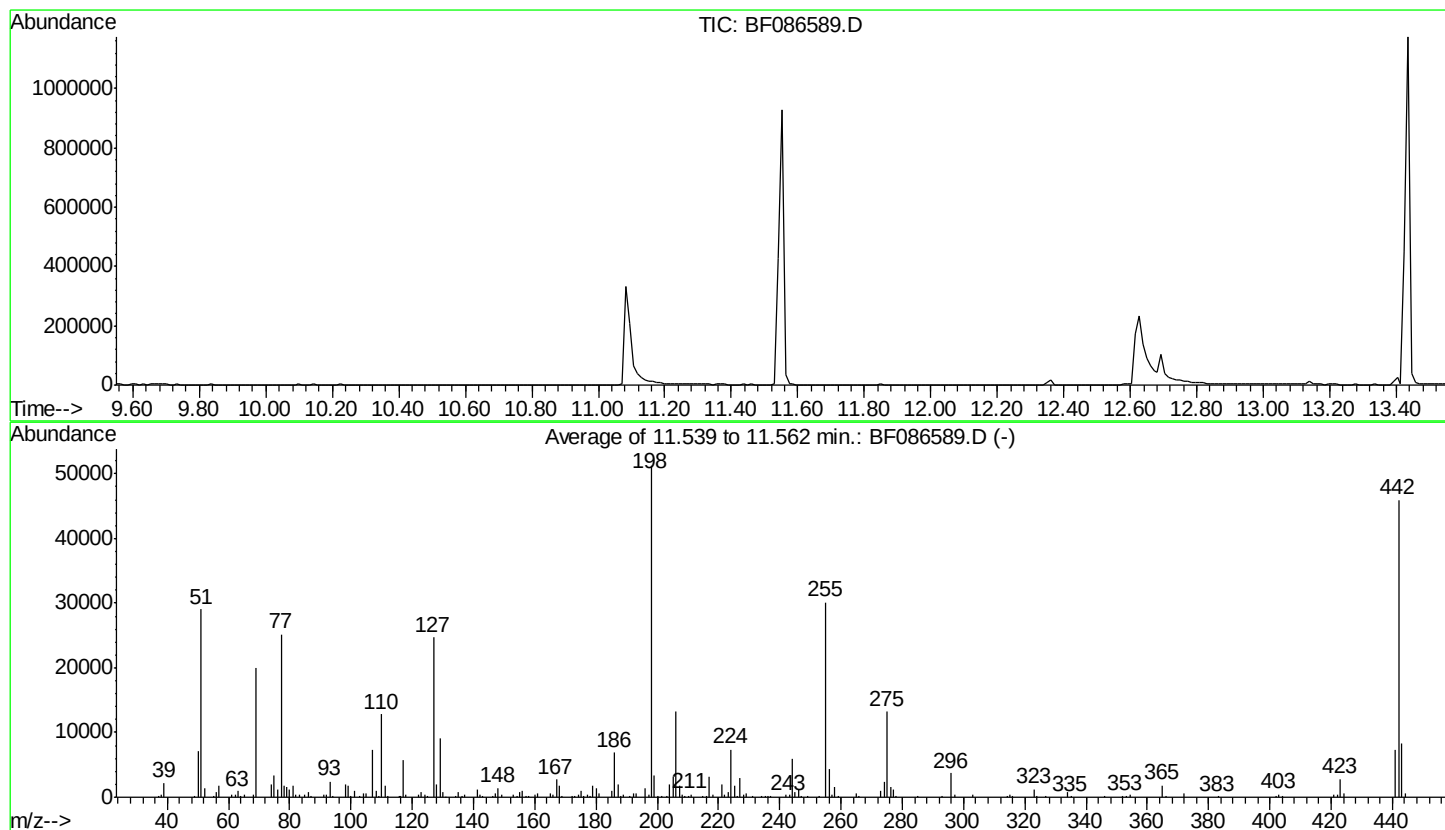

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.7	29078	PASS
68	69	0.00	2	1.7	342	PASS
69	198	0.00	100	39.0	19969	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	24657	PASS
197	198	0.00	2	0.9	465	PASS
198	198	100	100	100.0	51255	PASS
199	198	5	9	6.6	3403	PASS
275	198	10	60	25.7	13185	PASS
365	198	1	100	3.6	1865	PASS
441	442	0.01	24	16.0	7345	PASS
442	198	50	100	89.7	45960	PASS
443	442	15	24	18.2	8360	PASS