


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050117\
 Data File : BF094744.D
 Acq On : 1 May 2017 11:38
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 17 14:59:23 2017

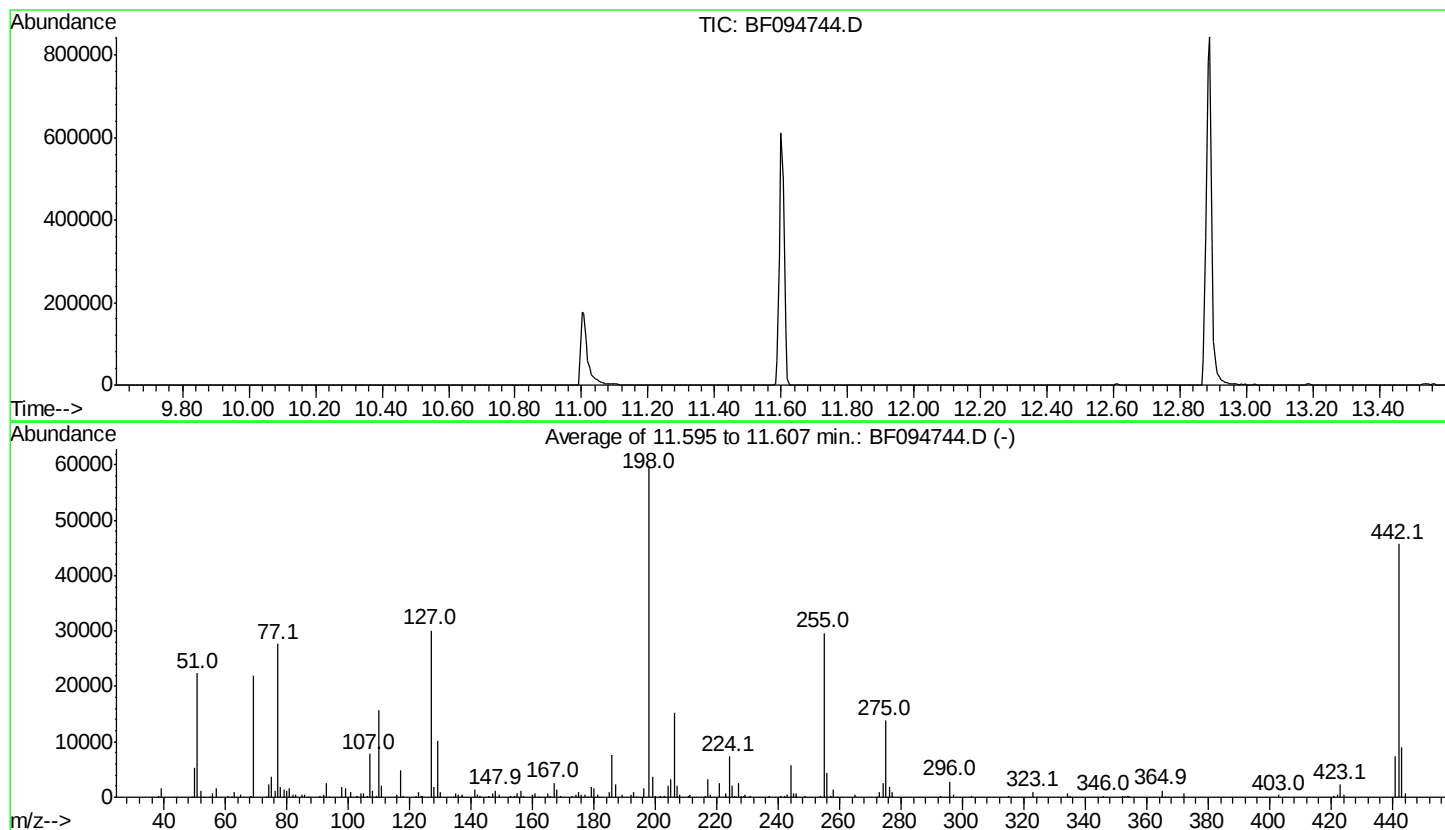

AutoFind: Scans 1642, 1643, 1644; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	22368	PASS
68	69	0.00	2	1.6	351	PASS
69	198	0.00	100	36.7	22000	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.4	30165	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59872	PASS
199	198	5	9	6.4	3821	PASS
275	198	10	60	23.0	13788	PASS
365	198	1	100	2.0	1186	PASS
441	442	0.01	24	16.1	7376	PASS
442	198	50	100	76.3	45709	PASS
443	442	15	24	19.9	9103	PASS