


Data Path : Z:\HPCHEM1\BNA_F\Data\BF050118\
 Data File : BF104975.D
 Acq On : 1 May 2018 11:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 01 16:13:08 2018

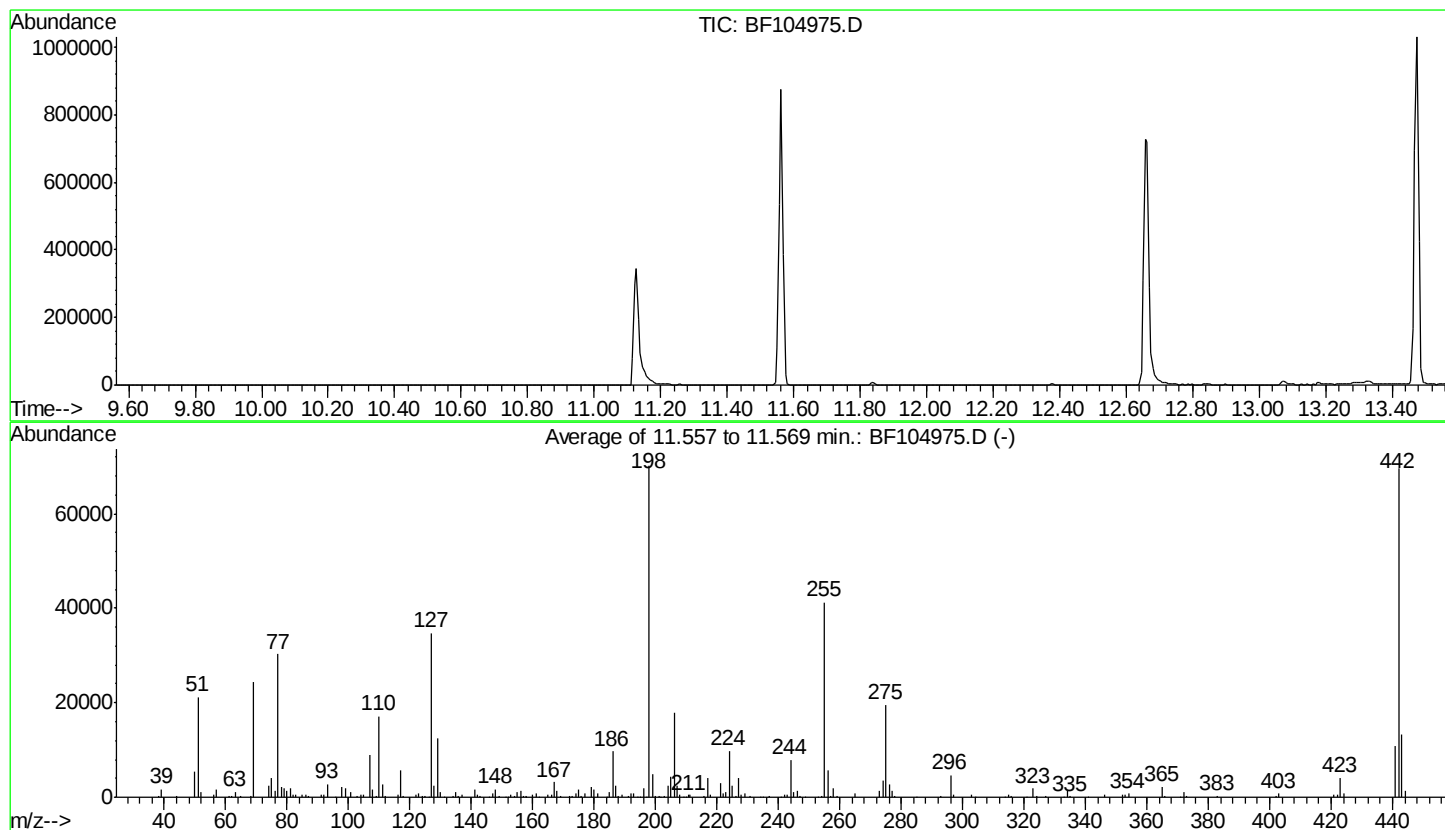

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	21204	PASS
68	69	0.00	2	1.5	363	PASS
69	198	0.00	100	34.6	24320	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.4	34712	PASS
197	198	0.00	2	0.2	115	PASS
198	198	100	100	100.0	70224	PASS
199	198	5	9	7.0	4920	PASS
275	198	10	60	27.8	19543	PASS
365	198	1	100	3.3	2289	PASS
441	443	0.01	100	80.5	10730	PASS
442	198	50	100	99.1	69597	PASS
443	442	15	24	19.1	13326	PASS