


Data Path : Z:\HPCHEM1\BNA_F\Data\BF050118\
 Data File : BF105002.D
 Acq On : 2 May 2018 00:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 01 16:13:08 2018

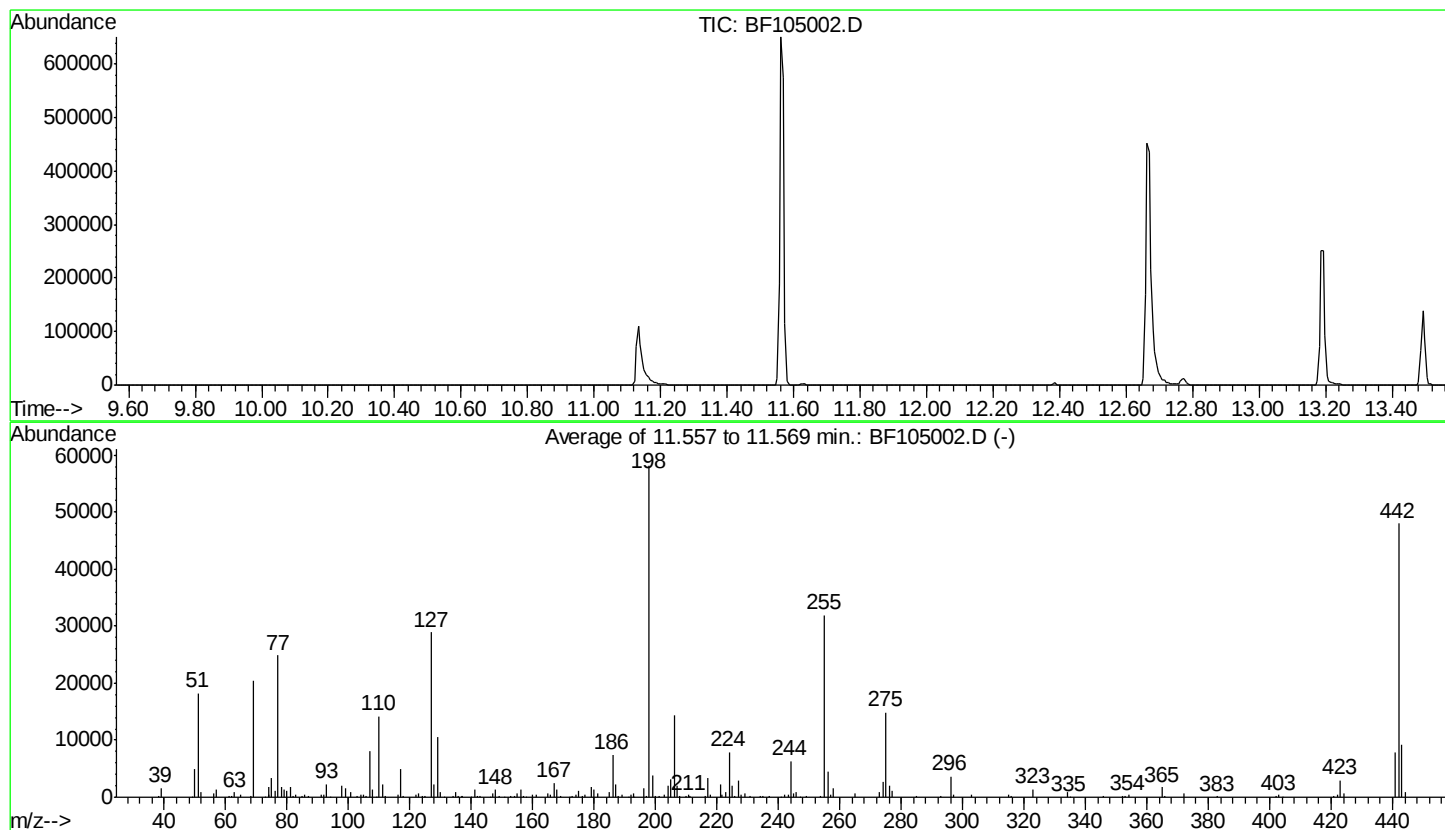

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	18232	PASS
68	69	0.00	2	1.6	327	PASS
69	198	0.00	100	35.0	20367	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	28908	PASS
197	198	0.00	2	0.4	206	PASS
198	198	100	100	100.0	58146	PASS
199	198	5	9	6.4	3734	PASS
275	198	10	60	25.5	14849	PASS
365	198	1	100	3.1	1792	PASS
441	443	0.01	100	85.7	7879	PASS
442	198	50	100	82.5	47963	PASS
443	442	15	24	19.2	9199	PASS