
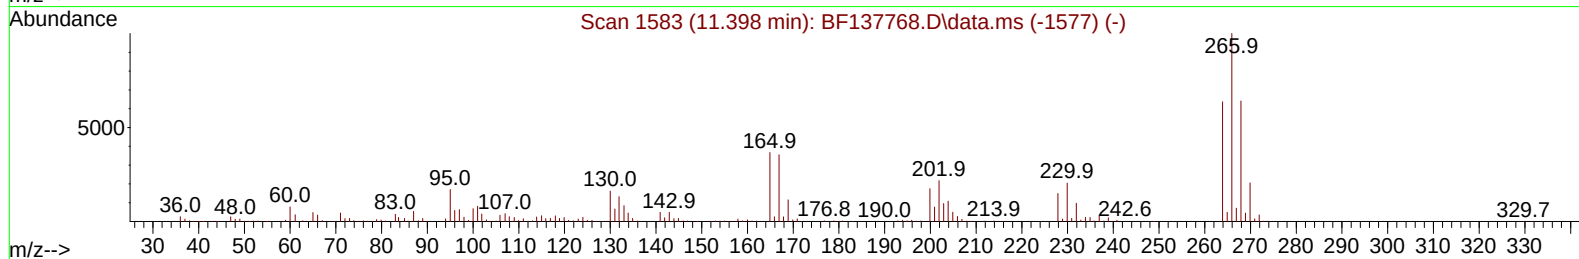
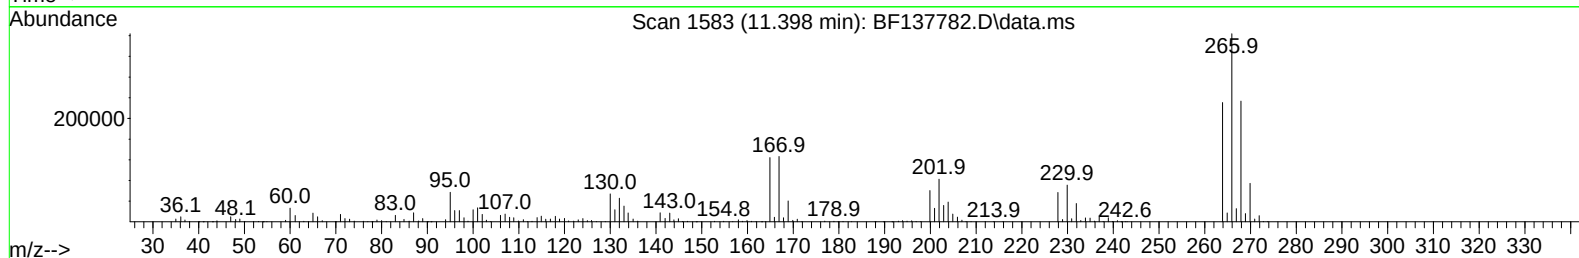


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
Data File : BF137782.D
Acq On : 01 May 2024 09:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 11:53:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

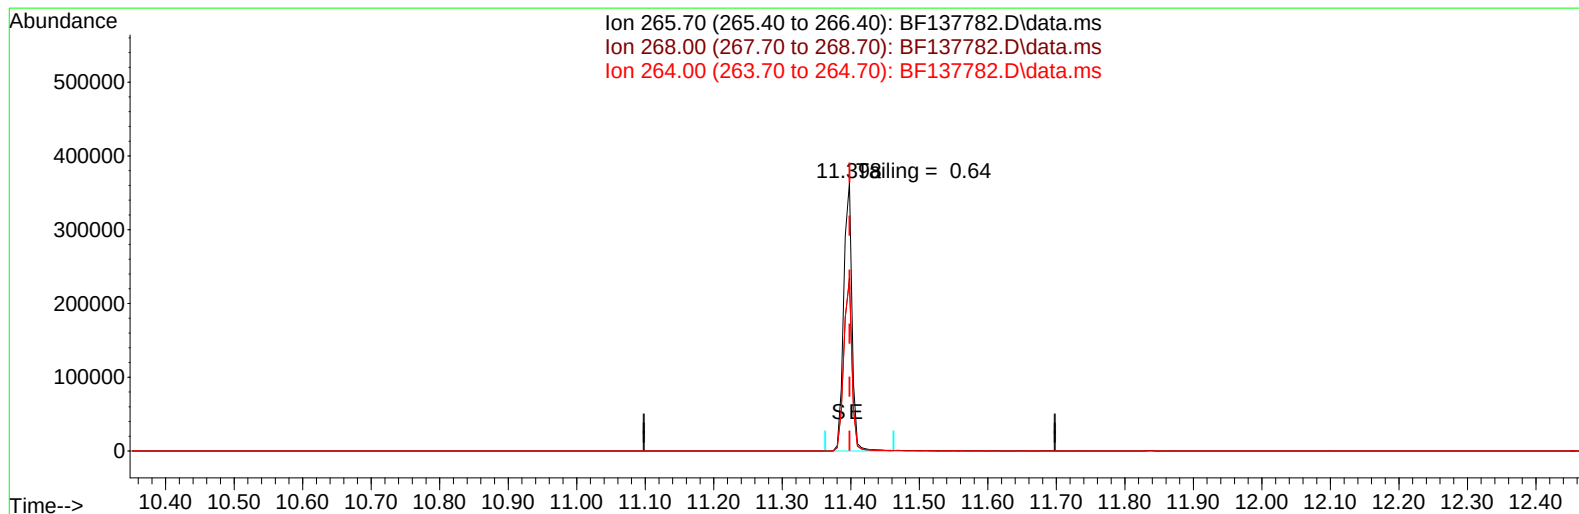

TIC: BF137782.D\data.ms

(70) Pentachlorophenol (C)




11.398min (-0.000) 448125.70 ng

response 305846

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.22
264.00	63.70	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
Data File : BF137782.D
Acq On : 01 May 2024 09:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 11:53:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

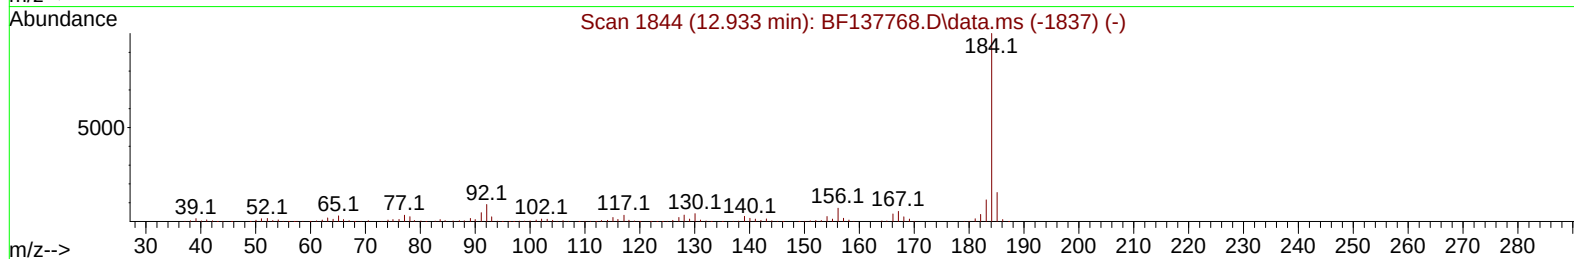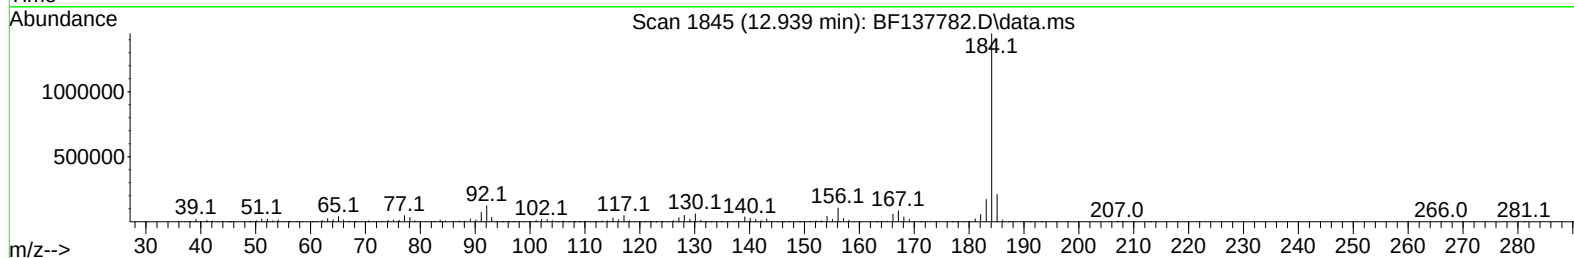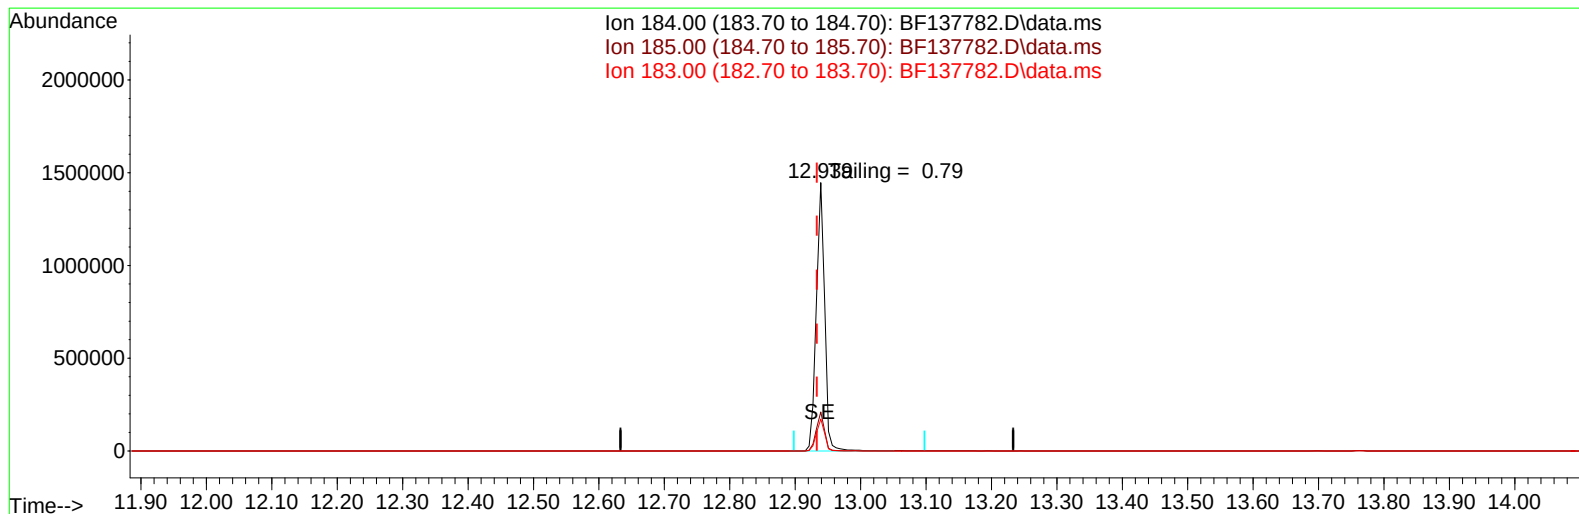

TIC: BF137782.D\data.ms

(77) Benzidine

12.939min (+ 0.006) 256256.71 ng

response 1280152

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.58
183.00	11.50	11.92
0.00	0.00	0.00