

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
 Data File : BF137784.D
 Acq On : 01 May 2024 10:41
 Operator : CG\JU
 Sample : PB160574BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB160574BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137784.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.146	7	10	27	rVB	222436	302495	3.19%	0.585%
2	5.692	607	613	616	rBV	5718676	6317096	66.65%	12.217%
3	6.675	773	780	783	rBV	5463219	6210717	65.53%	12.011%
4	7.057	841	845	848	rBV	1726440	1359811	14.35%	2.630%
5	7.622	935	941	944	rBV	3821353	4193760	44.25%	8.110%
6	8.339	1058	1063	1067	rBV	2015433	1845072	19.47%	3.568%
7	9.416	1240	1246	1249	rBV	7614834	8442126	89.07%	16.327%
8	10.104	1357	1363	1366	rBV	2633483	2238646	23.62%	4.329%
9	10.898	1492	1498	1501	rBV	5434684	5270296	55.60%	10.192%
10	11.598	1613	1617	1621	rBV	2614196	2369864	25.00%	4.583%
11	13.192	1883	1888	1891	rBV	8880672	9478243	100.00%	18.330%
12	14.251	2064	2068	2072	rBV	2300869	2037361	21.50%	3.940%
13	15.827	2330	2336	2346	rBV	1228106	1642553	17.33%	3.177%




Sum of corrected areas: 51708040

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
Data File : BF137784.D
Acq On : 01 May 2024 10:41
Operator : CG\JU
Sample : PB160574BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160574BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

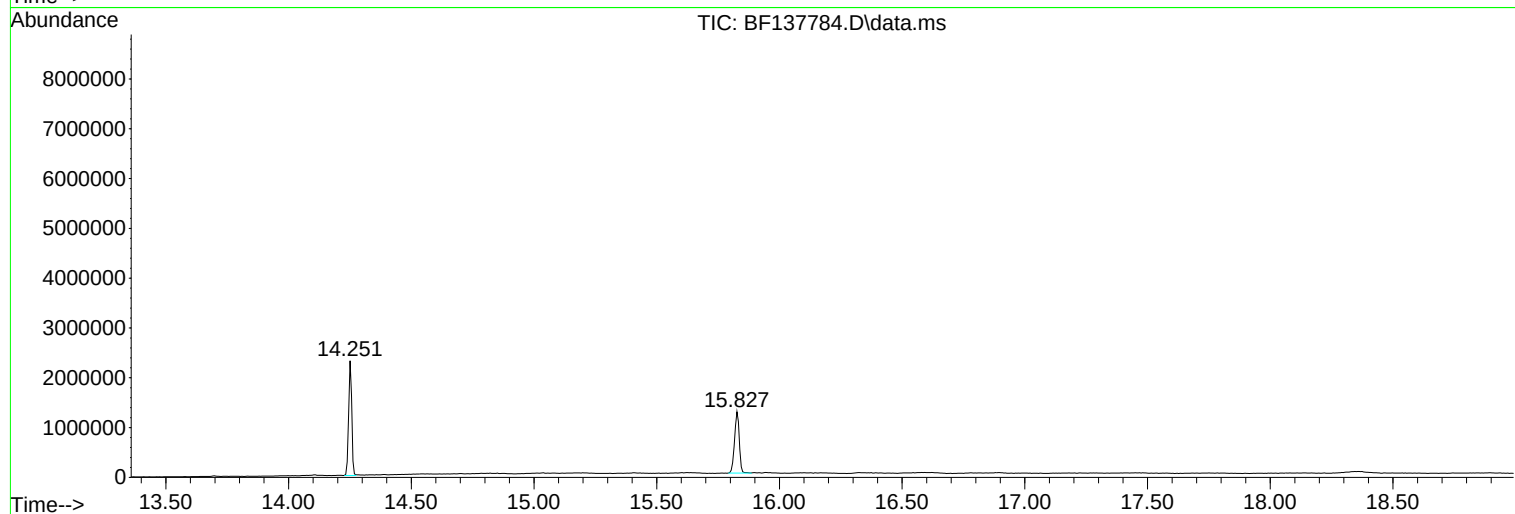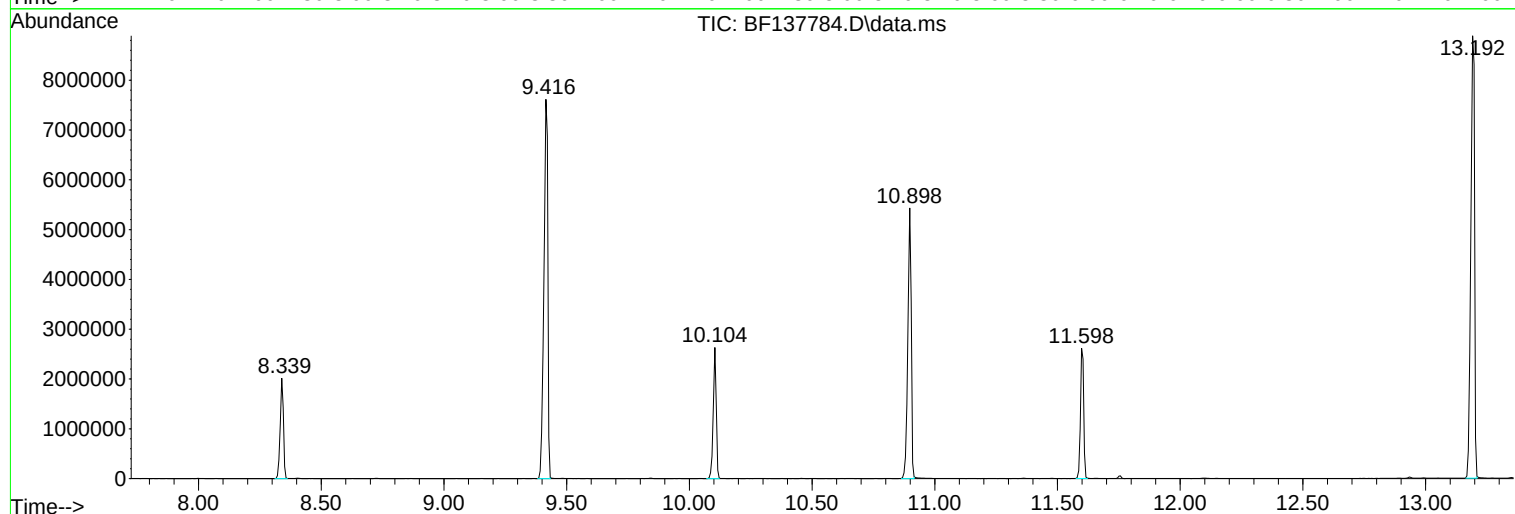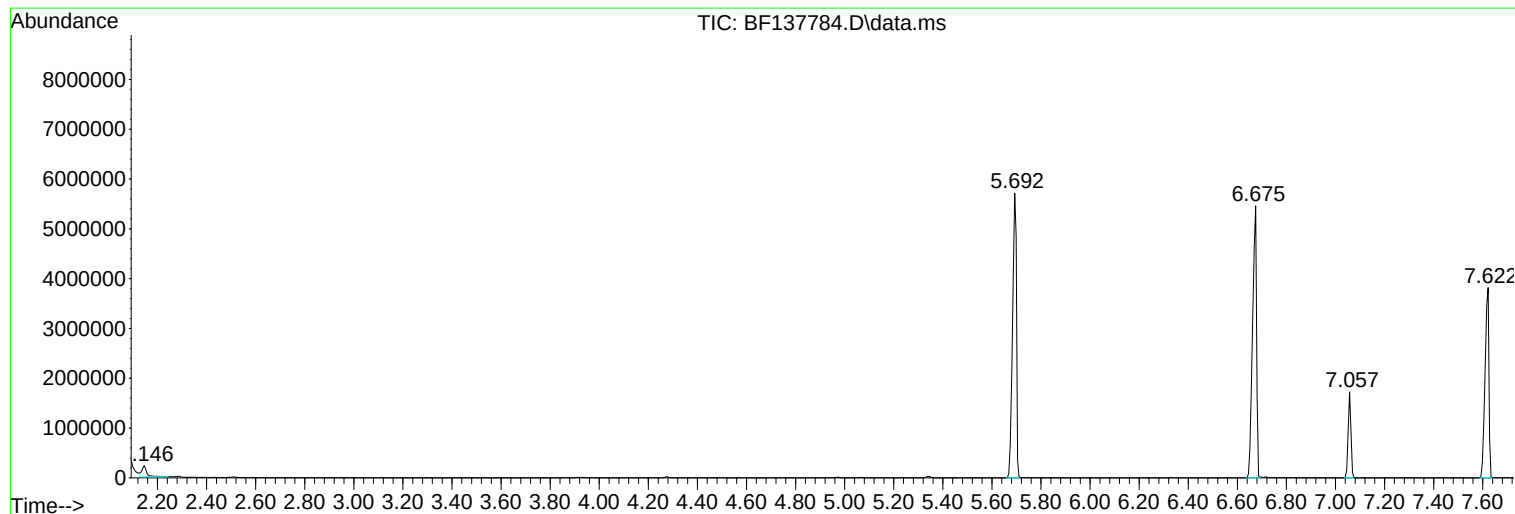

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
Data File : BF137784.D
Acq On : 01 May 2024 10:41
Operator : CG\JU
Sample : PB160574BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160574BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown2.146 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.146	4.45 ng	302495	1,4-Dichlorobenzene-d4	7.057

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2,2-dimethoxy-	104	C5H12O2	000077-76-9	39
2			1-Hexen-4-ol, 1-chloro-3,5-dimet...	162	C8H15ClO	100244-09-5	9
3			Propane, 2-methoxy-2-methyl-	88	C5H12O	001634-04-4	9
4			1,3-Dioxolane, 2-pentadecyl-	284	C18H36O2	004360-57-0	9
5			1-Hexanamine	101	C6H15N	000111-26-2	9

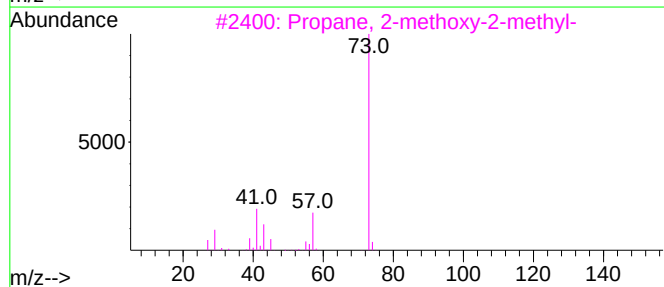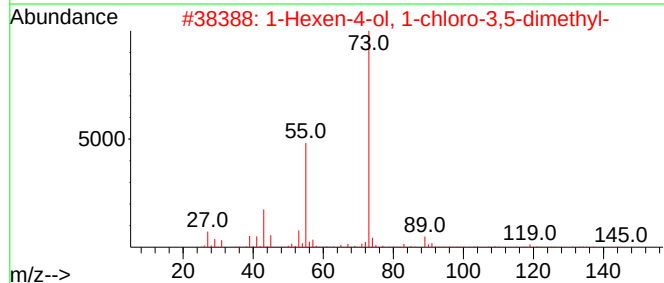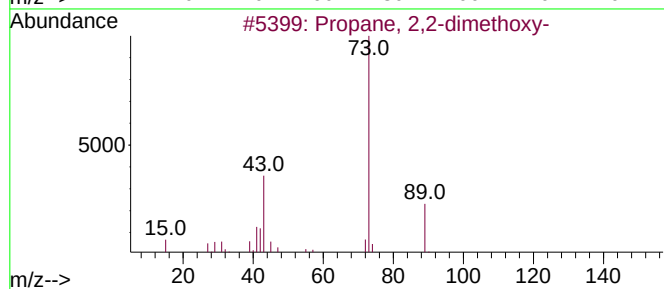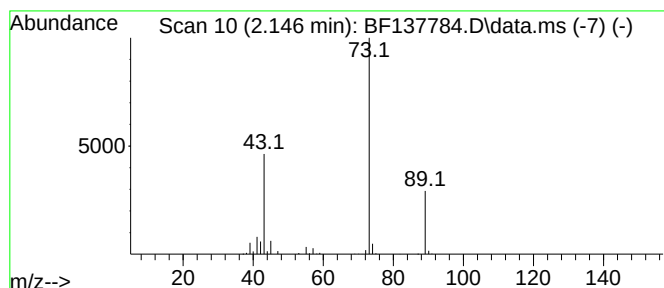

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
Data File : BF137784.D
Acq On : 01 May 2024 10:41
Operator : CG\JU
Sample : PB160574BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160574BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown2.146	2.146	4.5	ng	302495	1	7.057	1359810	20.0