

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
Data File : BF137786.D
Acq On : 01 May 2024 11:42
Operator : CG\JU
Sample : PB160621BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160621BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137786.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.693	608	613	616	rBV	5593164	6299142	67.32%	12.208%
2	6.675	773	780	783	rBV	5453505	6228823	66.57%	12.071%
3	7.057	841	845	848	rBV	1766436	1374324	14.69%	2.663%
4	7.616	934	940	943	rBV	3639767	4255315	45.48%	8.247%
5	8.339	1058	1063	1067	rBV	2028964	1879990	20.09%	3.643%
6	9.416	1240	1246	1249	rBV	7839958	8553814	91.42%	16.577%
7	10.104	1357	1363	1366	rBV	2612990	2266507	24.22%	4.392%
8	10.898	1491	1498	1501	rBV	5639597	5433666	58.07%	10.530%
9	11.598	1611	1617	1621	rBV	2778081	2357956	25.20%	4.570%
10	13.192	1882	1888	1891	rBV	9472792	9356949	100.00%	18.134%
11	14.251	2064	2068	2071	rBV	2218434	1963236	20.98%	3.805%
12	15.821	2329	2335	2342	rBV	1185554	1629778	17.42%	3.159%


Sum of corrected areas: 51599500

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
Data File : BF137786.D
Acq On : 01 May 2024 11:42
Operator : CG\JU
Sample : PB160621BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160621BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

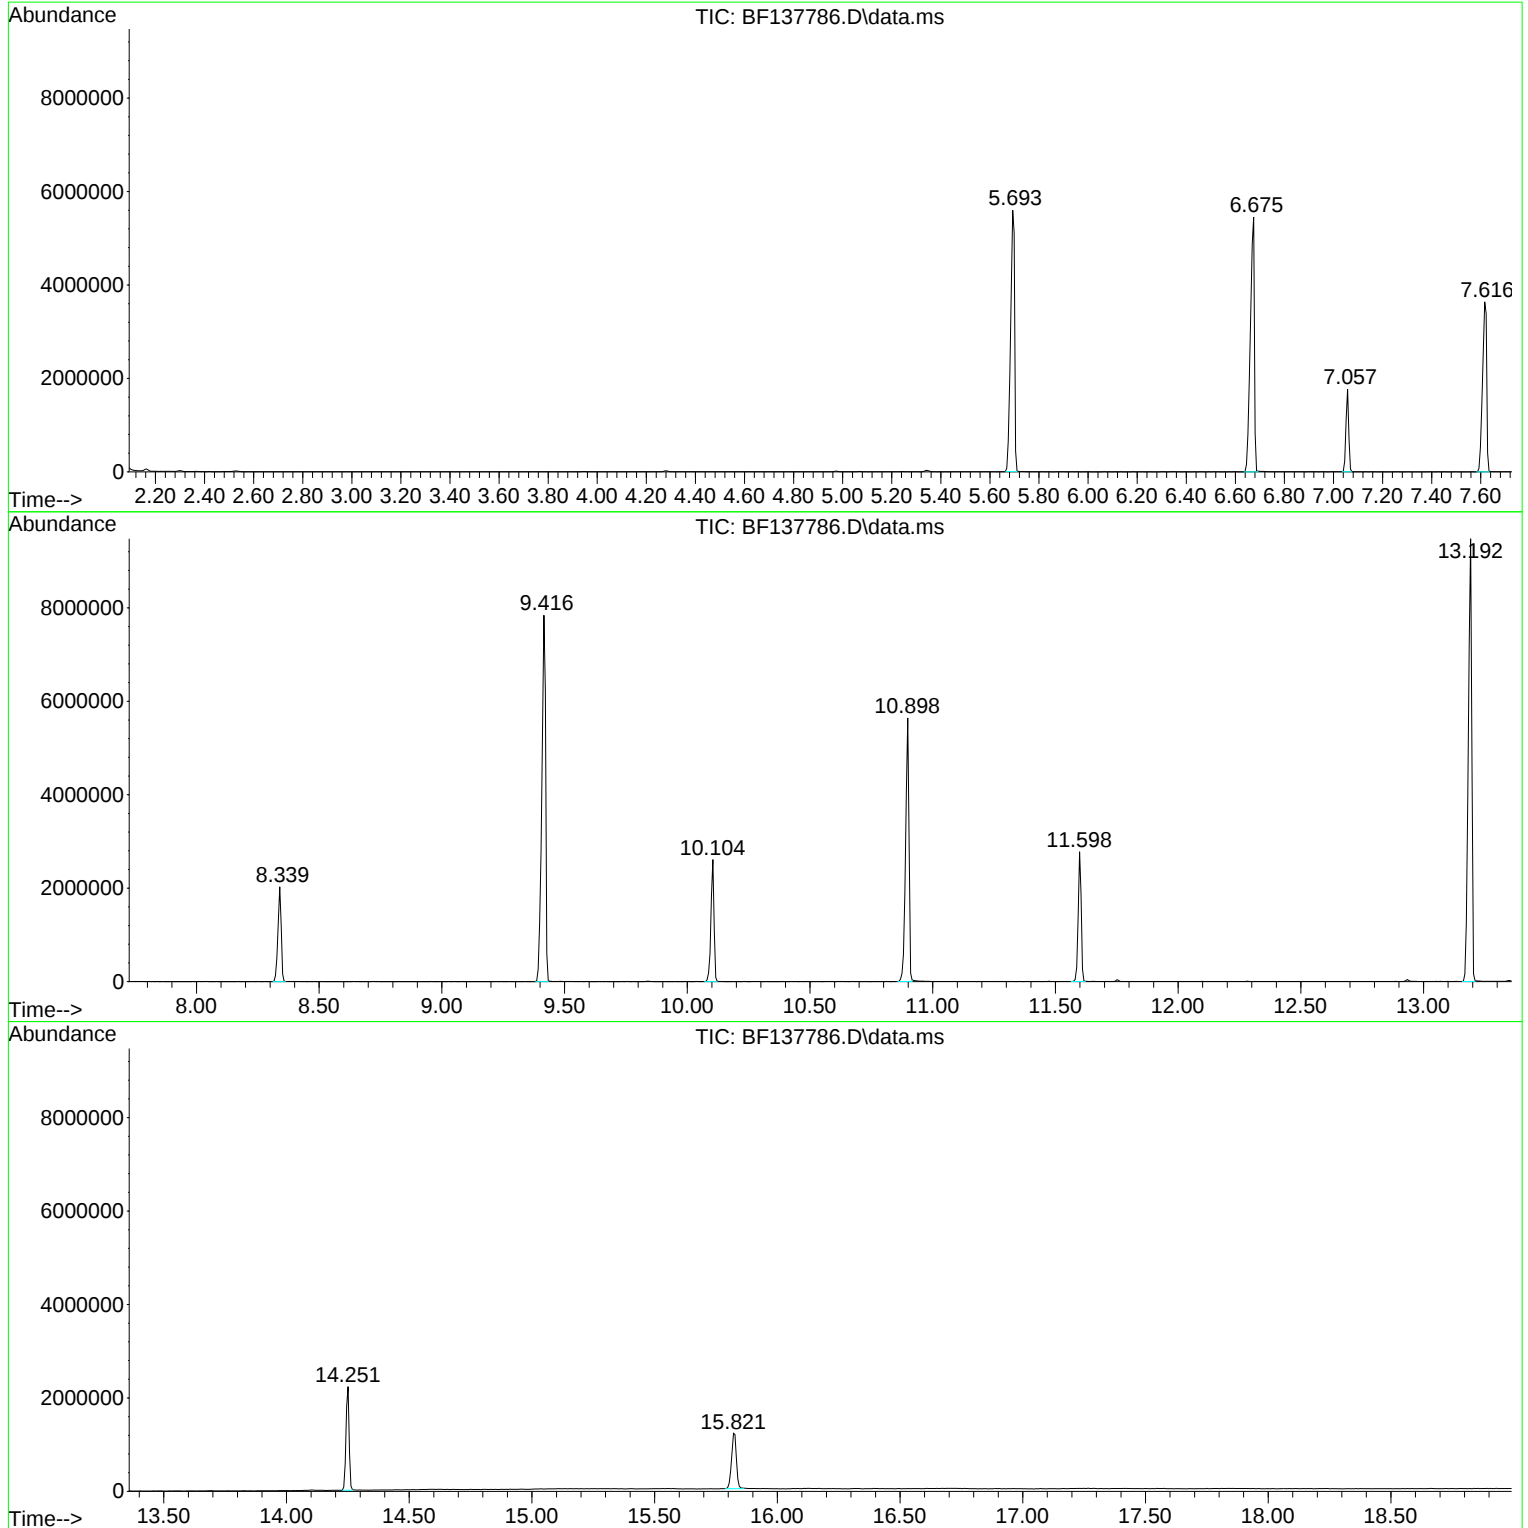

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
Data File : BF137786.D
Acq On : 01 May 2024 11:42
Operator : CG\JU
Sample : PB160621BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160621BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
Data File : BF137786.D
Acq On : 01 May 2024 11:42
Operator : CG\JU
Sample : PB160621BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160621BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------