

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
Data File : BF137788.D
Acq On : 01 May 2024 12:43
Operator : CG\JU
Sample : PB160608BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160608BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137788.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.692	607	613	616	rBV	5538862	5607636	66.78%	11.983%
2	6.675	773	780	782	rBV	4692377	5570247	66.33%	11.903%
3	7.057	841	845	848	rBV	1684387	1319514	15.71%	2.820%
4	7.616	935	940	943	rBV	3379949	3739422	44.53%	7.991%
5	8.339	1058	1063	1067	rBV	2080767	1838069	21.89%	3.928%
6	9.416	1240	1246	1249	rBV	7678121	7538886	89.77%	16.109%
7	10.104	1357	1363	1366	rBV	2650173	2240637	26.68%	4.788%
8	10.898	1492	1498	1501	rBV	4944844	4674870	55.67%	9.989%
9	11.598	1613	1617	1621	rBV	2852683	2354186	28.03%	5.031%
10	11.751	1640	1643	1647	rVB	109390	86674	1.03%	0.185%
11	13.192	1883	1888	1891	rBV	8504620	8397635	100.00%	17.944%
12	14.251	2064	2068	2071	rBV	2188204	1899211	22.62%	4.058%
13	15.821	2329	2335	2343	rBV	1137294	1531100	18.23%	3.272%


Sum of corrected areas: 46798087

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
Data File : BF137788.D
Acq On : 01 May 2024 12:43
Operator : CG\JU
Sample : PB160608BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160608BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

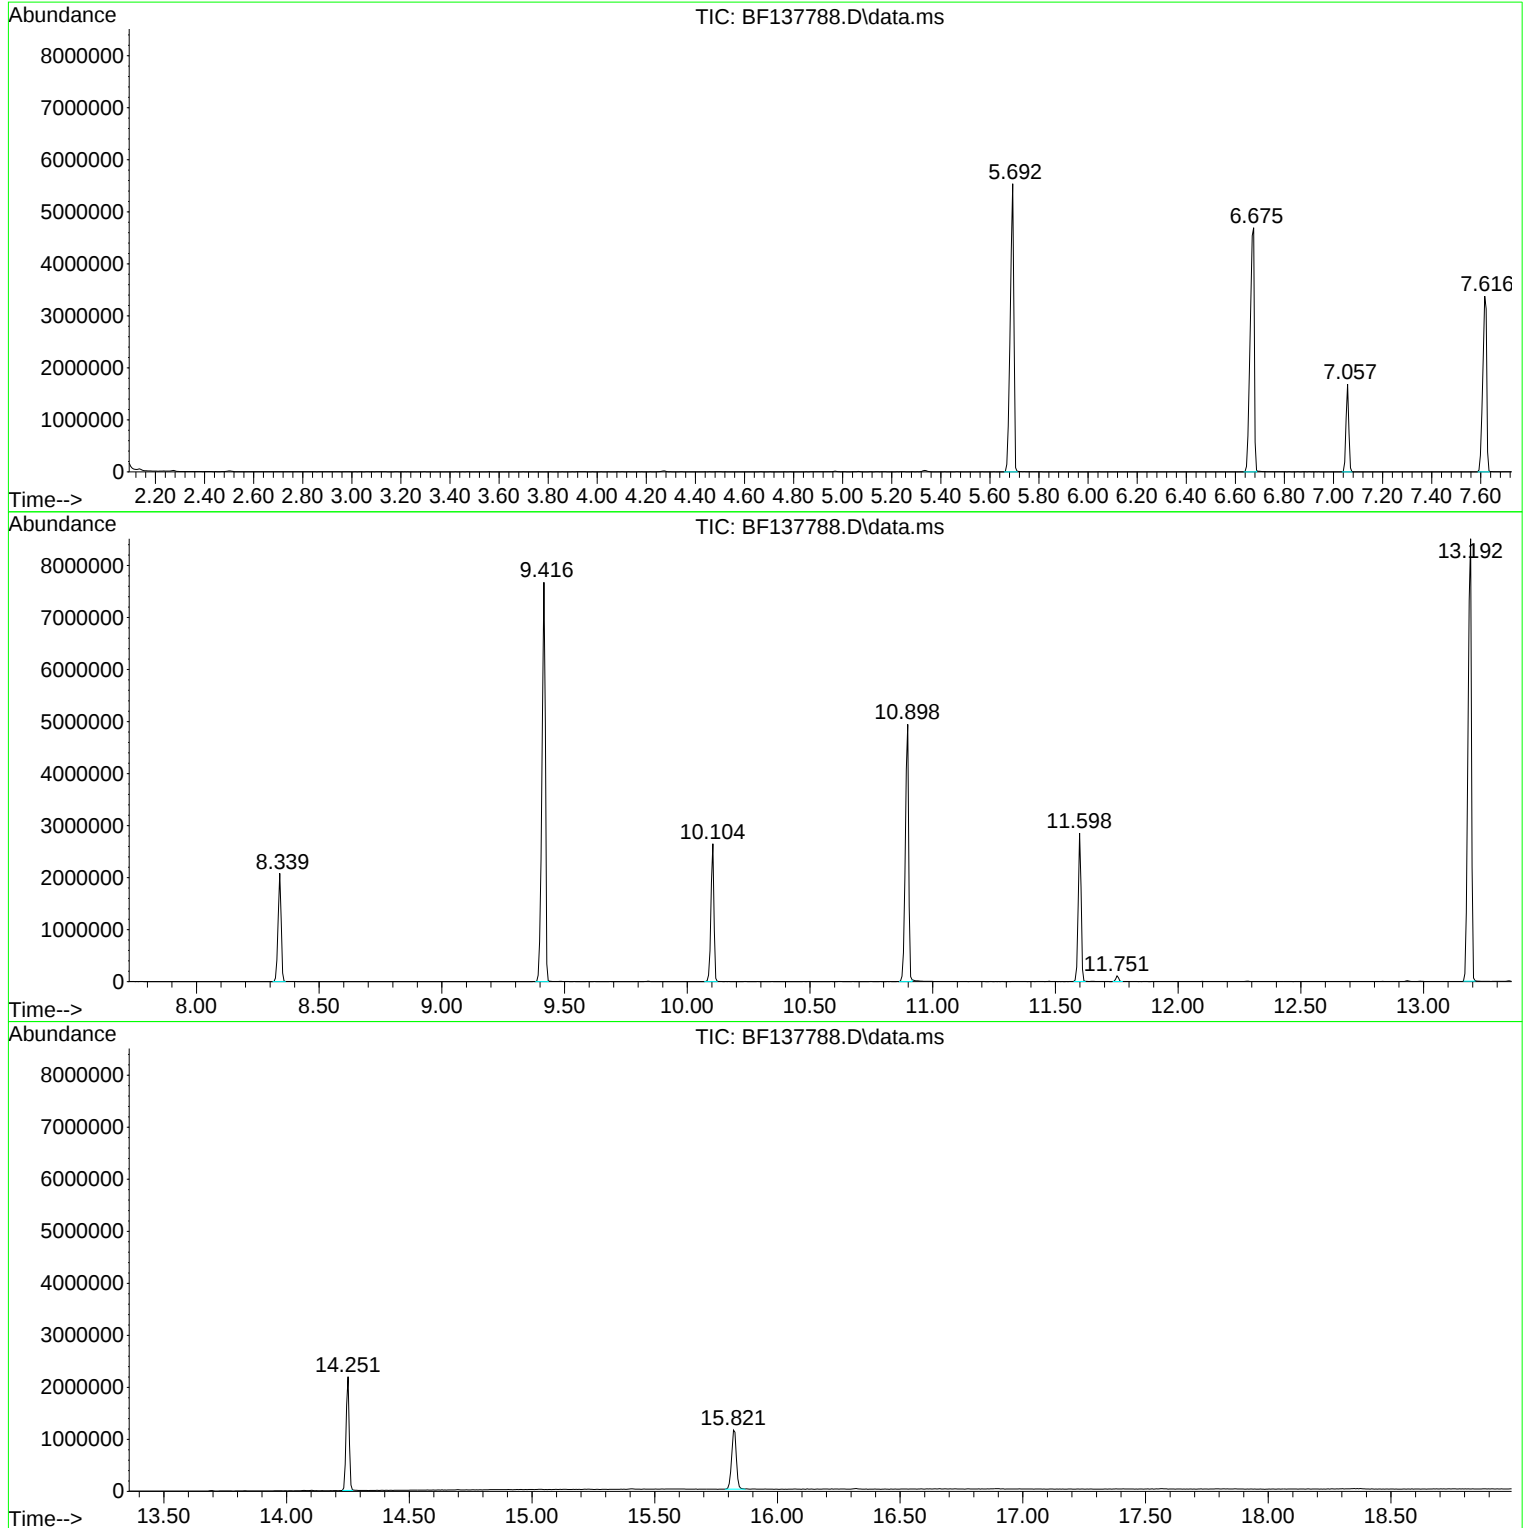

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
Data File : BF137788.D
Acq On : 01 May 2024 12:43
Operator : CG\JU
Sample : PB160608BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160608BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
Data File : BF137788.D
Acq On : 01 May 2024 12:43
Operator : CG\JU
Sample : PB160608BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB160608BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------