


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
Data File : BF137782.D
Acq On : 01 May 2024 09:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 03:25:08 2024

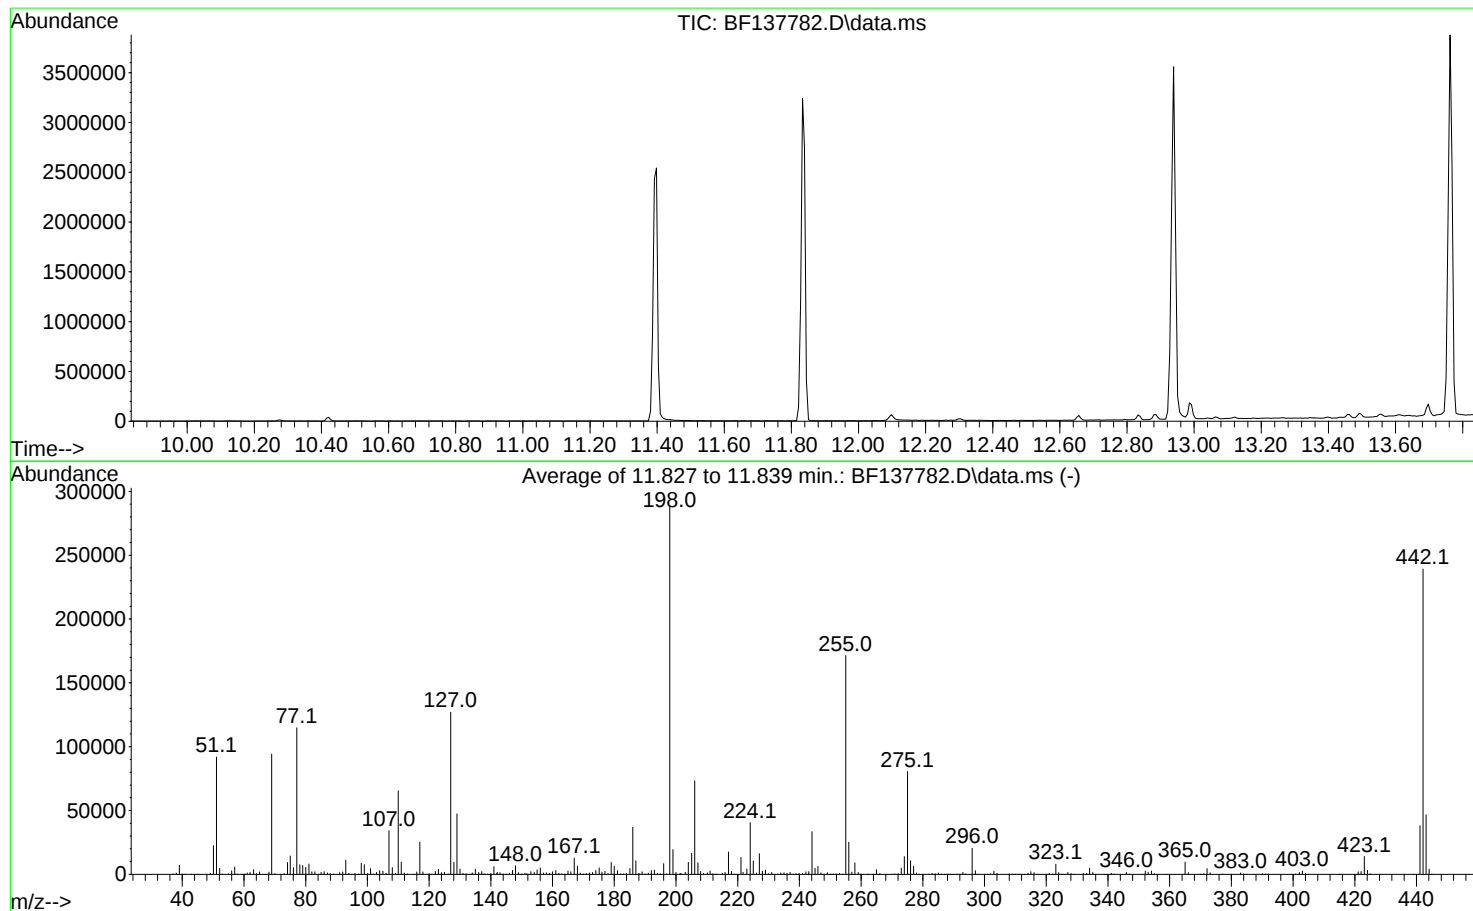

AutoFind: Scans 1656, 1657, 1658; Background Corrected with Scan 1651

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	31.9	91835	PASS
68	69	0.00	2	1.9	1806	PASS
69	198	0.00	100	32.7	94101	PASS
70	69	0.00	2	0.6	533	PASS
127	198	10	80	44.1	127040	PASS
197	198	0.00	2	0.1	333	PASS
198	198	100	100	100.0	288192	PASS
199	198	5	9	6.8	19454	PASS
275	198	10	60	27.9	80547	PASS
365	198	1	100	3.3	9564	PASS
441	198	0.01	100	13.2	38056	PASS
442	442	50	100	100.0	239120	PASS
443	442	15	24	19.5	46619	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/1/2024	BNA_F	<u>BF1376782.D</u>
Compound Name	Response	Retention Time
DDT	656435	13.762
DDD	12436	13.462
DDE	1081	13.121
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13517	669952	2.02

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
Data File : BF137782.D
Acq On : 01 May 2024 09:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 01 11:53:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

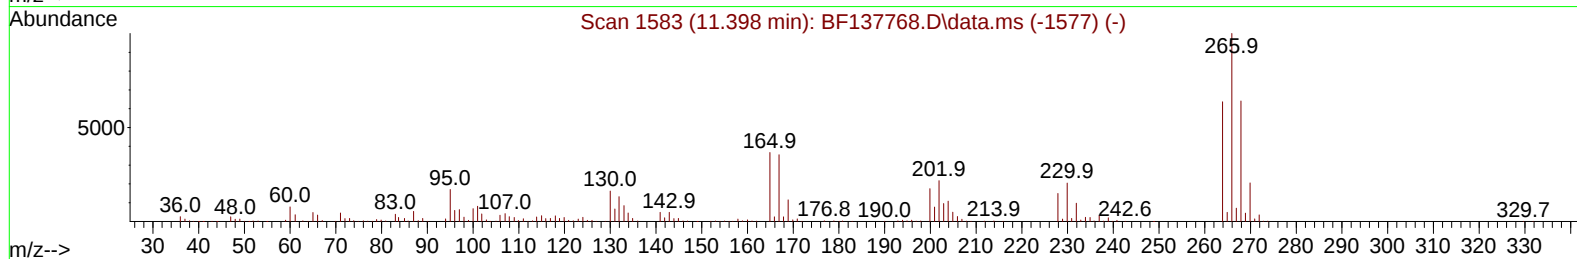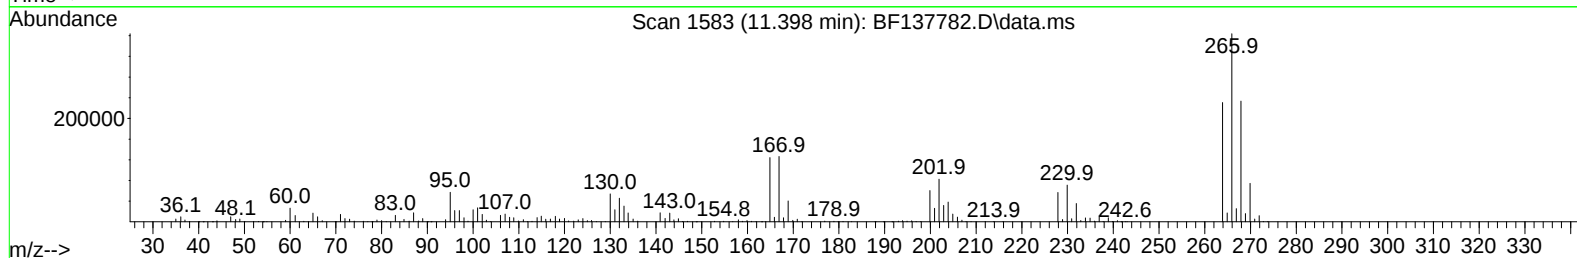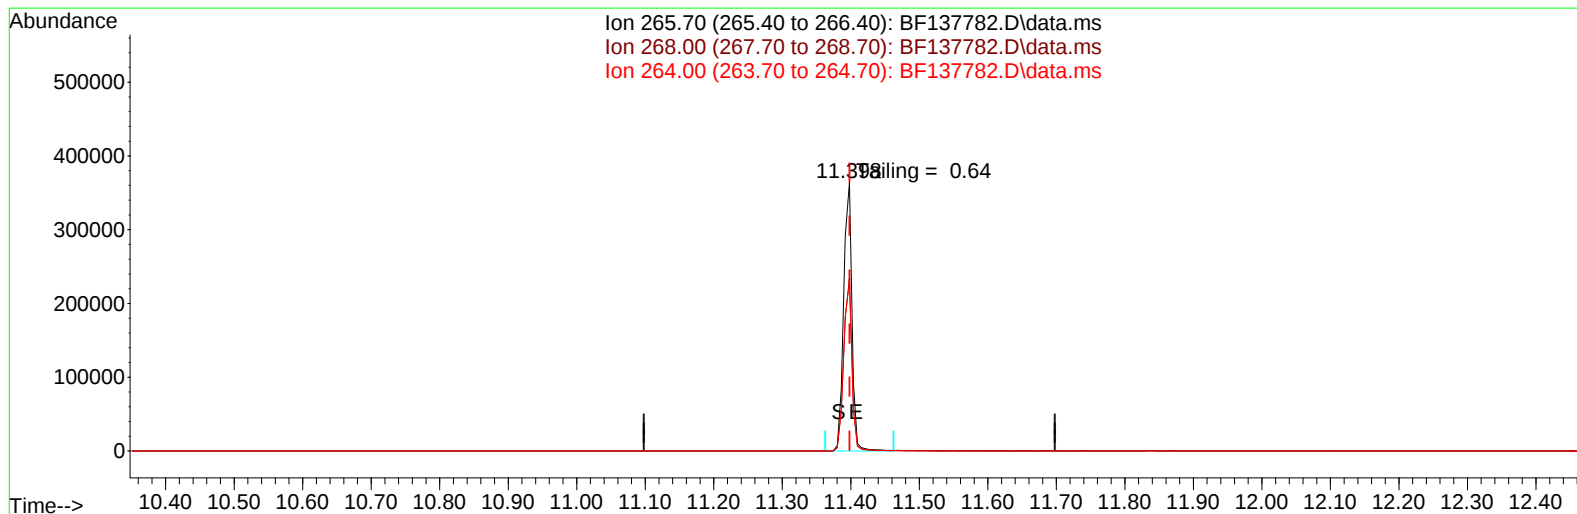

TIC: BF137782.D\data.ms

(70) Pentachlorophenol (C)

11.398min (-0.000) 448125.70 ng




response 305846

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.22
264.00	63.70	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050124\
Data File : BF137782.D
Acq On : 01 May 2024 09:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 01 11:53:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

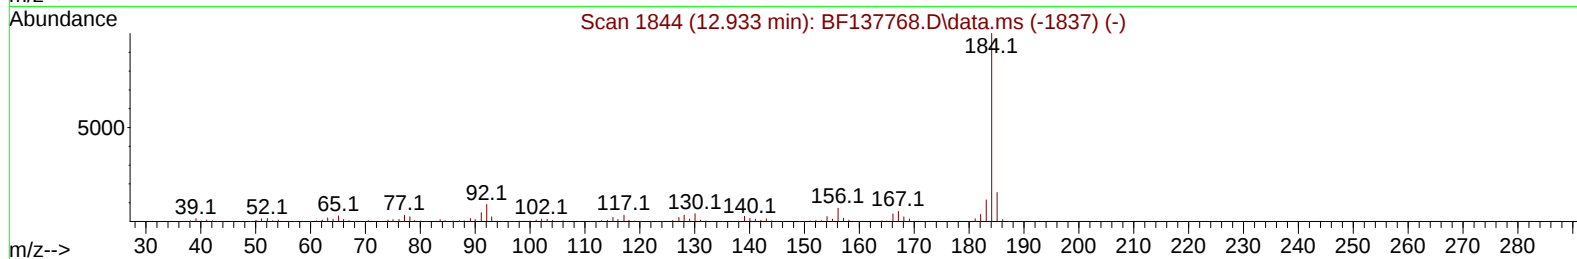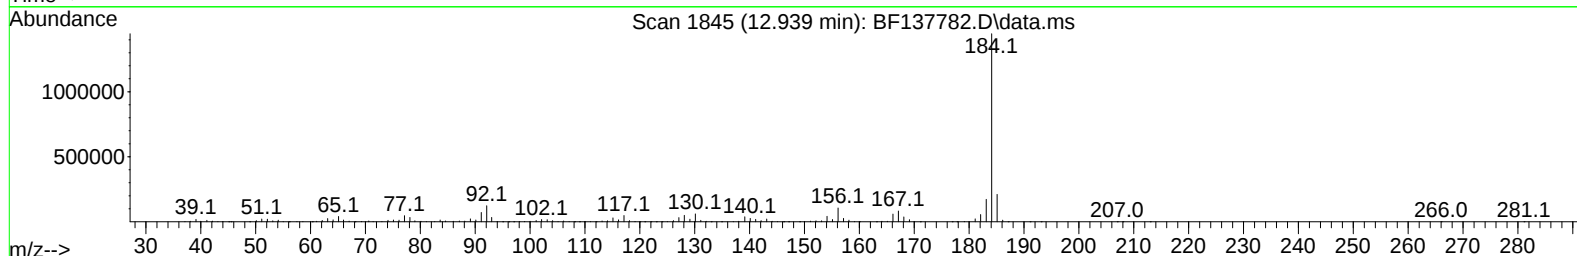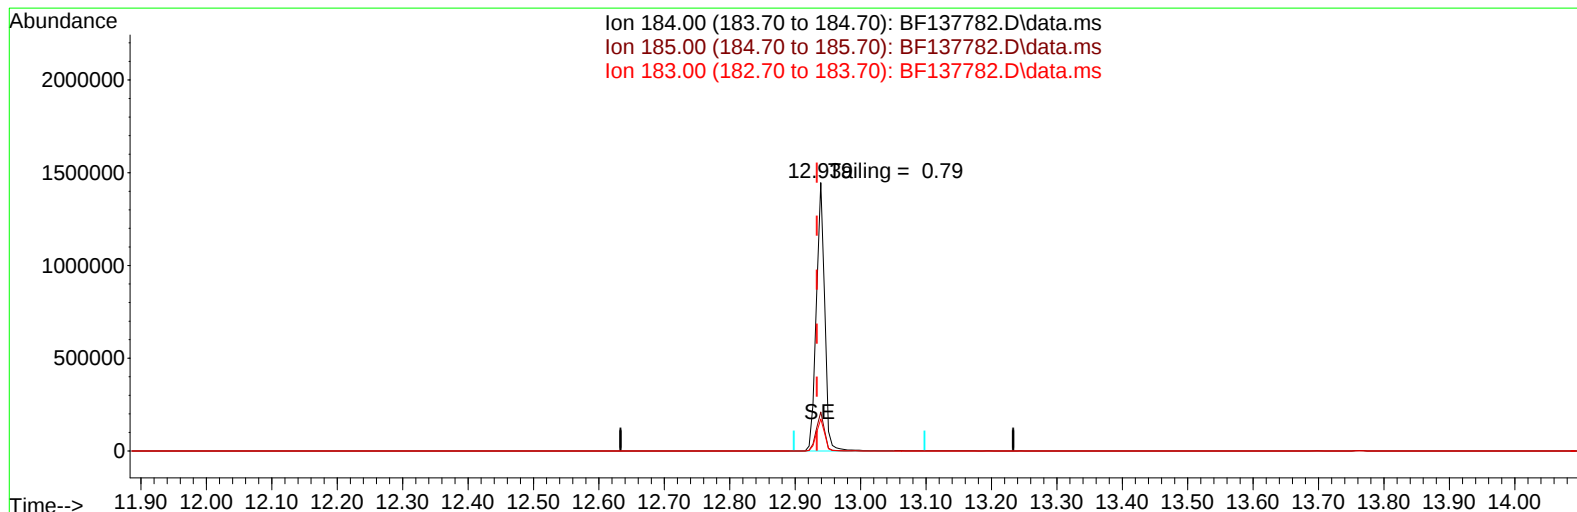

TIC: BF137782.D\data.ms

(77) Benzidine

12.939min (+ 0.006) 256256.71 ng

response 1280152

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.58
183.00	11.50	11.92
0.00	0.00	0.00