

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050216\
 Data File : BF086629.D
 Acq On : 2 May 2016 20:49
 Operator : UM/SJ
 Sample : H2716-16
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 26WARD-3-CS-5(12-25FTBGS)

Quant Time: May 03 01:51:47 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF042716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 27 14:20:52 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	173922	20.00	ng	-0.06
21) Naphthalene-d8	8.04	136	759930	20.00	ng	-0.06
38) Acenaphthene-d10	9.79	164	193546	20.00	ng	-0.06
63) Phenanthrene-d10	11.26	188	553481	20.00	ng	-0.06
75) Chrysene-d12	13.89	240	110058	20.00	ng	-0.07
86) Perylene-d12	15.29	264	1507	20.00	ng	-0.07
System Monitoring Compounds						
5) 2-Fluorophenol	5.34	112	373172	37.01	ng	-0.04
7) Phenol-d6	6.38	99	378716	26.91	ng	-0.06
23) Nitrobenzene-d5	7.32	82	244989	17.38	ng	-0.06
41) 2,4,6-Tribromophenol	10.58	330	119399	58.50	ng	-0.06
44) 2-Fluorobiphenyl	9.12	172	592596	47.66	ng	-0.06
78) Terphenyl-d14	12.85	244	982493	196.67	ng	-0.06


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050216\
Data File : BF086629.D
Acq On : 2 May 2016 20:49
Operator : UM/SJ
Sample : H2716-16
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
26WARD-3-CS-5(12-25FTBGS)

Quant Time: May 03 01:51:47 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 14:20:52 2016
Response via : Initial Calibration

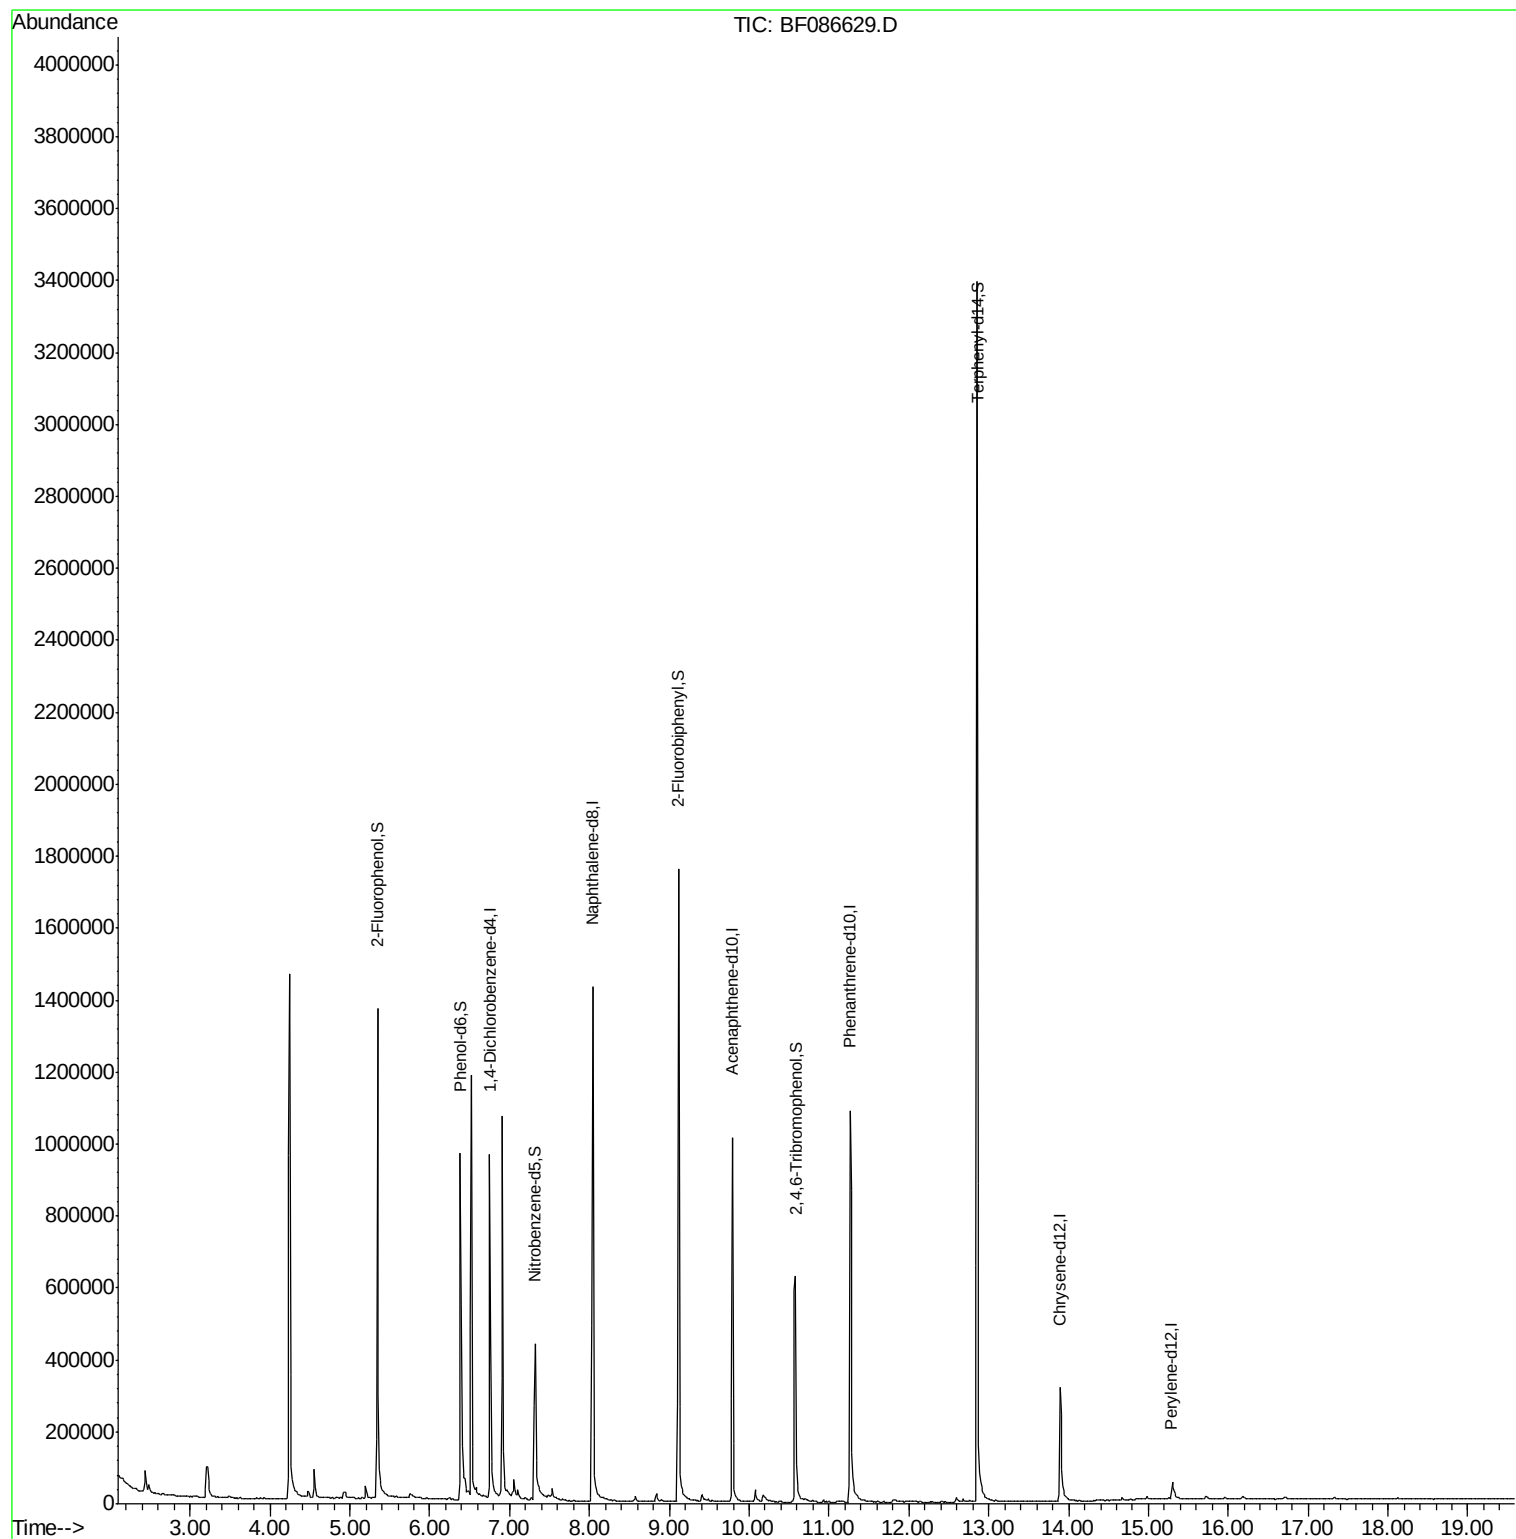



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.75 min Scan# 408

Delta R.T. -0.06 min

Lab File: BF086629.D

Acq: 2 May 2016 20:49

Instrument :

BNA_F

ClientSampleId :

26WARD-3-CS-5(12-25FTBGS)


Tot Ion:152 Resp: 173922

Ion Ratio Lower Upper

152 100

150 157.8 125.8 188.6




115 70.5 51.5 77.3

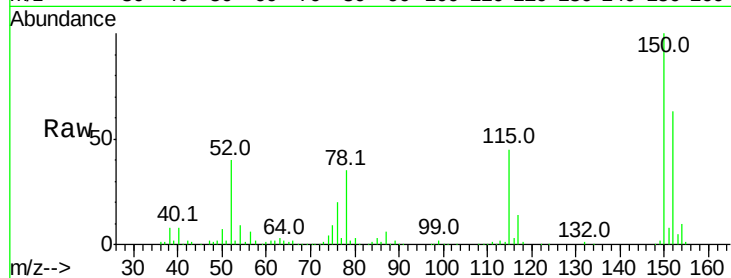

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

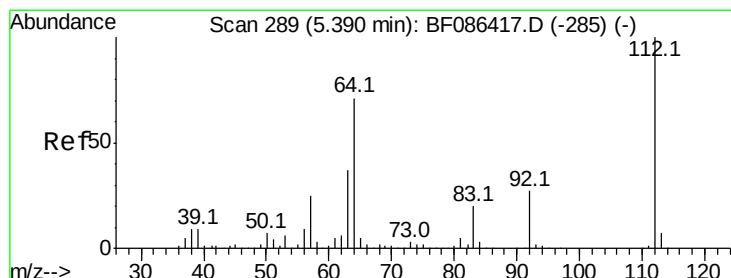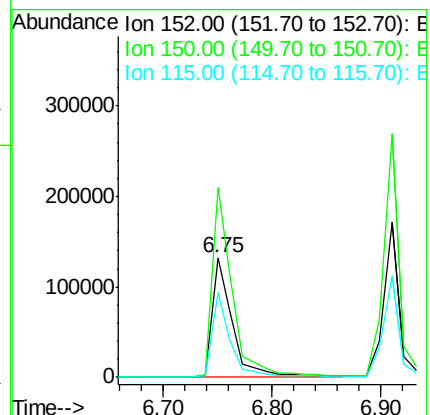

#5

2-Fluorophenol

Concen: 37.01 ng

RT: 5.34 min Scan# 285

Delta R.T. -0.04 min

Lab File: BF086629.D

Acq: 2 May 2016 20:49


Tgt Ion:112 Resp: 373172

Ion Ratio Lower Upper

112 100

64 68.1 52.1 78.1



63 36.2 25.7 38.5

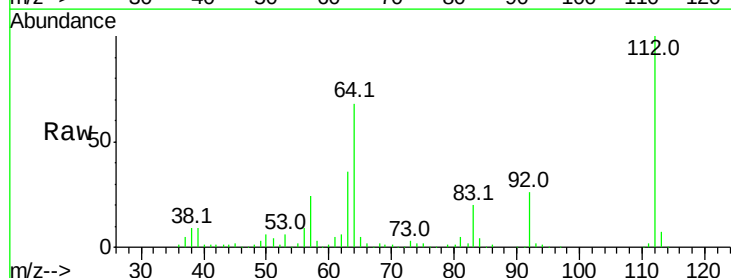


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

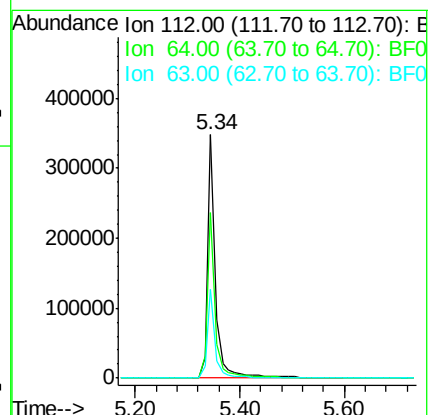



#7

Phenol-d6

Concen: 26.91 ng

RT: 6.38 min Scan# 376

Delta R.T. -0.06 min

Lab File: BF086629.D

Acq: 2 May 2016 20:49

Instrument :

BNA_F

ClientSampleId :

26WARD-3-CS-5(12-25FTBGS)


Tot Ion: 99 Resp: 378716

Ion Ratio Lower Upper

99 100

42 29.7 13.6 20.4#




71 37.0 24.6 36.8#

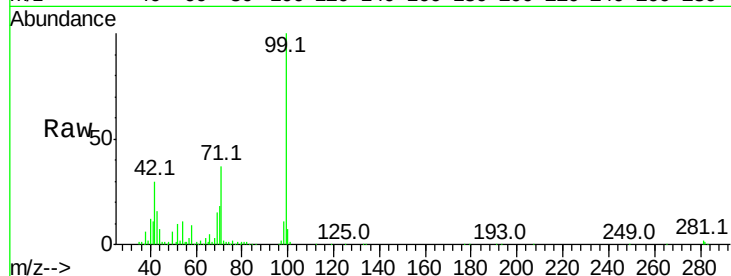

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

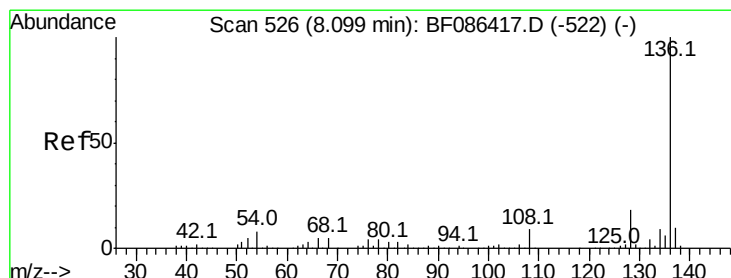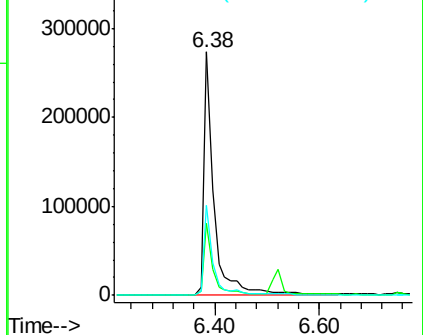

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.04 min Scan# 521

Delta R.T. -0.06 min

Lab File: BF086629.D

Acq: 2 May 2016 20:49

Tgt Ion: 136 Resp: 759930


Ion Ratio Lower Upper

136 100

137 10.8 8.8 13.2

54 10.1 5.0 7.4#

68 6.2 4.4 6.6


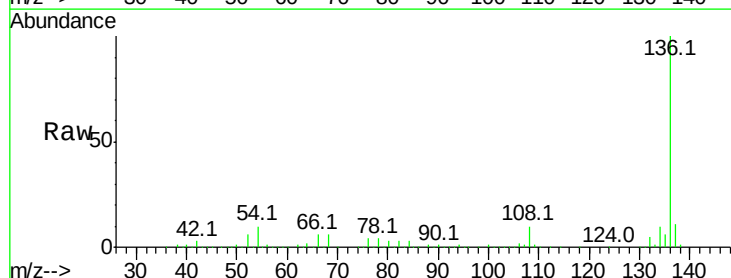



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

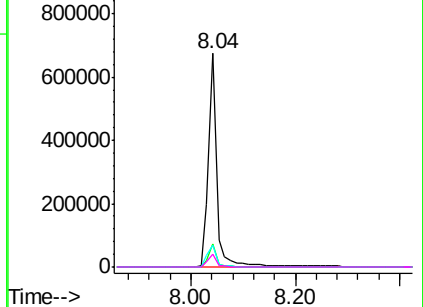


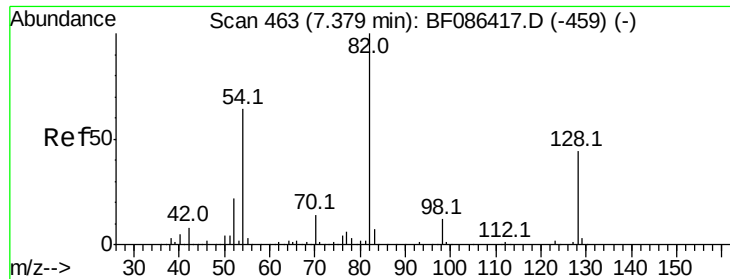




#23
 Nitrobenzene-d5
 Concen: 17.38 ng
 RT: 7.32 min Scan# 458
 Delta R.T. -0.06 min
 Lab File: BF086629.D
 Acq: 2 May 2016 20:49

Instrument :
 BNA_F
 ClientSampleId :
 26WARD-3-CS-5(12-25FTBGS)

Tot Ion: 82 Resp: 244989
 Ion Ratio Lower Upper
 82 100
 128 46.9 40.6 61.0
 54 60.9 38.1 57.1#

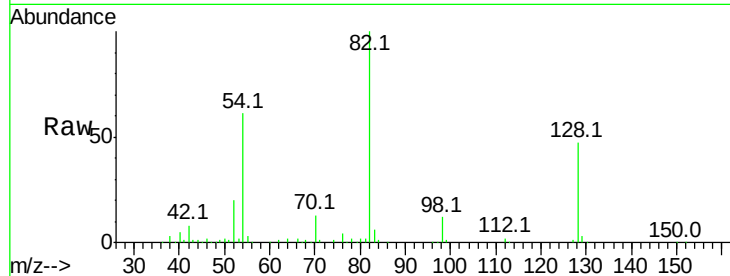


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

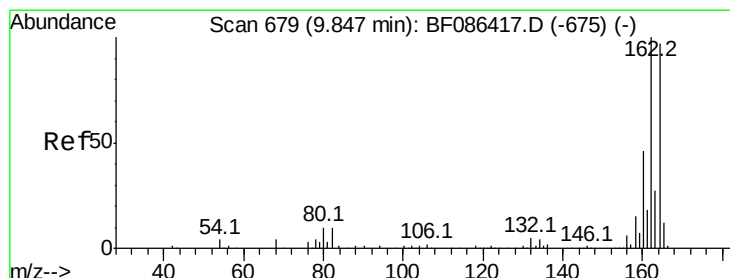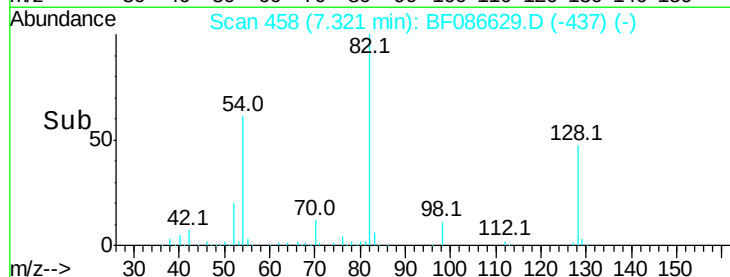
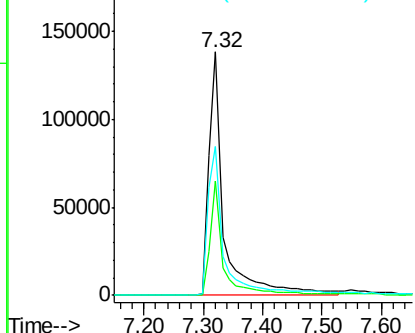



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.79 min Scan# 674
 Delta R.T. -0.06 min
 Lab File: BF086629.D
 Acq: 2 May 2016 20:49

Tgt Ion: 164 Resp: 193546
 Ion Ratio Lower Upper
 164 100
 162 109.6 82.8 124.2
 160 53.8 36.9 55.3

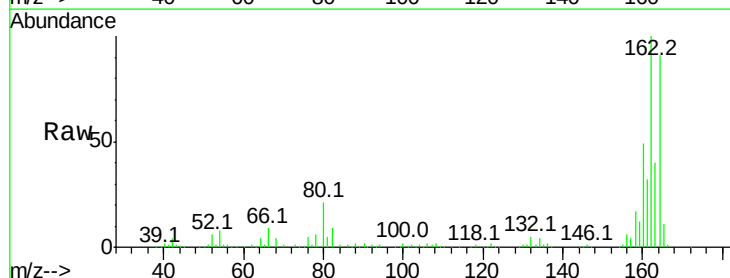

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

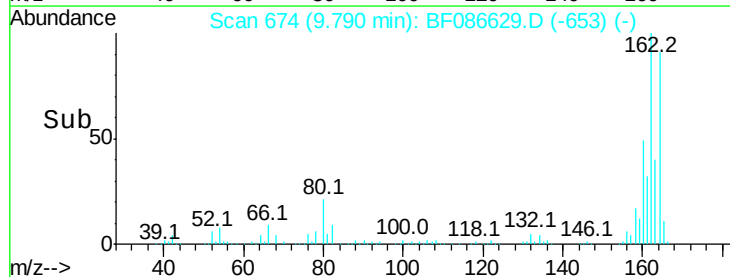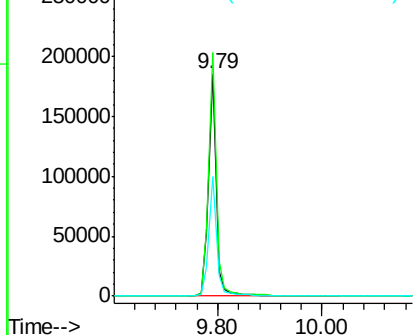







#41
 2,4,6-Tribromophenol
 Concen: 58.50 ng
 RT: 10.58 min Scan# 743
 Delta R.T. -0.06 min
 Lab File: BF086629.D
 Acq: 2 May 2016 20:49

Instrument :
 BNA_F
 ClientSampleId :
 26WARD-3-CS-5(12-25FTBGS)

Tot Ion	Ratio	Lower	Upper
330	100		
332	98.2	79.0	118.4
141	35.9	31.2	46.8

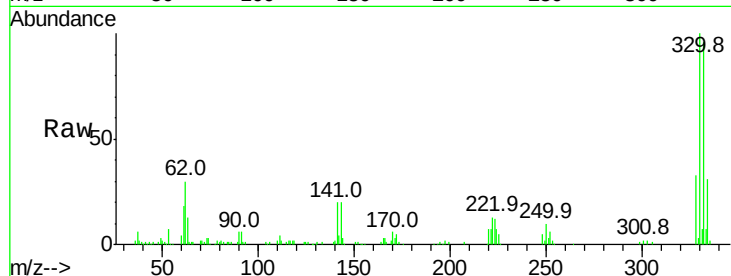


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

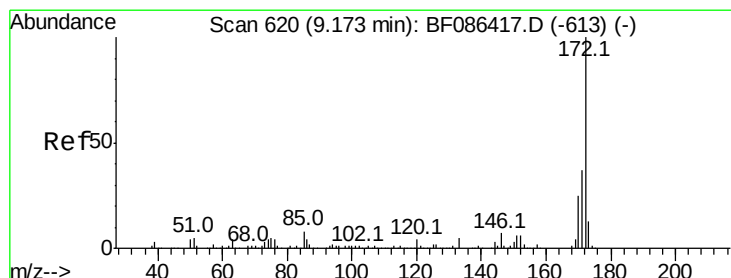
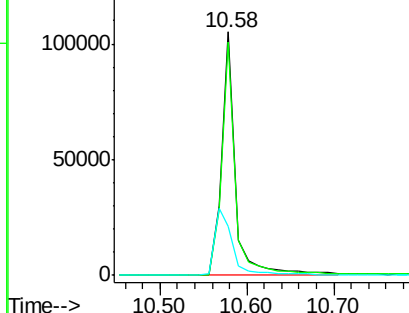



#44
 2-Fluorobiphenyl
 Concen: 47.66 ng
 RT: 9.12 min Scan# 615
 Delta R.T. -0.06 min
 Lab File: BF086629.D
 Acq: 2 May 2016 20:49

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.1	29.0	43.6
170	23.8	19.8	29.8

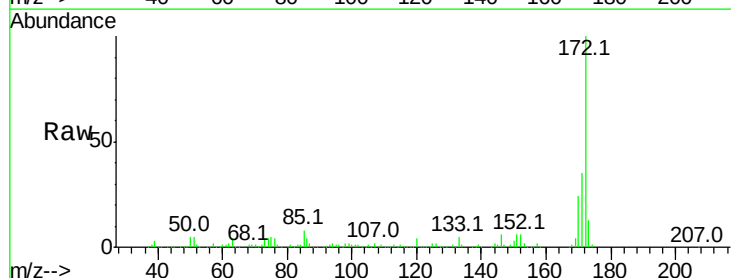

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

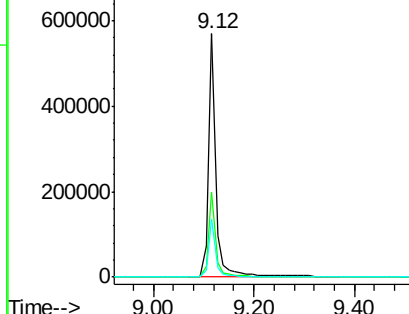

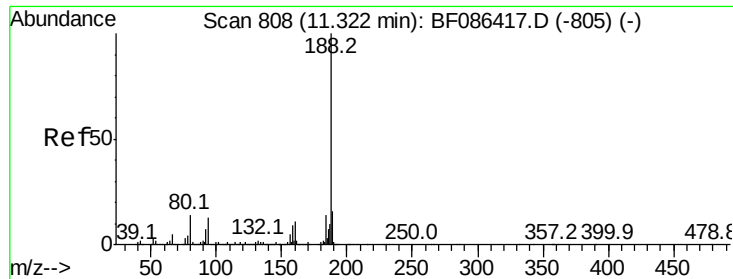

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.26 min Scan# 803

Delta R.T. -0.06 min

Lab File: BF086629.D

Acq: 2 May 2016 20:49

Instrument :

BNA_F

ClientSampleId :

26WARD-3-CS-5(12-25FTBGS)


Tot Ion:188 Resp: 553481

Ion Ratio Lower Upper

188 100

94 14.4 6.8 10.2#




80 16.2 7.1 10.7#

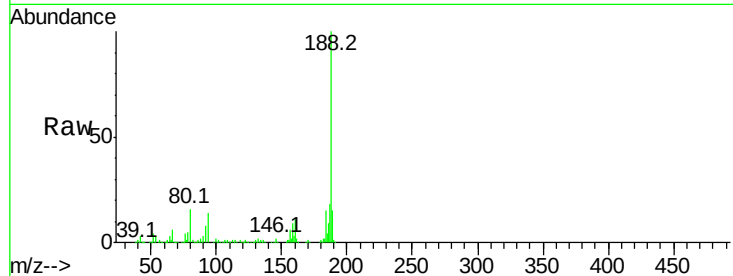

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

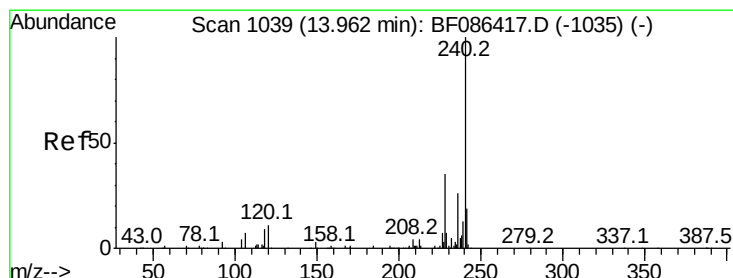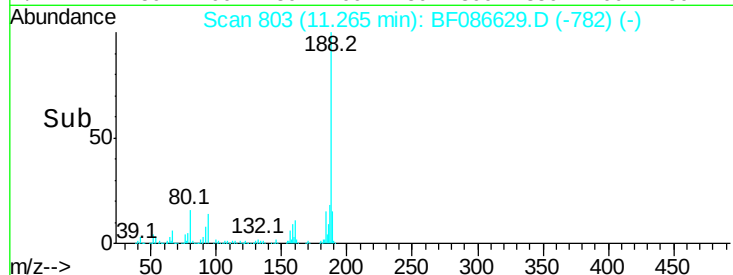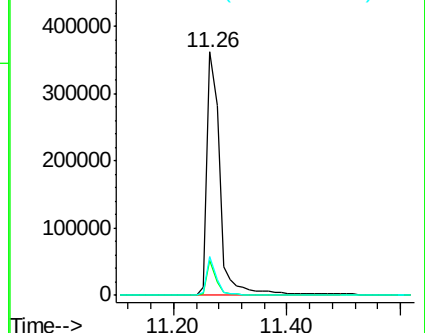

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.89 min Scan# 1033

Delta R.T. -0.07 min

Lab File: BF086629.D

Acq: 2 May 2016 20:49


Tgt Ion:240 Resp: 110058

Ion Ratio Lower Upper

240 100

120 14.5 11.2 16.8



236 33.7 21.2 31.8#

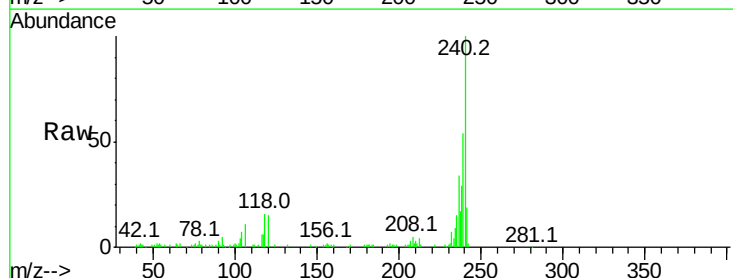


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

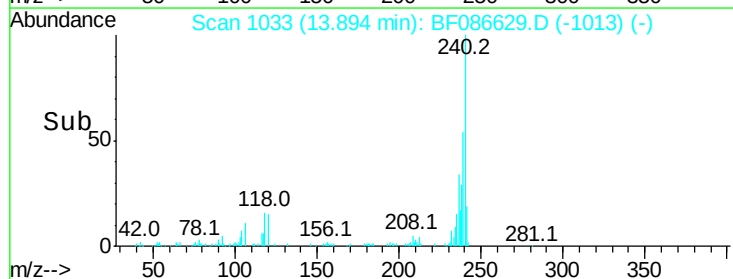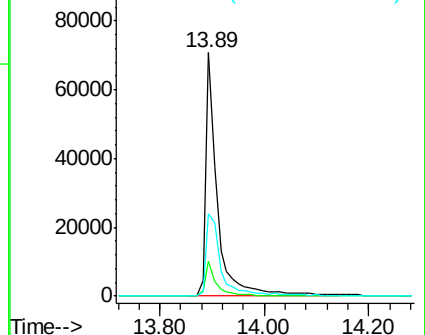

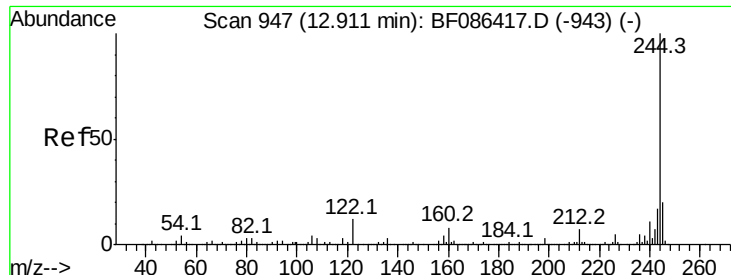

#78

Terphenyl-d14

Concen: 196.67 ng

RT: 12.85 min Scan# 942

Delta R.T. -0.06 min

Lab File: BF086629.D

Acq: 2 May 2016 20:49

Instrument :

BNA_F

ClientSampleId :

26WARD-3-CS-5(12-25FTBGS)


Tot Ion:244 Resp: 982493

Ion Ratio Lower Upper

244 100

212 8.2 6.2 9.2




122 14.9 12.0 18.0

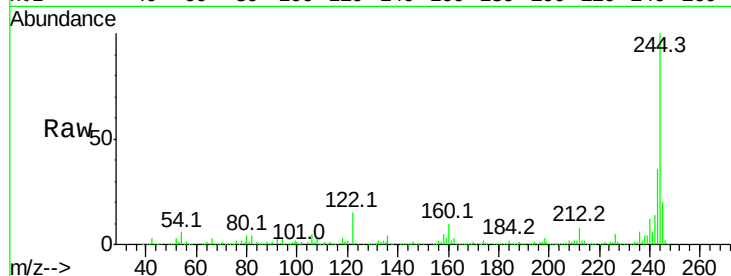

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

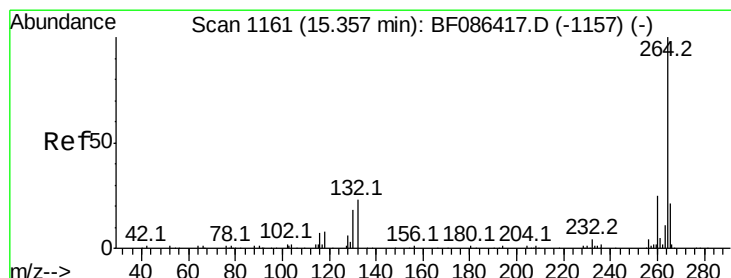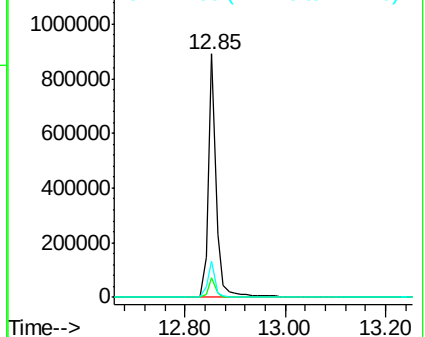

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.29 min Scan# 1155

Delta R.T. -0.07 min

Lab File: BF086629.D

Acq: 2 May 2016 20:49


Tgt Ion:264 Resp: 1507

Ion Ratio Lower Upper

264 100

260 154.1 19.5 29.3#

265 29.1 17.3 25.9#

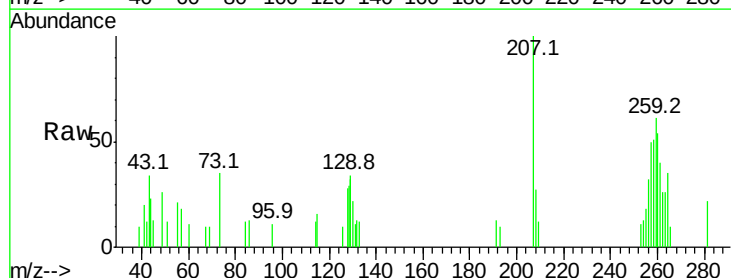

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

