
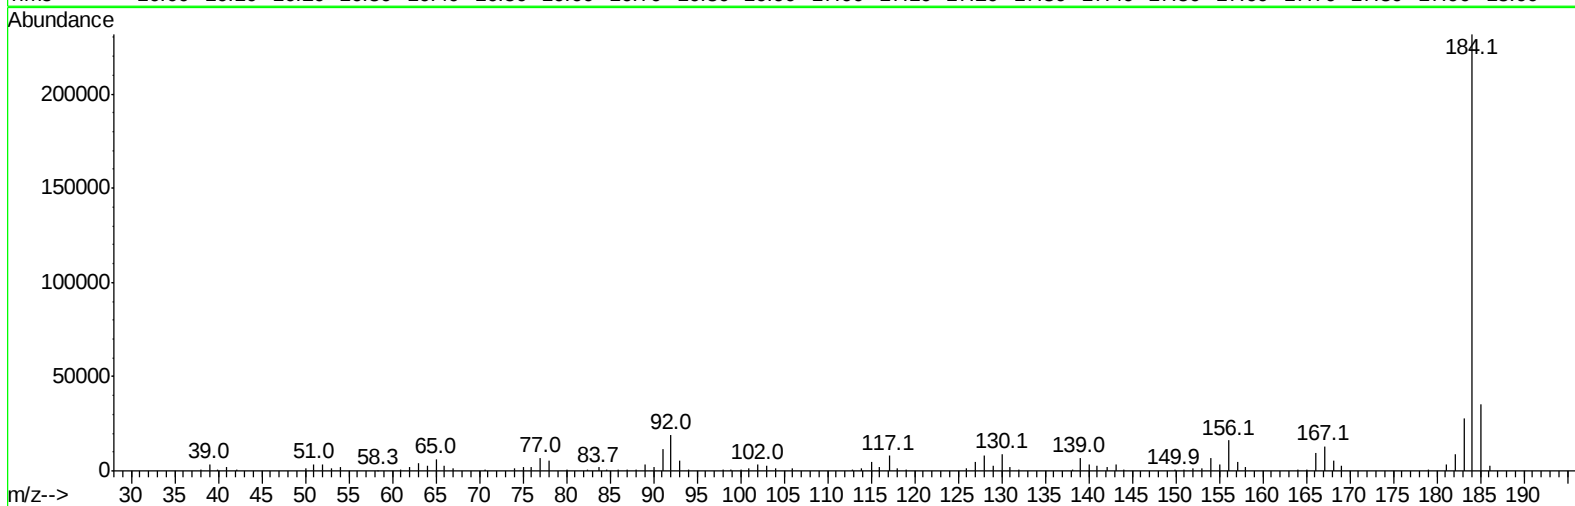


Data Path : Z:\HPCHEM1\BNA F\DATA\BF050217\
Data File : BF094797.D
Acq On : 2 May 2017 17:05
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 05:22:39 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 02 17:18:57 2017
Response via : Initial Calibration

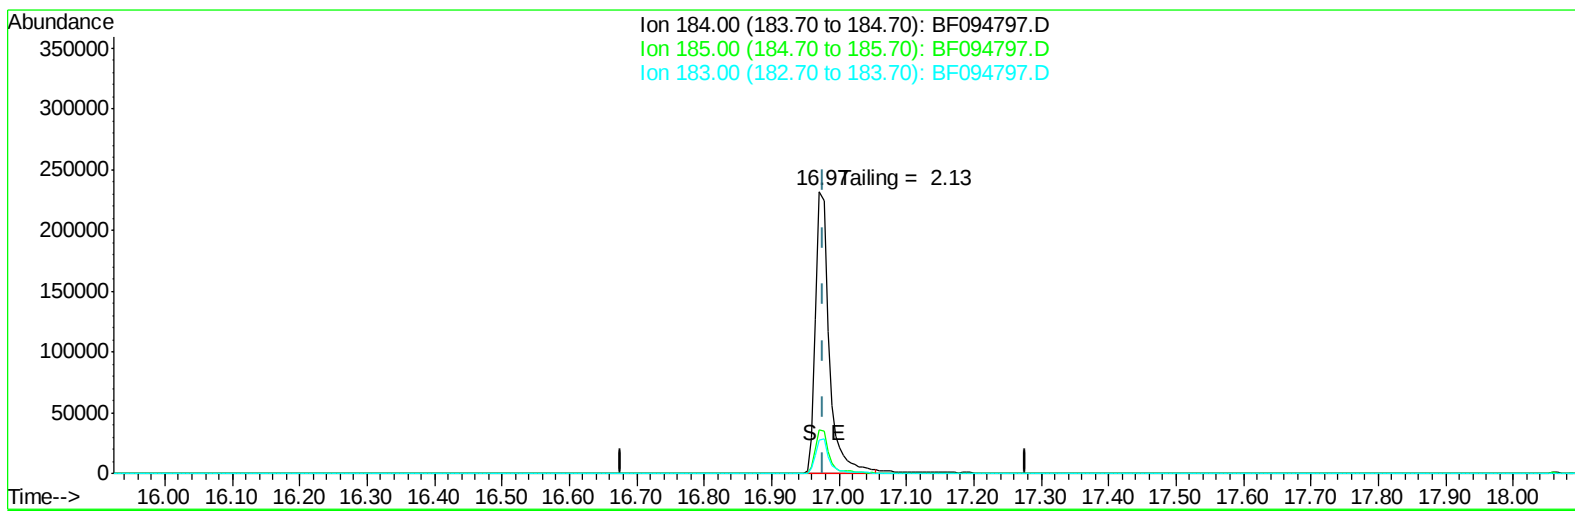

TIC: BF094797.D

(76) Benzidine



16.971min (-0.006) 0.00ng

response 321507

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	15.33#
183.00	12.20	12.03
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050217\
Data File : BF094797.D
Acq On : 2 May 2017 17:05
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 05:22:39 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 02 17:18:57 2017
Response via : Initial Calibration

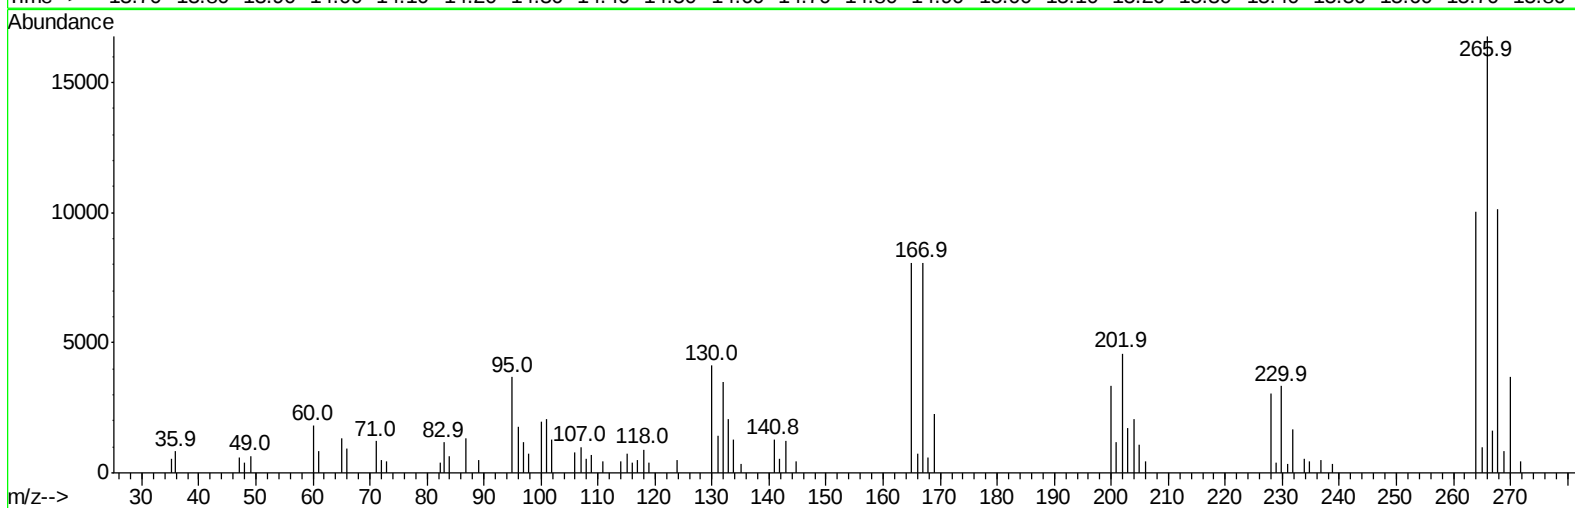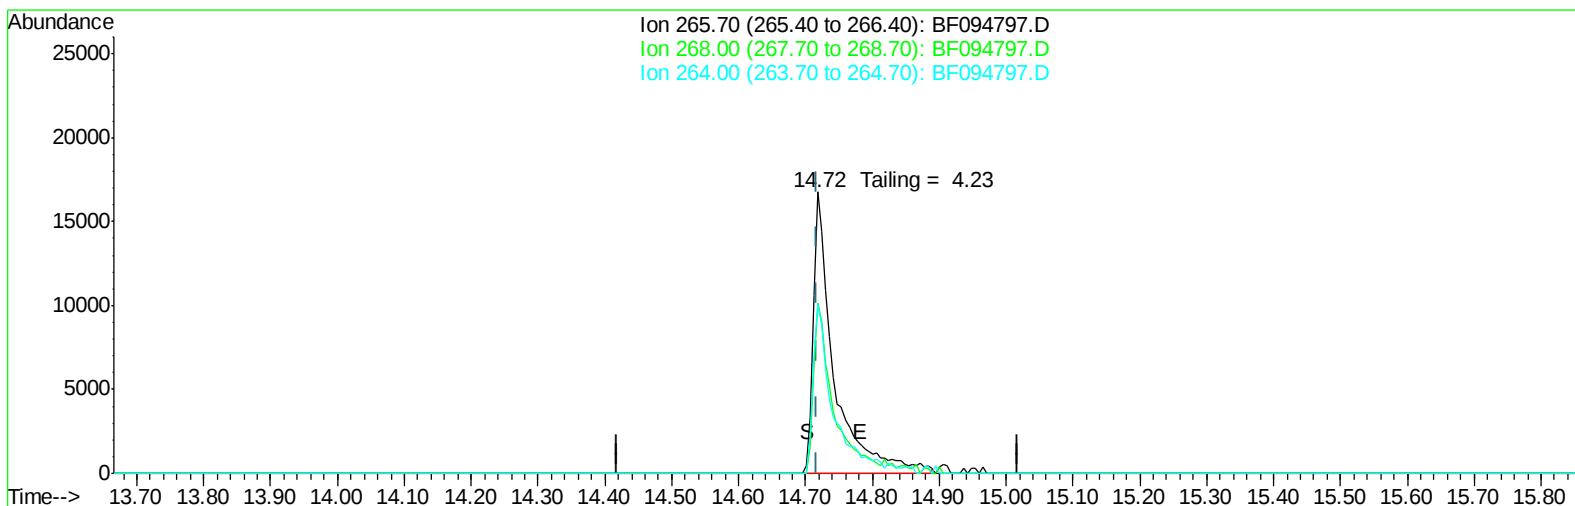

TIC: BF094797.D

(69) Pentachlorophenol (C)

14.718min (+0.000) 0.00ng

response 35744

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.32
264.00	64.60	59.86
0.00	0.00	0.00