

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050217\
 Data File : BF094810.D
 Acq On : 3 May 2017 00:08
 Operator : SJ/MA
 Sample : I2916-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RINSATEBLANK

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.025	521	525	530	rBV2	6779	11671	1.63%	0.191%
2	5.695	635	639	659	rBV	57638	130595	18.26%	2.138%
3	7.295	907	911	923	rBV	30227	71163	9.95%	1.165%
4	7.389	923	927	941	rVB	231448	353590	49.44%	5.788%
5	7.725	980	984	994	rBV	441225	495643	69.31%	8.113%
6	7.960	1020	1024	1034	rBV	279797	332878	46.55%	5.449%
7	8.619	1132	1136	1150	rBV	174727	249499	34.89%	4.084%
8	9.748	1323	1328	1345	rBV	528698	660269	92.33%	10.808%
9	11.519	1625	1629	1645	rBV	444192	562733	78.69%	9.211%
10	12.577	1804	1809	1824	rBV2	532426	715148	100.00%	11.706%
11	13.871	2025	2029	2043	rBV	160933	257278	35.98%	4.211%
12	14.977	2212	2217	2232	rBV	487864	650534	90.96%	10.648%
13	17.301	2608	2612	2618	rBV	520684	532971	74.53%	8.724%
14	18.642	2836	2840	2851	rBV	410529	505216	70.64%	8.270%
15	20.071	3077	3083	3087	rBV4	9287	13238	1.85%	0.217%
16	20.306	3119	3123	3137	rBV	360777	451759	63.17%	7.395%
17	20.412	3137	3141	3147	rVB7	14616	21672	3.03%	0.355%
18	20.794	3201	3206	3211	rVB5	12981	17941	2.51%	0.294%
19	21.224	3274	3279	3286	rBV4	14647	23623	3.30%	0.387%
20	21.718	3356	3363	3370	rBV4	9327	21252	2.97%	0.348%
21	22.294	3455	3461	3467	rBV7	10676	20925	2.93%	0.343%
22	22.977	3575	3577	3583	rVB7	6998	9684	1.35%	0.159%


Sum of corrected areas: 6109282

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050217\
Data File : BF094810.D
Acq On : 3 May 2017 00:08
Operator : SJ/MA
Sample : I2916-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RINSATEBLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

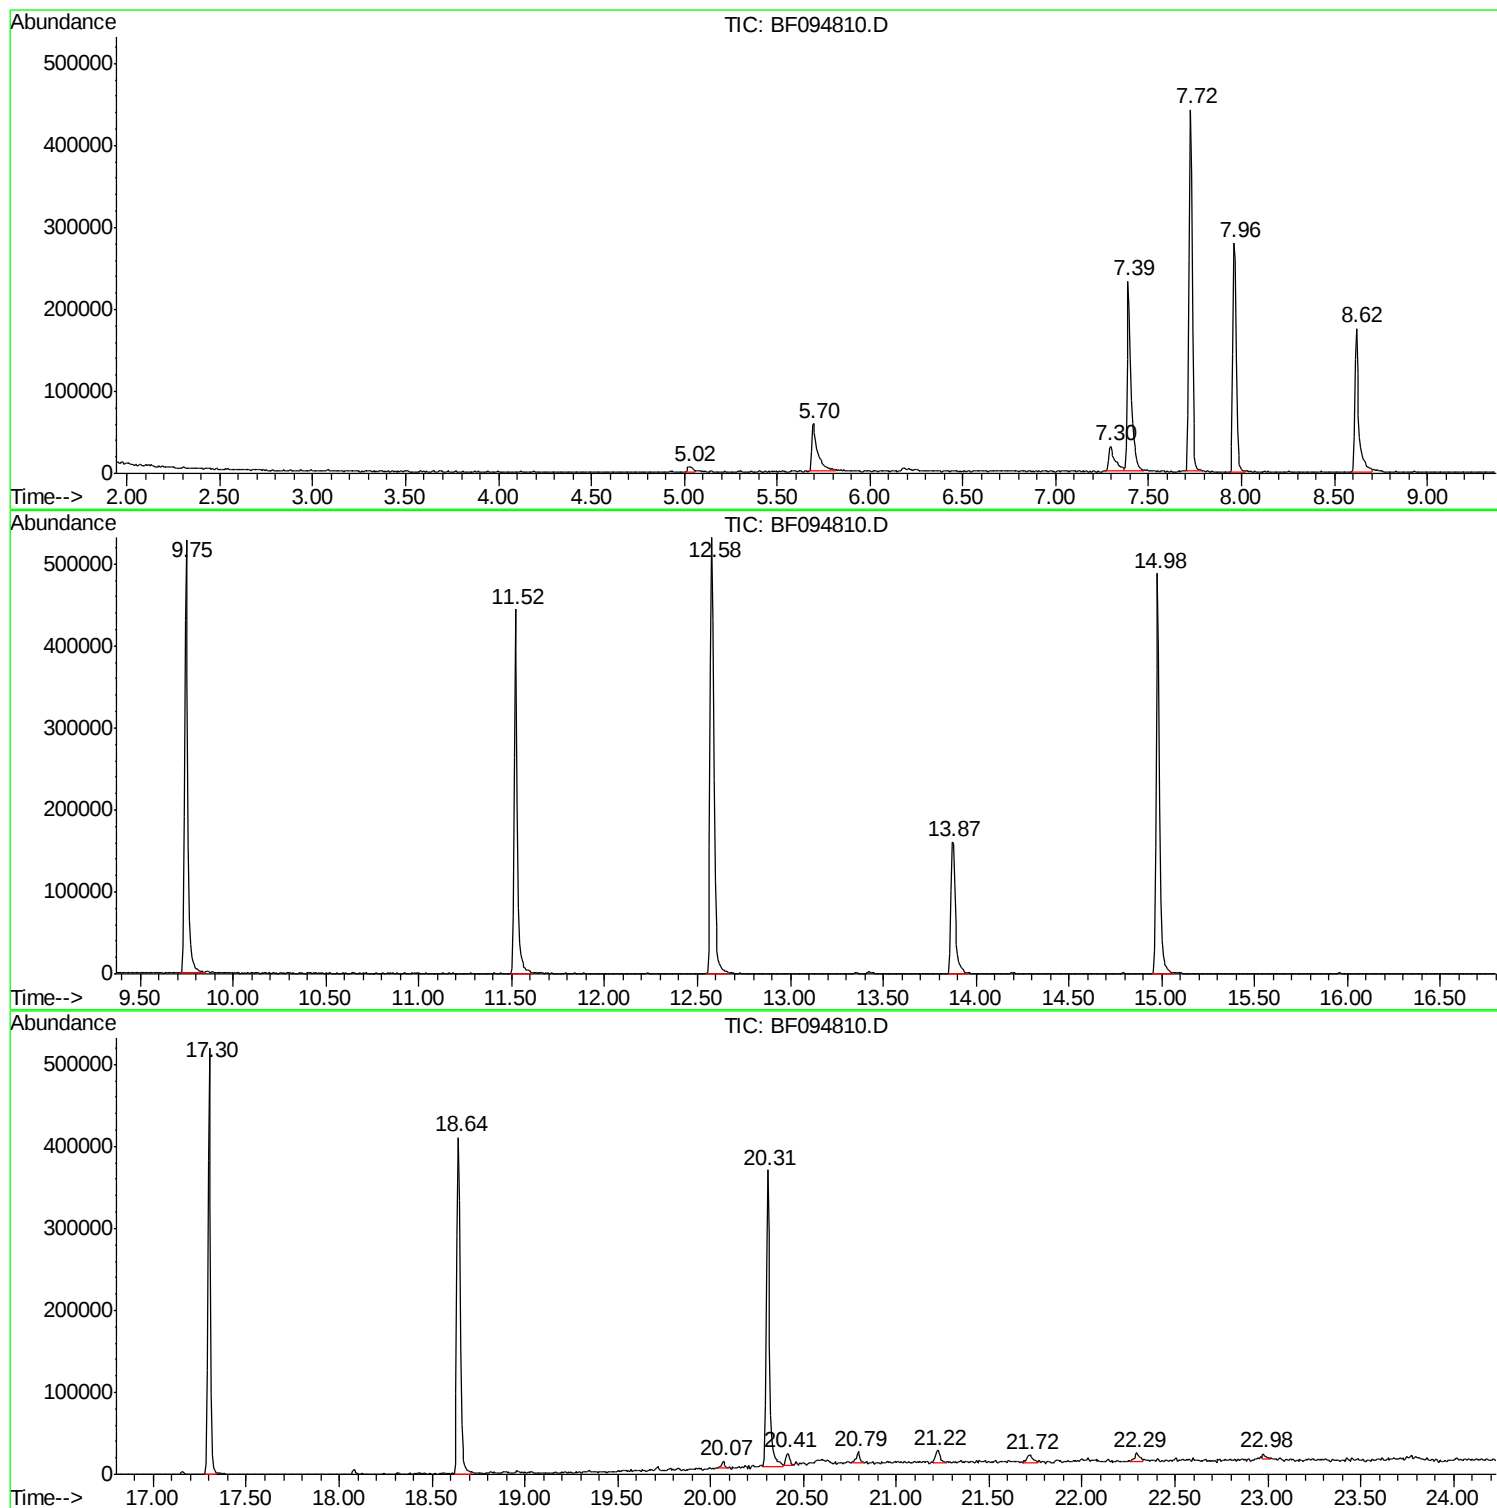

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050217\
Data File : BF094810.D
Acq On : 3 May 2017 00:08
Operator : SJ/MA
Sample : I2916-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RINSATEBLANK










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.39 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.39	14.27 ng	353590	1,4-Dichlorobenzene-d4	7.72

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	10
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

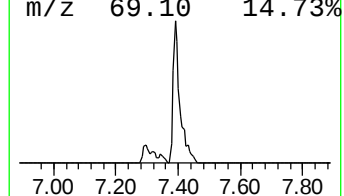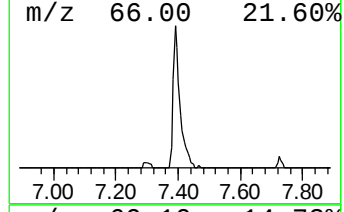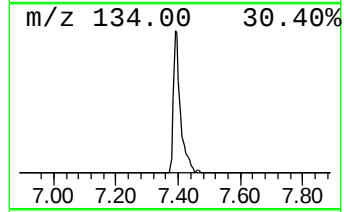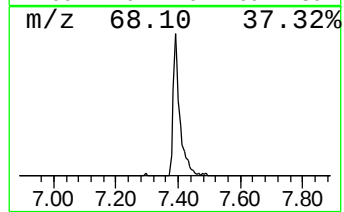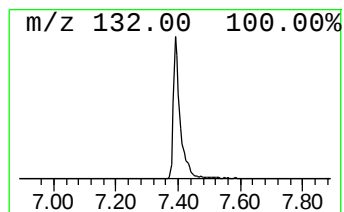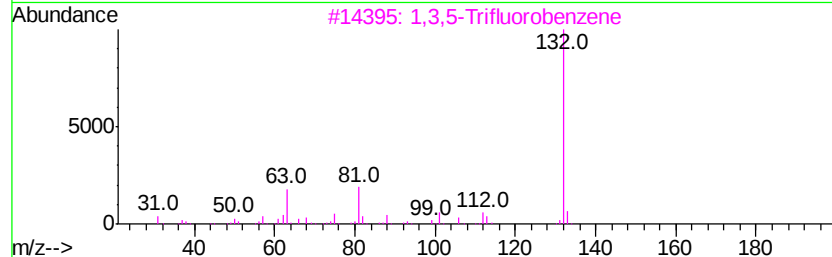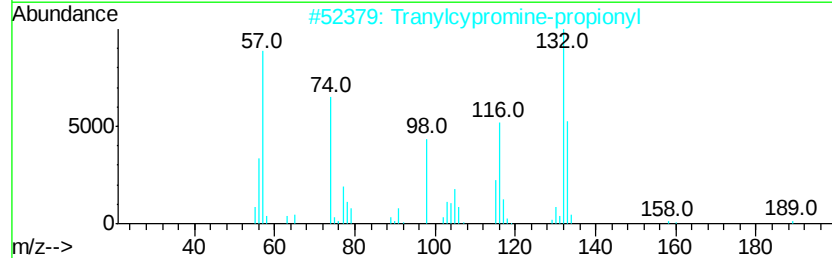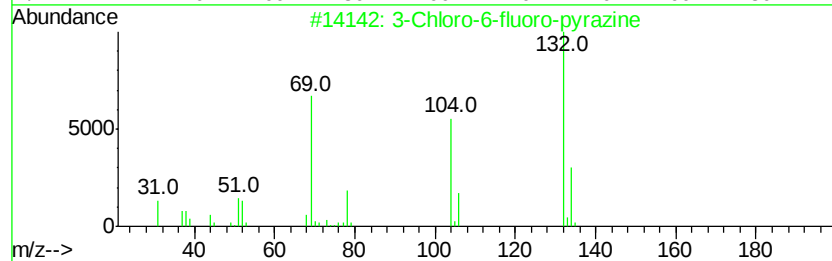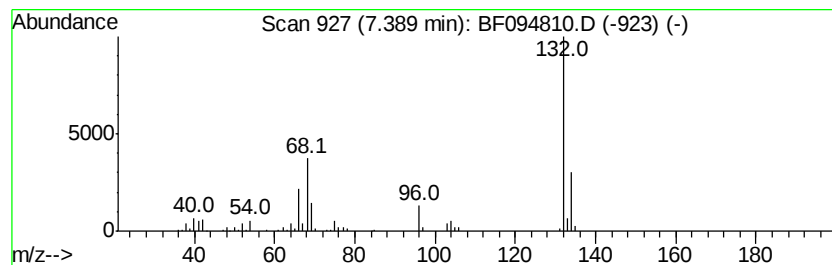

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050217\
Data File : BF094810.D
Acq On : 3 May 2017 00:08
Operator : SJ/MA
Sample : I2916-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RINSATEBLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.39	7.39	14.3	ng	353590	1	7.72	495643	20.0