


Data Path : Z:\HPCHEM1\BNA F\DATA\BF050217\
 Data File : BF094788.D
 Acq On : 2 May 2017 12:19
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 03 17:24:51 2017

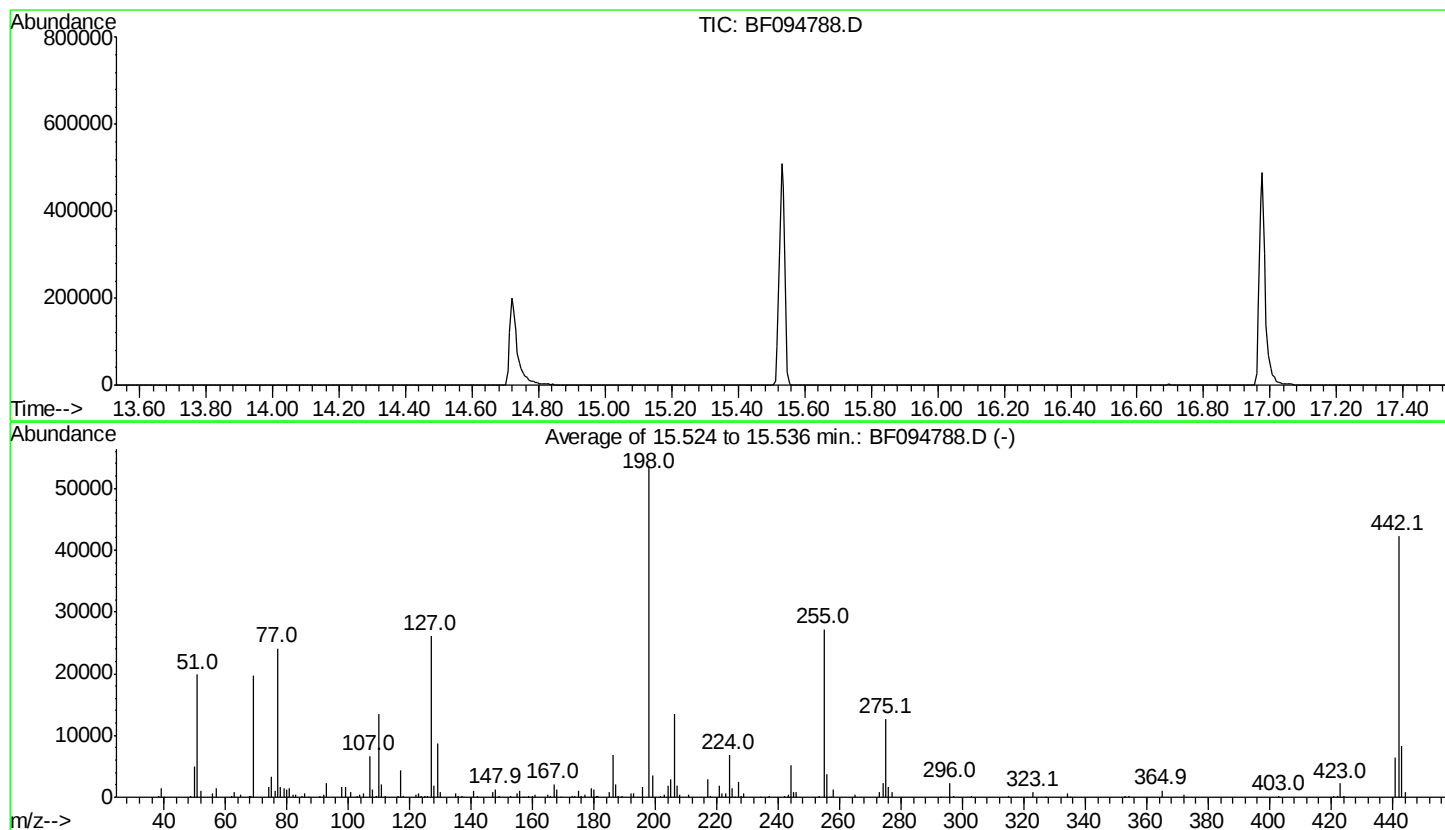

AutoFind: Scans 2310, 2311, 2312; Background Corrected with Scan 2305

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	19845	PASS
68	69	0.00	2	1.5	292	PASS
69	198	0.00	100	36.6	19661	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.6	26112	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	53680	PASS
199	198	5	9	6.6	3522	PASS
275	198	10	60	23.6	12687	PASS
365	198	1	100	2.1	1108	PASS
441	442	0.01	24	15.3	6485	PASS
442	198	50	100	78.9	42368	PASS
443	442	15	24	19.7	8351	PASS