
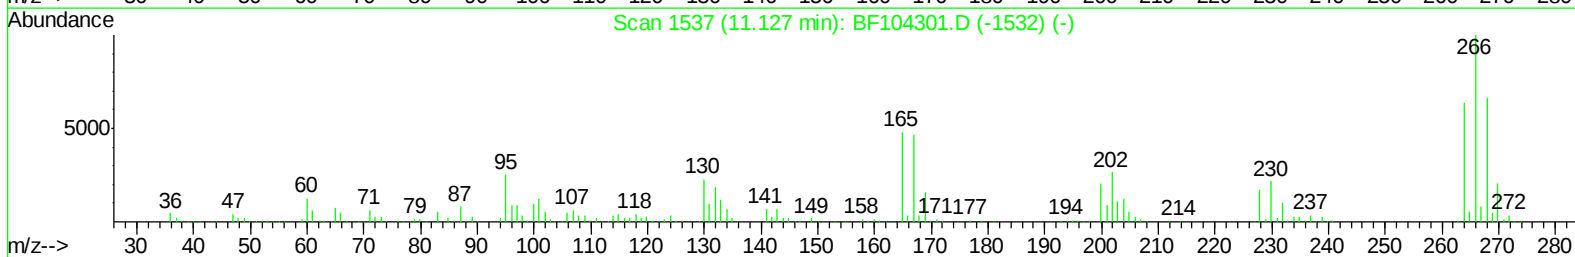
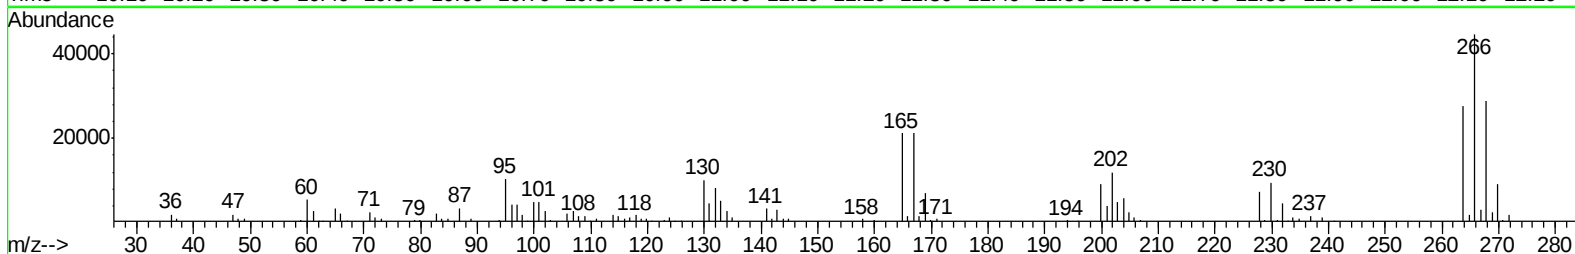


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050218\
Data File : BF105019.D
Acq On : 2 May 2018 9:57
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 09:12:17 2018
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 02 17:25:18 2018
Response via : Initial Calibration

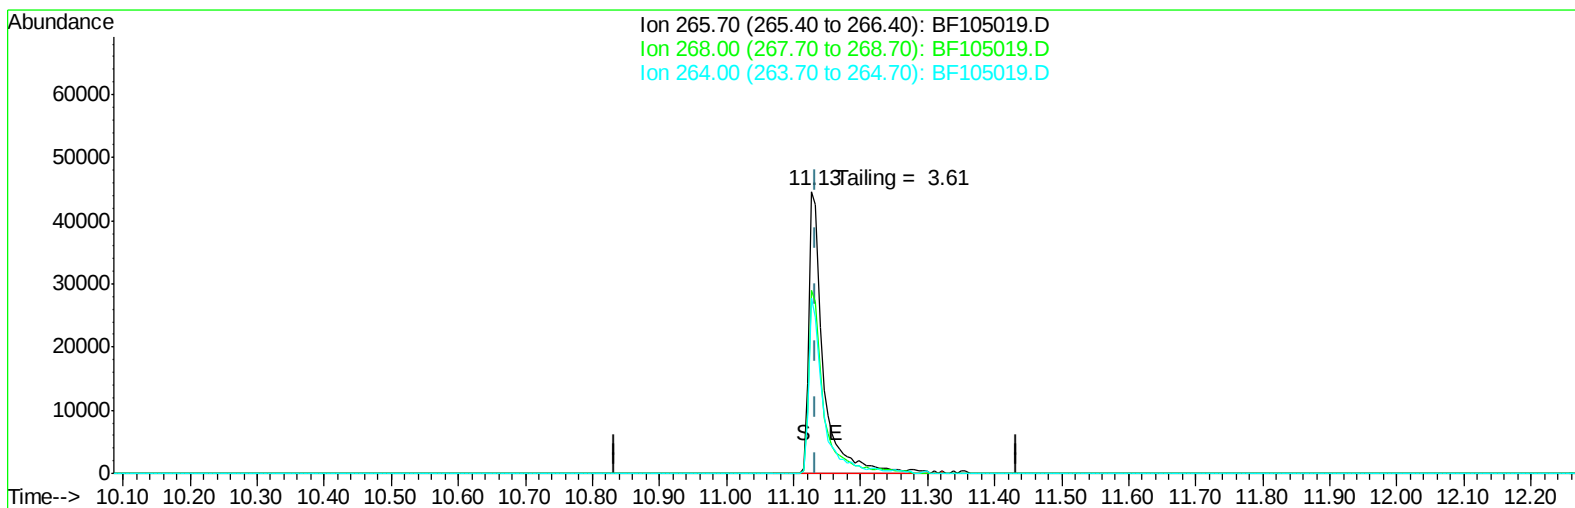

TIC: BF105019.D

(69) Pentachlorophenol (C)

11.127min (-0.006) 29432.89ng

response 65162

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.94
264.00	61.90	62.15
0.00	0.00	0.00