

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050218\
 Data File : BF105043.D
 Acq On : 2 May 2018 20:43
 Operator : JU/SJ
 Sample : PB108660BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB108660BL

Quant Time: May 03 08:52:53 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 02 17:25:18 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.79	152	80837	20.00	ng	0.00
21) Naphthalene-d8	8.07	136	335871	20.00	ng	0.00
38) Acenaphthene-d10	9.83	164	152758	20.00	ng	0.00
63) Phenanthrene-d10	11.32	188	263798	20.00	ng	0.00
75) Chrysene-d12	14.02	240	191860	20.00	ng	-0.01
86) Perylene-d12	15.58	264	152391	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.41	112	643664	121.75	ng	0.00
7) Phenol-d6	6.43	99	764692	117.72	ng	0.00
23) Nitrobenzene-d5	7.36	82	462754	89.97	ng	-0.01
41) 2,4,6-Tribromophenol	10.63	330	180920	114.17	ng	0.00
44) 2-Fluorobiphenyl	9.15	172	899641	93.04	ng	0.00
78) Terphenyl-d14	12.92	244	787910	93.63	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050218\
Data File : BF105043.D
Acq On : 2 May 2018 20:43
Operator : JU/SJ
Sample : PB108660BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB108660BL

Quant Time: May 03 08:52:53 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 02 17:25:18 2018
Response via : Initial Calibration

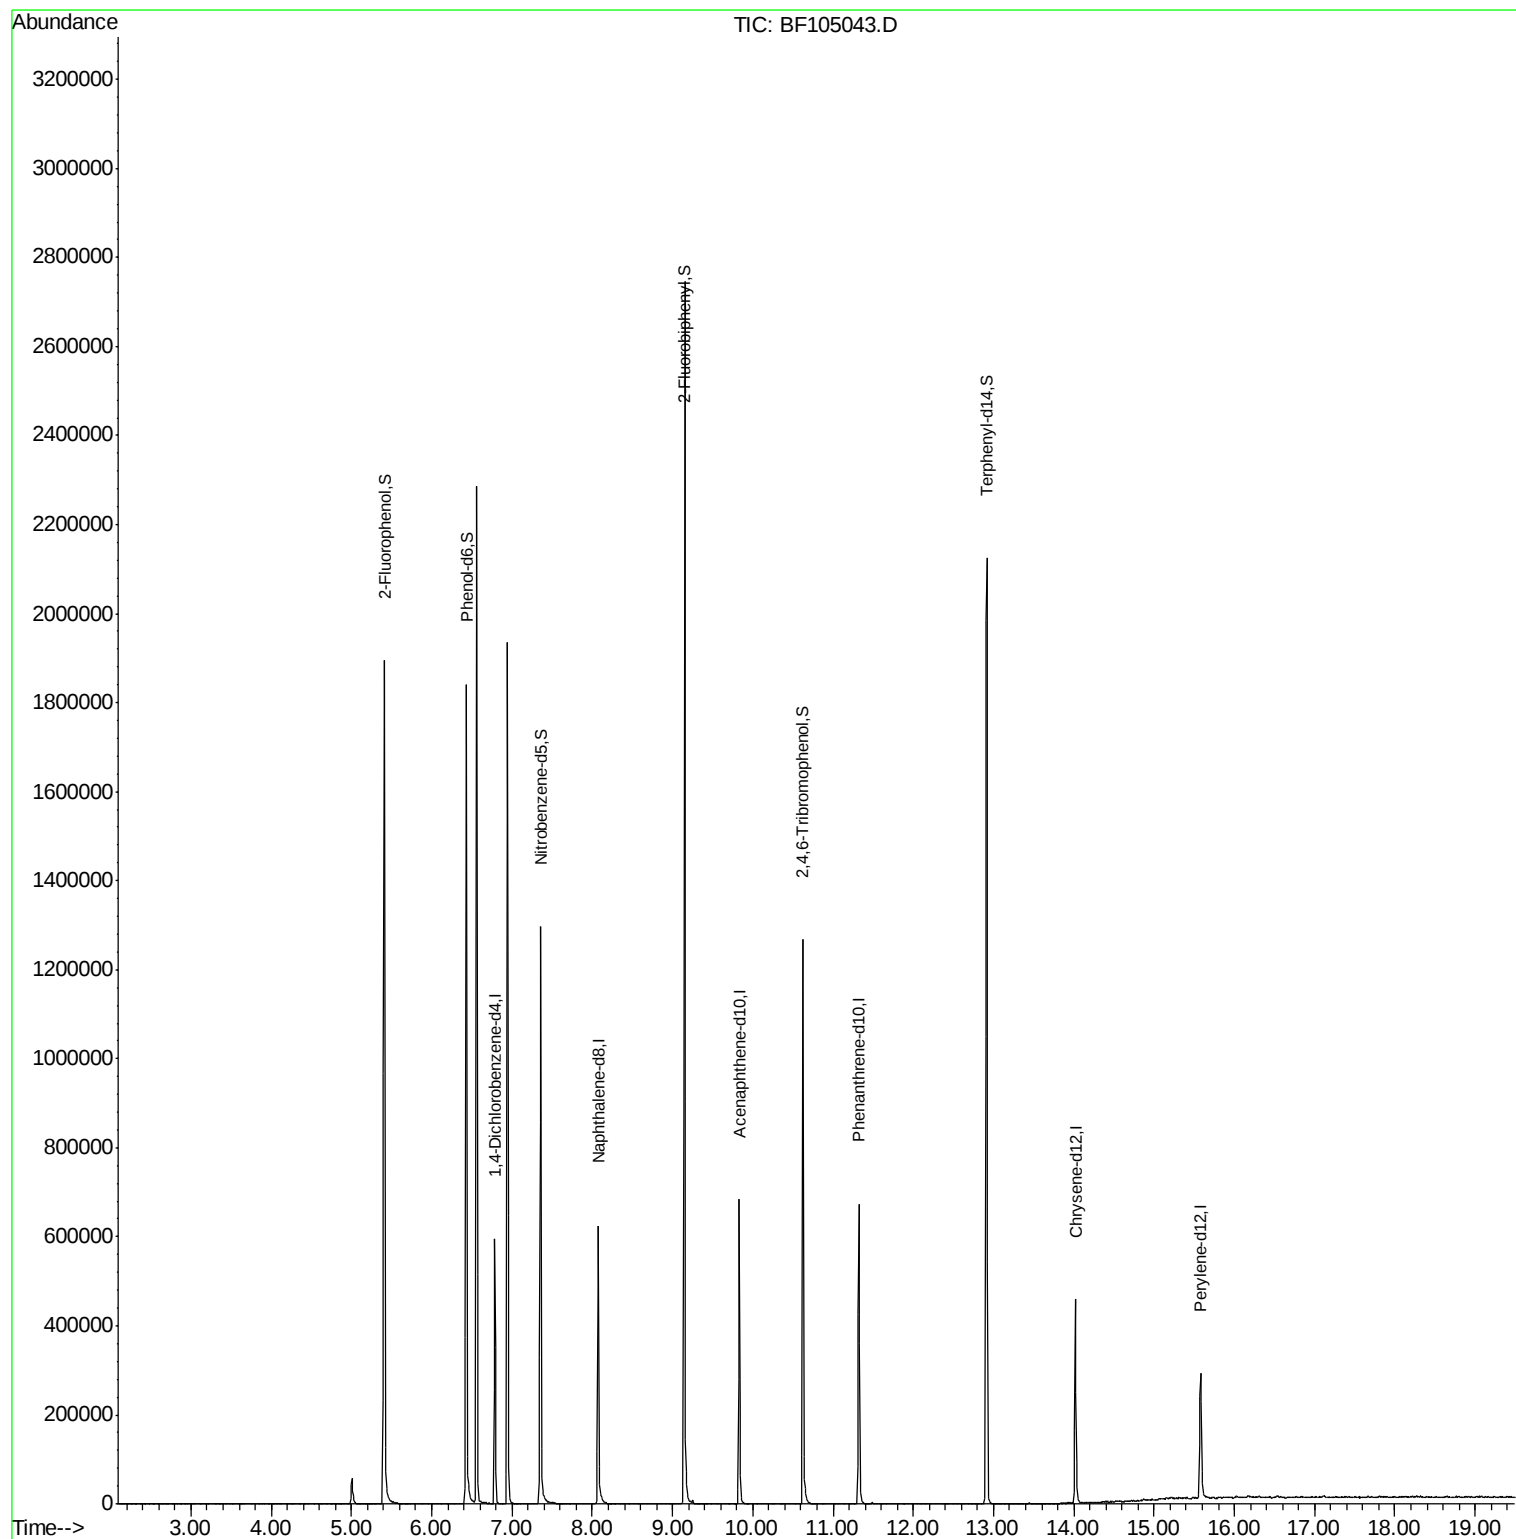




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.79 min Scan# 799
Delta R.T. 0.00 min
Lab File: BF105043.D
Acq: 2 May 2018 20:43

Instrument :
BNA_F
ClientSampleId :
PB108660BL

Tot Ion:152 Resp: 80837
Ion Ratio Lower Upper
152 100
150 159.7 124.6 186.8
115 66.0 50.1 75.1

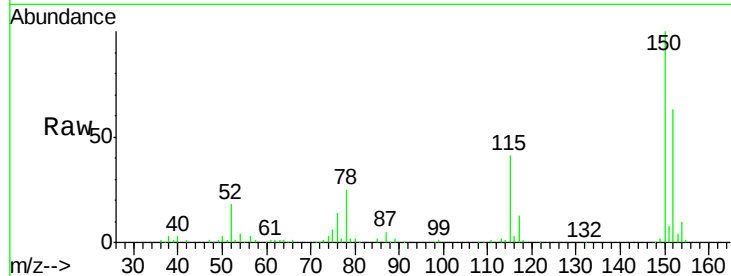


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

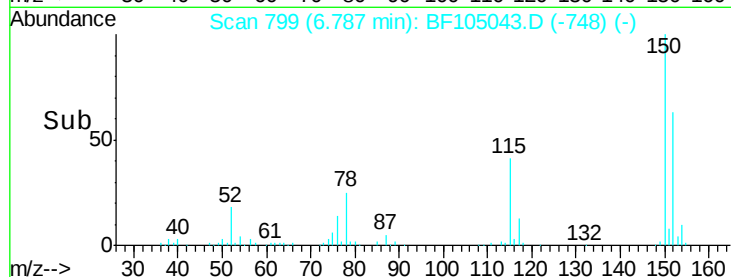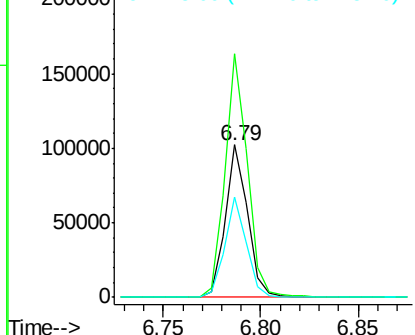



#5

2-Fluorophenol
Concen: 121.751 ng
RT: 5.41 min Scan# 565
Delta R.T. 0.01 min
Lab File: BF105043.D
Acq: 2 May 2018 20:43

Tgt Ion:112 Resp: 643664
Ion Ratio Lower Upper
112 100
64 52.0 47.9 71.9
63 27.1 23.7 35.5

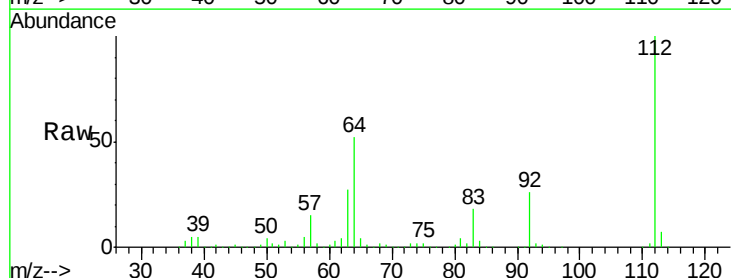

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

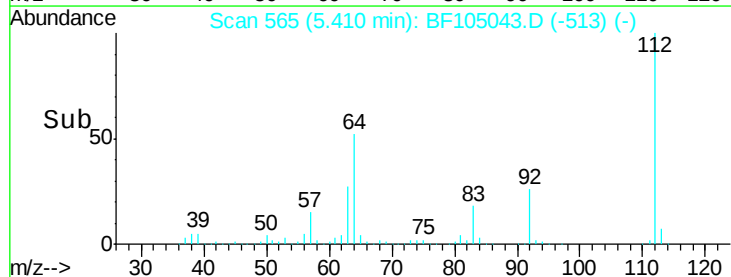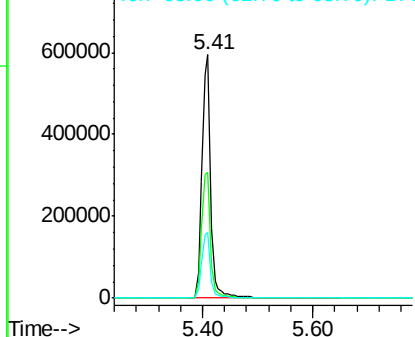



#7

Phenol-d6

Concen: 117.723 ng

RT: 6.43 min Scan# 739

Delta R.T. -0.01 min

Lab File: BF105043.D

Acq: 2 May 2018 20:43

Instrument :

BNA_F

ClientSampleId :

PB108660BL


Tot Ion: 99 Resp: 764692

Ion Ratio Lower Upper

99 100

42 15.1 14.5 21.7



71 34.0 25.4 38.0

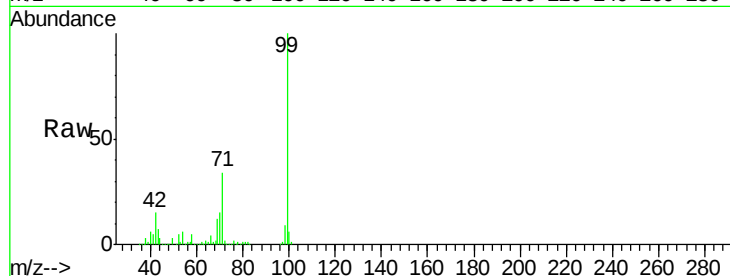

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

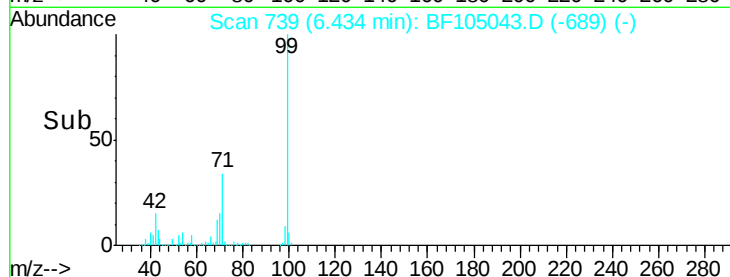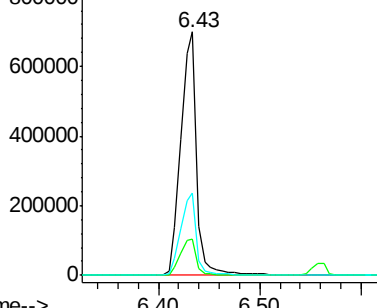

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.07 min Scan# 1018

Delta R.T. 0.00 min

Lab File: BF105043.D

Acq: 2 May 2018 20:43

Tgt Ion: 136 Resp: 335871


Ion Ratio Lower Upper

136 100

137 10.7 8.9 13.3

54 6.1 6.6 9.8#

68 5.2 5.0 7.4


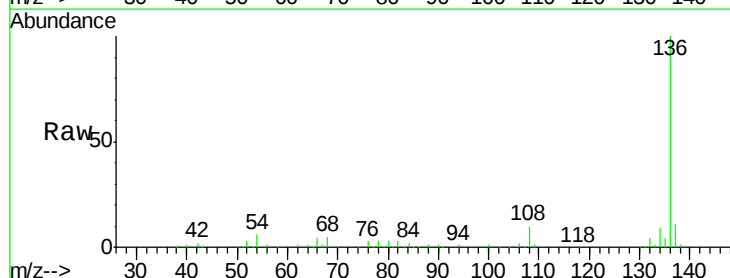


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

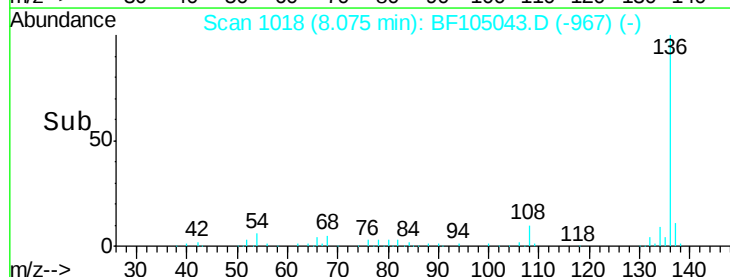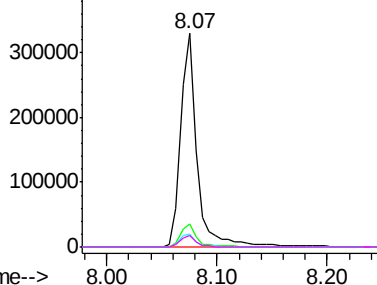






#23
Nitrobenzene-d5
Concen: 89.966 ng
RT: 7.36 min Scan# 896
Delta R.T. -0.01 min
Lab File: BF105043.D
Acq: 2 May 2018 20:43

Instrument :
BNA_F
ClientSampleId :
PB108660BL

Tot Ion: 82 Resp: 462754
Ion Ratio Lower Upper
82 100
128 47.5 36.1 54.1
54 44.0 41.4 62.2

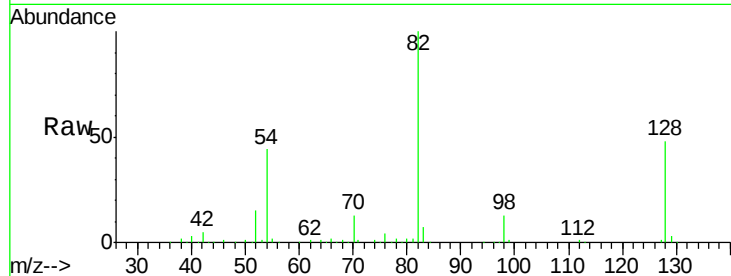


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

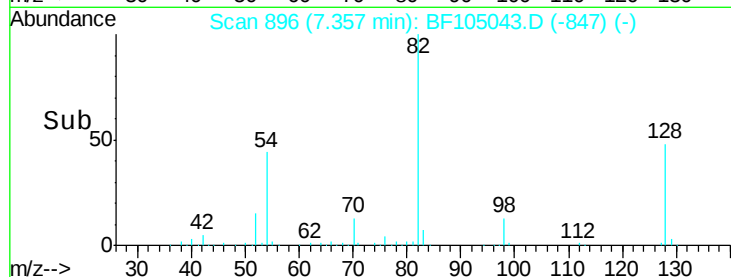
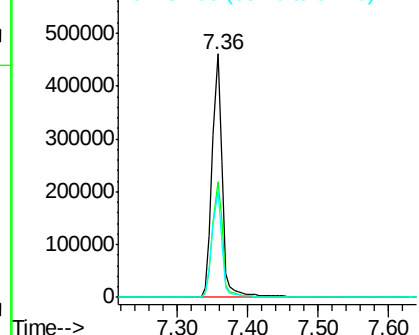


#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.83 min Scan# 1316
Delta R.T. -0.01 min
Lab File: BF105043.D
Acq: 2 May 2018 20:43

Tgt Ion: 164 Resp: 152758
Ion Ratio Lower Upper
164 100
162 104.8 86.1 129.1
160 44.7 38.3 57.5

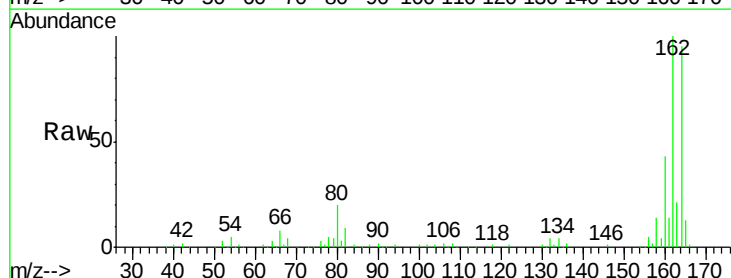

Abundance Ion 164.00 (163.70 to 164.70): BF1
Ion 162.00 (161.70 to 162.70): BF1
Ion 160.00 (159.70 to 160.70): BF1

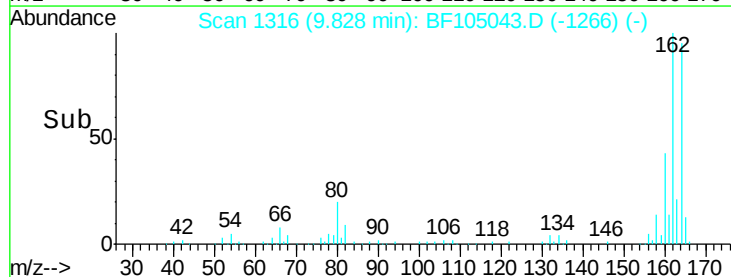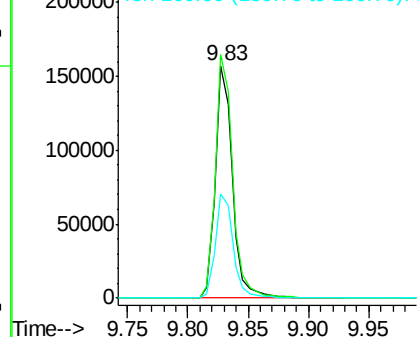







#41
 2,4,6-Tribromophenol
 Concen: 114.174 ng
 RT: 10.63 min Scan# 1452
 Delta R.T. -0.01 min
 Lab File: BF105043.D
 Acq: 2 May 2018 20:43

Instrument :
 BNA_F
 ClientSampleId :
 PB108660BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.1	77.0	115.6
141	33.9	29.9	44.9

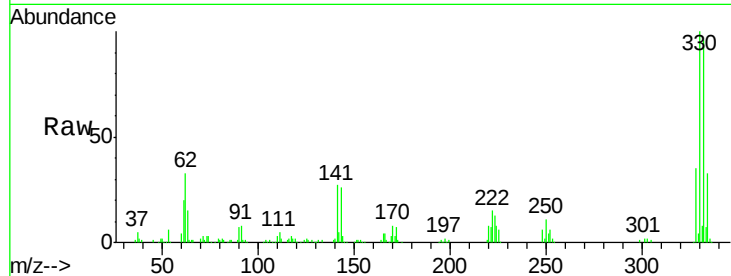


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

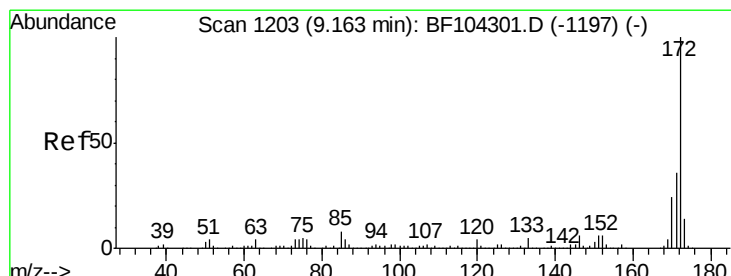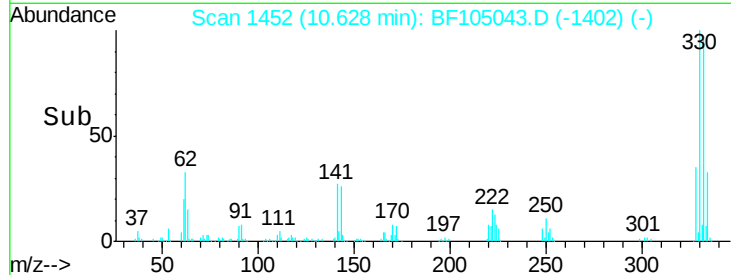
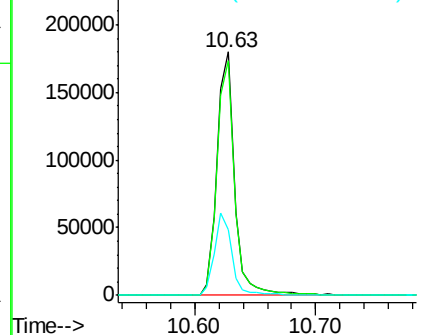


#44
 2-Fluorobiphenyl
 Concen: 93.037 ng
 RT: 9.15 min Scan# 1201
 Delta R.T. -0.01 min
 Lab File: BF105043.D
 Acq: 2 May 2018 20:43

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	29.7	44.5
170	24.1	19.6	29.4

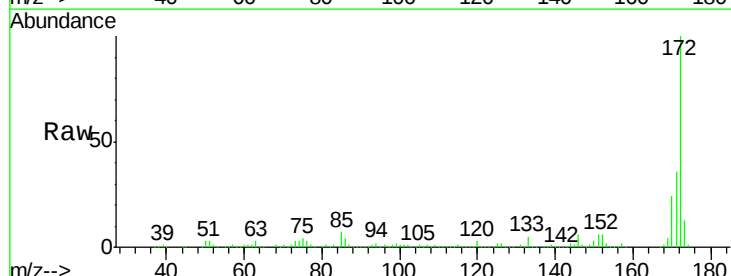

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

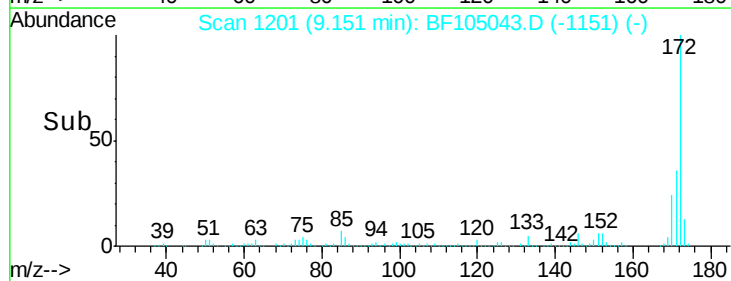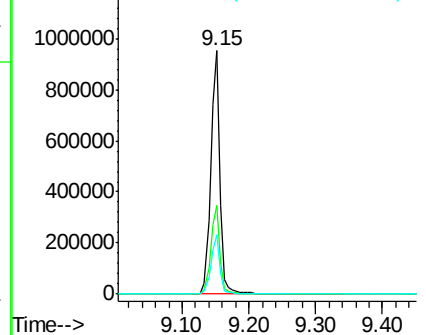







#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.32 min Scan# 1570
Delta R.T. 0.00 min
Lab File: BF105043.D
Acq: 2 May 2018 20:43

Instrument :
BNA_F
ClientSampleId :
PB108660BL

Tot Ion:188 Resp: 263798
Ion Ratio Lower Upper
188 100
94 9.5 8.5 12.7
80 10.2 9.2 13.8

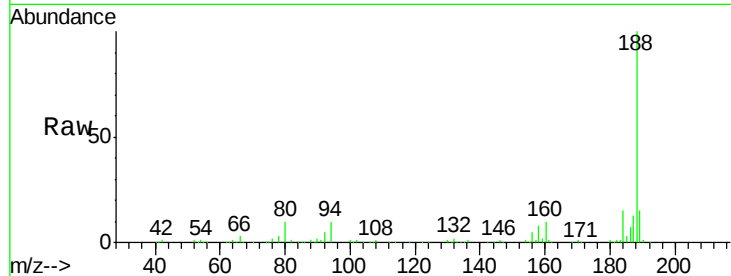


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

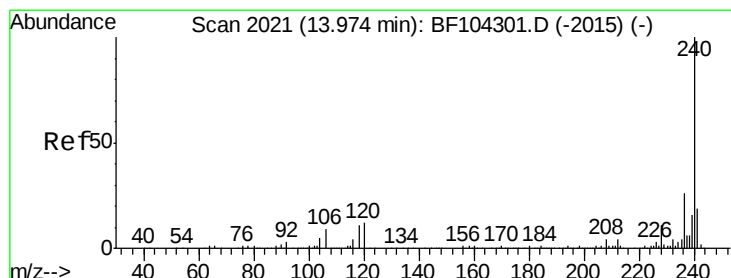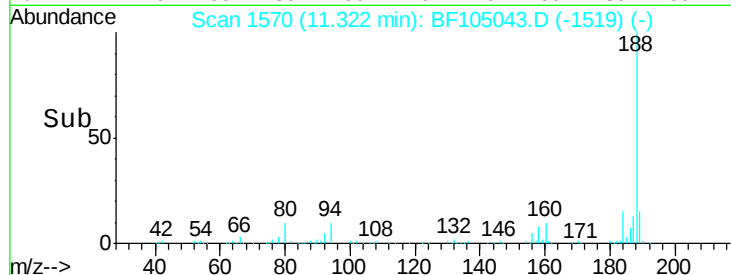
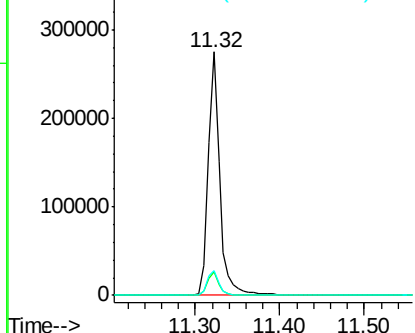


#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.02 min Scan# 2029
Delta R.T. -0.01 min
Lab File: BF105043.D
Acq: 2 May 2018 20:43

Tgt Ion:240 Resp: 191860
Ion Ratio Lower Upper
240 100
120 12.2 9.5 14.3
236 26.2 20.7 31.1

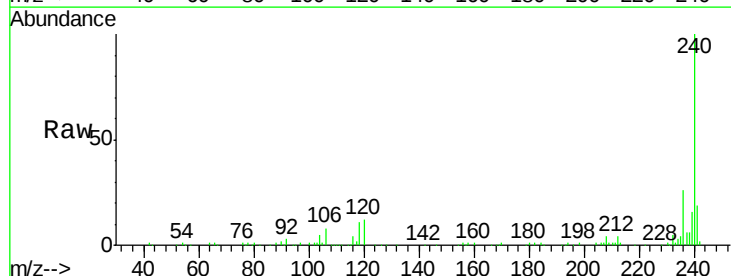

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



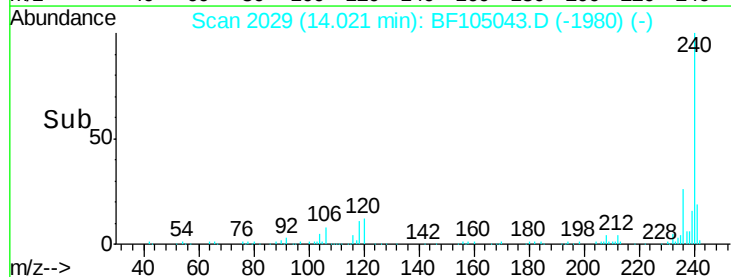
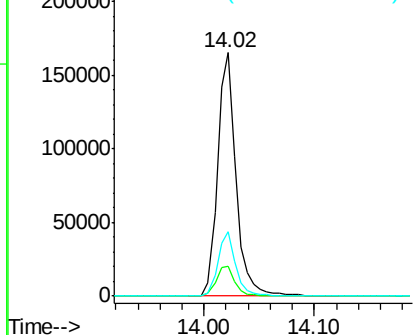




#78
 Terphenyl-d14
 Concen: 93.626 ng
 RT: 12.92 min Scan# 1841
 Delta R.T. 0.00 min
 Lab File: BF105043.D
 Acq: 2 May 2018 20:43

Instrument :
 BNA_F
 ClientSampleId :
 PB108660BL

Tot Ion:244 Resp: 787910
 Ion Ratio Lower Upper
 244 100
 212 6.8 5.4 8.0
 122 10.7 11.0 16.4#

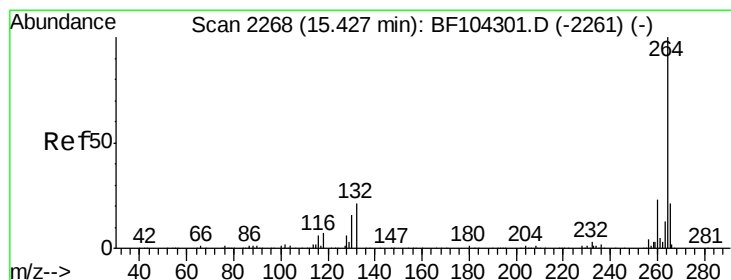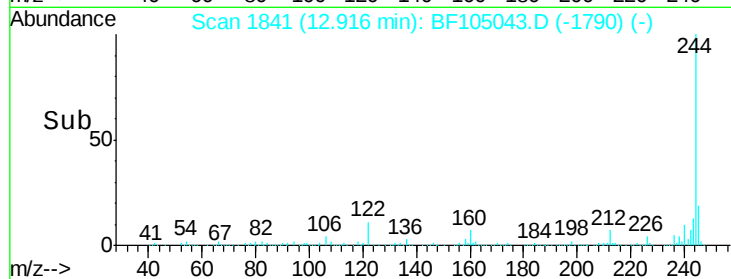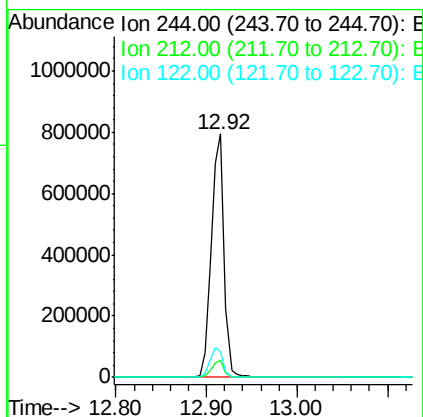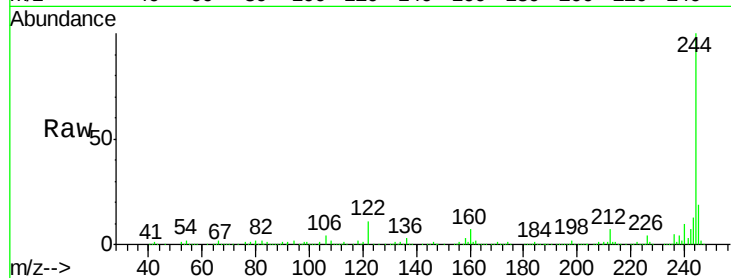

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.58 min Scan# 2294
 Delta R.T. -0.01 min
 Lab File: BF105043.D
 Acq: 2 May 2018 20:43

Tgt Ion:264 Resp: 152391
 Ion Ratio Lower Upper
 264 100
 260 23.0 19.2 28.8
 265 20.8 17.5 26.3

