

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050218\
 Data File : BF105059.D
 Acq On : 3 May 2018 4:42
 Operator : JU/SJ
 Sample : J2684-05
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 043018-DBRI-E-D-B

Quant Time: May 03 07:17:12 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 02 17:25:18 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.79	152	86037	20.00	ng	0.00
21) Naphthalene-d8	8.07	136	348625	20.00	ng	0.00
38) Acenaphthene-d10	9.83	164	150025	20.00	ng	0.00
63) Phenanthrene-d10	11.32	188	251611	20.00	ng	0.00
75) Chrysene-d12	14.00	240	221286	20.00	ng	-0.03
86) Perylene-d12	15.54	264	173823	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	248617	44.18	ng	0.00
7) Phenol-d6	6.42	99	180571	26.12	ng	-0.02
23) Nitrobenzene-d5	7.36	82	535379	100.28	ng	-0.01
41) 2,4,6-Tribromophenol	10.62	330	138311	88.87	ng	-0.01
44) 2-Fluorobiphenyl	9.15	172	937934	98.76	ng	0.00
78) Terphenyl-d14	12.91	244	872646	89.91	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050218\
Data File : BF105059.D
Acq On : 3 May 2018 4:42
Operator : JU/SJ
Sample : J2684-05
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
043018-DBRI-E-D-B

Quant Time: May 03 07:17:12 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 02 17:25:18 2018
Response via : Initial Calibration

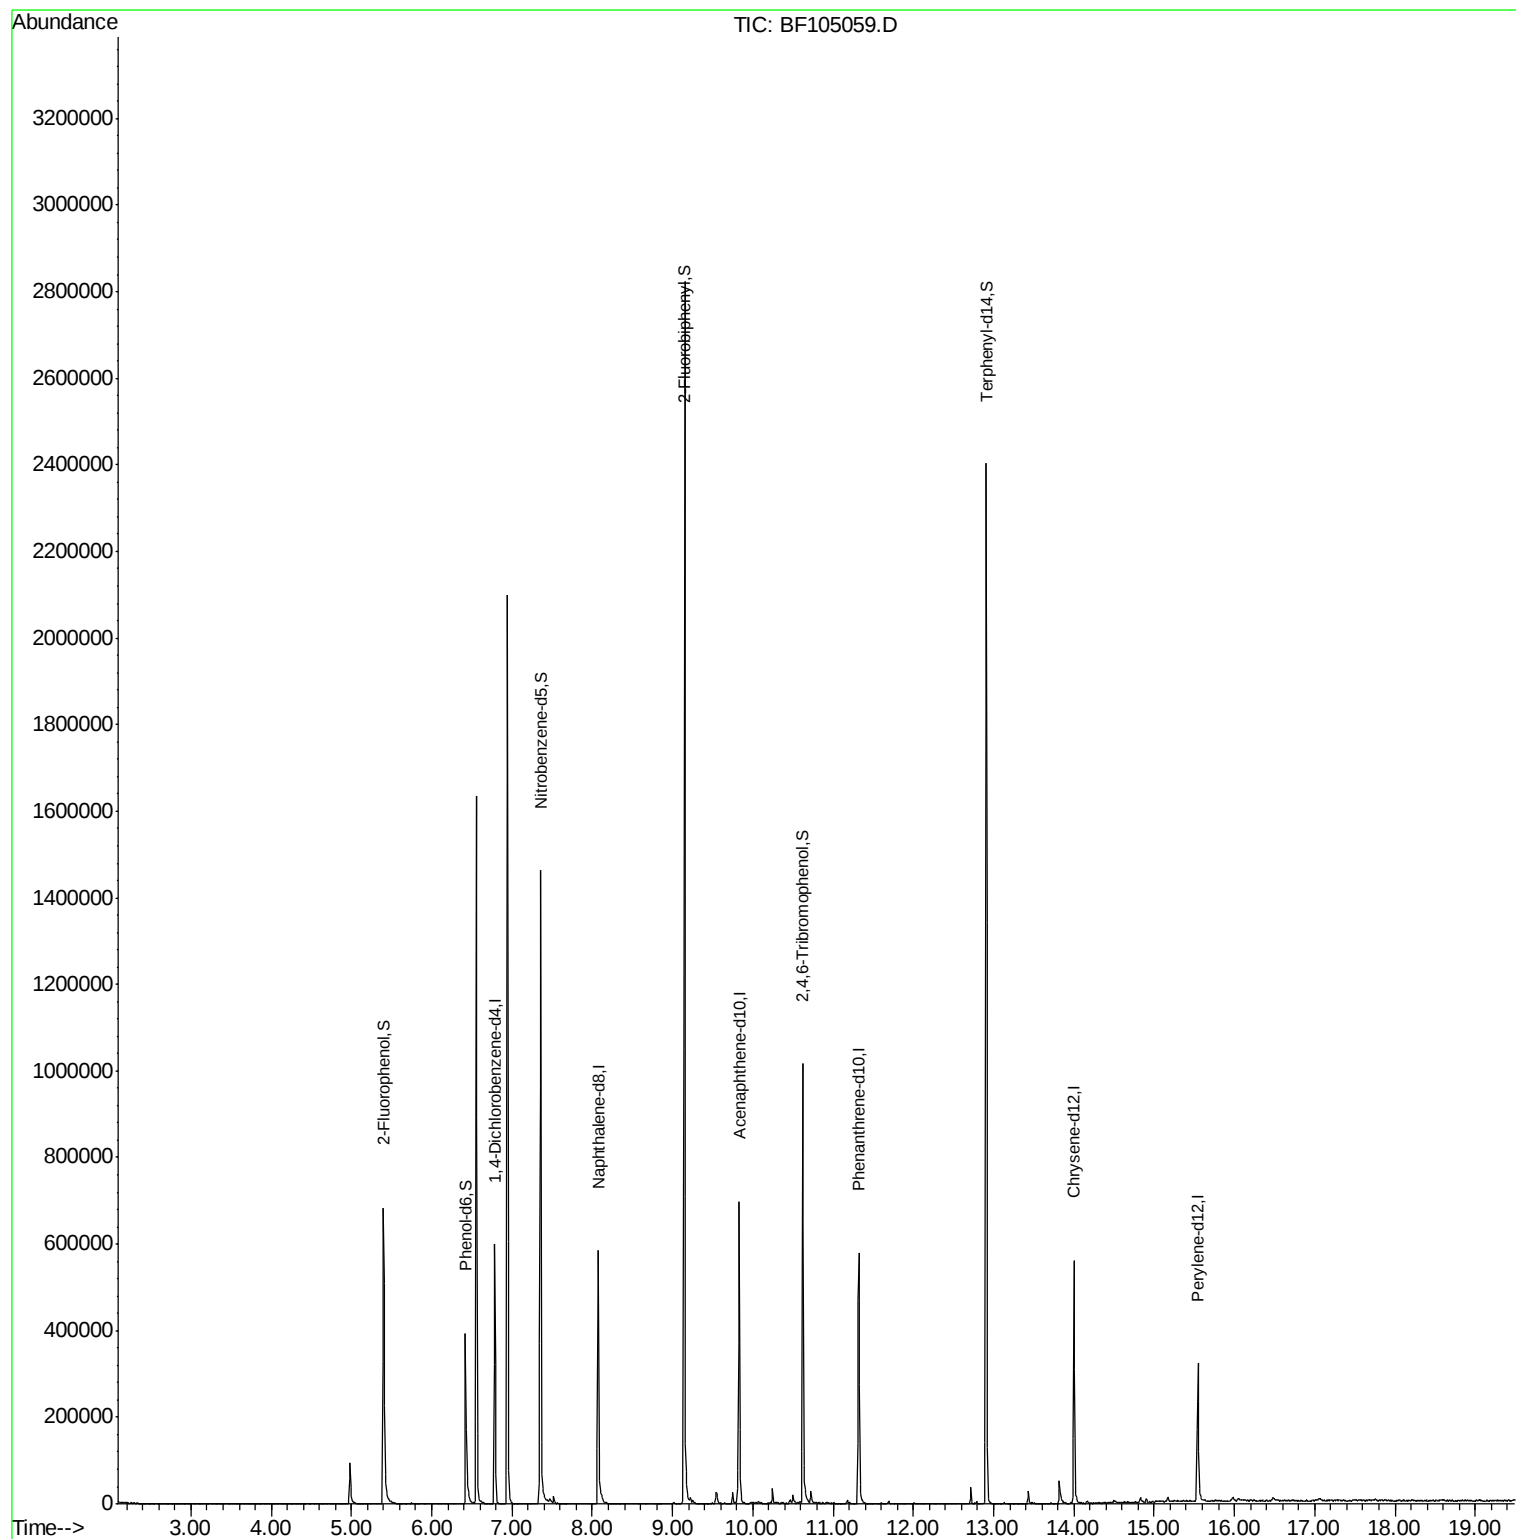



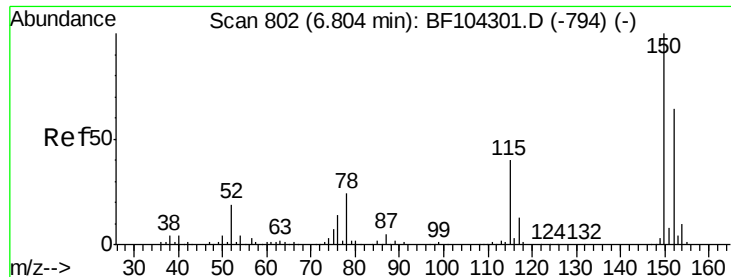


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.79 min Scan# 799
Delta R.T. -0.00 min
Lab File: BF105059.D
Acq: 3 May 2018 4:42

Instrument :
BNA_F
ClientSampleId :
043018-DBRI-E-D-B




Tot Ion:152 Resp: 86037
Ion Ratio Lower Upper
152 100
150 156.1 124.6 186.8
115 63.6 50.1 75.1

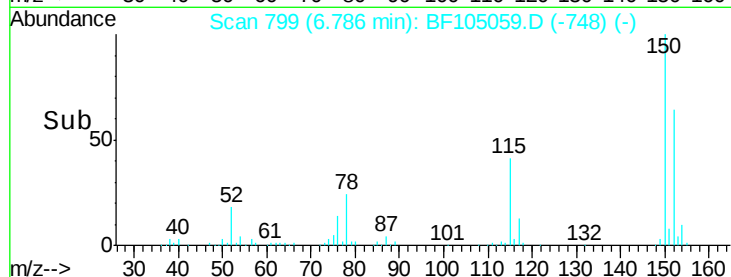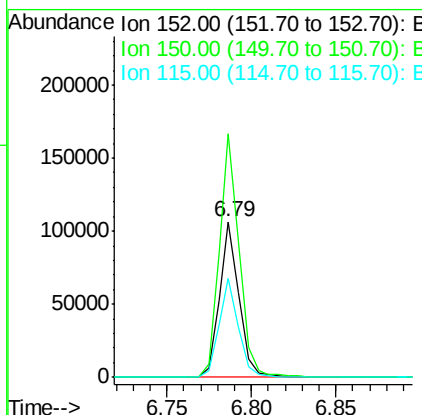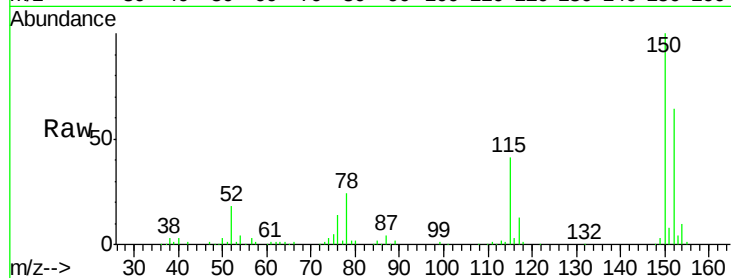

#5

2-Fluorophenol
Concen: 44.184 ng
RT: 5.40 min Scan# 563
Delta R.T. -0.01 min
Lab File: BF105059.D
Acq: 3 May 2018 4:42

Tgt Ion:112 Resp: 248617
Ion Ratio Lower Upper
112 100
64 54.1 47.9 71.9
63 25.9 23.7 35.5

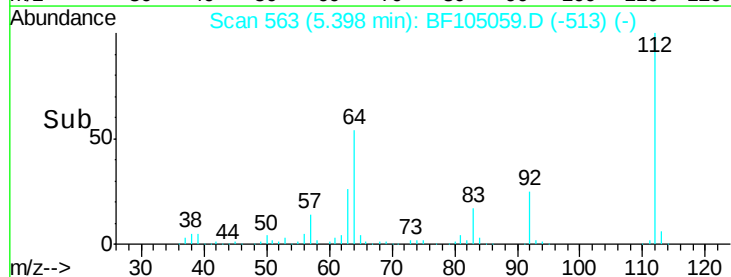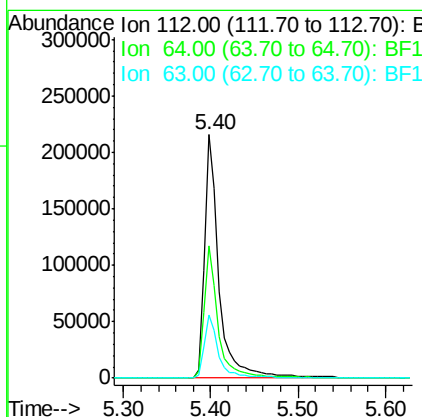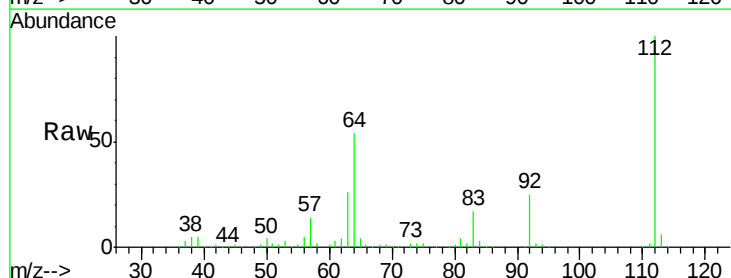



#7

Phenol-d6

Concen: 26.119 ng

RT: 6.42 min Scan# 737

Delta R.T. -0.02 min

Lab File: BF105059.D

Acq: 3 May 2018 4:42

Instrument :

BNA_F

ClientSampleId :

043018-DBRI-E-D-B


Tot Ion: 99 Resp: 180571

Ion Ratio Lower Upper

99 100

42 15.1 14.5 21.7




71 32.5 25.4 38.0

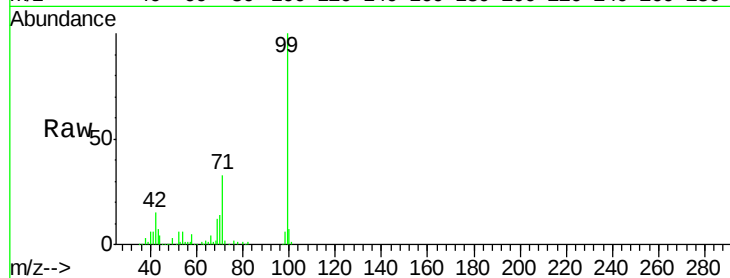

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

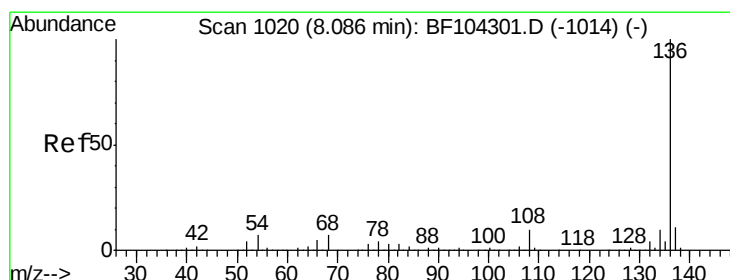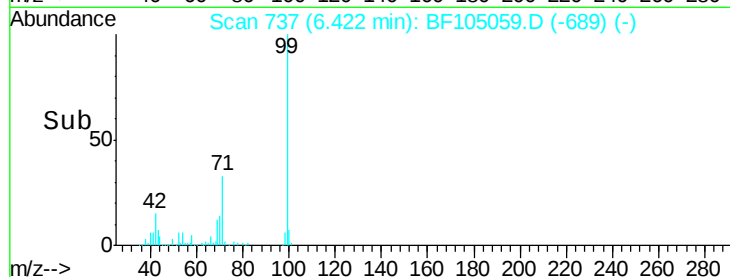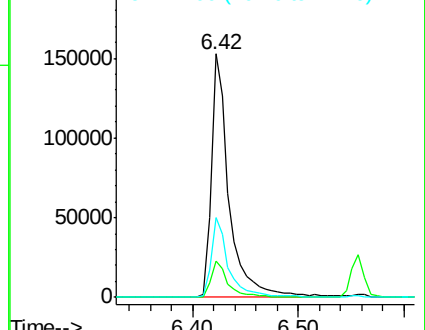

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.07 min Scan# 1018

Delta R.T. -0.00 min

Lab File: BF105059.D

Acq: 3 May 2018 4:42

Tgt Ion: 136 Resp: 348625


Ion Ratio Lower Upper

136 100

137 10.5 8.9 13.3

54 5.6 6.6 9.8#

68 4.8 5.0 7.4#


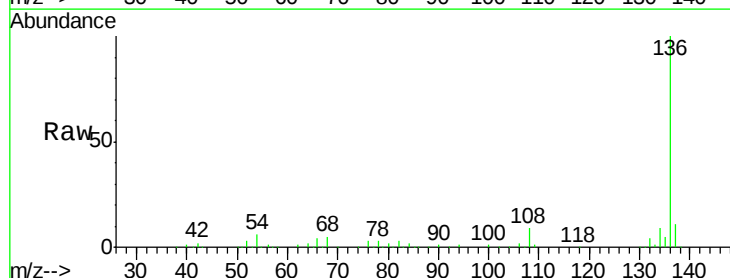


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

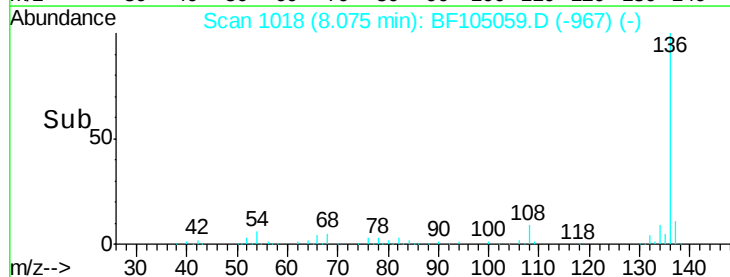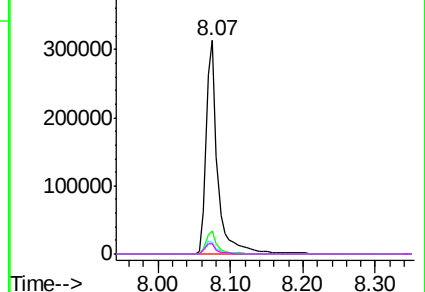







#23
 Nitrobenzene-d5
 Concen: 100.277 ng
 RT: 7.36 min Scan# 896
 Delta R.T. -0.01 min
 Lab File: BF105059.D
 Acq: 3 May 2018 4:42

Instrument :
 BNA_F
 ClientSampleId :
 043018-DBRI-E-D-B

Tot Ion: 82 Resp: 535379
 Ion Ratio Lower Upper
 82 100
 128 46.8 36.1 54.1
 54 43.7 41.4 62.2

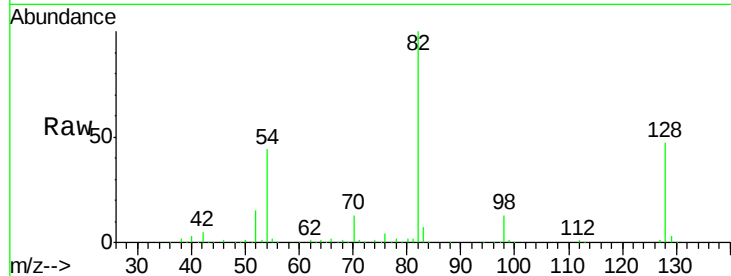


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

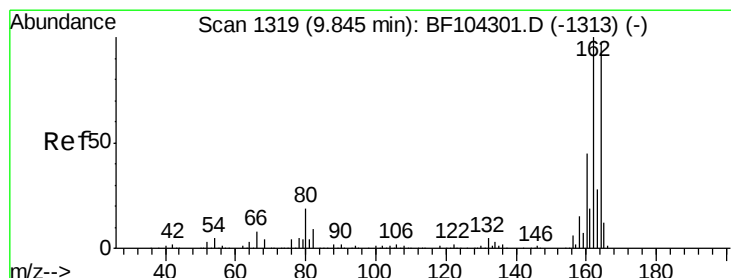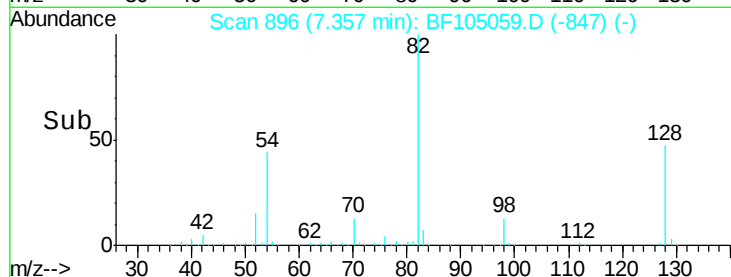
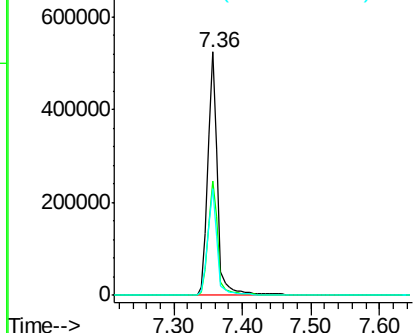


#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.83 min Scan# 1316
 Delta R.T. -0.01 min
 Lab File: BF105059.D
 Acq: 3 May 2018 4:42

Tgt Ion: 164 Resp: 150025
 Ion Ratio Lower Upper
 164 100
 162 104.7 86.1 129.1
 160 45.3 38.3 57.5

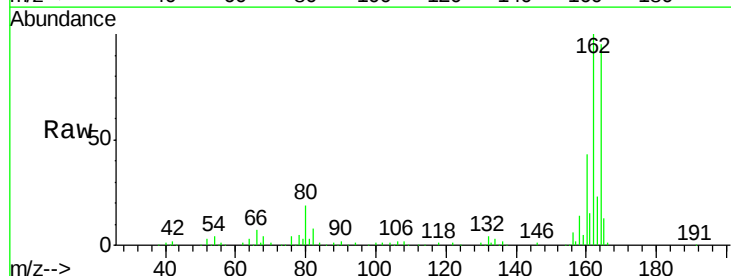

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

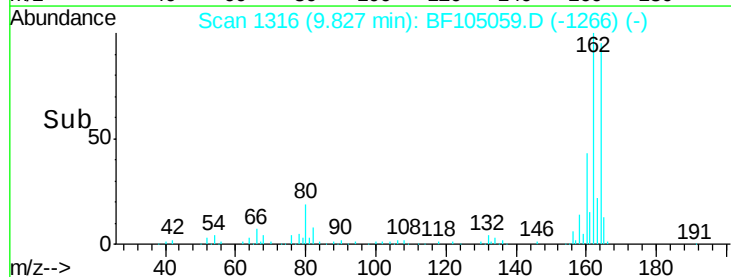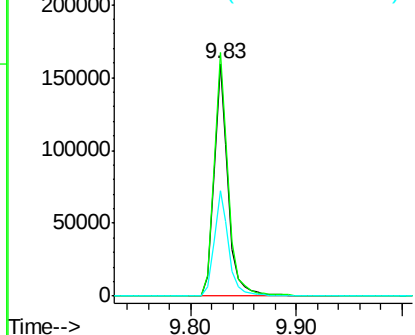







#41
 2,4,6-Tribromophenol
 Concen: 88.875 ng
 RT: 10.62 min Scan# 1451
 Delta R.T. -0.01 min
 Lab File: BF105059.D
 Acq: 3 May 2018 4:42

Instrument :
 BNA_F
 ClientSampleId :
 043018-DBRI-E-D-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.8	77.0	115.6
141	33.4	29.9	44.9

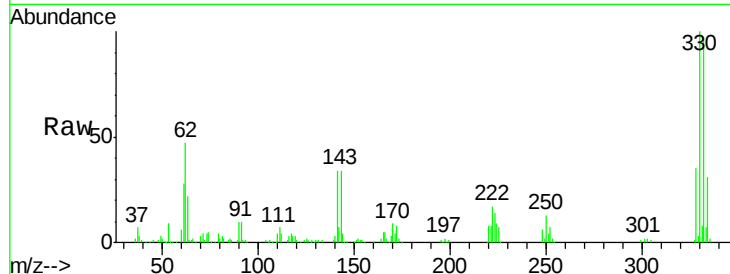


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

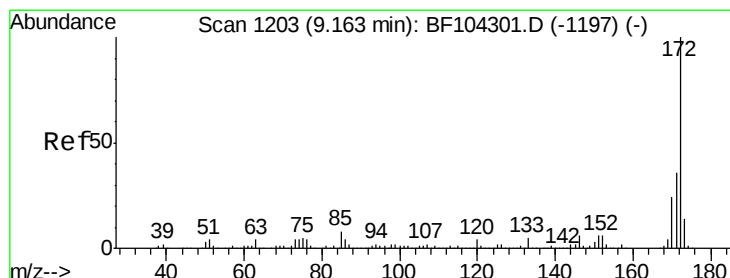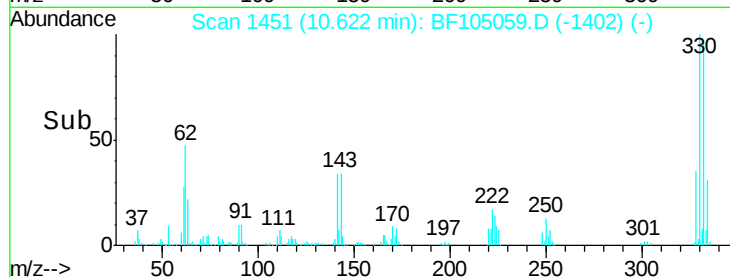
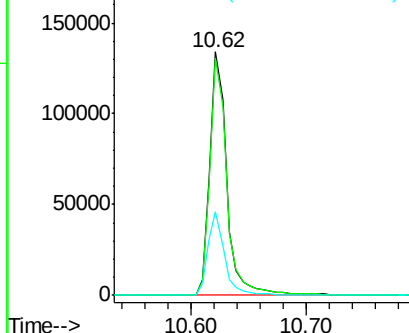


#44
 2-Fluorobiphenyl
 Concen: 98.764 ng
 RT: 9.15 min Scan# 1201
 Delta R.T. -0.01 min
 Lab File: BF105059.D
 Acq: 3 May 2018 4:42

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.6	29.7	44.5
170	24.0	19.6	29.4

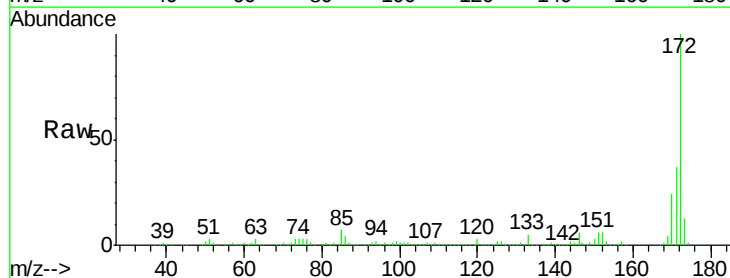

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



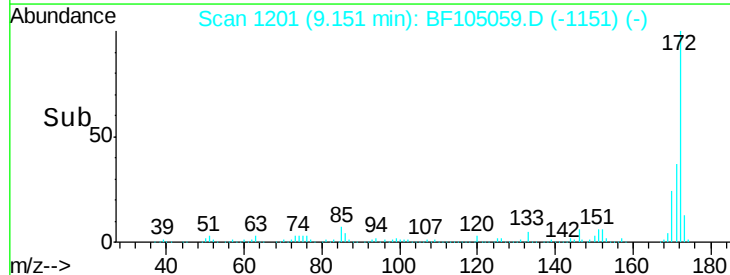
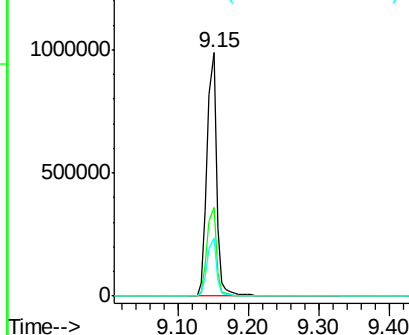




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.32 min Scan# 1570
Delta R.T. -0.00 min
Lab File: BF105059.D
Acq: 3 May 2018 4:42




Instrument :
BNA_F
ClientSampleId :
043018-DBRI-E-D-B

Tot Ion:188 Resp: 251611
Ion Ratio Lower Upper
188 100
94 9.3 8.5 12.7
80 9.5 9.2 13.8

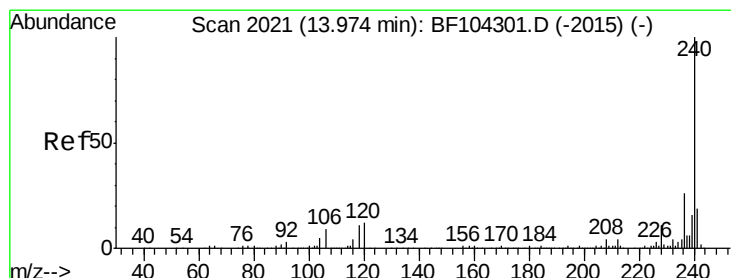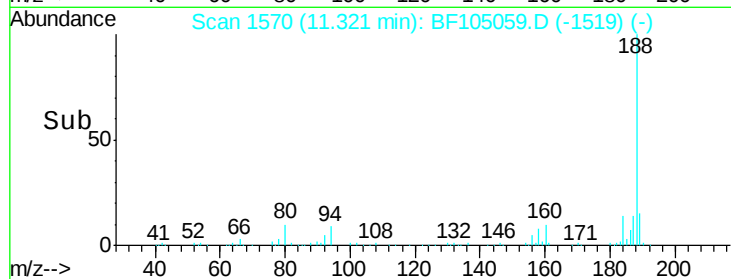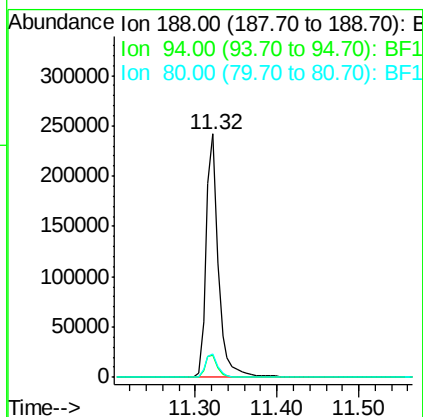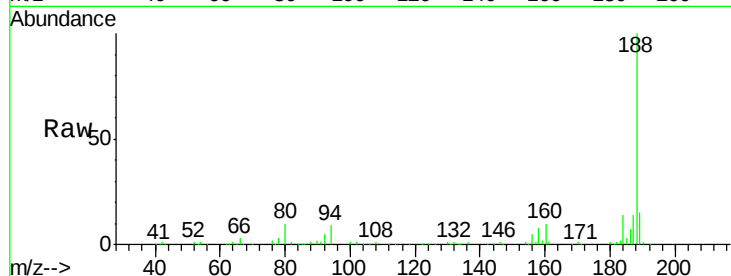

#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.00 min Scan# 2026
Delta R.T. -0.03 min
Lab File: BF105059.D
Acq: 3 May 2018 4:42

Tgt Ion:240 Resp: 221286
Ion Ratio Lower Upper
240 100
120 11.3 9.5 14.3
236 25.0 20.7 31.1

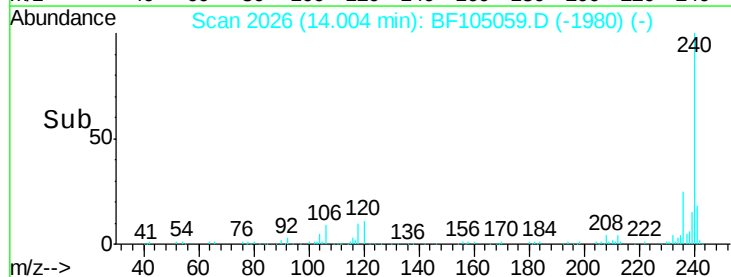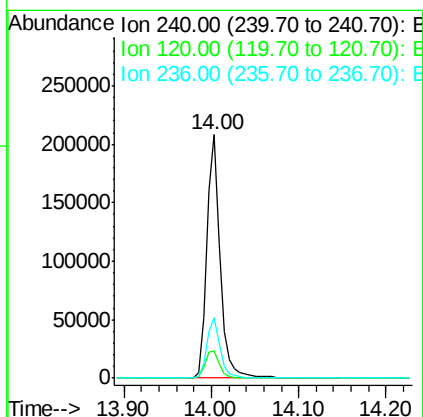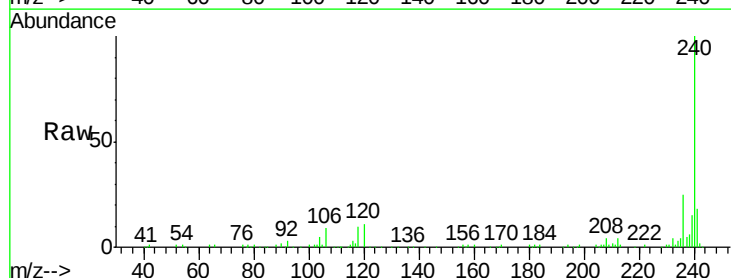



#78

Terphenyl-d14

Concen: 89.906 ng

RT: 12.91 min Scan# 1840

Delta R.T. -0.01 min

Lab File: BF105059.D

Acq: 3 May 2018 4:42

Instrument :

BNA_F

ClientSampleId :

043018-DBRI-E-D-B


Tot Ion:244 Resp: 872646

Ion Ratio Lower Upper




244 100

212 6.9 5.4 8.0

122 12.3 11.0 16.4

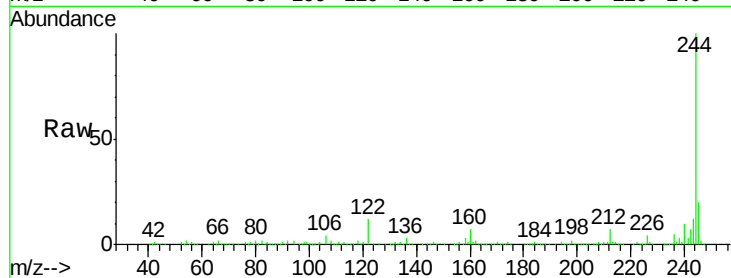

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

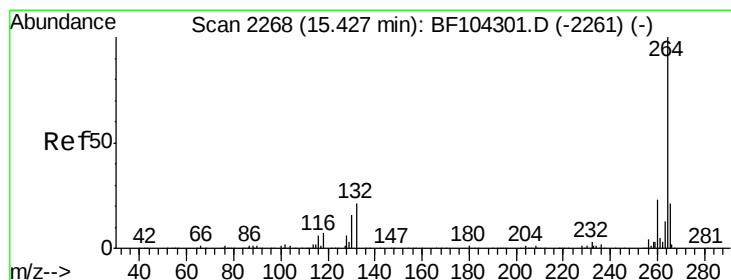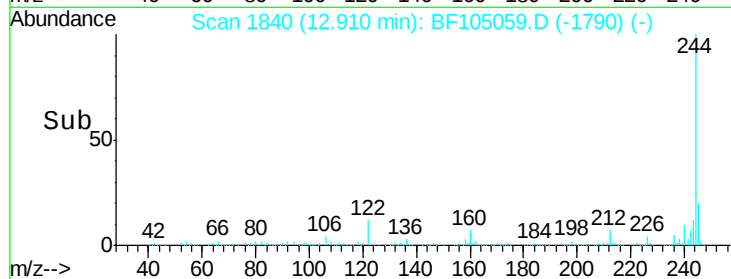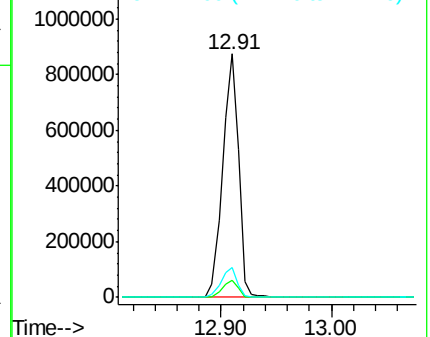

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.54 min Scan# 2288

Delta R.T. -0.05 min

Lab File: BF105059.D

Acq: 3 May 2018 4:42


Tgt Ion:264 Resp: 173823

Ion Ratio Lower Upper

264 100

260 24.2 19.2 28.8

265 21.1 17.5 26.3

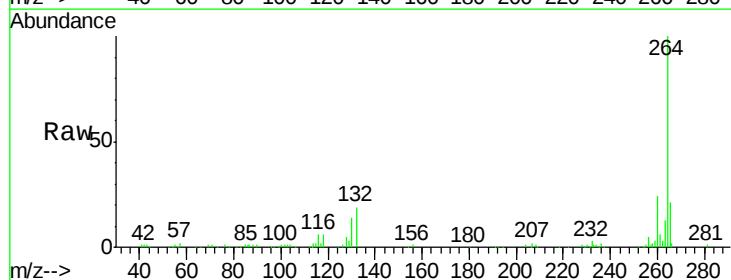

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

