


Data Path : Z:\HPCHEM1\BNA F\Data\BF050218\
 Data File : BF105019.D
 Acq On : 2 May 2018 9:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 02 17:25:18 2018

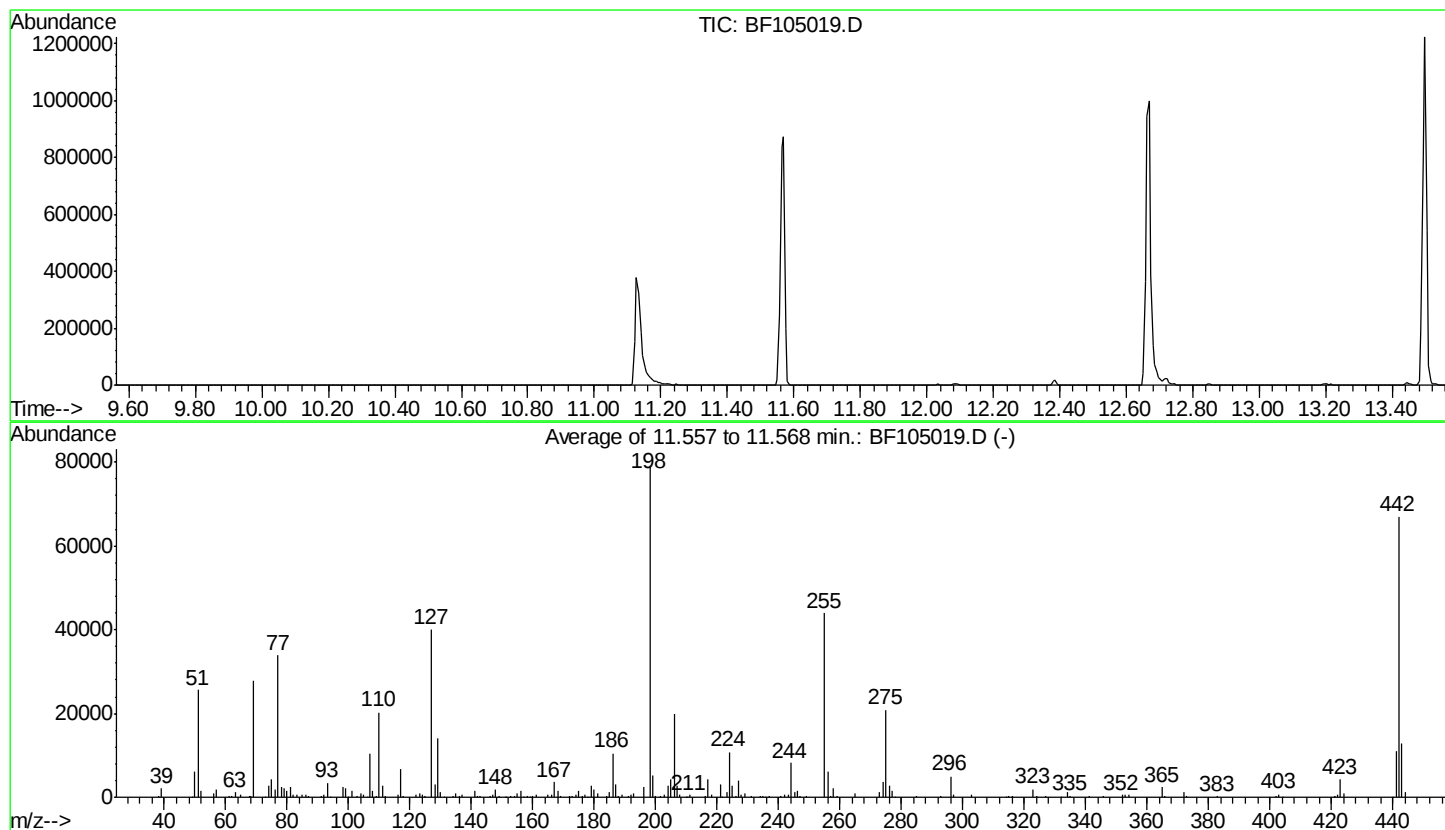

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	25555	PASS
68	69	0.00	2	0.9	260	PASS
69	198	0.00	100	35.2	27902	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.5	40000	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	79176	PASS
199	198	5	9	6.5	5164	PASS
275	198	10	60	26.4	20878	PASS
365	198	1	100	3.1	2415	PASS
441	443	0.01	100	84.8	10898	PASS
442	198	50	100	84.6	66988	PASS
443	442	15	24	19.2	12853	PASS