


Data Path : Z:\HPCHEM1\BNA F\Data\BF050218\
 Data File : BF105046.D
 Acq On : 2 May 2018 22:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 02 17:25:18 2018

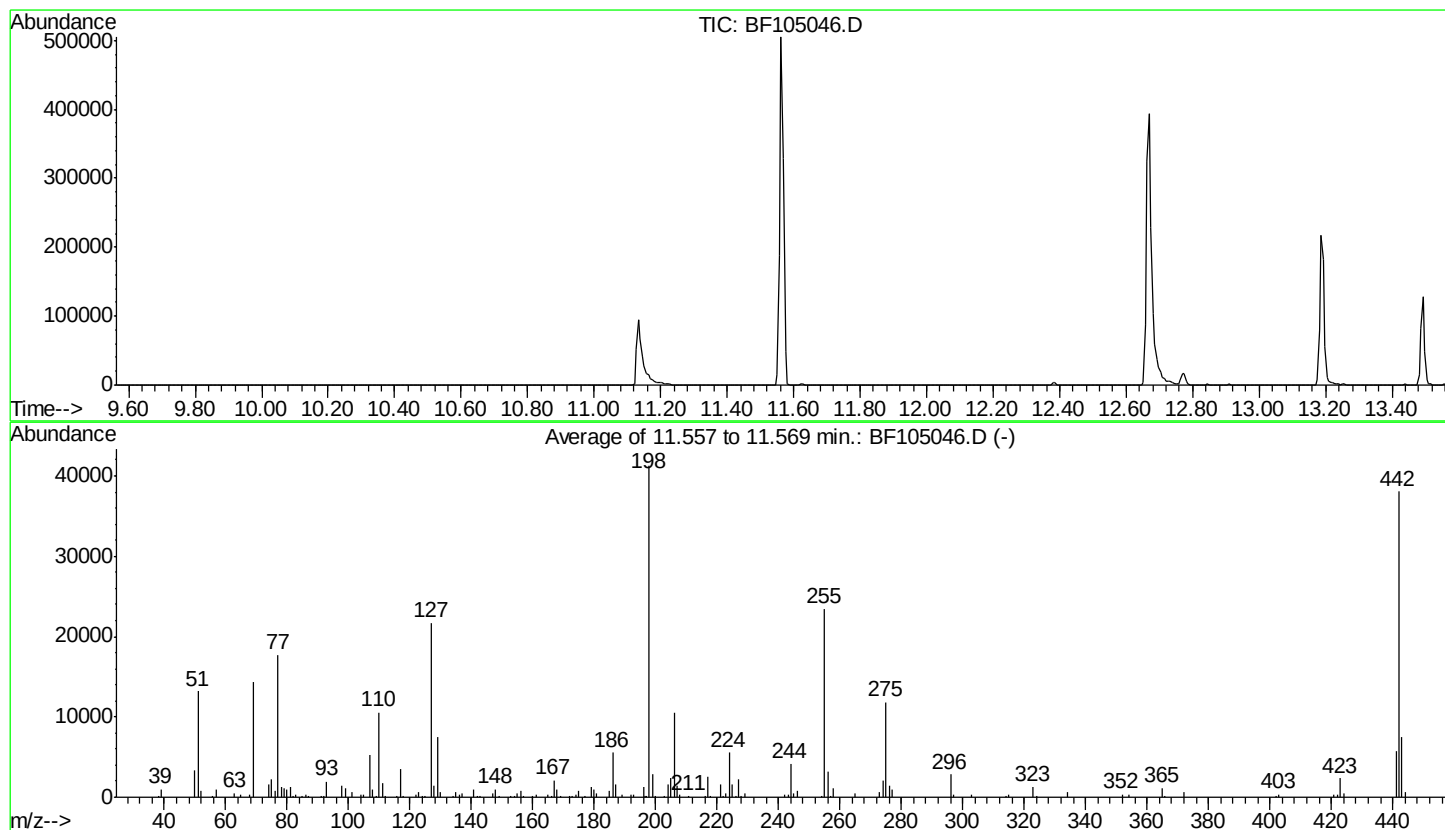

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	13155	PASS
68	69	0.00	2	1.9	272	PASS
69	198	0.00	100	34.7	14338	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.7	21736	PASS
197	198	0.00	2	0.3	114	PASS
198	198	100	100	100.0	41272	PASS
199	198	5	9	7.1	2922	PASS
275	198	10	60	28.8	11866	PASS
365	198	1	100	2.8	1158	PASS
441	443	0.01	100	77.4	5794	PASS
442	198	50	100	92.1	38013	PASS
443	442	15	24	19.7	7487	PASS