
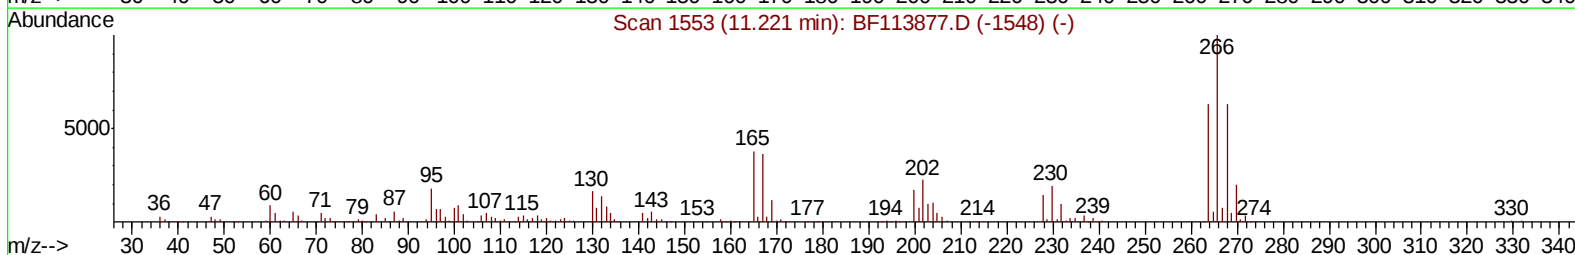
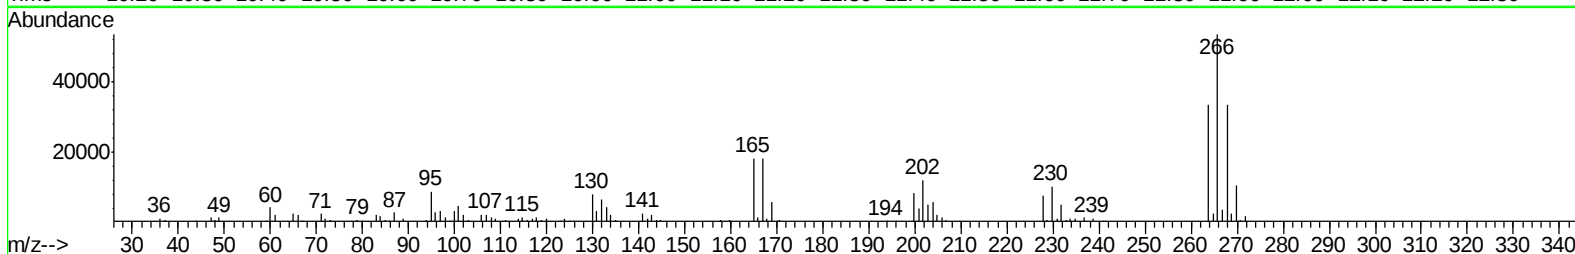


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF050219\
Data File : BF114079.D
Acq On : 2 May 2019 11:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 04:16:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 23 03:32:35 2019
Response via : Initial Calibration

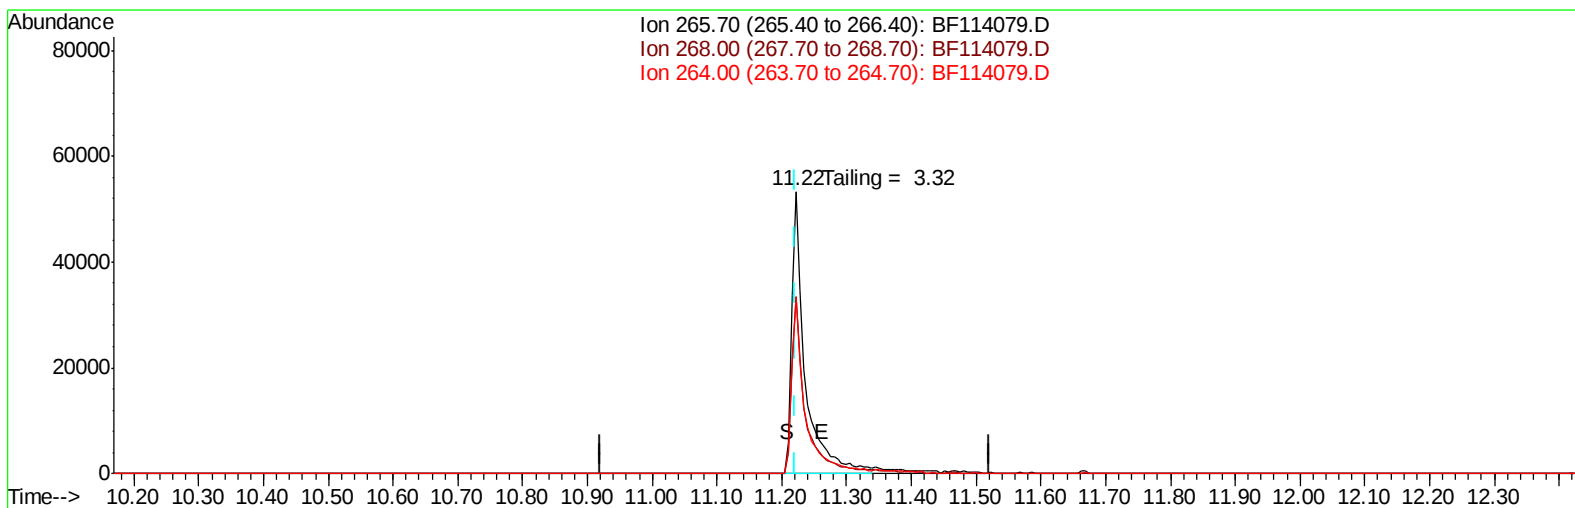

TIC: BF114079.D

(70) Pentachlorophenol (C)




11.222min (+0.000) 28532.57ng

response 79778

Ion	Exp%	Act%
265.70	100	100
268.00	66.90	62.82
264.00	63.80	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF050219\
 Data File : BF114079.D
 Acq On : 2 May 2019 11:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 04:16:31 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF042219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 23 03:32:35 2019
 Response via : Initial Calibration

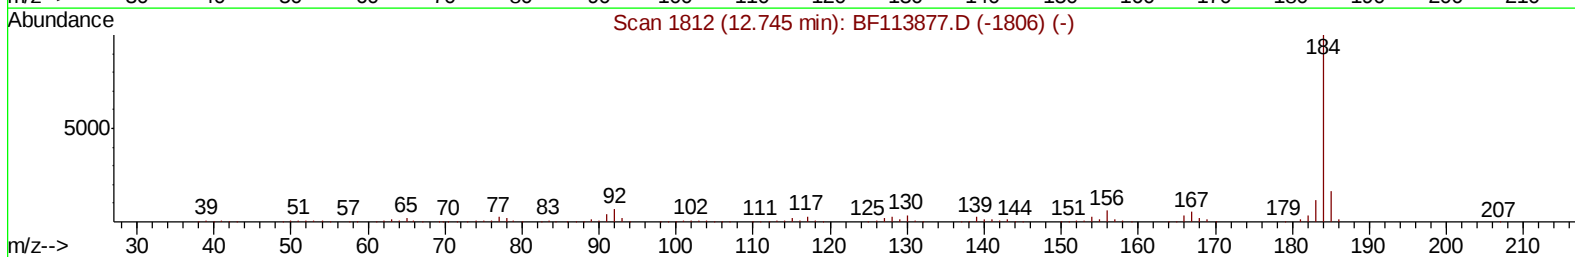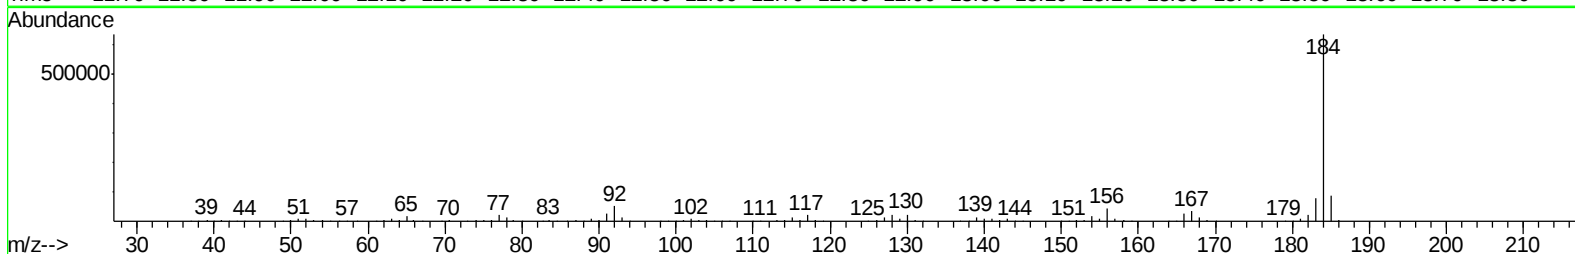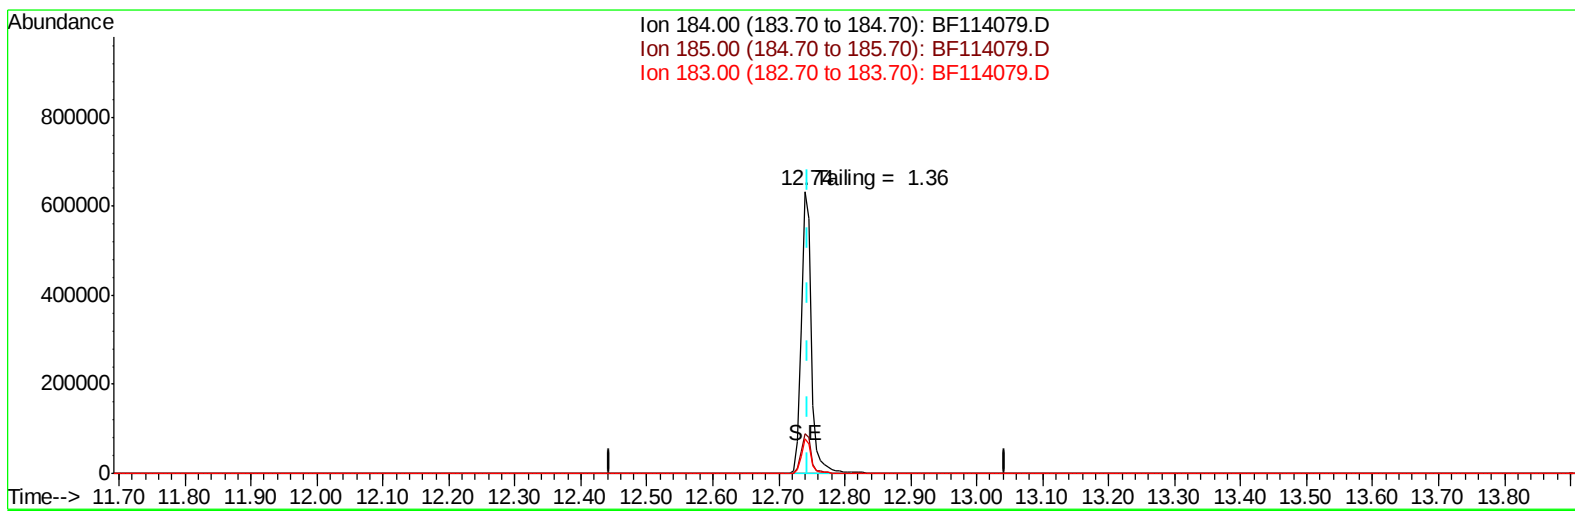

TIC: BF114079.D

(77) Benzidine

12.739min (-0.005) 0.00ng

response 676160

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.01
183.00	11.70	12.22
0.00	0.00	0.00