


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050219\
 Data File : BF114079.D
 Acq On : 2 May 2019 11:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 23 03:32:35 2019

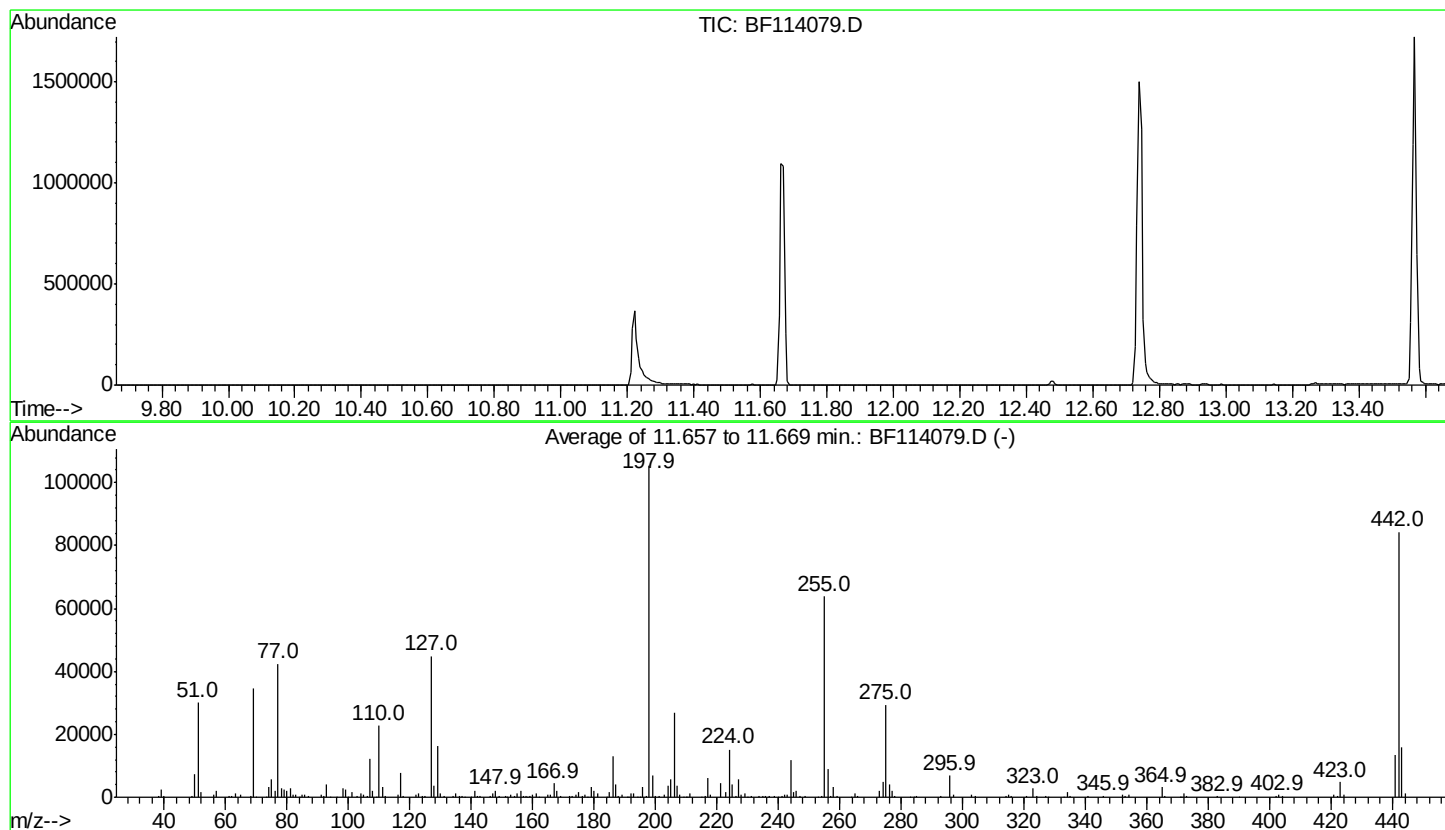

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.5	30026	PASS
68	69	0.00	2	1.7	593	PASS
69	198	0.00	100	32.8	34557	PASS
70	69	0.00	2	0.3	118	PASS
127	198	10	80	42.5	44840	PASS
197	198	0.00	2	0.5	554	PASS
198	198	100	100	100.0	105426	PASS
199	198	5	9	6.7	7108	PASS
275	198	10	60	27.8	29360	PASS
365	198	1	100	3.1	3240	PASS
441	198	0.01	100	12.9	13625	PASS
442	198	50	100	80.0	84371	PASS
443	442	15	24	18.8	15863	PASS