Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050222\
Data File : BF128037.D
Acq On : 02 May 2022 20:34
Operator : CG\JU
Sample : N2611-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Quant Time: May 03 07:29:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 05:13:03 2022
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Dichlorobenzene-d4	6.934	152	92990	20.000 ng	0.00
21) Naphthalene-d8	8.222	136	320405	20.000 ng	0.00
39) Acenaphthene-d10	9.980	164	151057	20.000 ng	0.00
64) Phenanthrene-d10	11.475	188	253903	20.000 ng	0.00
76) Chrysene-d12	14.127	240	142873	20.000 ng	# 0.01
86) Perylene-d12	15.651	264	110797	20.000 ng	0.03
System Monitoring Compounds					
5) 2-Fluorophenol	5.563	112	600794	102.907 ng	0.01
7) Phenol-d6	6.563	99	774870	102.287 ng	0.00
23) Nitrobenzene-d5	7.498	82	506077	74.274 ng	0.00
42) 2,4,6-Tribromophenol	10.775	330	150630	99.057 ng	0.00
45) 2-Fluorobiphenyl	9.292	172	761750	85.311 ng	0.00
79) Terphenyl-d14	13.063	244	744145	95.239 ng	0.00
Target Compounds					Qvalue
9) Benzaldehyde	6.487	77	25371	5.414 ng	# 1
18) Hexachloroethane	7.463	117	38746	15.138 ng	# 1
19) n-Nitroso-di-n-propyla...	7.351	70	17716	3.820 ng	# 77
20) 3+4-Methylphenols	7.334	107	24195	3.831 ng	86
22) Acetophenone	7.322	105	36283	4.646 ng	# 64
25) Isophorone	7.498	82	505453	44.076 ng	# 68
31) Naphthalene	8.251	128	2800293	171.599 ng	98
33) 4-Chloroaniline	8.251	127	381674	59.112 ng	# 31
37) 2-Methylnaphthalene	8.934	142	423081	39.229 ng	99
38) 1-Methylnaphthalene	9.033	142	235291	22.445 ng	99
46) 1,1'-Biphenyl	9.392	154	54610	4.880 ng	98
49) Acenaphthylene	9.839	152	38881	2.984 ng	# 97
52) Acenaphthene	10.010	154	52270	5.967 ng	96
55) Dibenzofuran	10.180	168	69421	5.493 ng	# 96
57) 2,4-Dinitrotoluene	10.151	165	6944	2.390 ng	# 39
58) Fluorene	10.528	166	82161	8.712 ng	97
67) 4-Bromophenyl-phenylether	10.775	248	9430	3.350 ng	# 1
71) Phenanthrene	11.498	178	511648	38.497 ng	99
72) Anthracene	11.551	178	141624	10.697 ng	99
73) Carbazole	11.704	167	29318	2.298 ng	94
75) Fluoranthene	12.698	202	685190	48.984 ng	97
78) Pyrene	12.927	202	653664	56.676 ng	99
81) Benzo(a)anthracene	14.116	228	248273	26.071 ng	95
83) Chrysene	14.151	228	214405	23.575 ng	98
87) Indeno(1,2,3-cd)pyrene	17.204	276	98125	13.268 ng	# 94
88) Benzo(b)fluoranthene	15.198	252	296577	42.618 ng	# 97
89) Benzo(k)fluoranthene	15.198	252	296577	42.301 ng	# 95
90) Benzo(a)pyrene	15.580	252	162037	28.071 ng	97
91) Dibenzo(a,h)anthracene	17.209	278	24345	4.105 ng	# 69
92) Benzo(g,h,i)perylene	17.680	276	101911	16.304 ng	# 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050222\
Data File : BF128037.D
Acq On : 02 May 2022 20:34
Operator : CG\JU
Sample : N2611-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Quant Time: May 03 07:29:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 05:13:03 2022
Response via : Initial Calibration

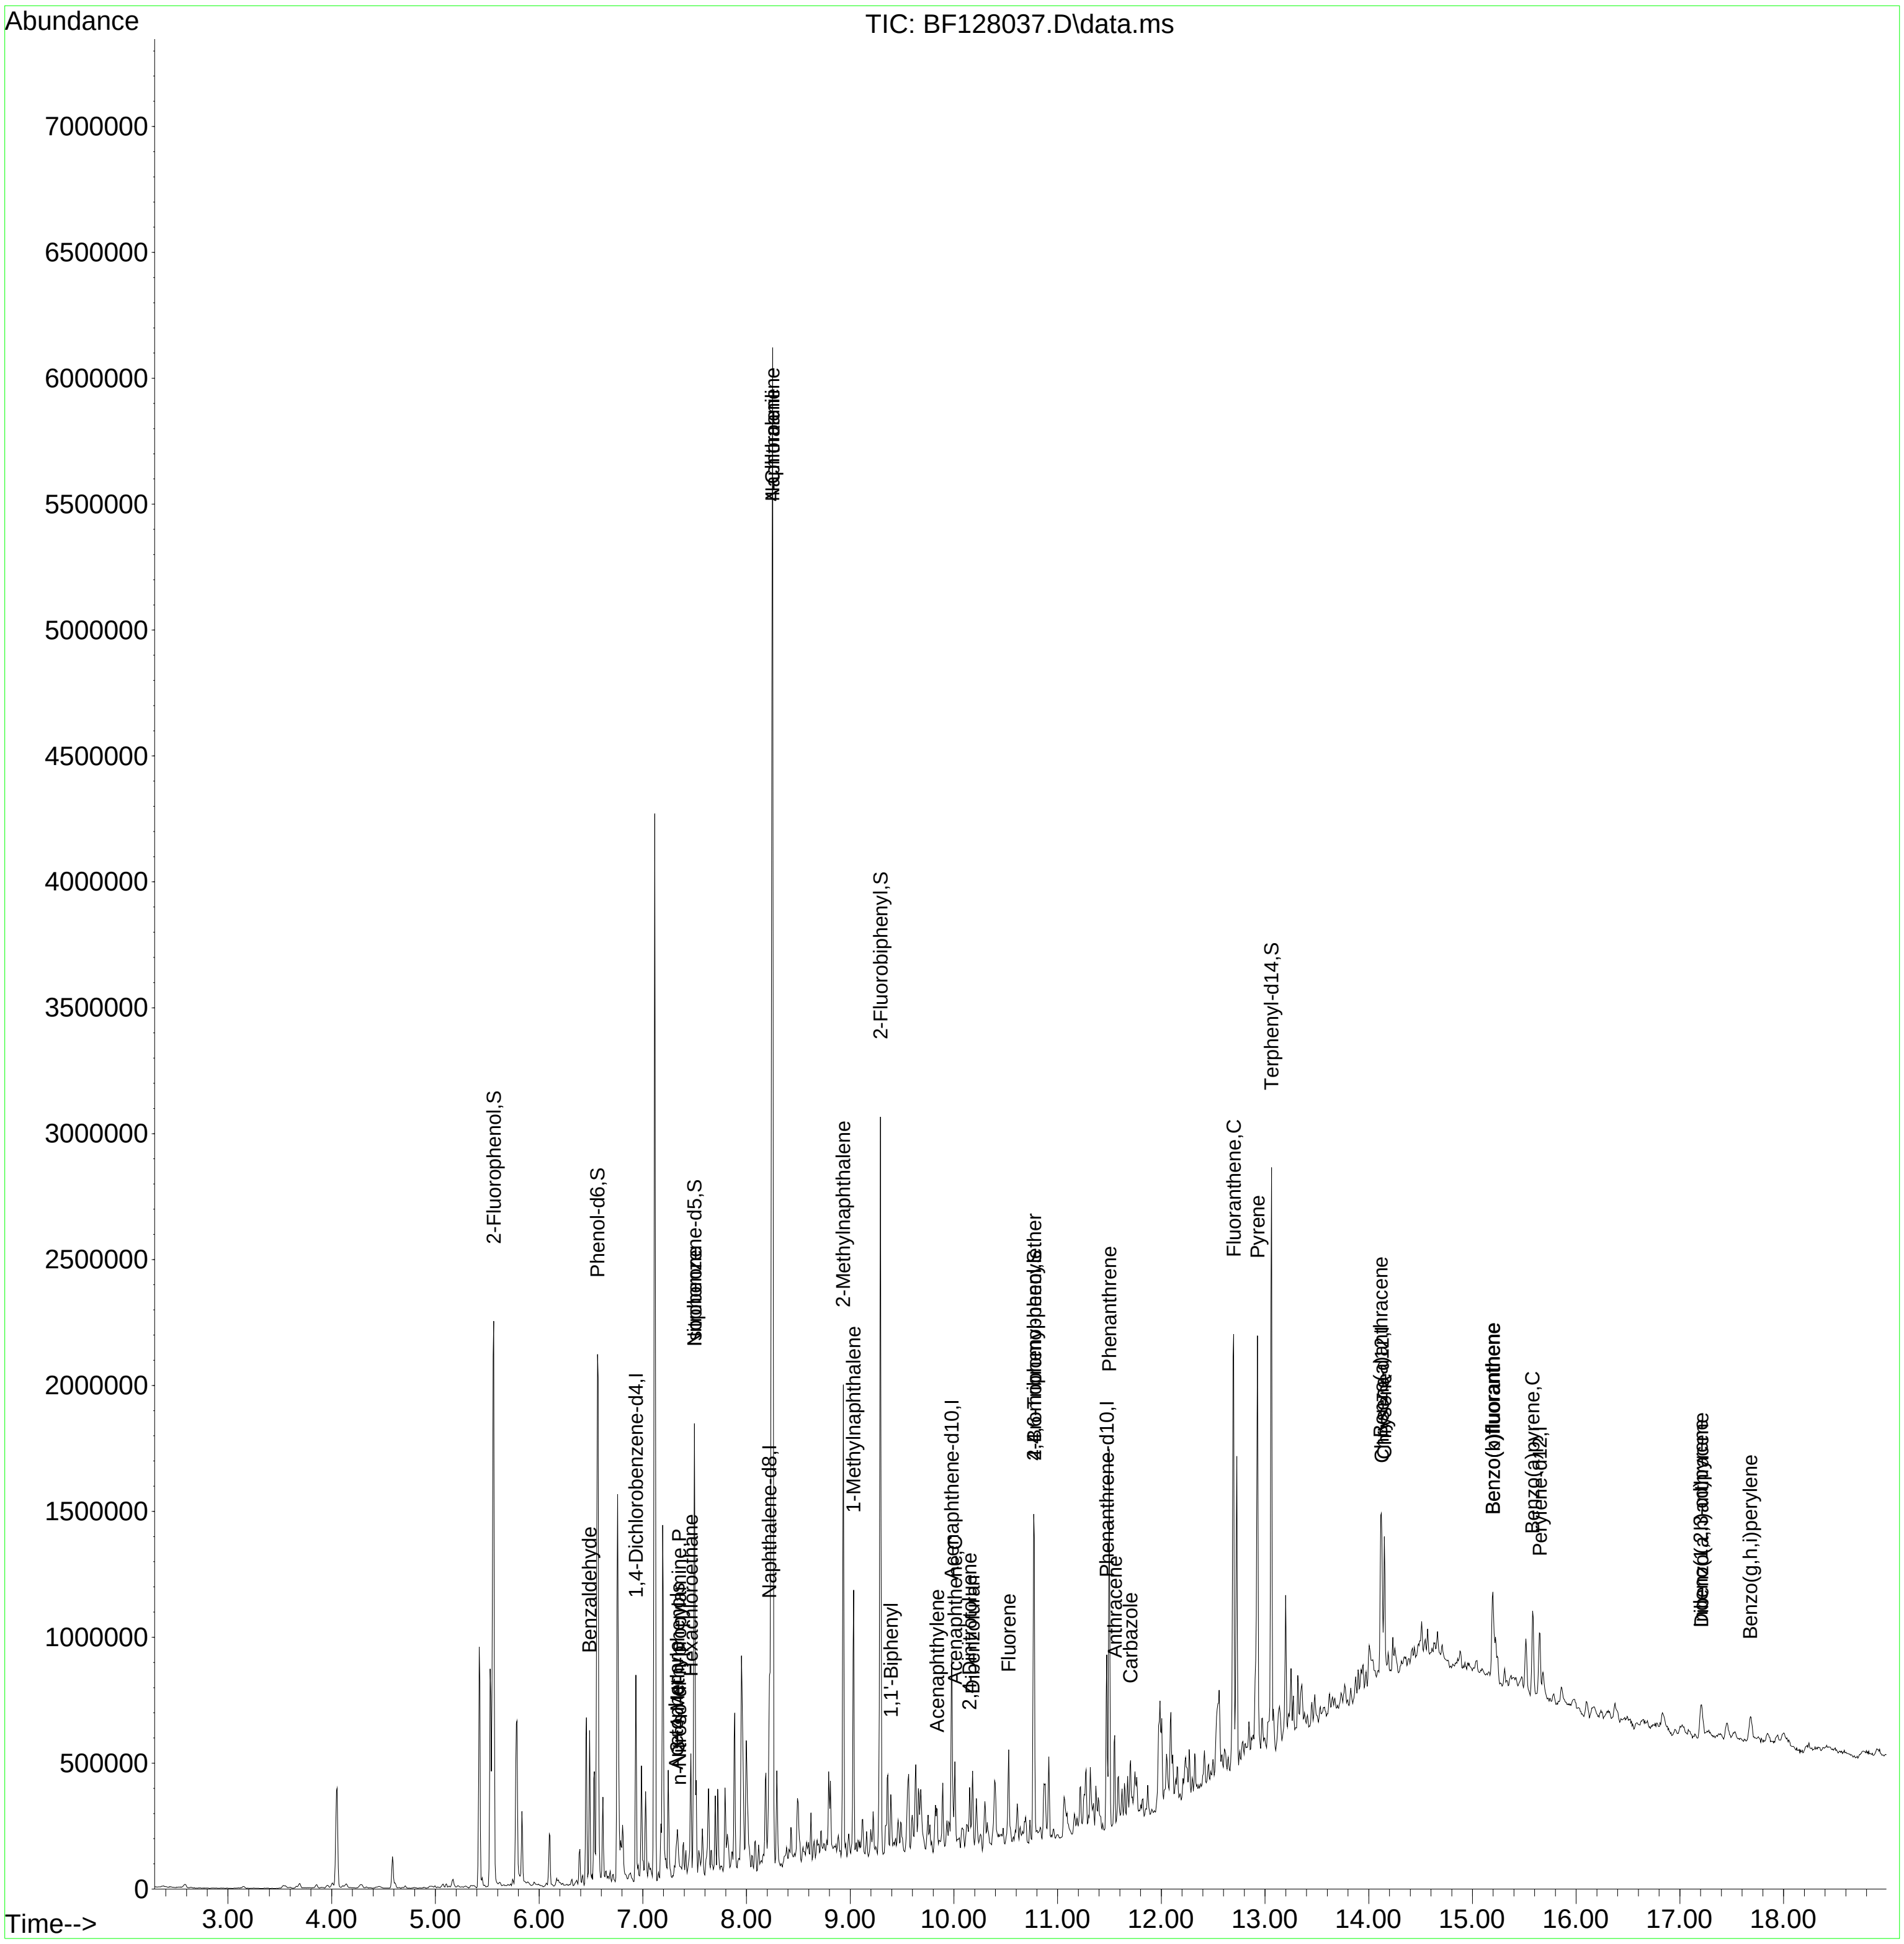

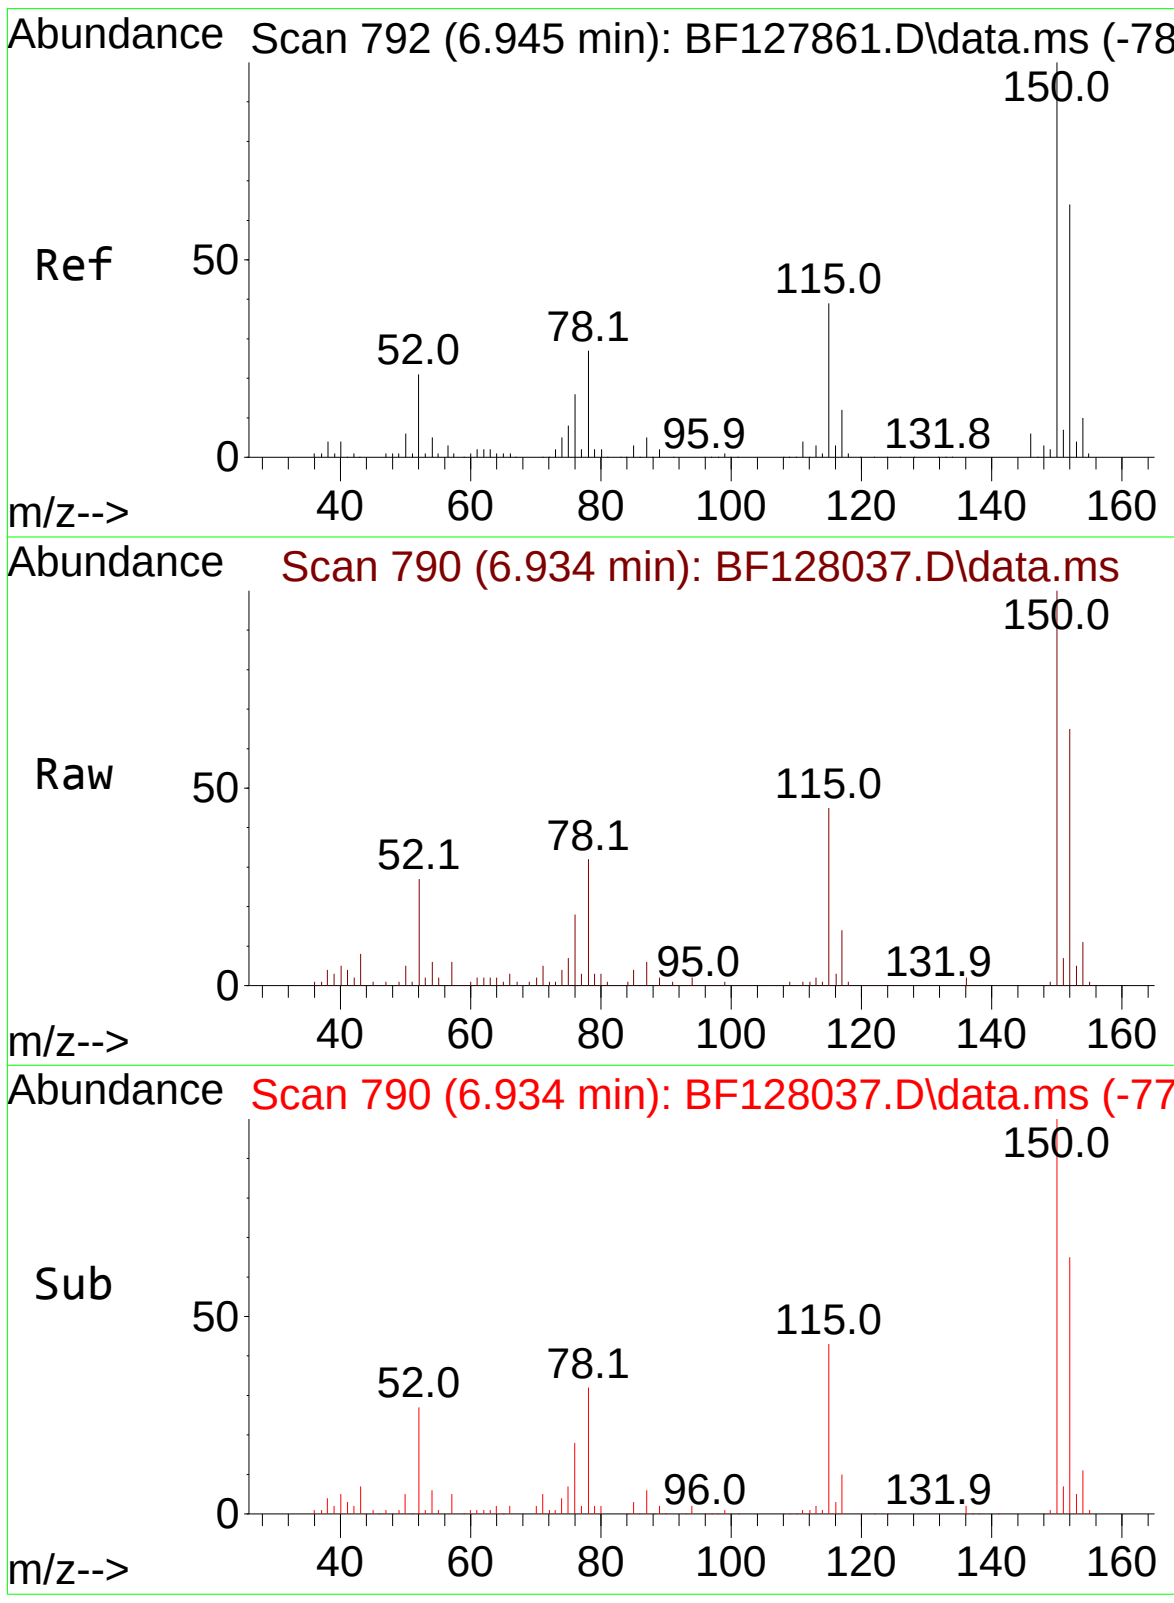

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.934 min   Scan# 7

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Delta R.T.   -0.000 min
Lab File: BF128037.D
Acq: 02 May 2022   20:34

Tgt Ion:152 Resp: 92990

Ion	Ratio	Lower	Upper
152	100		
150	153.0	125.3	187.9
115	68.4	48.8	73.2



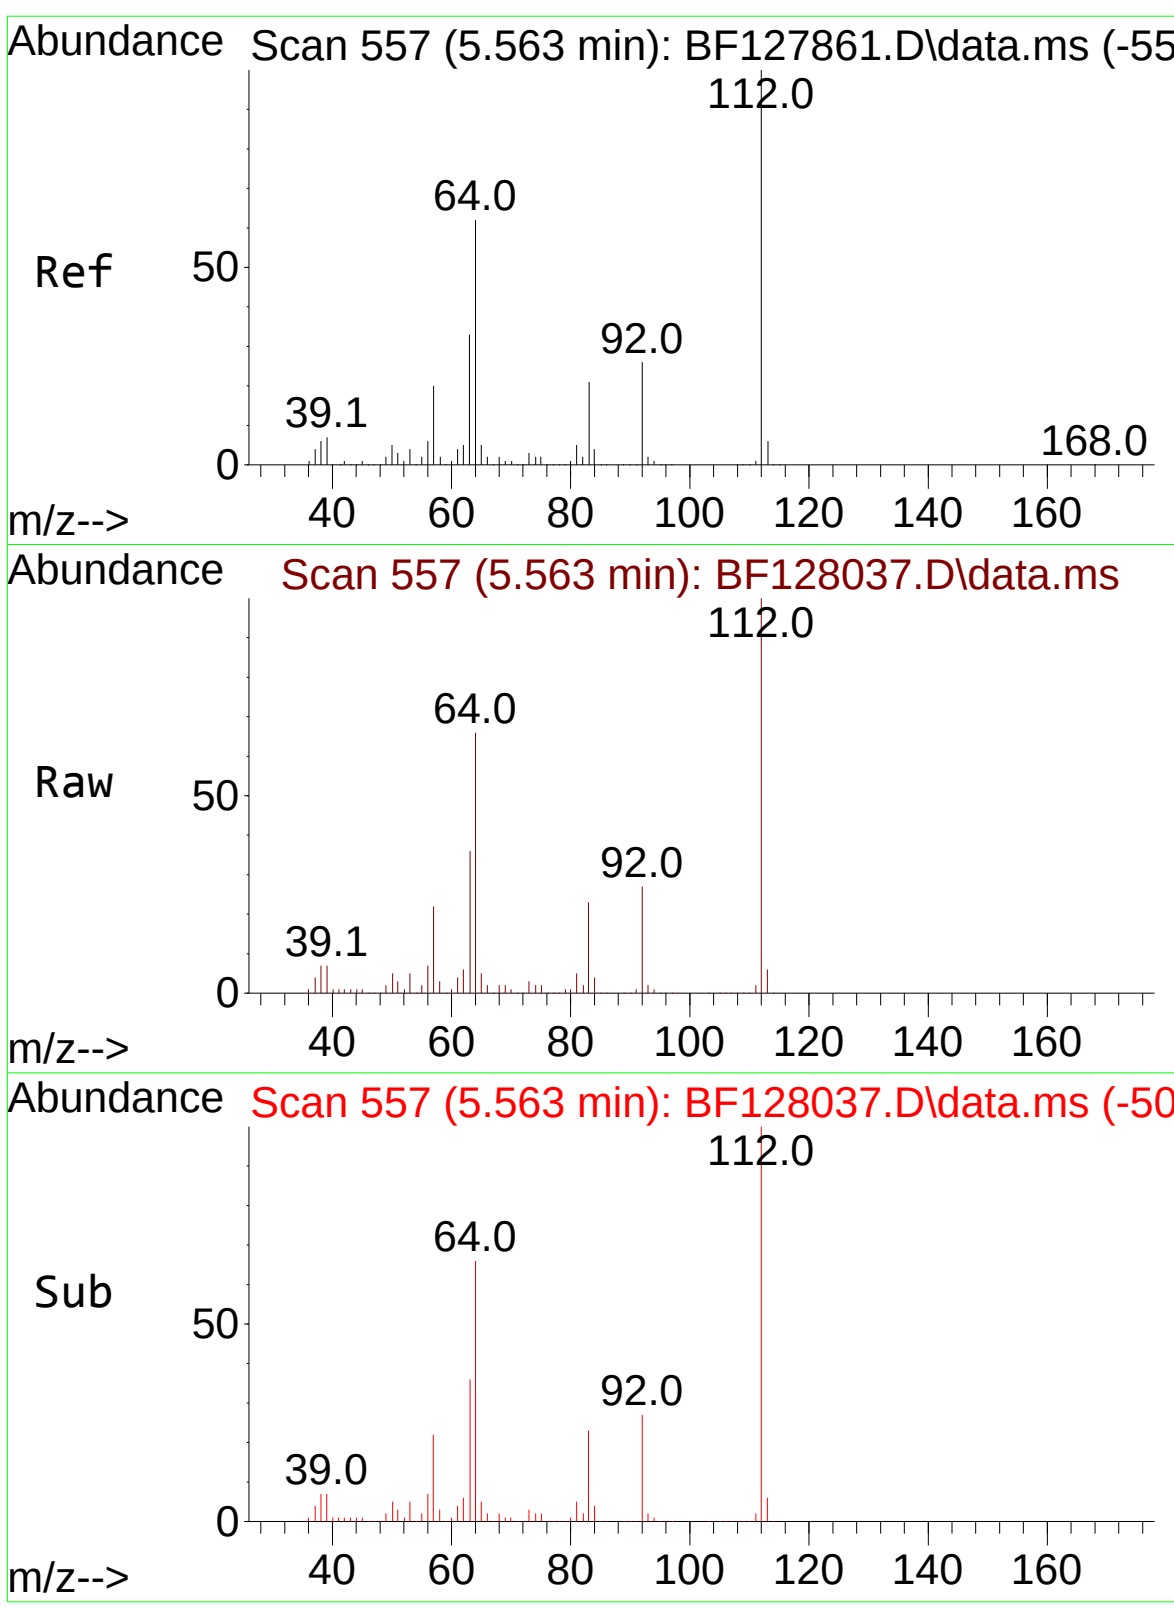

#5
2-Fluorophenol
Concen: 102.907 ng
RT: 5.563 min   Scan# 557
Delta R.T.   0.012 min
Lab File: BF128037.D
Acq: 02 May 2022   20:34

Tgt Ion:112 Resp: 600794

Ion	Ratio	Lower	Upper
112	100		
64	65.6	49.5	74.3
63	35.9	26.3	39.5



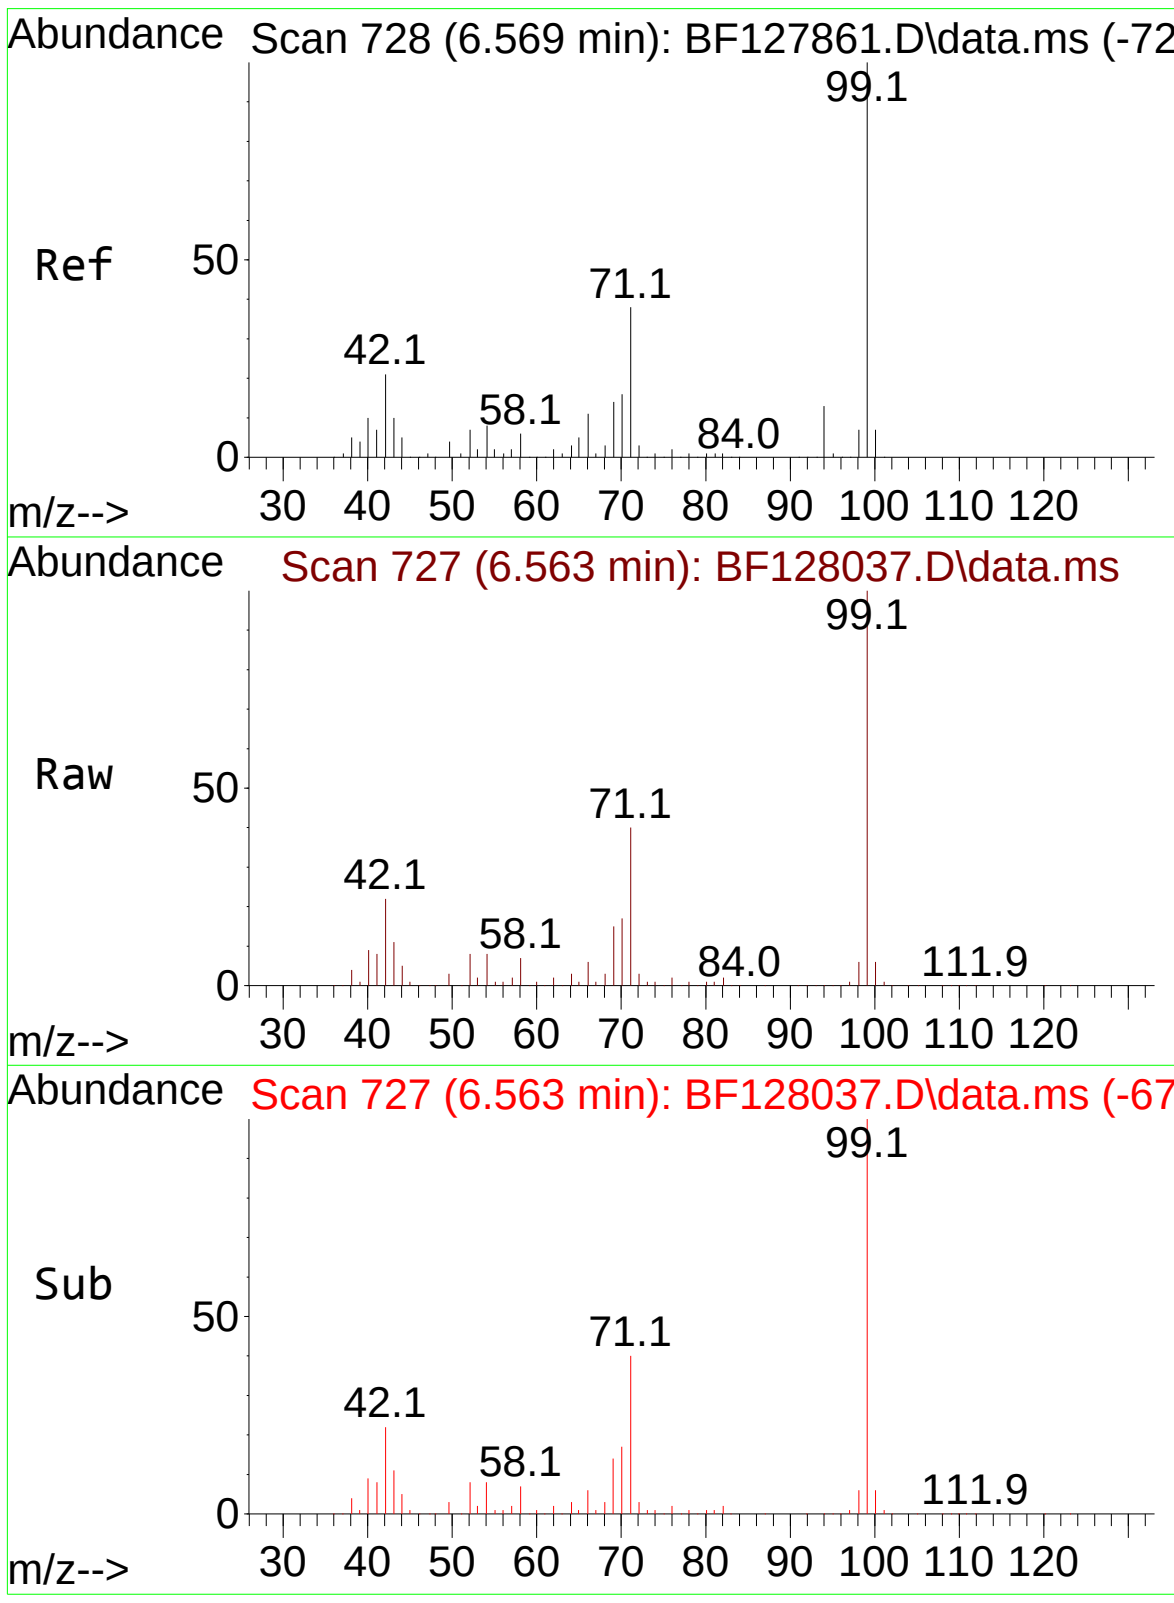

#7
Phenol-d6
Concen: 102.287 ng
RT: 6.563 min Scan# 7
Delta R.T. 0.000 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Tgt Ion: 99 Resp: 774870

Ion	Ratio	Lower	Upper
99	100		
42	22.1	16.6	24.8
71	40.3	30.0	45.0



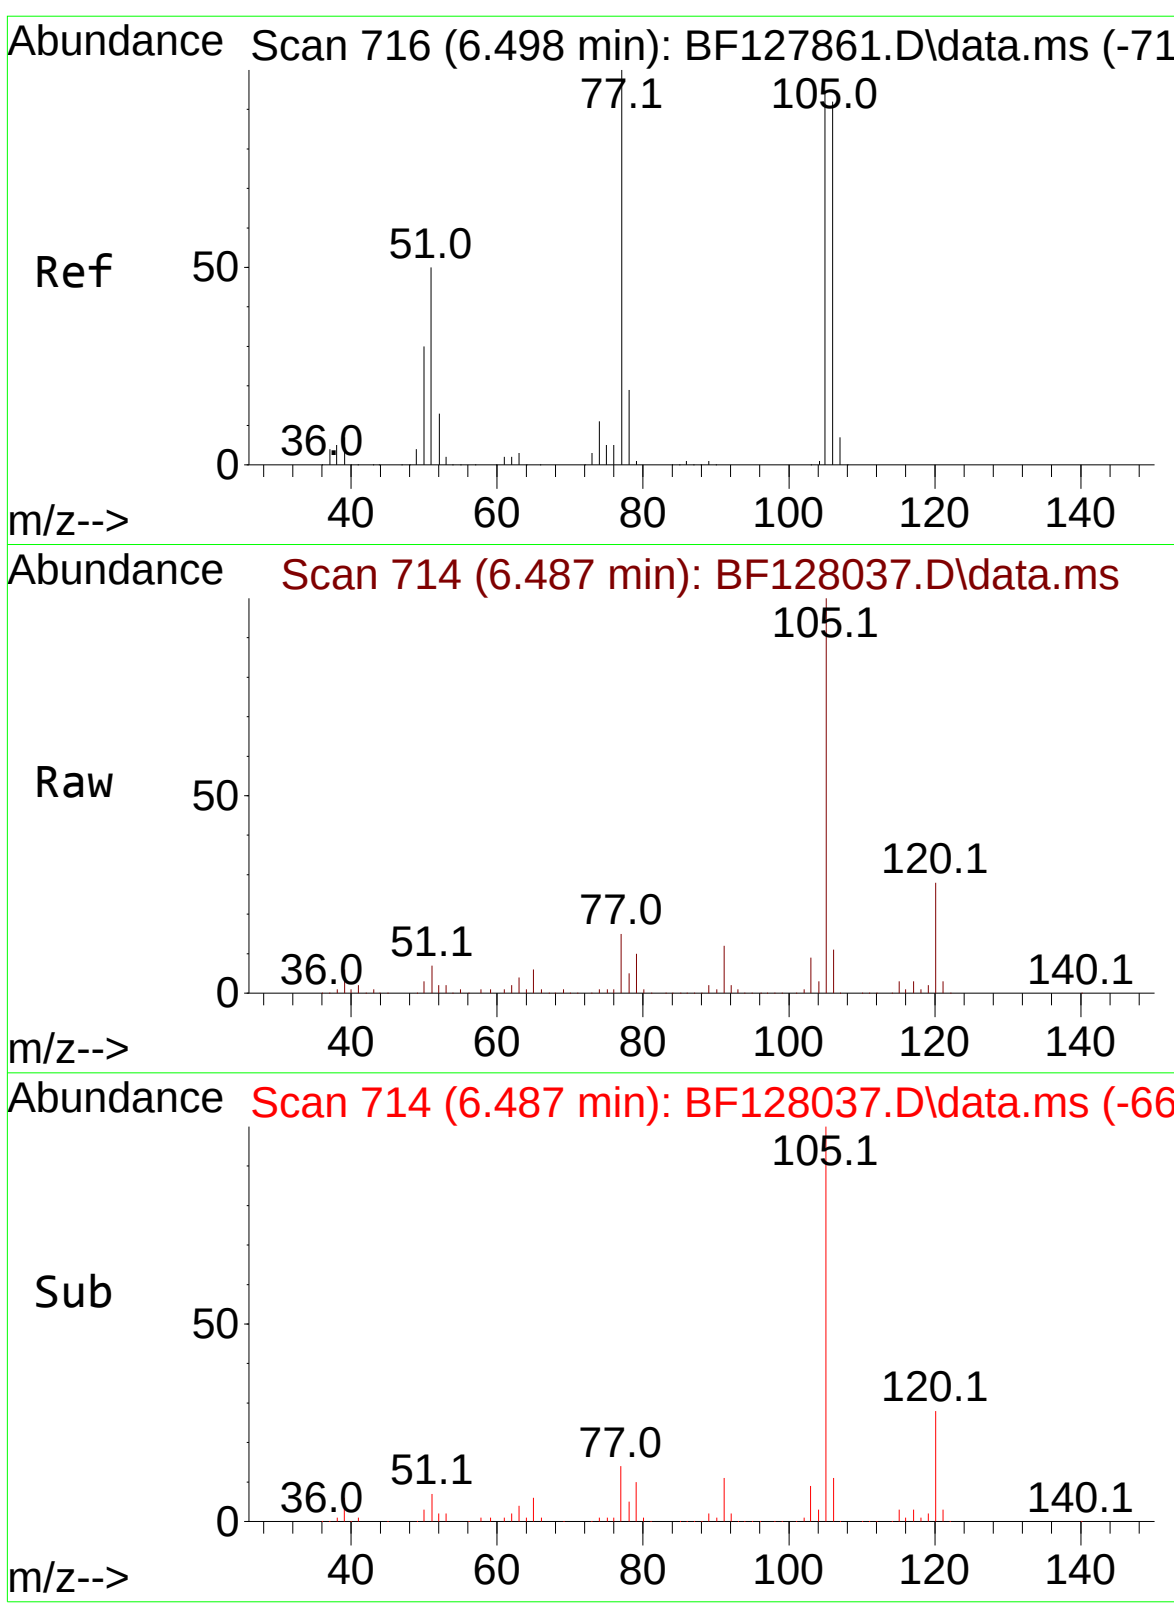

#9
Benzaldehyde
Concen: 5.414 ng
RT: 6.487 min Scan# 714
Delta R.T. 0.000 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion: 77 Resp: 25371

Ion	Ratio	Lower	Upper
77	100		
105	686.0	74.9	114.9#
106	75.4	72.2	112.2



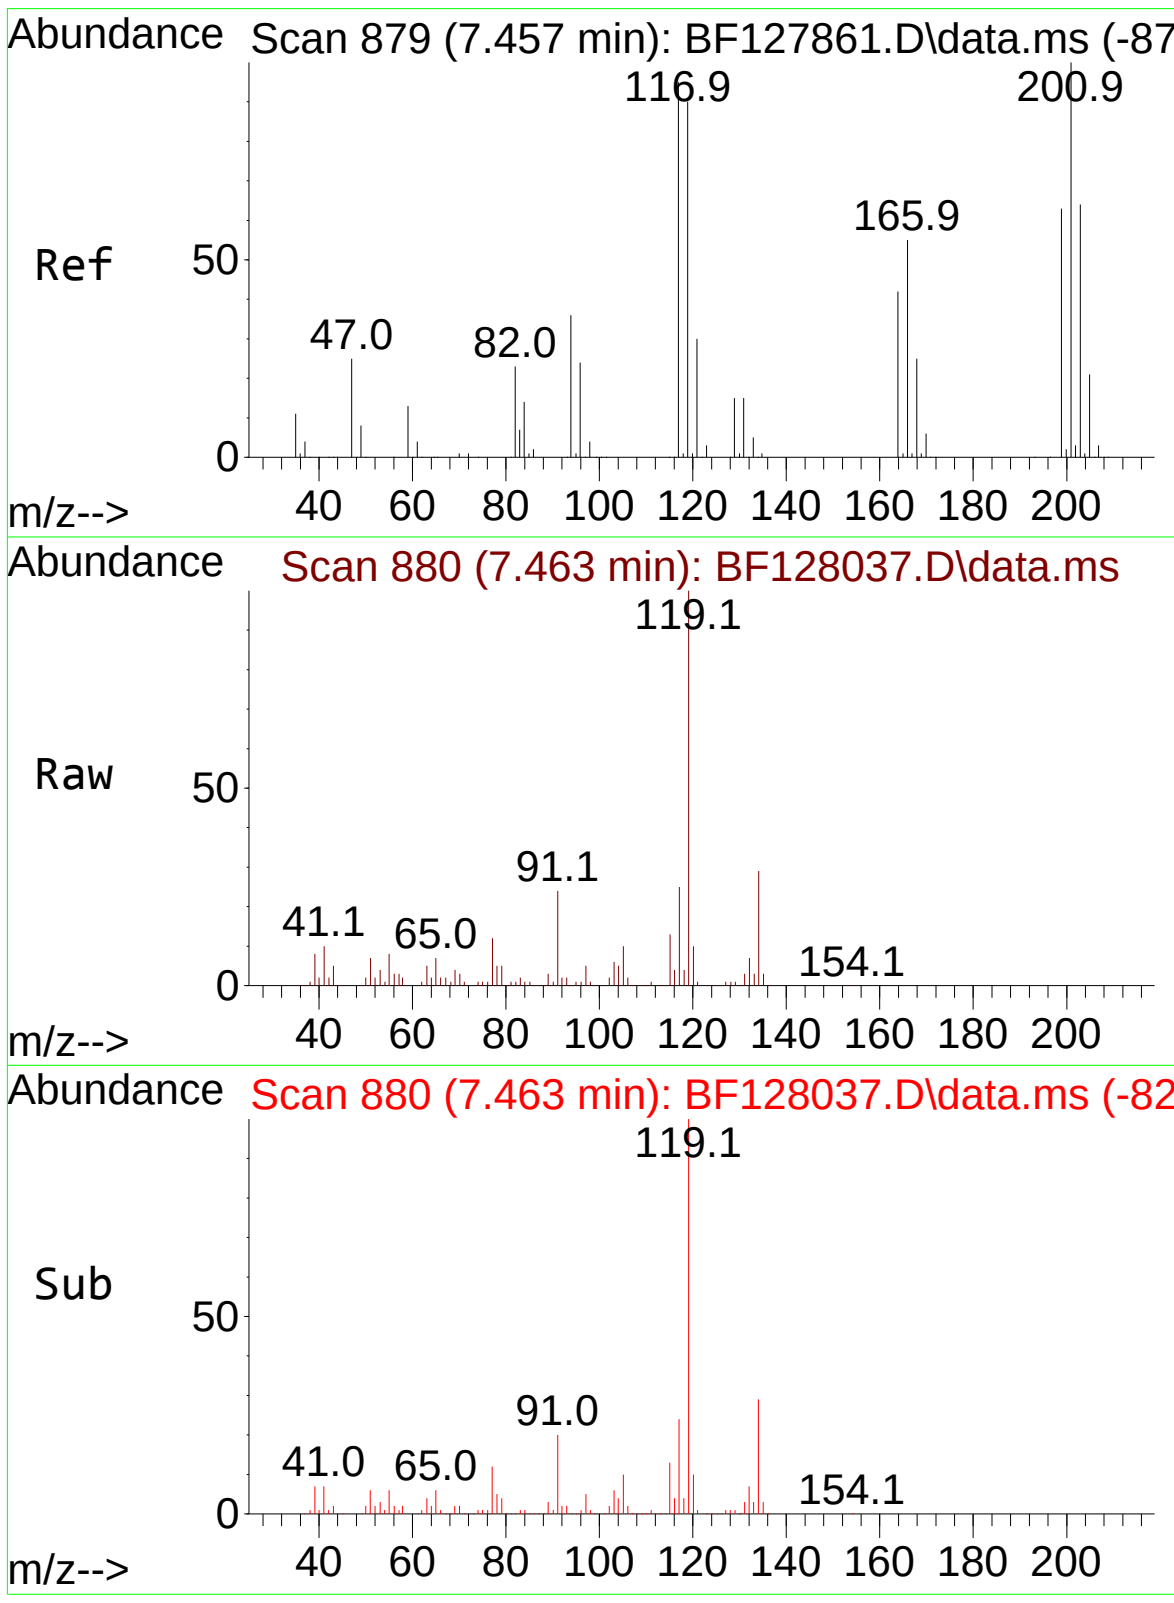

#18
Hexachloroethane
Concen: 15.138 ng
RT: 7.463 min   Scan# 8

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Delta R.T.   0.018 min
Lab File: BF128037.D
Acq: 02 May 2022   20:34

Tgt Ion:117 Resp: 38746

Ion	Ratio	Lower	Upper
117	100		
119	394.7	76.2	114.4#
201	0.0	84.4	126.6#

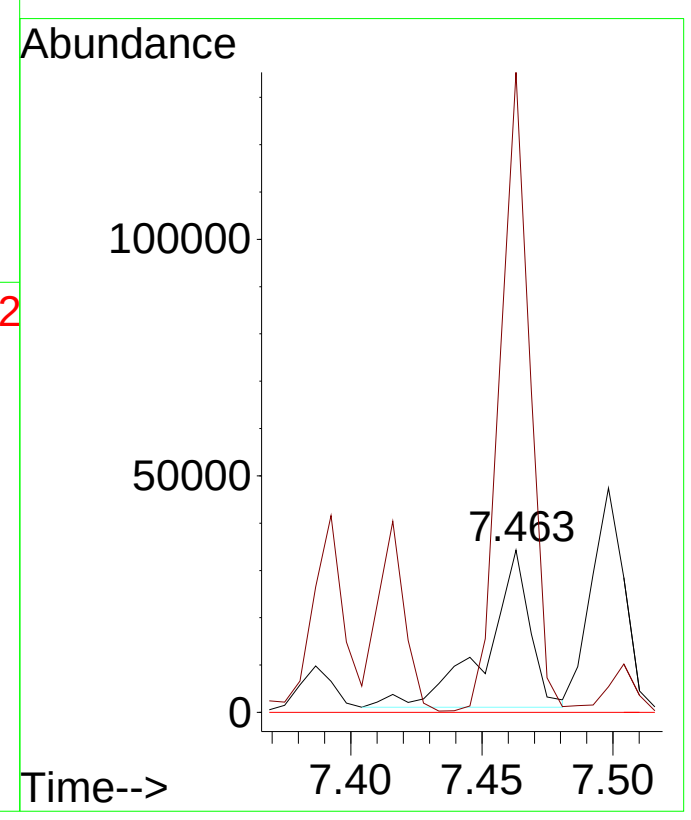

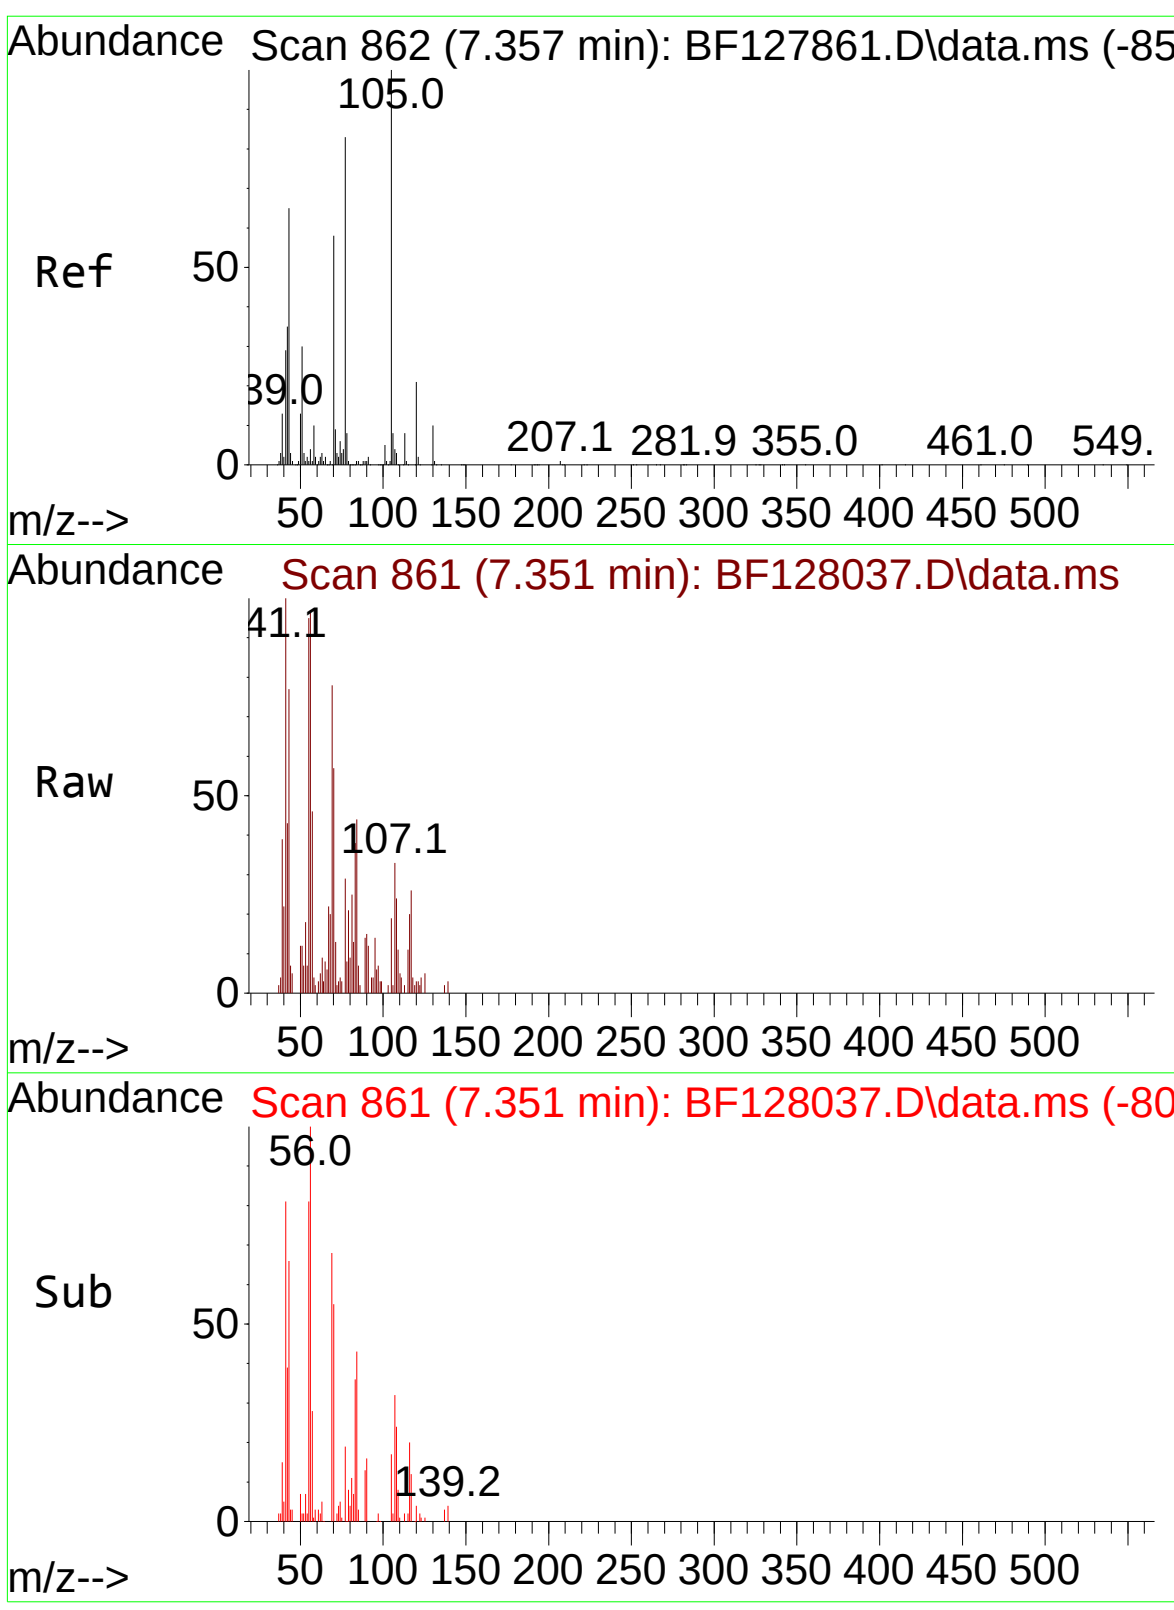

#19
n-Nitroso-di-n-propylamine
Concen: 3.820 ng
RT: 7.351 min   Scan# 861
Delta R.T.   0.006 min
Lab File: BF128037.D
Acq: 02 May 2022   20:34

Tgt Ion: 70 Resp: 17716

Ion	Ratio	Lower	Upper
70	100		
42	74.5	48.7	73.1#
101	0.0	7.2	10.8#
130	0.0	14.4	21.6#

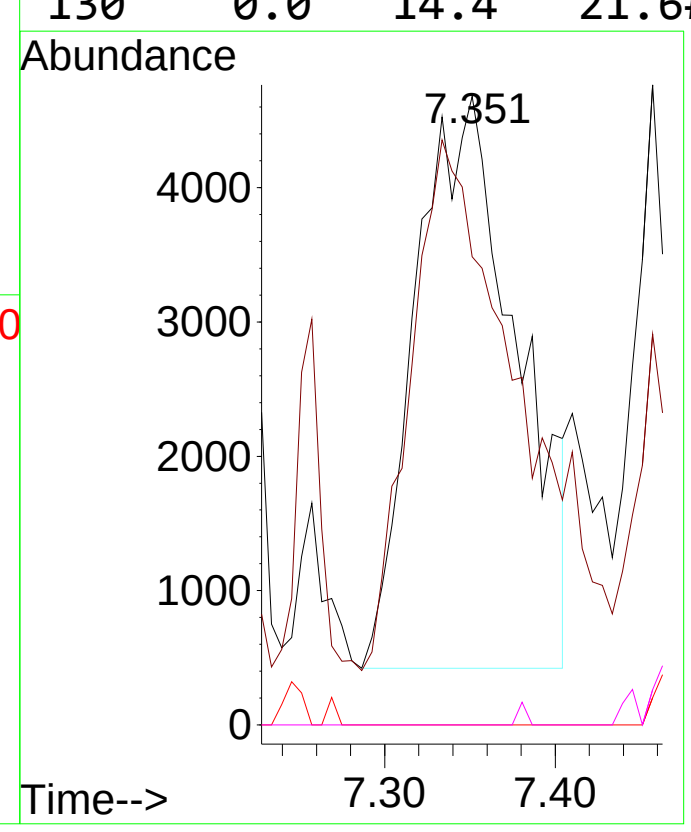

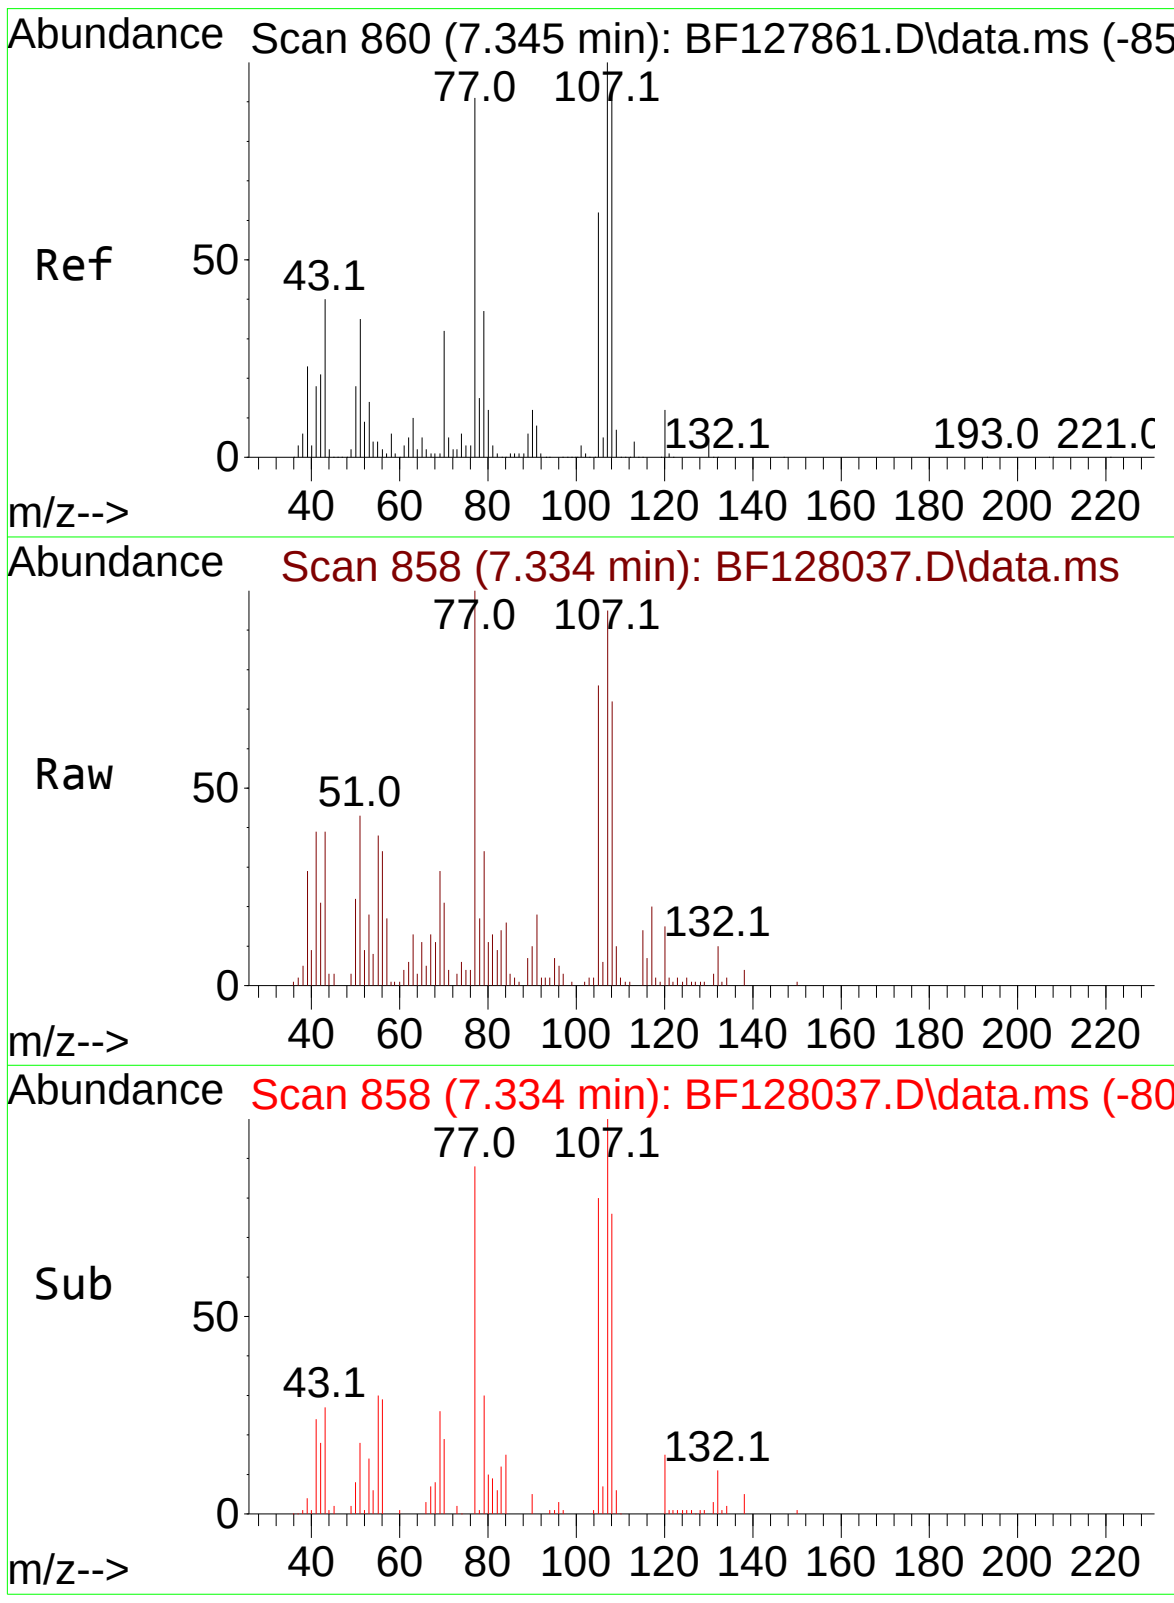

#20
3+4-Methylphenols
Concen: 3.831 ng
RT: 7.334 min Scan# 8

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Delta R.T. 0.000 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:107 Resp: 24195

Ion	Ratio	Lower	Upper
107	100		
108	76.4	73.4	113.4
77	105.5	71.1	111.1
79	35.5	17.1	57.1

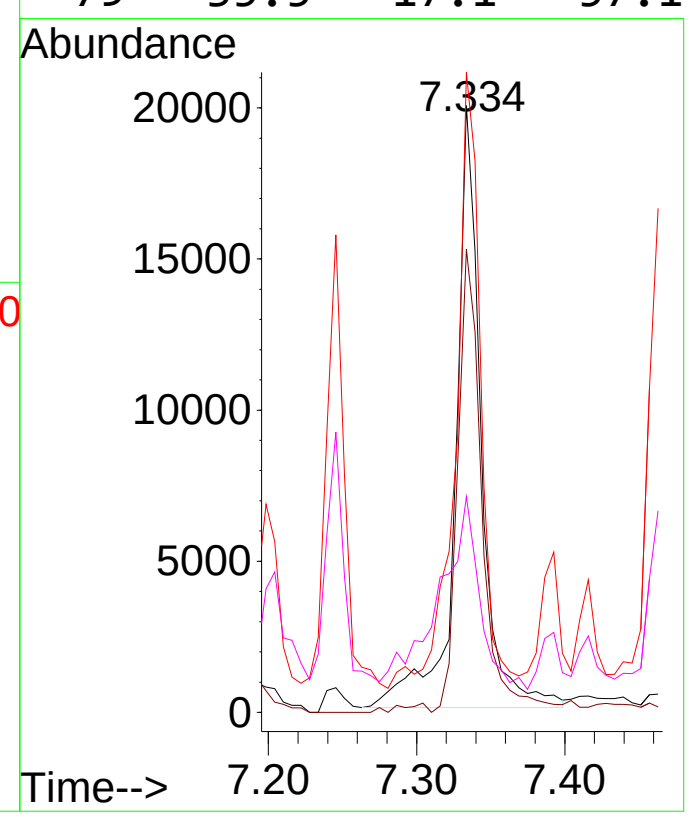

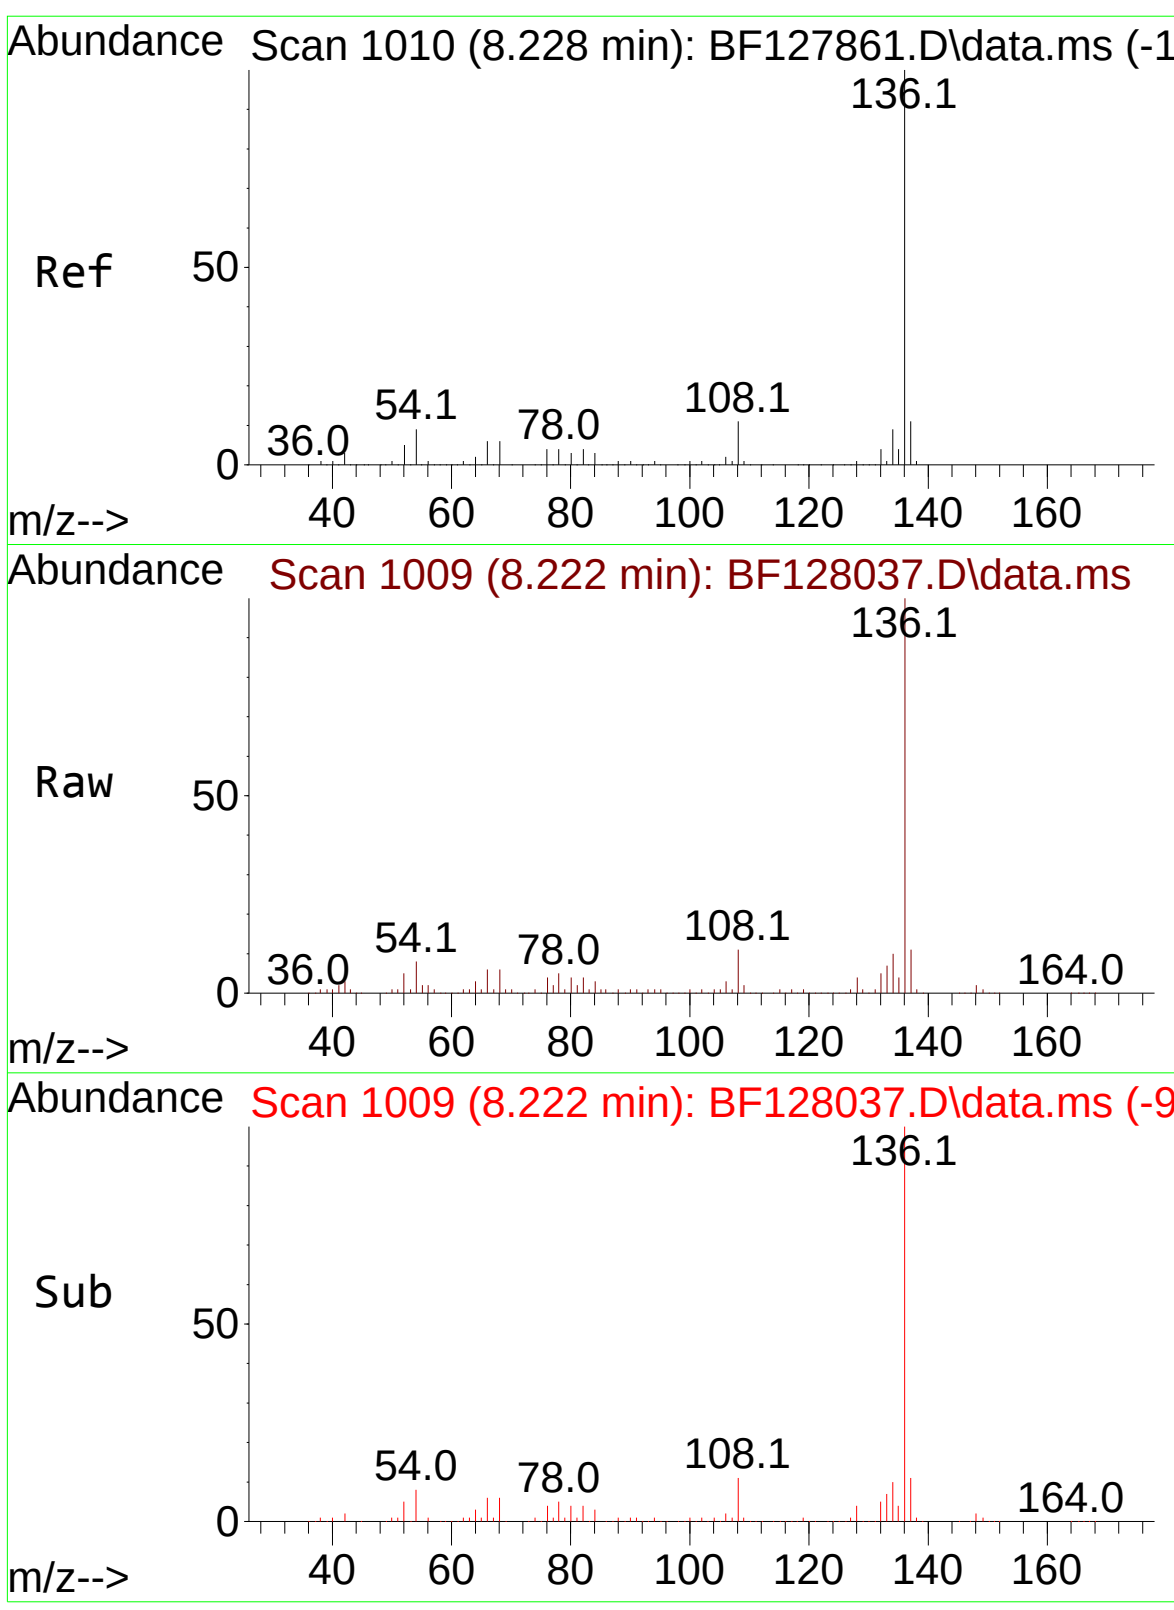

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.222 min Scan# 1009
Delta R.T. 0.006 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:136 Resp: 320405

Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.6	13.0
54	8.4	6.8	10.2
68	6.2	5.1	7.7

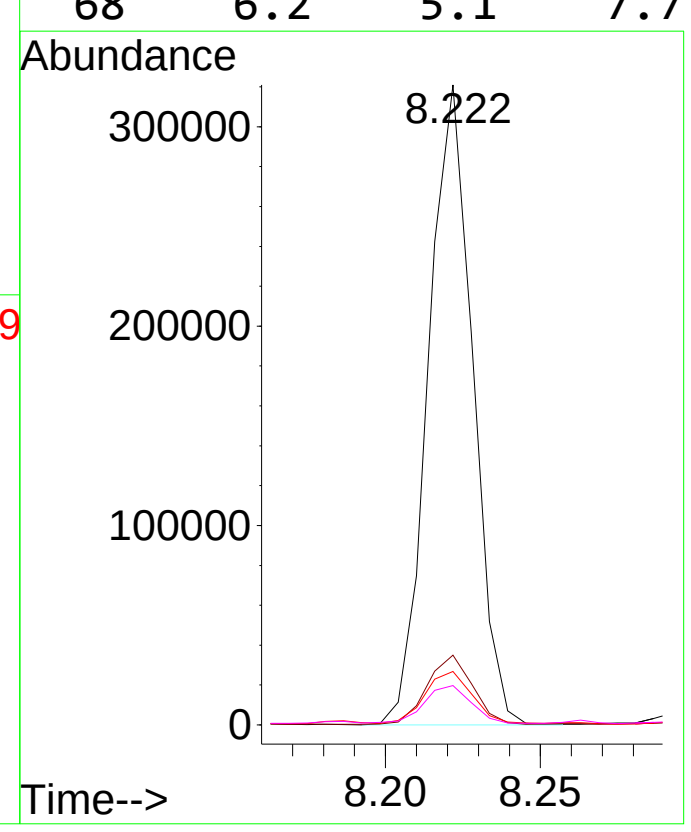

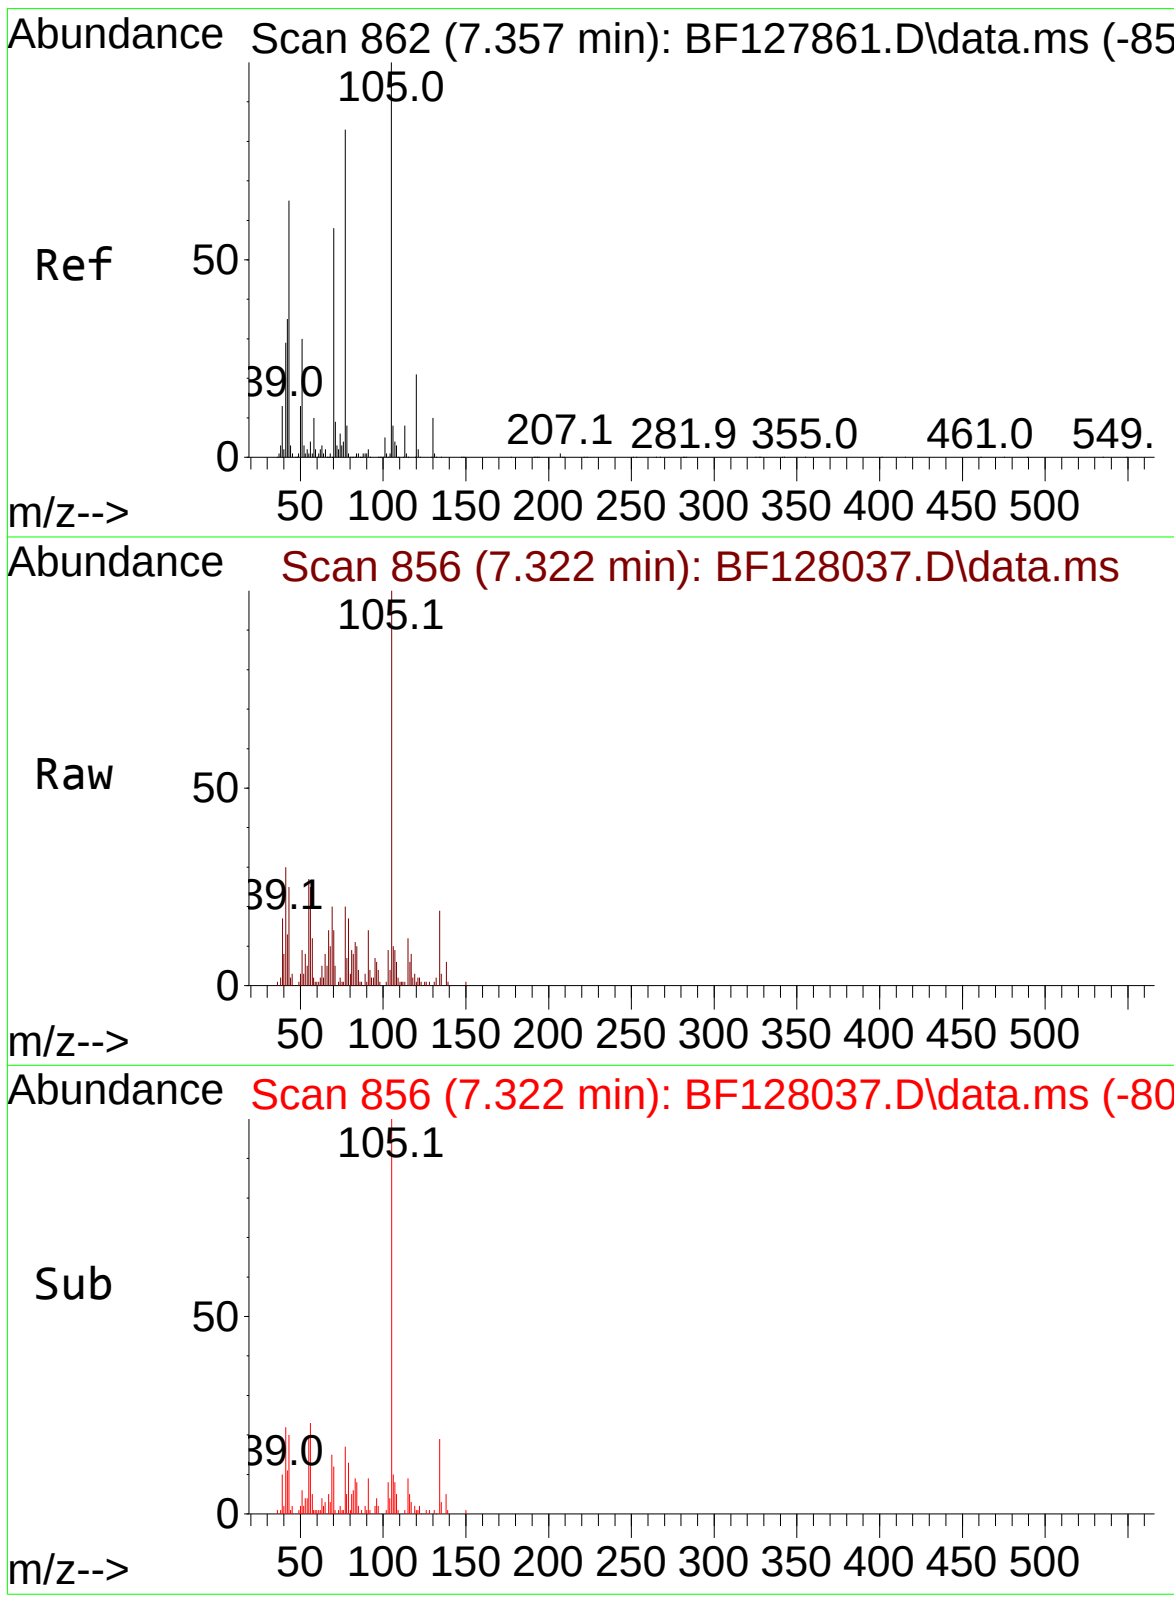

#22
Acetophenone
Concen: 4.646 ng
RT: 7.322 min Scan# 8
Delta R.T. -0.023 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Tgt Ion:105 Resp: 36283

Ion	Ratio	Lower	Upper
105	100		
71	4.9	7.3	10.9#
51	9.1	23.7	35.5#
120	1.1	17.0	25.6#

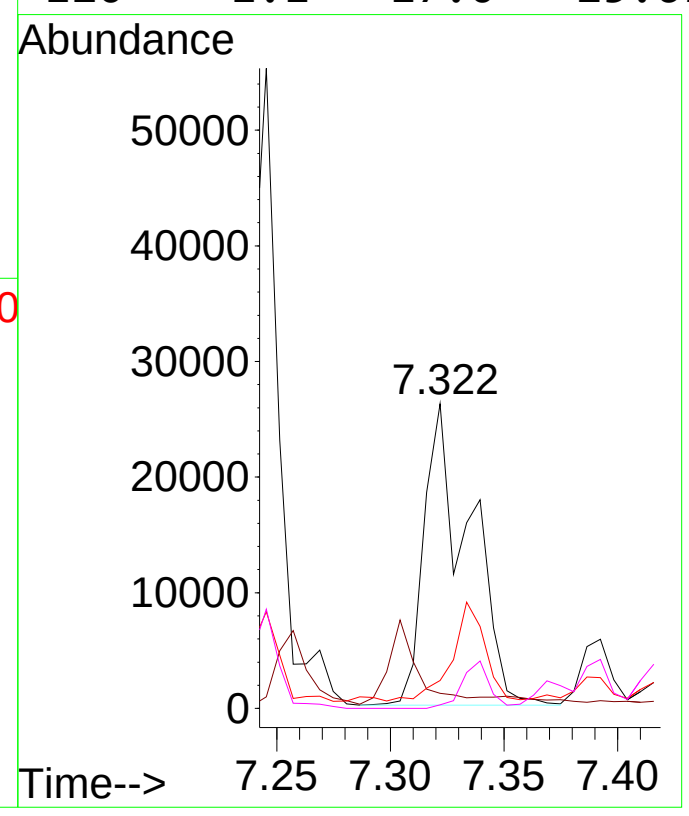

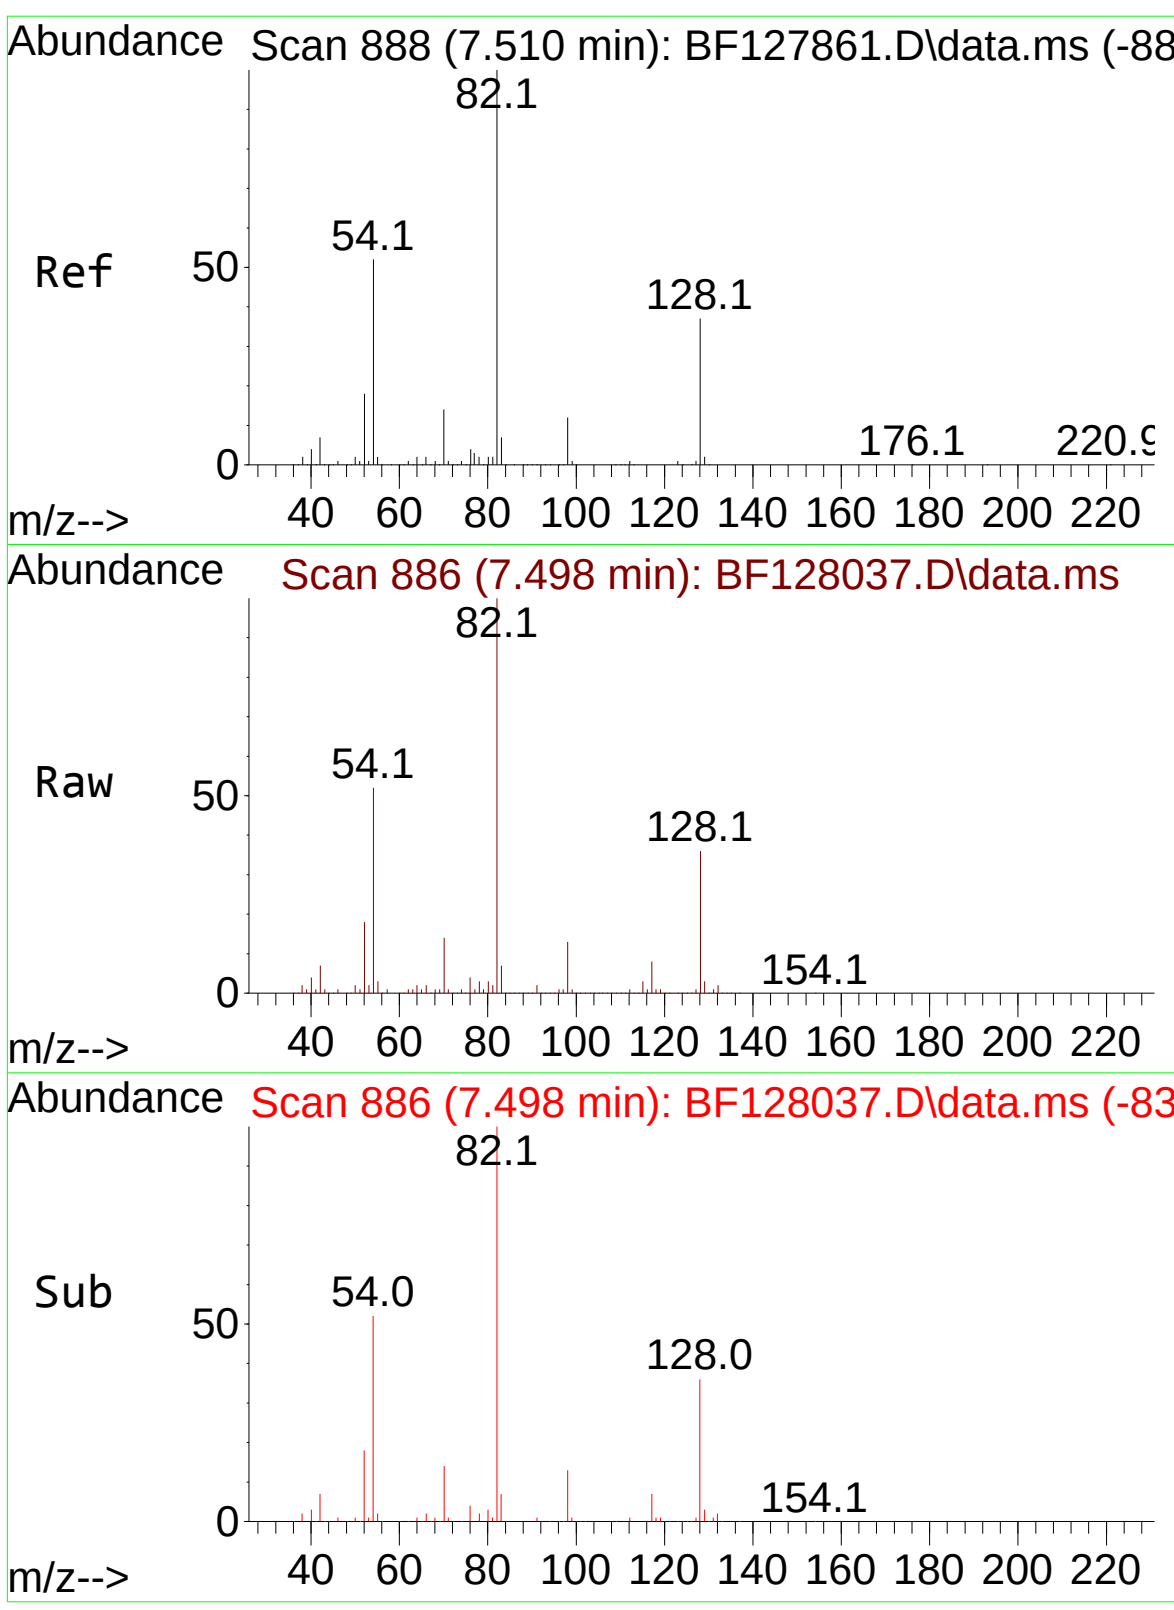

#23
Nitrobenzene-d5
Concen: 74.274 ng
RT: 7.498 min Scan# 886
Delta R.T. -0.006 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion: 82 Resp: 506077

Ion	Ratio	Lower	Upper
82	100		
128	36.5	30.0	45.0
54	52.2	41.3	61.9



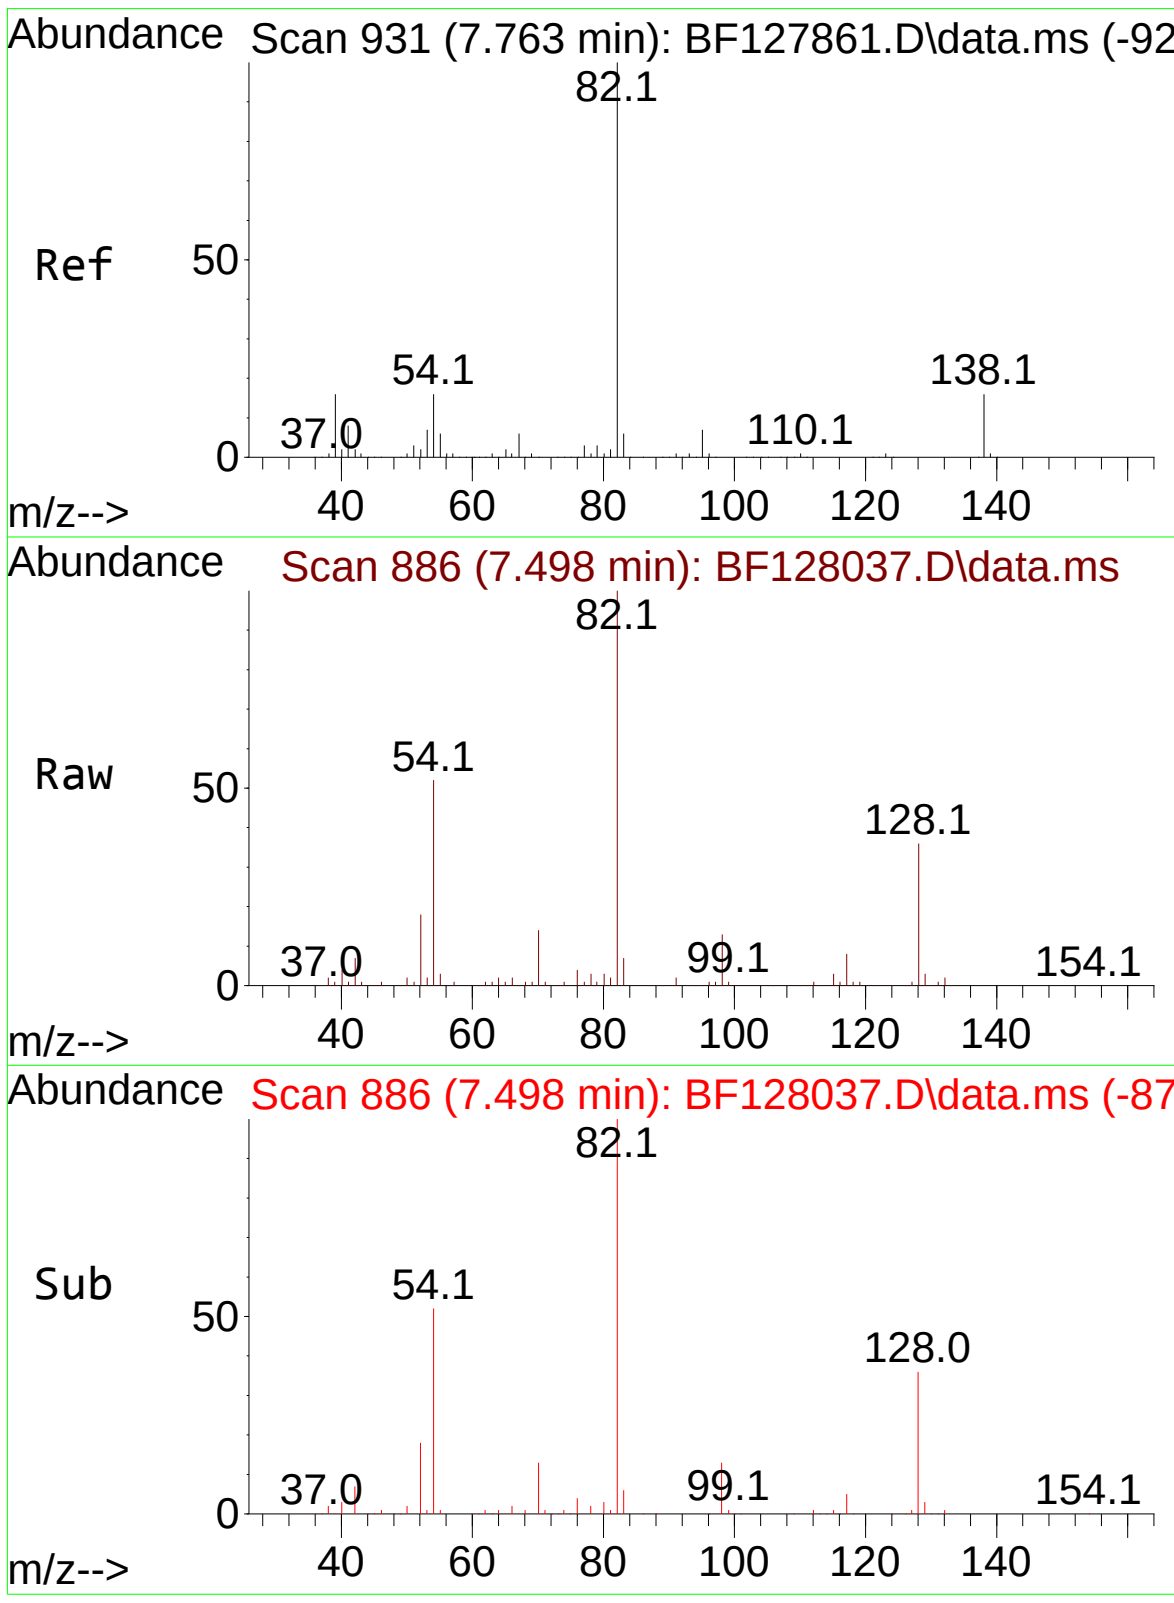

#25
Isophorone
Concen: 44.076 ng
RT: 7.498 min Scan# 8
Delta R.T. -0.259 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Tgt Ion: 82 Resp: 505453

Ion	Ratio	Lower	Upper
82	100		
95	0.2	5.6	8.4#
138	0.0	12.5	18.7#

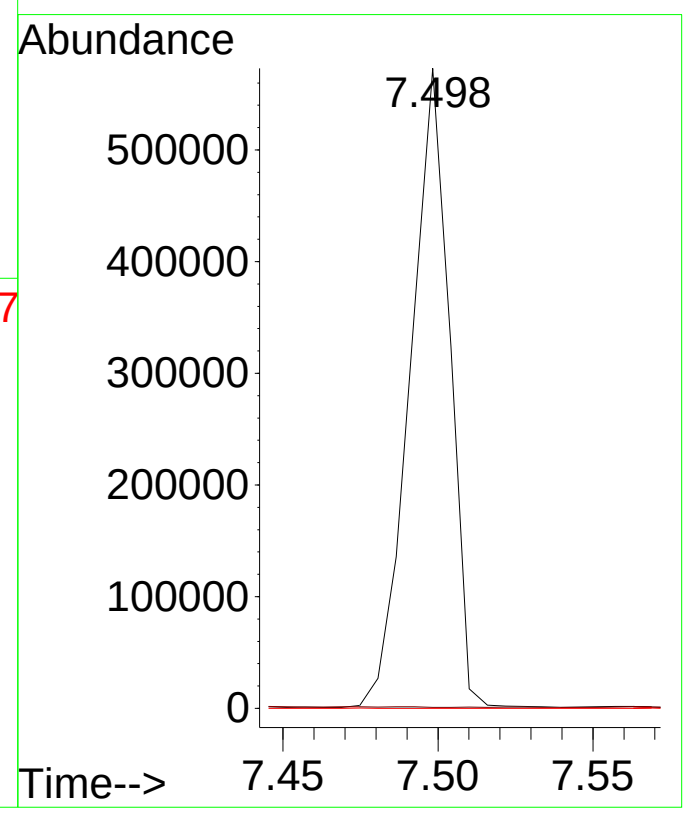

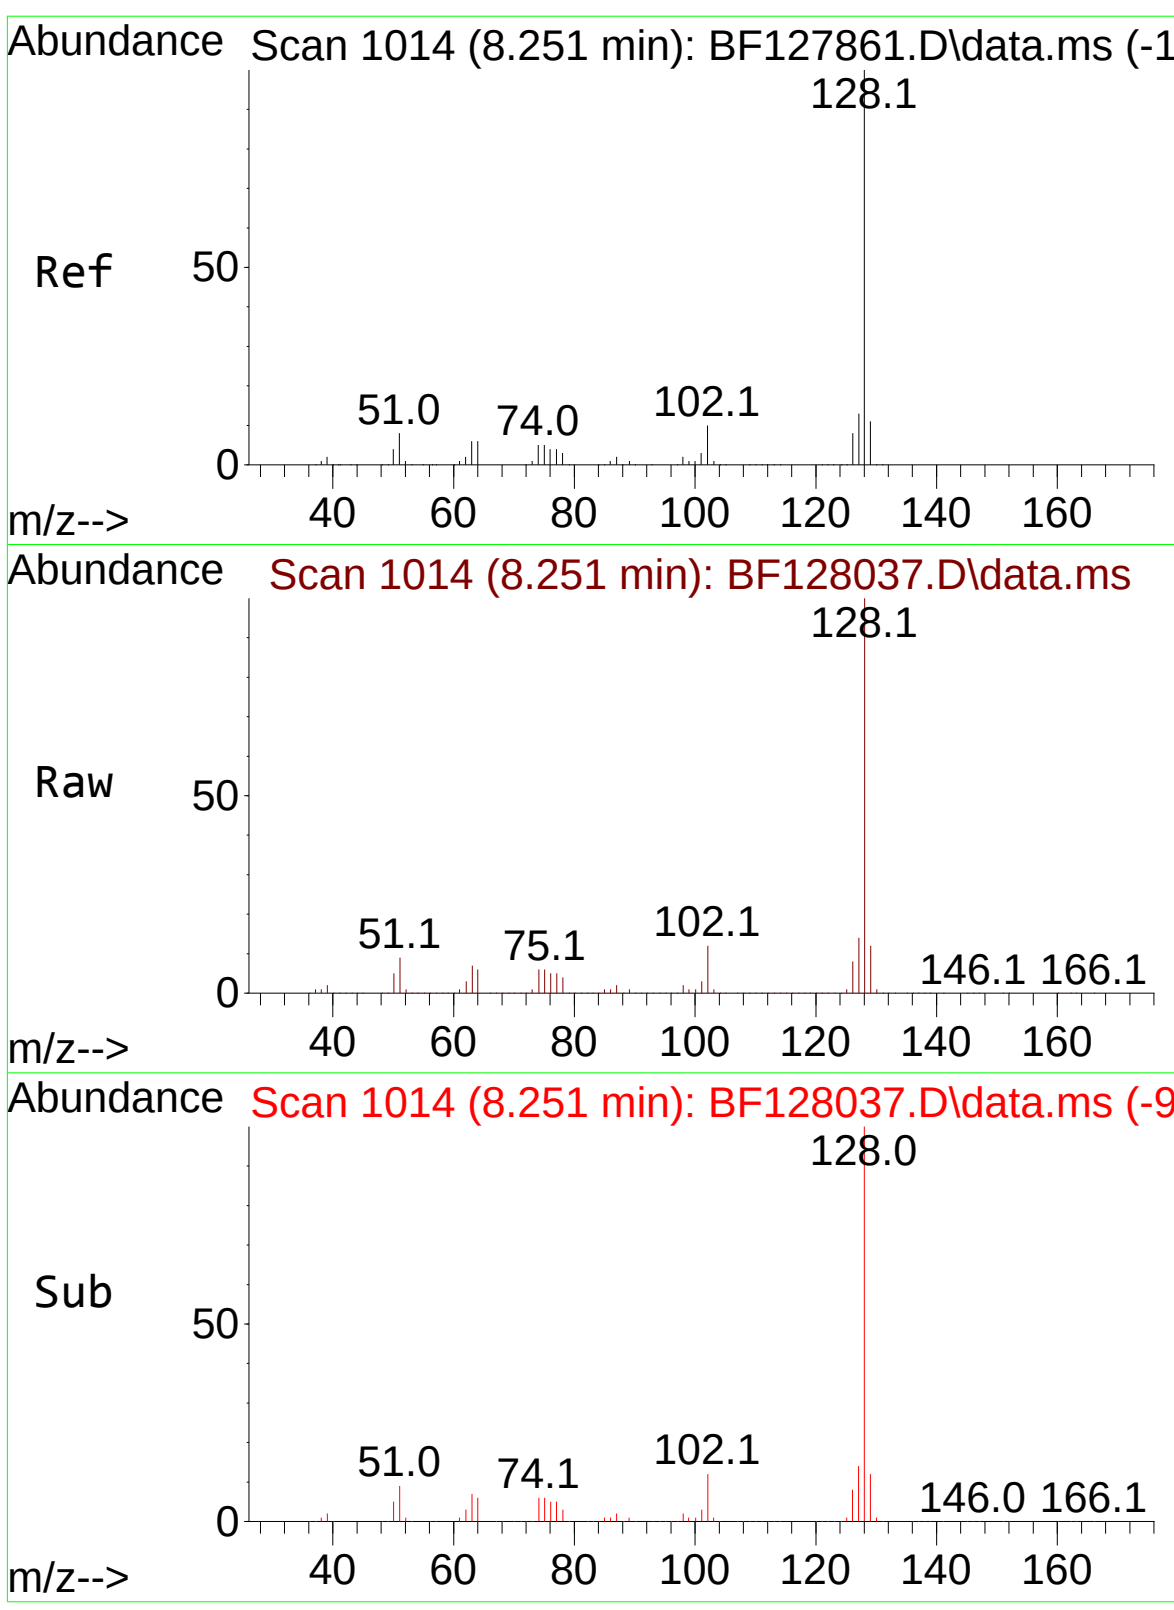

#31
Naphthalene
Concen: 171.599 ng
RT: 8.251 min Scan# 1014
Delta R.T. 0.012 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:128 Resp: 2800293

Ion	Ratio	Lower	Upper
128	100		
129	12.2	9.0	13.4
127	14.1	10.6	16.0

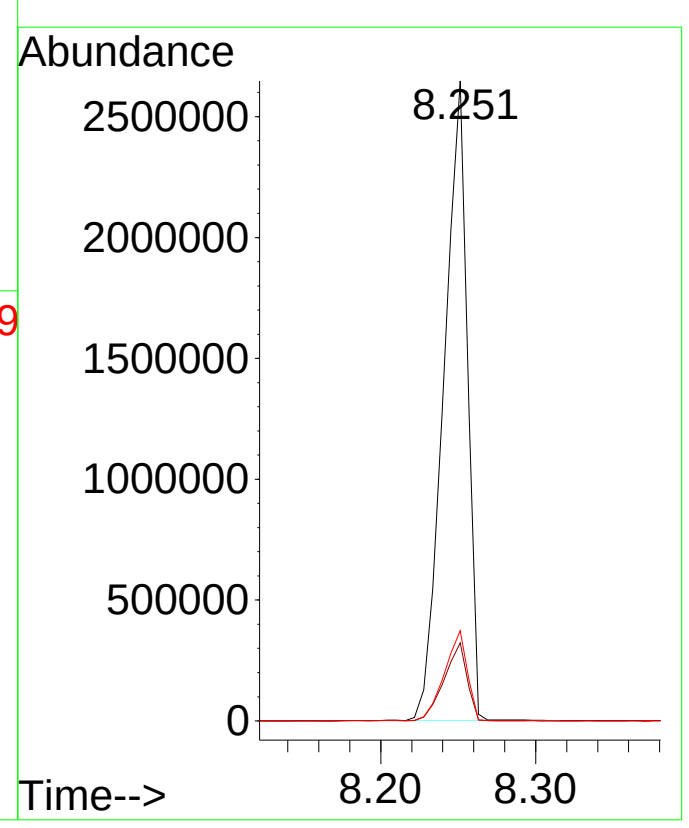

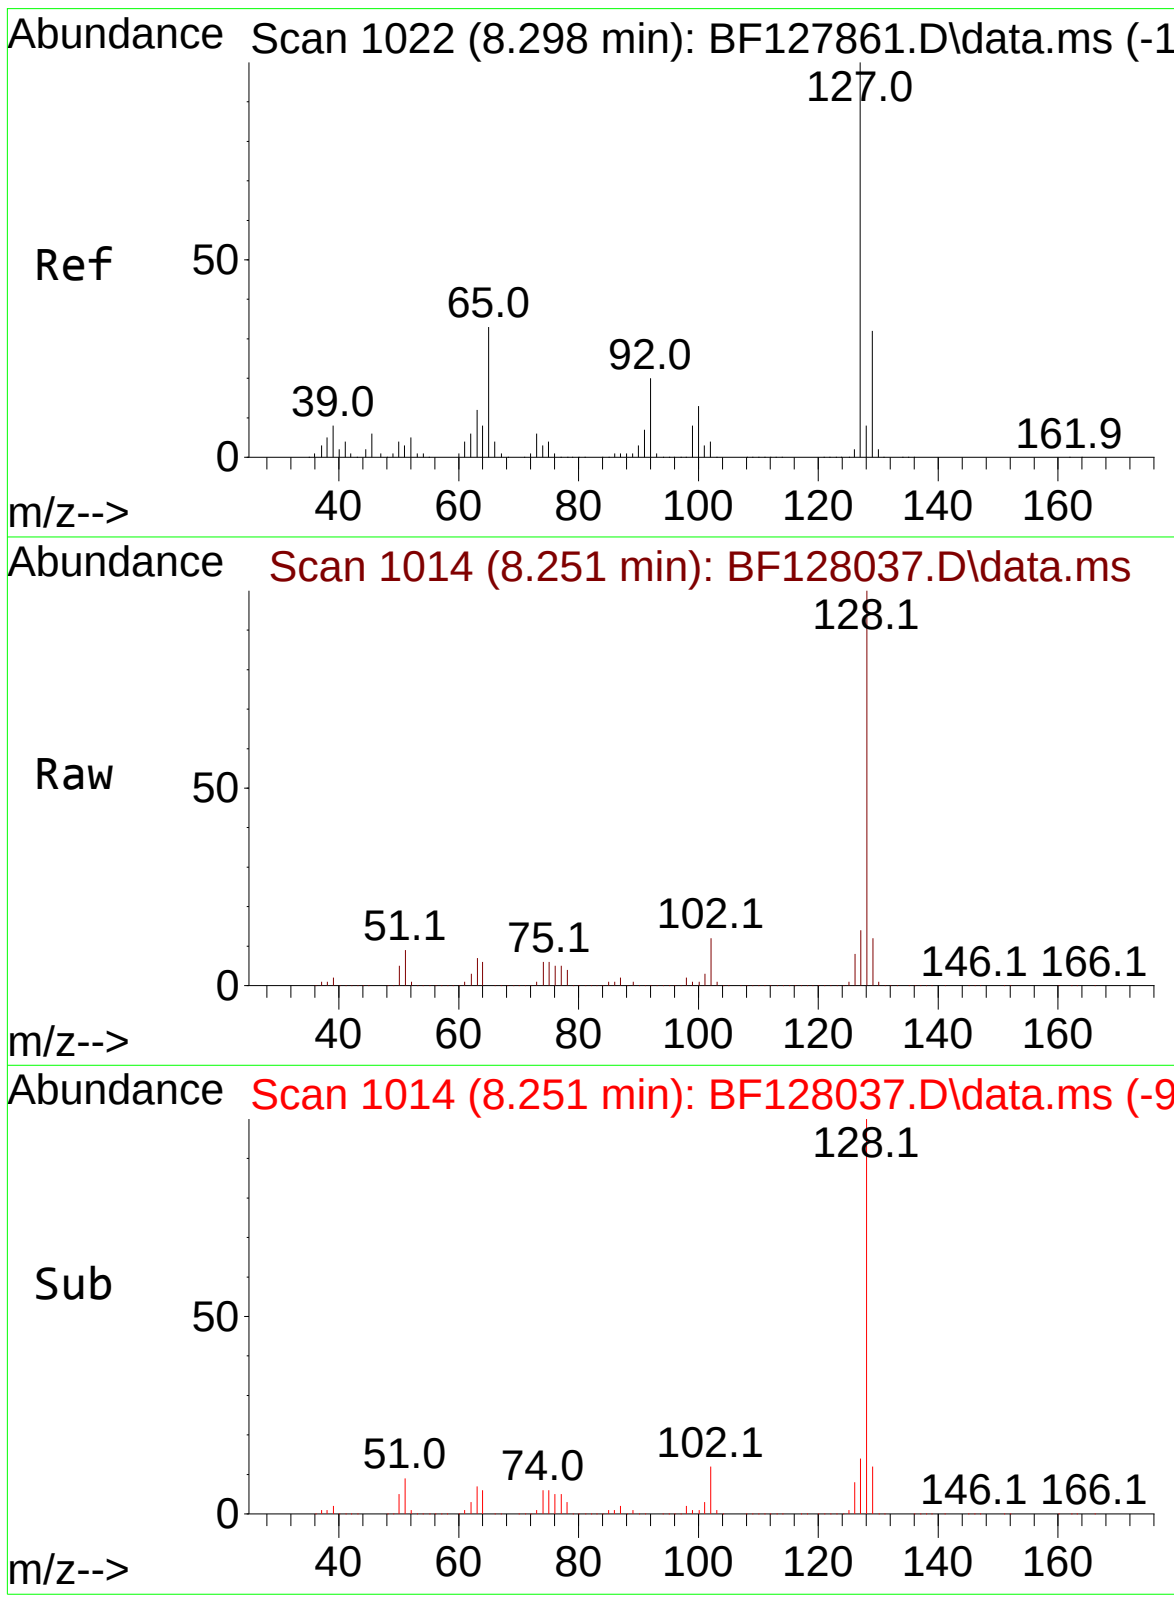

#33
4-Chloroaniline
Concen: 59.112 ng
RT: 8.251 min Scan# 1

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Delta R.T. -0.035 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:127 Resp: 381674

Ion	Ratio	Lower	Upper
127	100		
129	86.5	25.8	38.8#
65	0.0	26.7	40.1#
92	0.2	16.0	24.0#

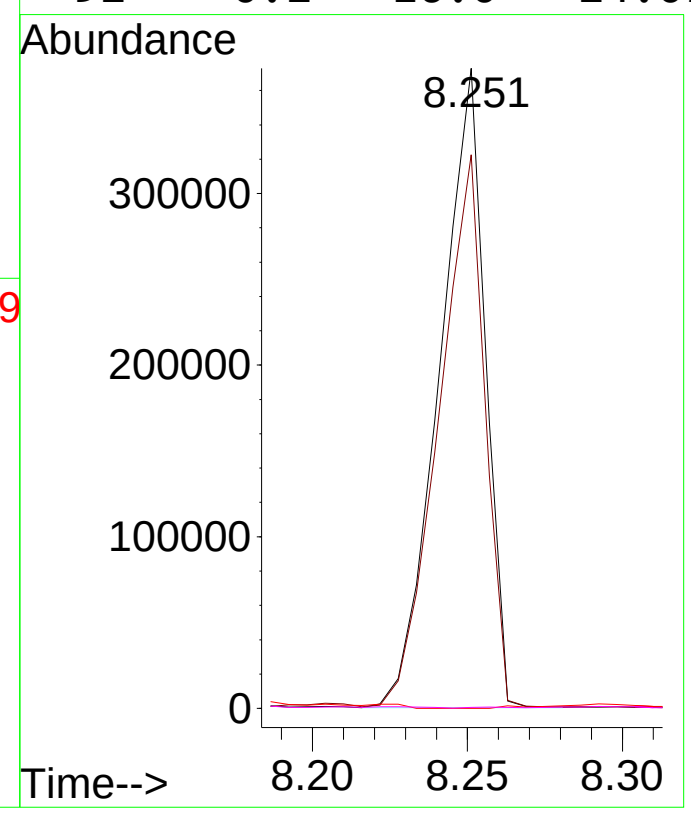

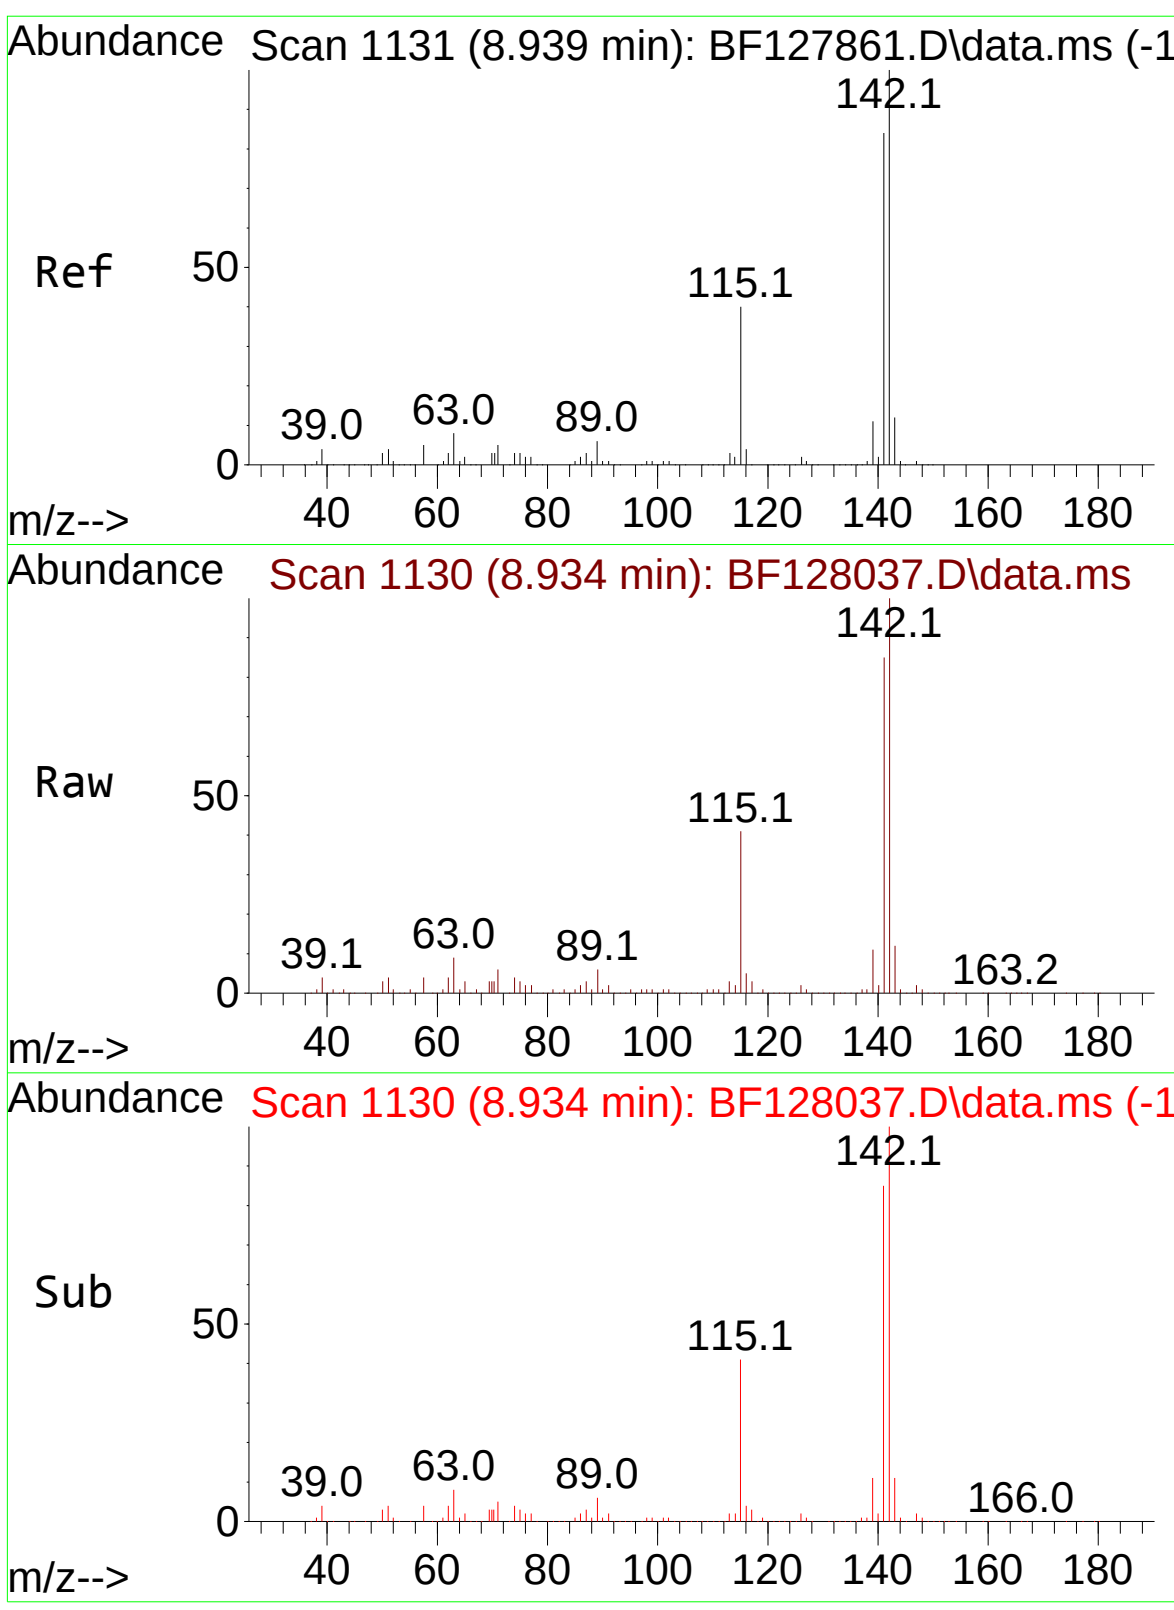

#37
2-Methylnaphthalene
Concen: 39.229 ng
RT: 8.934 min Scan# 1130
Delta R.T. 0.000 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:142 Resp: 423081

Ion	Ratio	Lower	Upper
142	100		
141	85.2	67.4	101.2

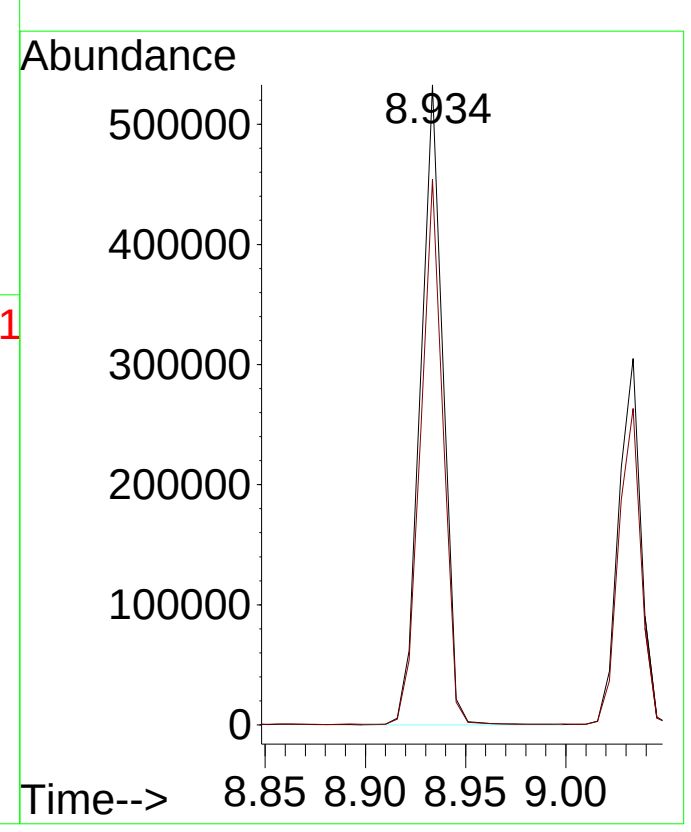

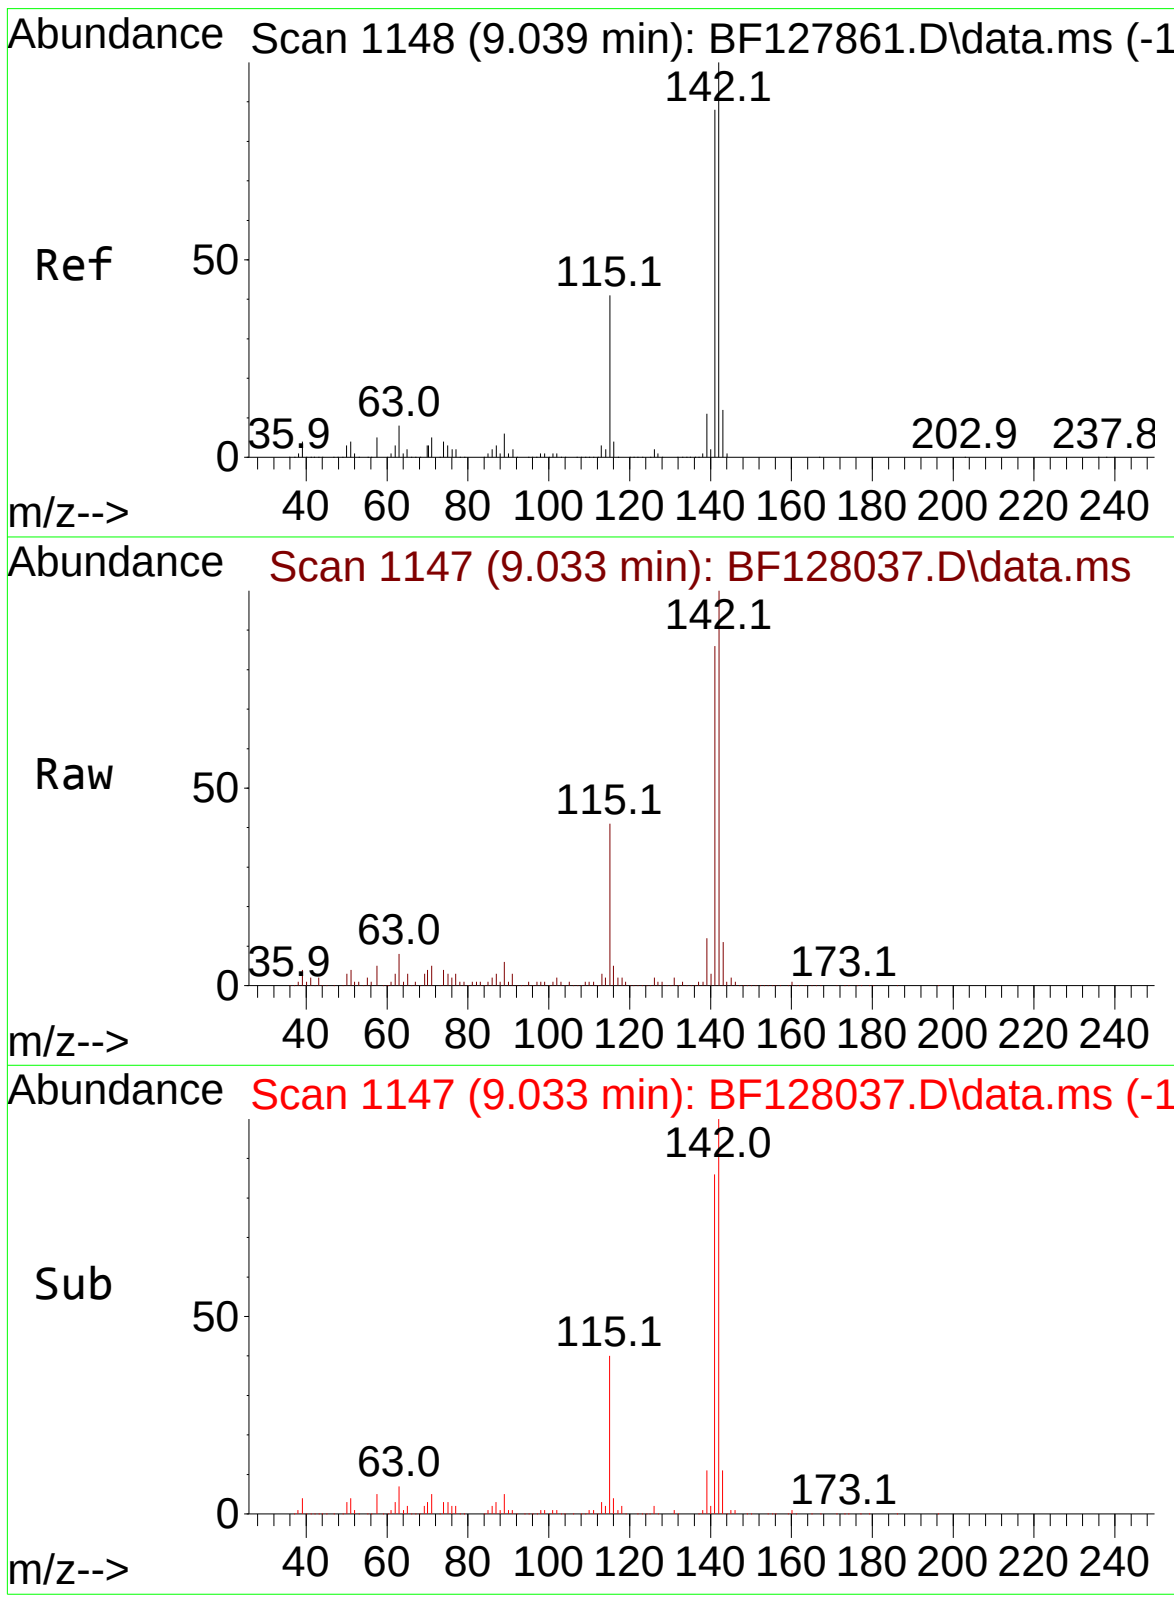

#38
1-Methylnaphthalene
Concen: 22.445 ng
RT: 9.033 min Scan# 1

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Delta R.T. 0.000 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:142 Resp: 235291

Ion	Ratio	Lower	Upper
142	100		
141	86.4	70.1	105.1

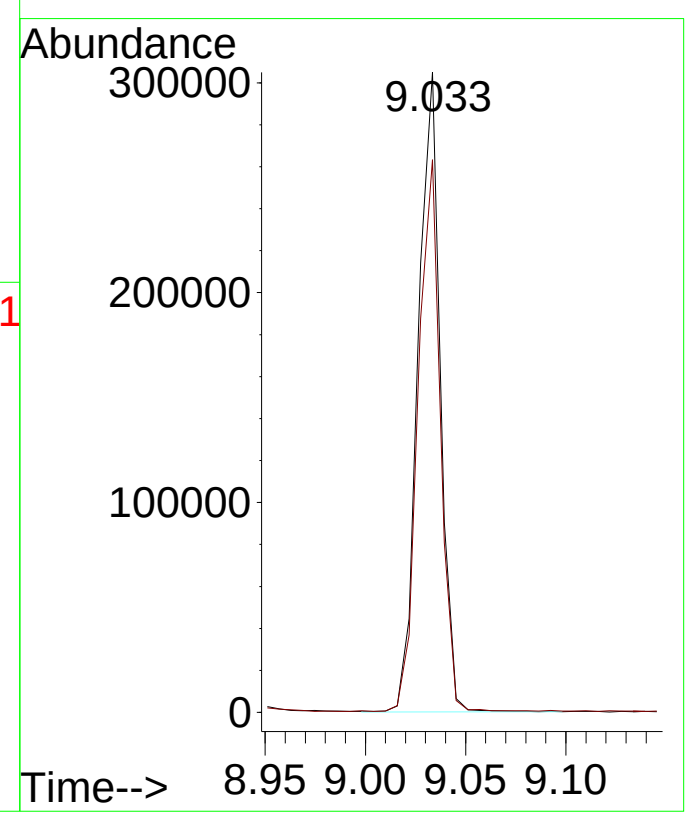

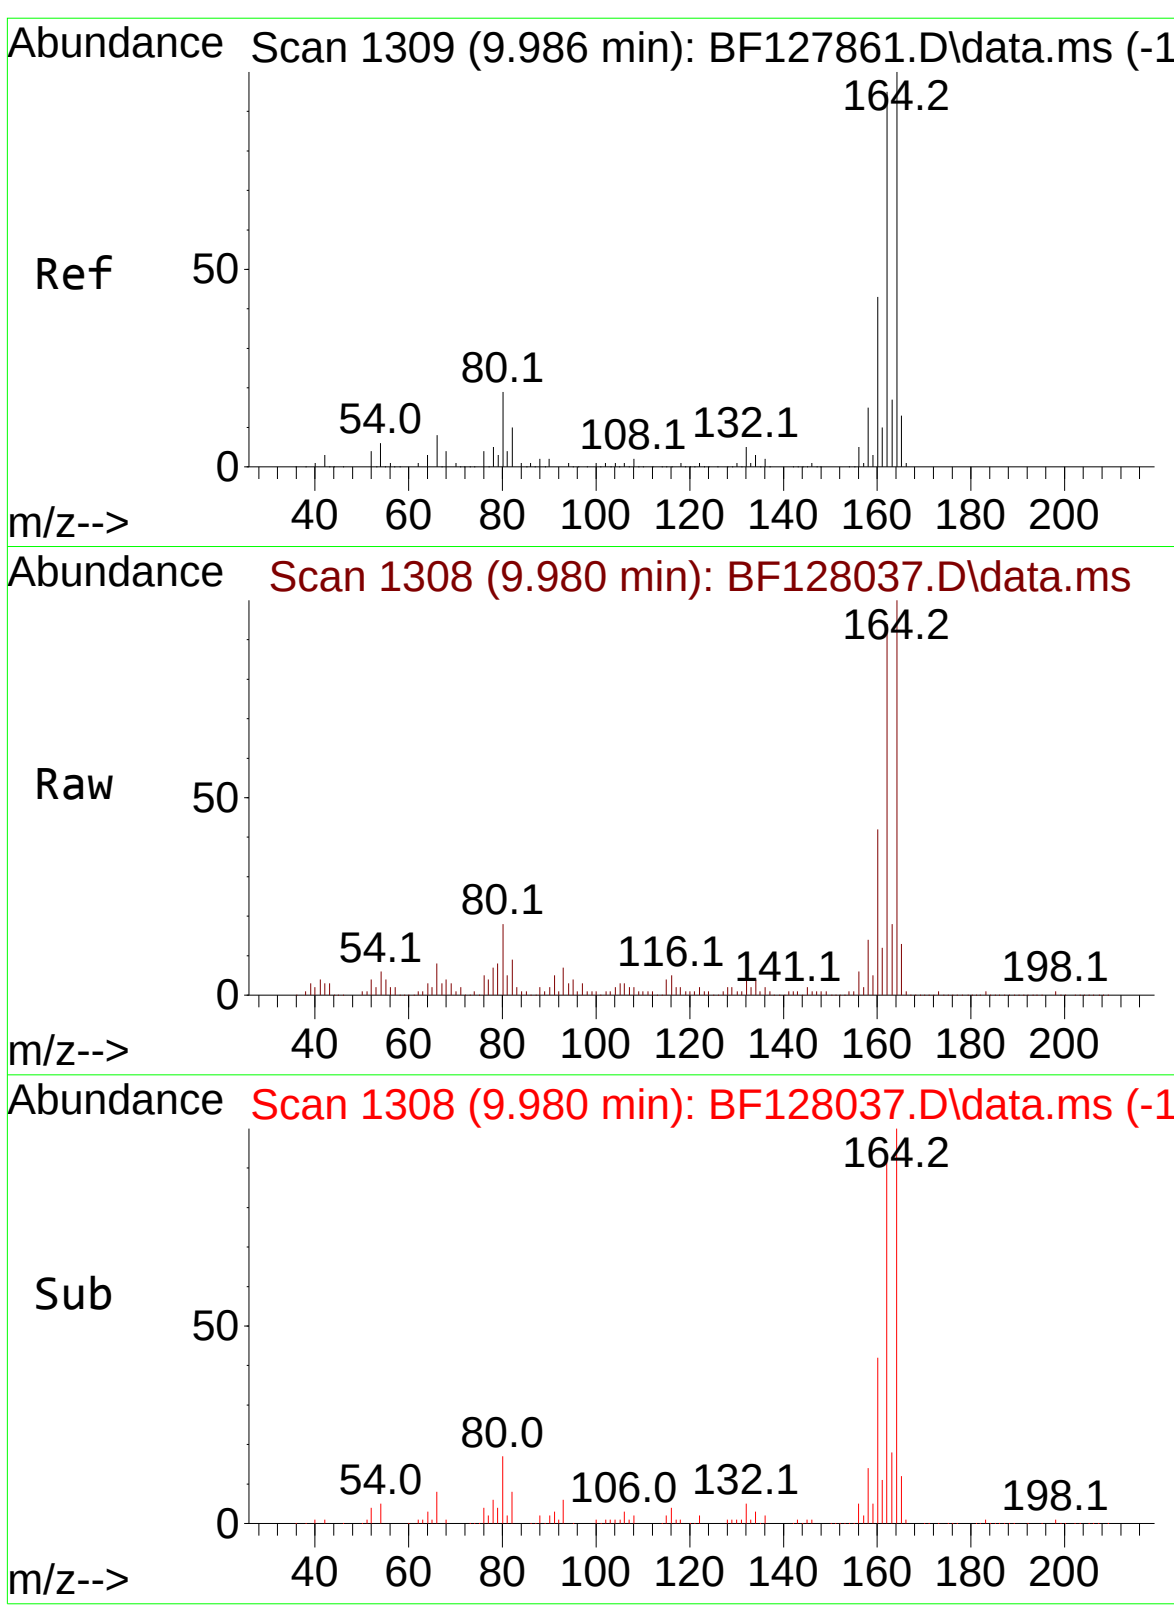

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.980 min Scan# 1308
Delta R.T. 0.006 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:164 Resp: 151057

Ion	Ratio	Lower	Upper
164	100		
162	94.0	76.0	114.0
160	42.2	34.8	52.2

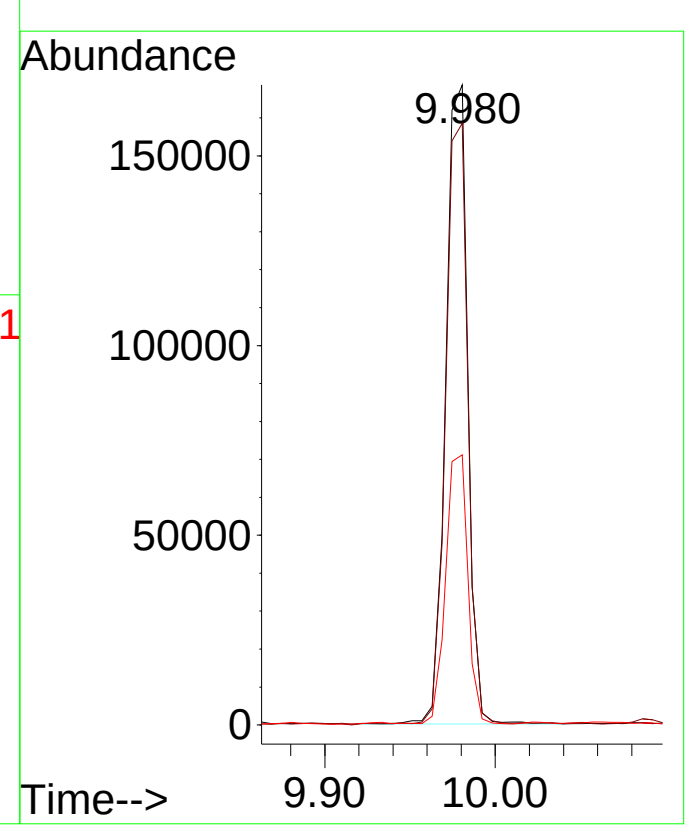

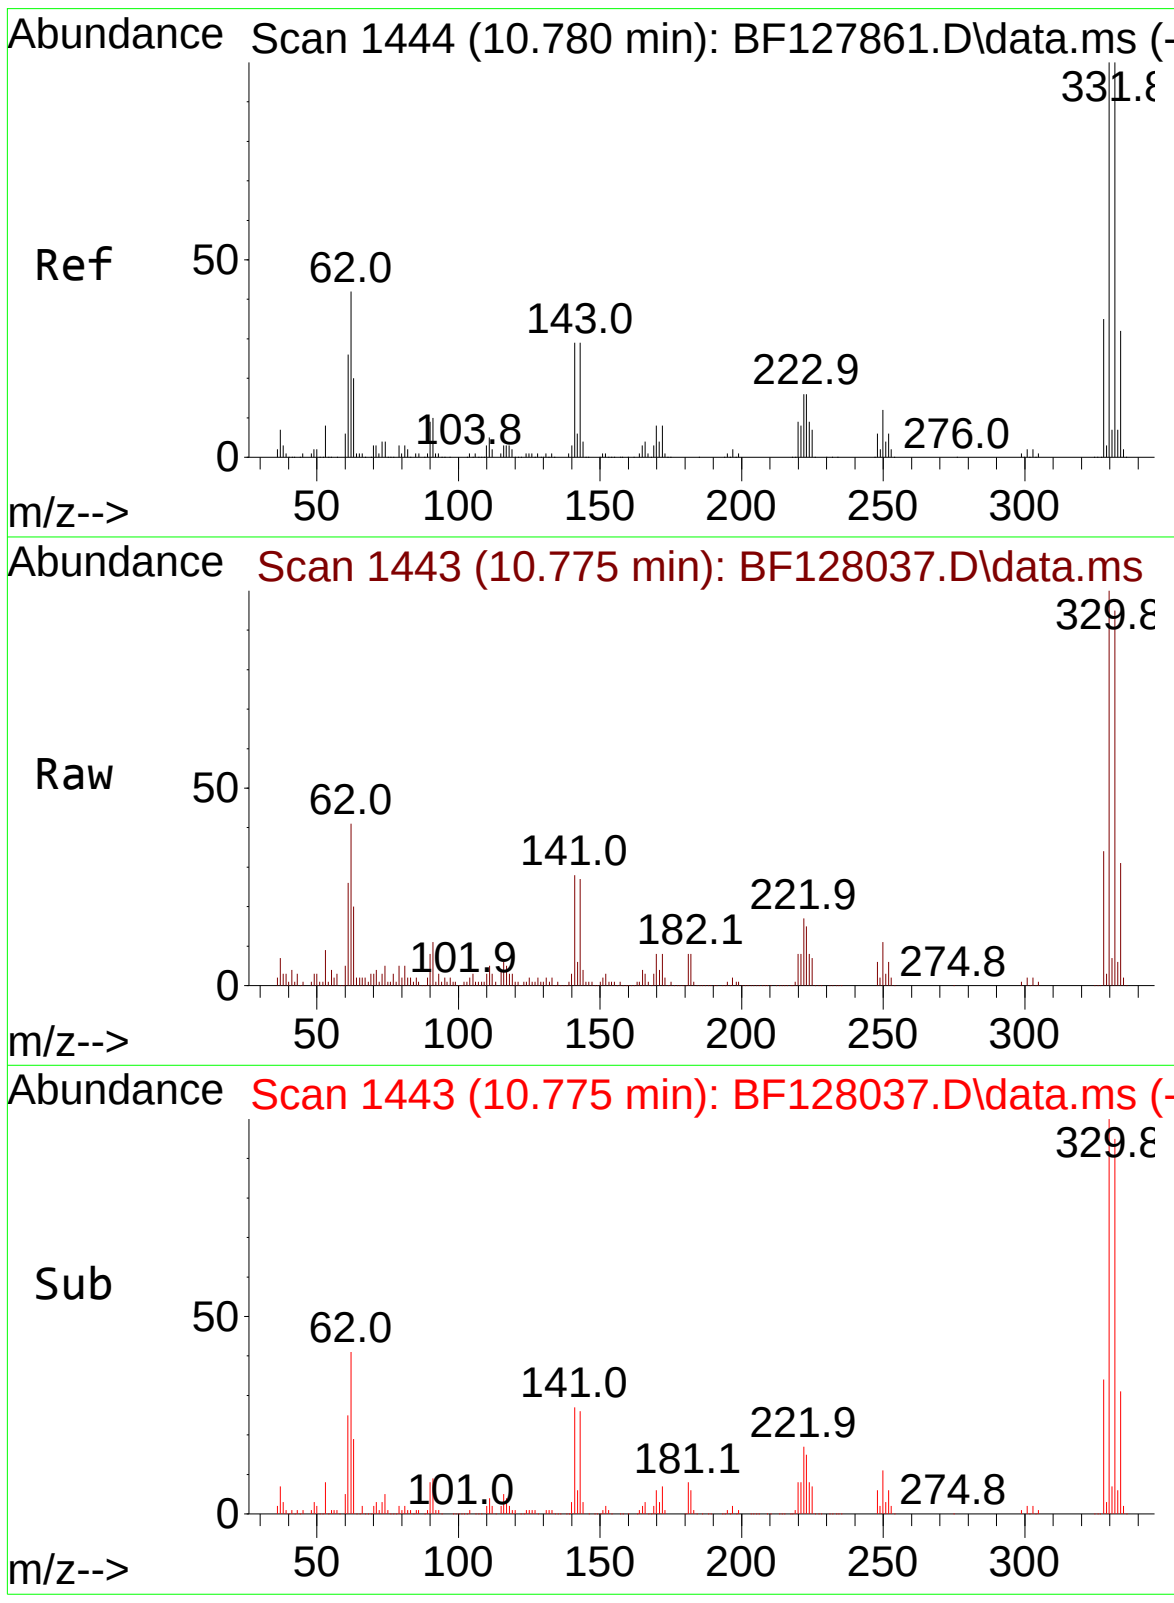

#42
2,4,6-Tribromophenol
Concen: 99.057 ng
RT: 10.775 min Scan# 14
Delta R.T. 0.006 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Tgt Ion:330 Resp: 150630

Ion	Ratio	Lower	Upper
330	100		
332	96.9	79.0	118.4
141	34.1	28.9	43.3

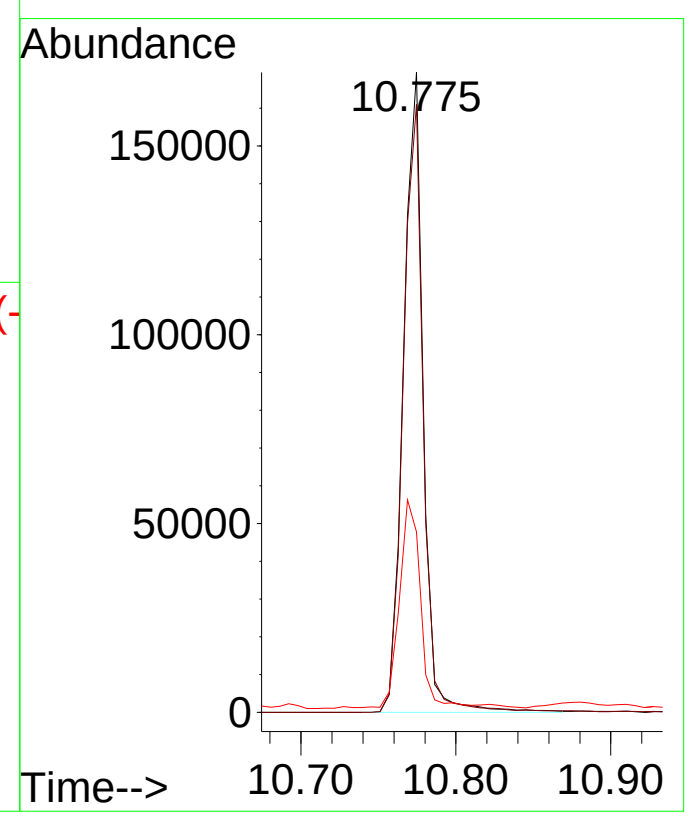

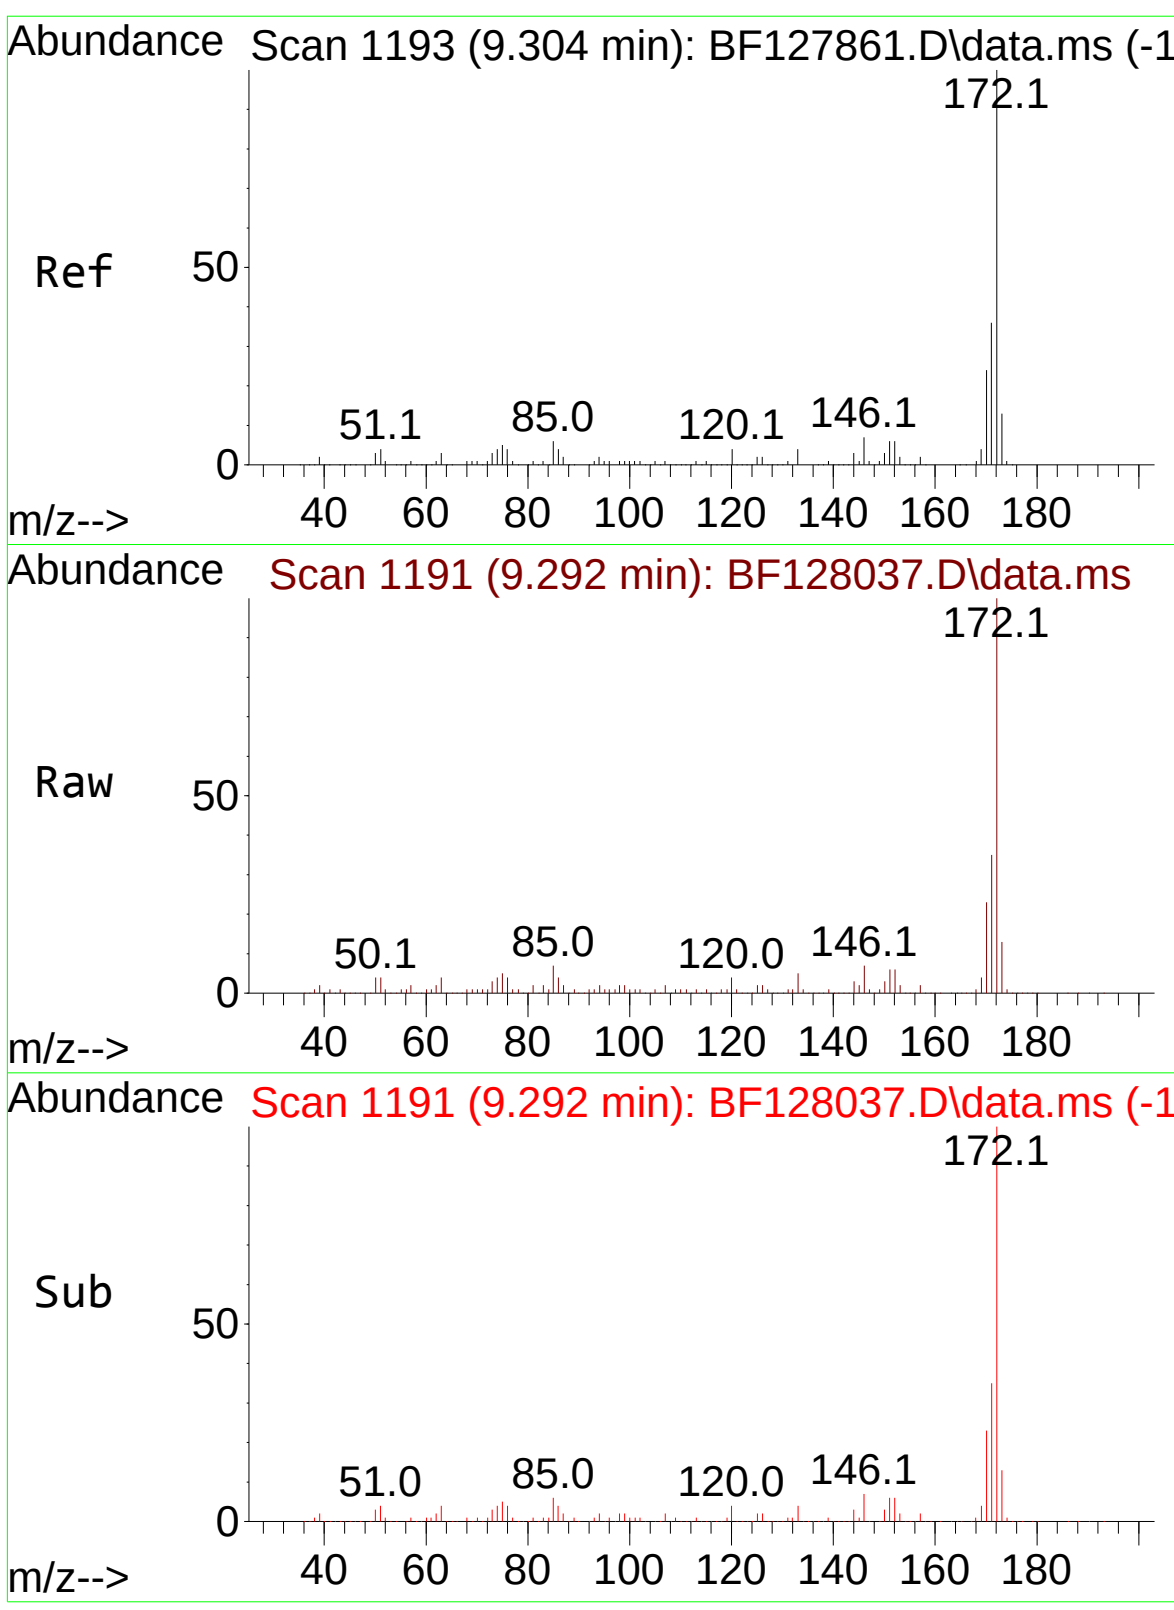

#45
2-Fluorobiphenyl
Concen: 85.311 ng
RT: 9.292 min Scan# 1191
Delta R.T. 0.000 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:172 Resp: 761750

Ion	Ratio	Lower	Upper
172	100		
171	35.2	28.6	42.8
170	23.4	19.1	28.7

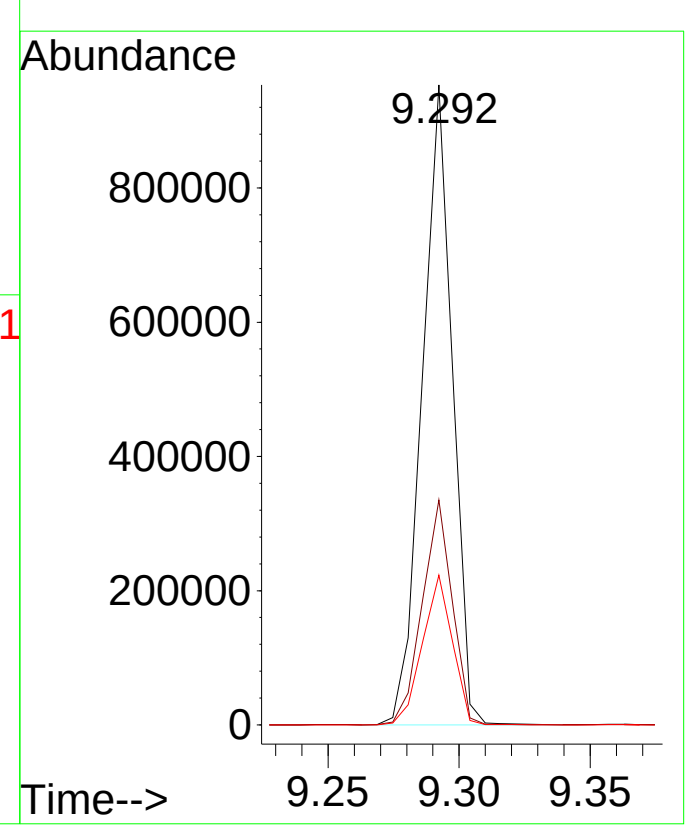

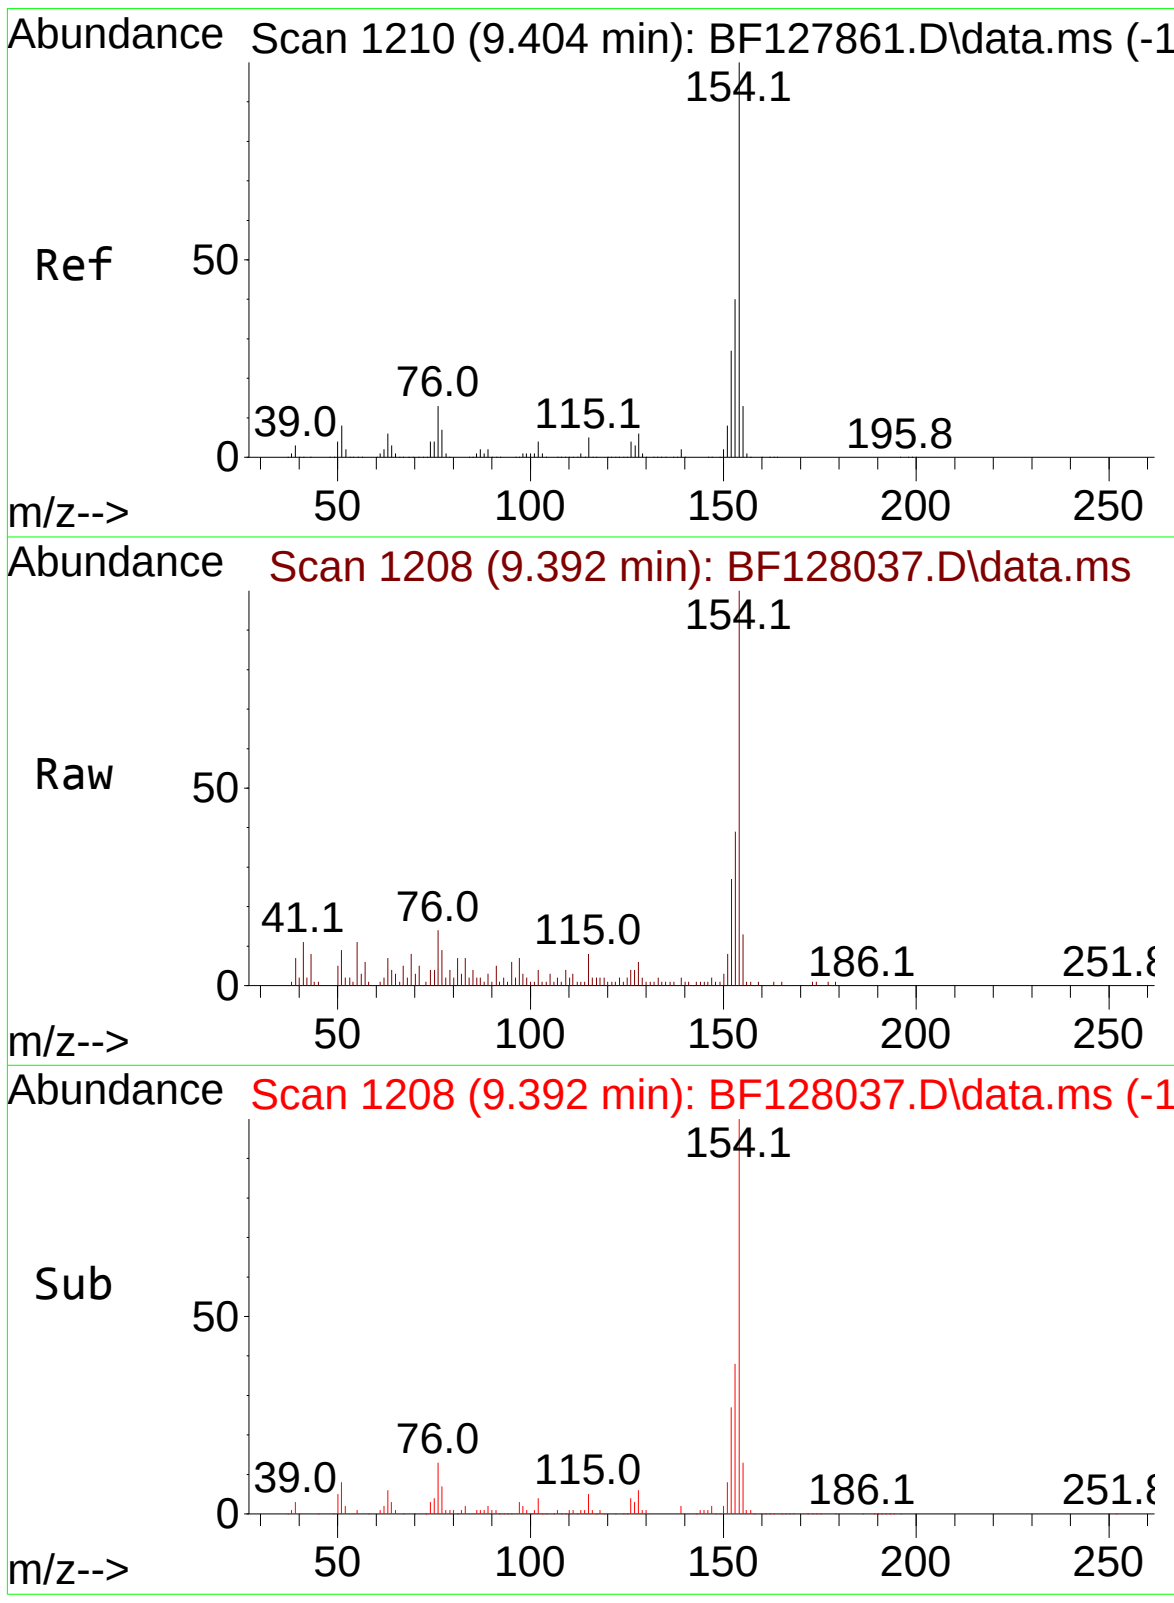

#46
1,1'-Biphenyl
Concen: 4.880 ng
RT: 9.392 min Scan# 1
Delta R.T. -0.006 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Tgt Ion:154 Resp: 54610

Ion	Ratio	Lower	Upper
154	100		
153	38.6	20.4	60.4
76	13.6	0.0	33.2



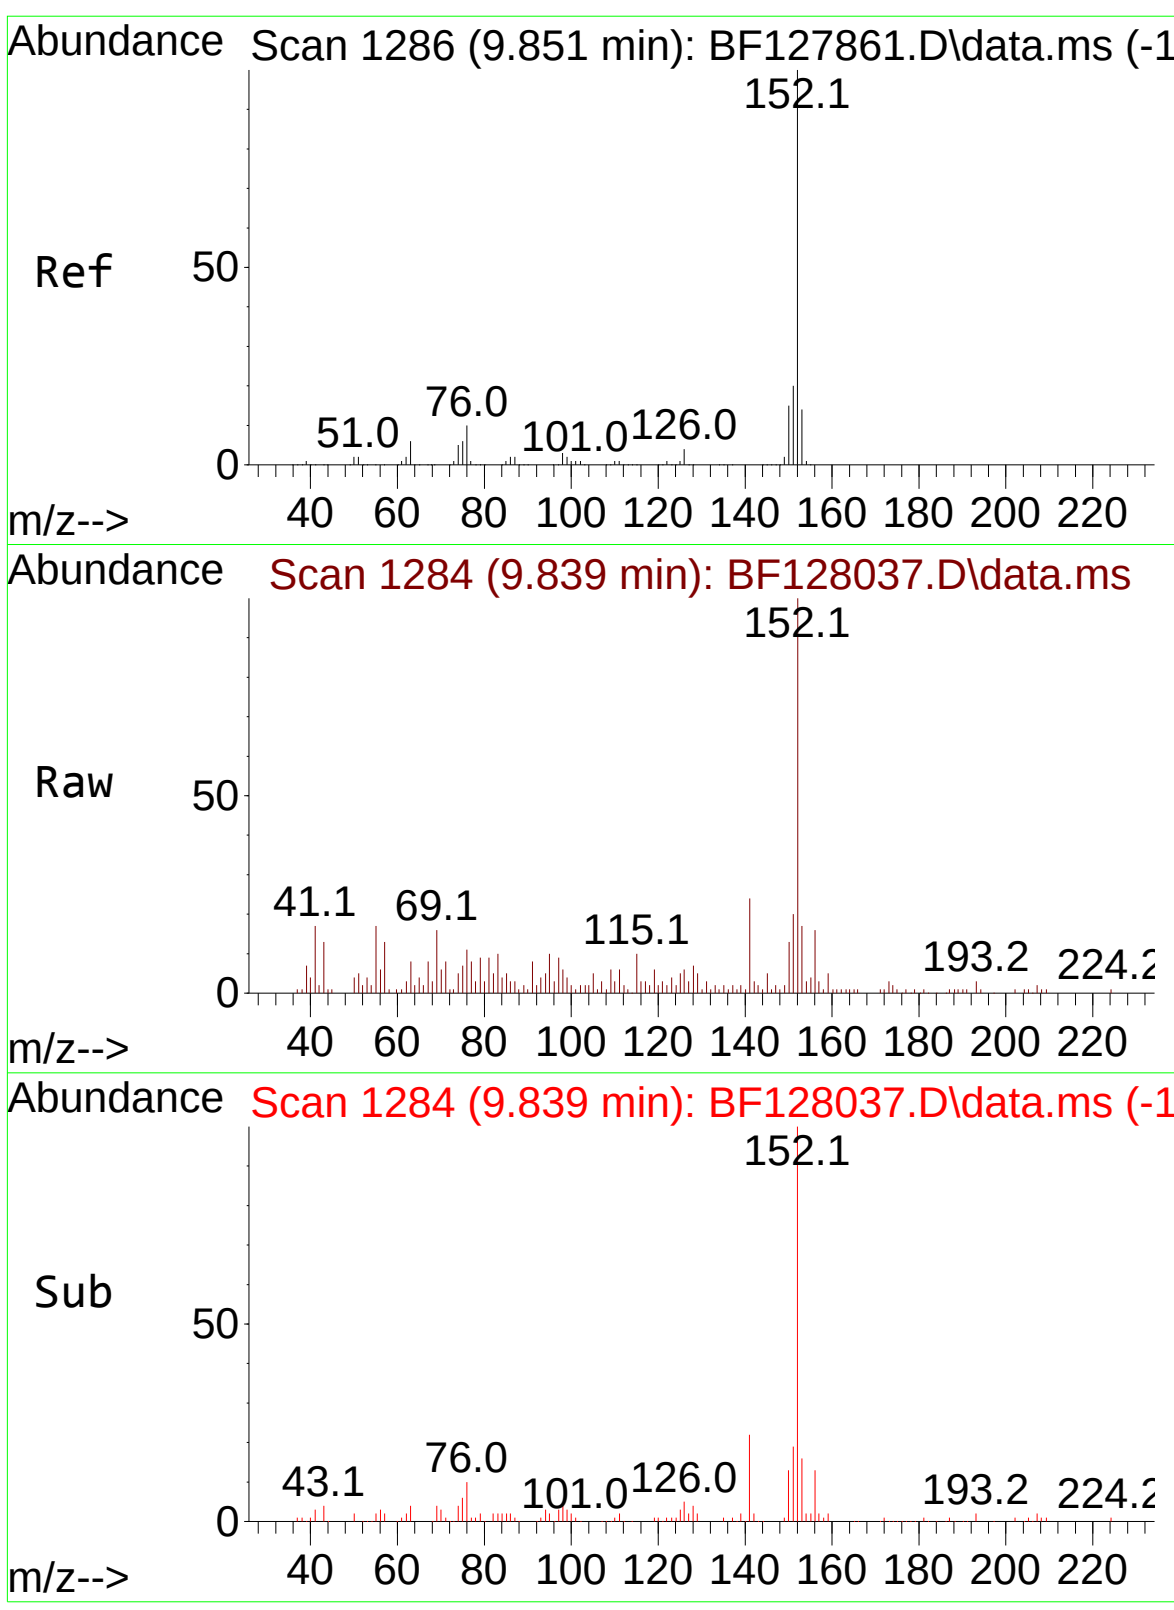

#49
Acenaphthylene
Concen: 2.984 ng
RT: 9.839 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:152 Resp: 38881

Ion	Ratio	Lower	Upper
152	100		
151	20.2	16.2	24.2
153	16.8	11.2	16.8#



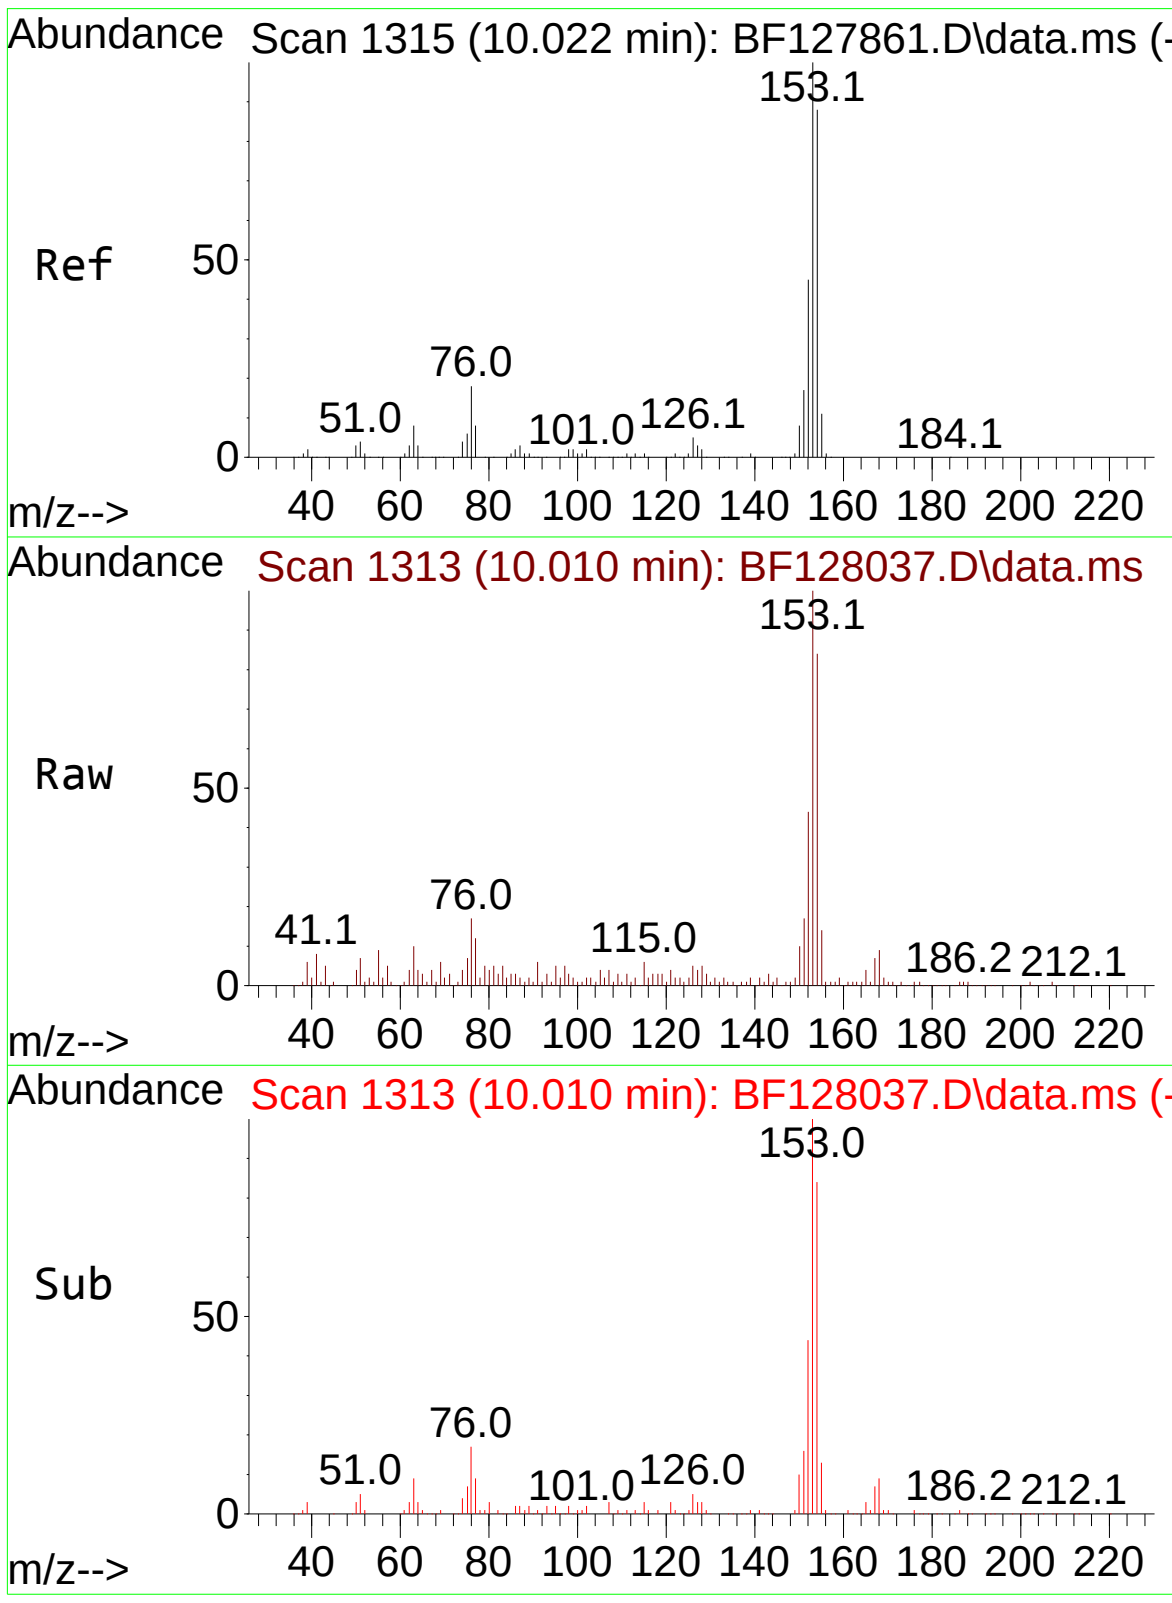

#52
Acenaphthene
Concen: 5.967 ng
RT: 10.010 min Scan# 1
Delta R.T. 0.000 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Tgt Ion:154 Resp: 52270

Ion	Ratio	Lower	Upper
154	100		
153	118.6	90.5	135.7
152	52.6	41.0	61.6



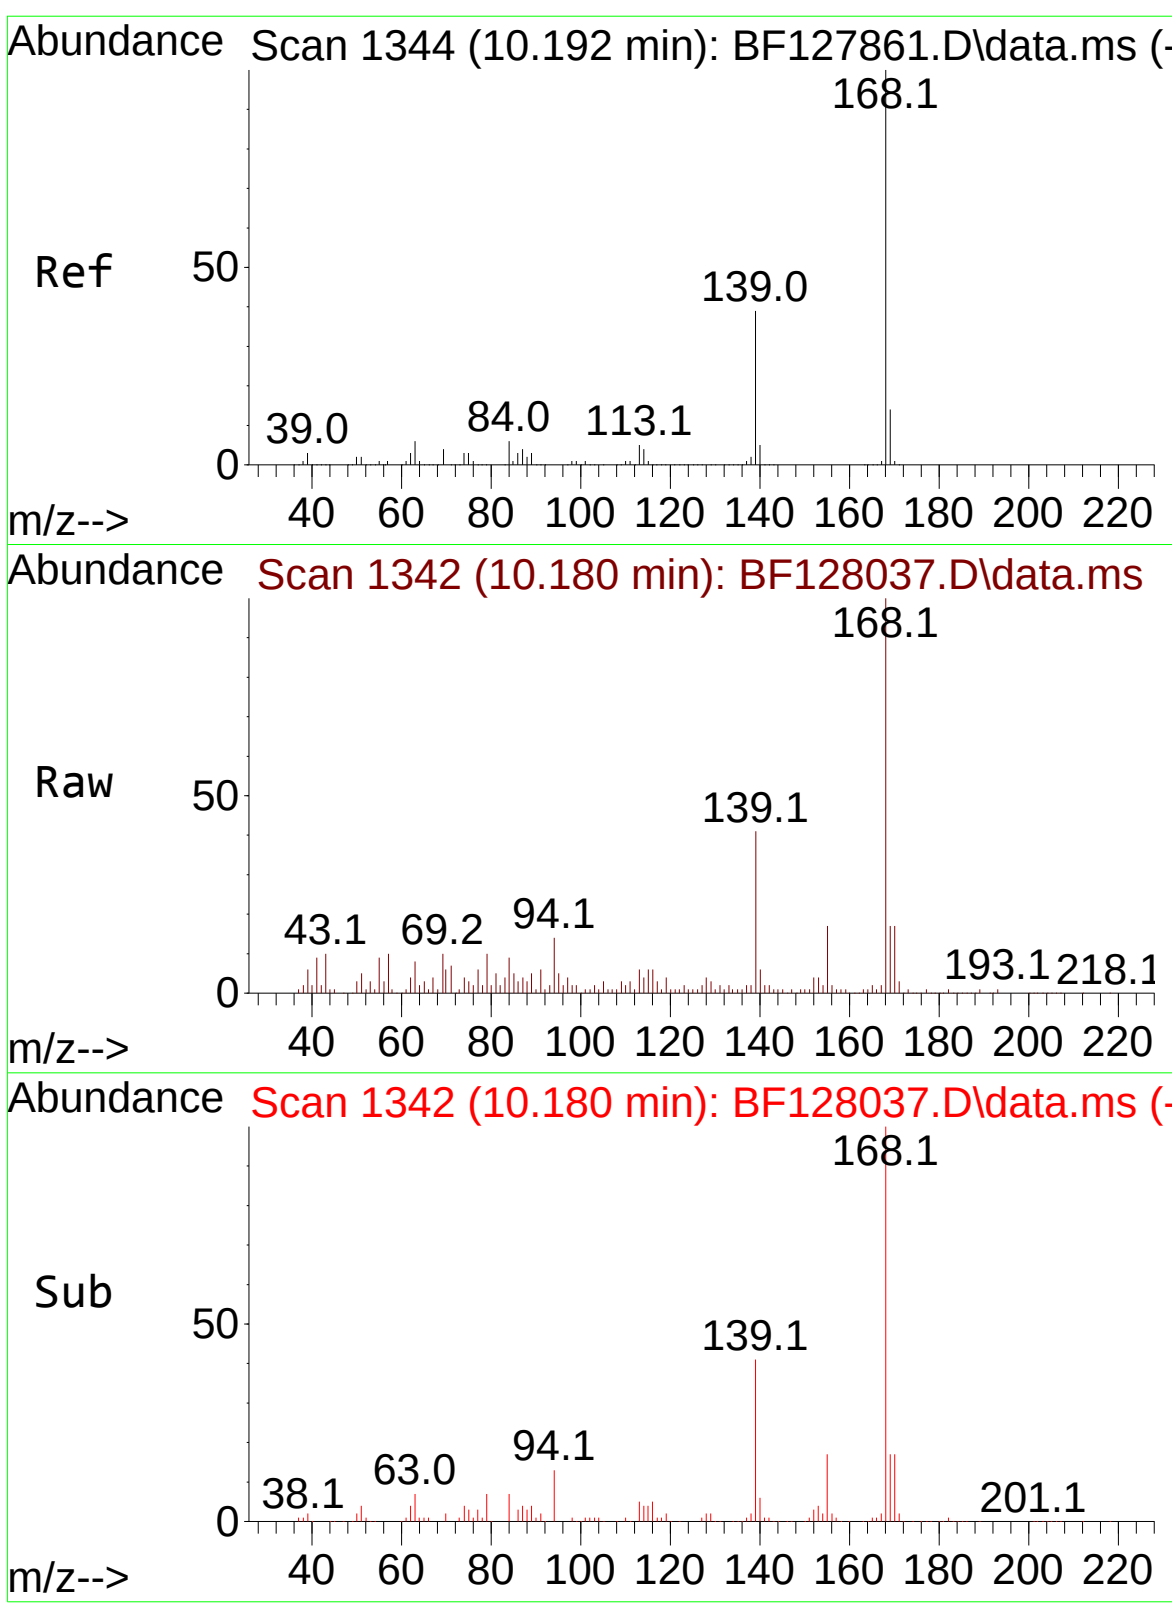

#55
Dibenzofuran
Concen: 5.493 ng
RT: 10.180 min Scan# 1342
Delta R.T. 0.000 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:168 Resp: 69421

Ion	Ratio	Lower	Upper
168	100		
139	41.3	31.7	47.5
169	17.0	10.9	16.3#



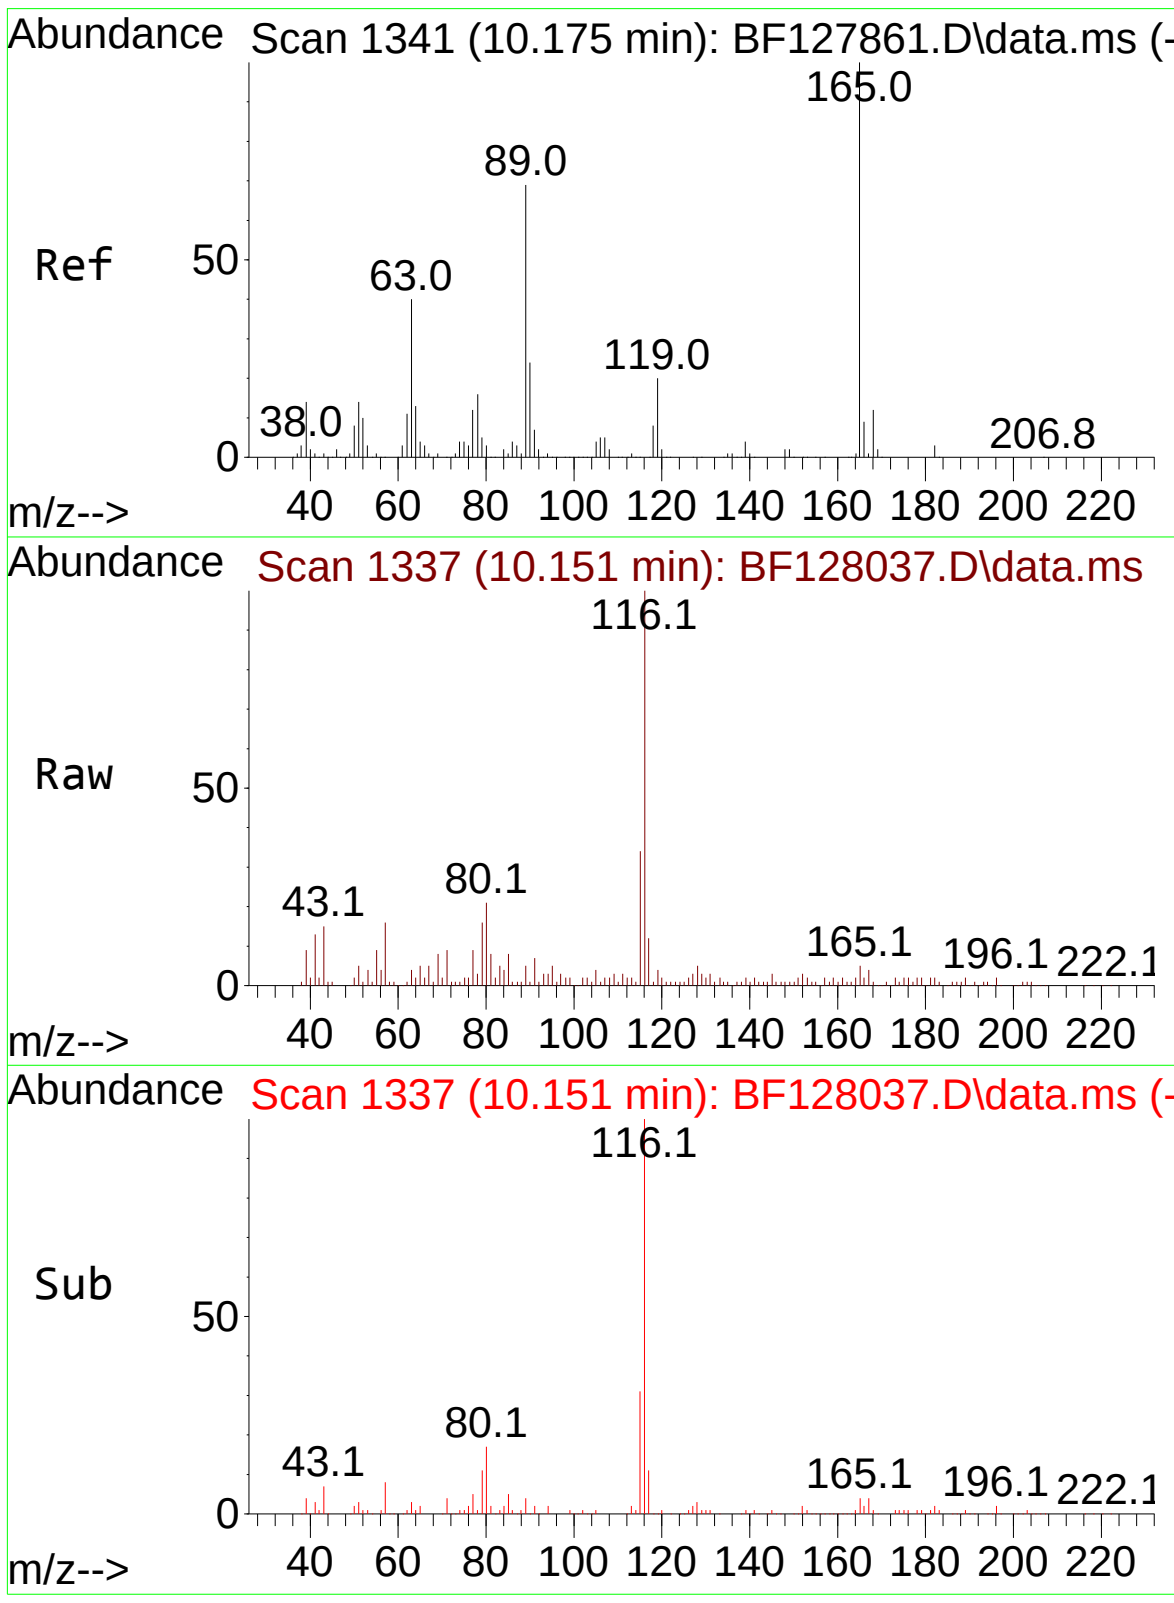

#57
2,4-Dinitrotoluene
Concen: 2.390 ng
RT: 10.151 min Scan# 1
Delta R.T. -0.012 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Tgt Ion:165 Resp: 6944

Ion	Ratio	Lower	Upper
165	100		
63	90.1	32.6	49.0#
89	107.6	55.2	82.8#
182	49.0	2.0	3.0#

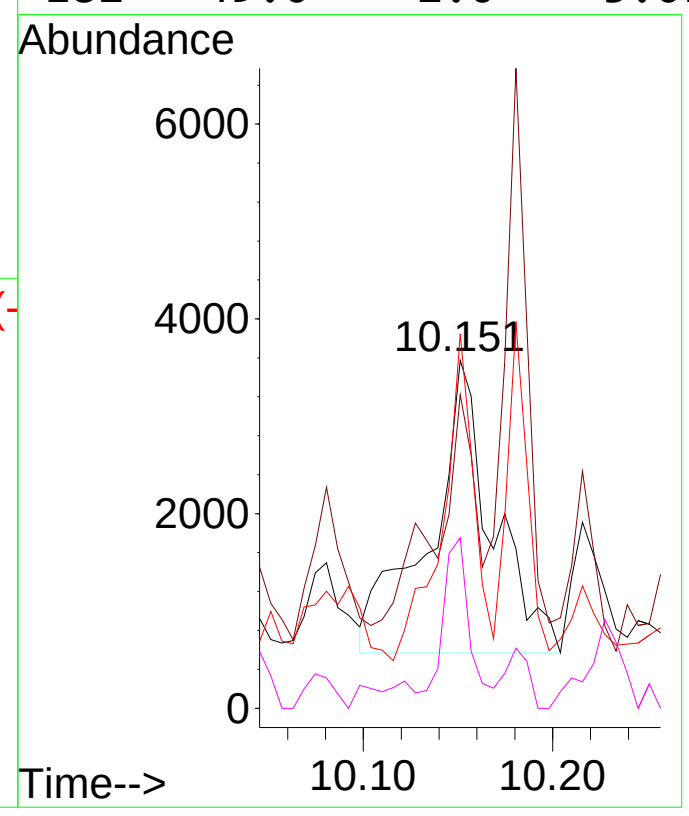

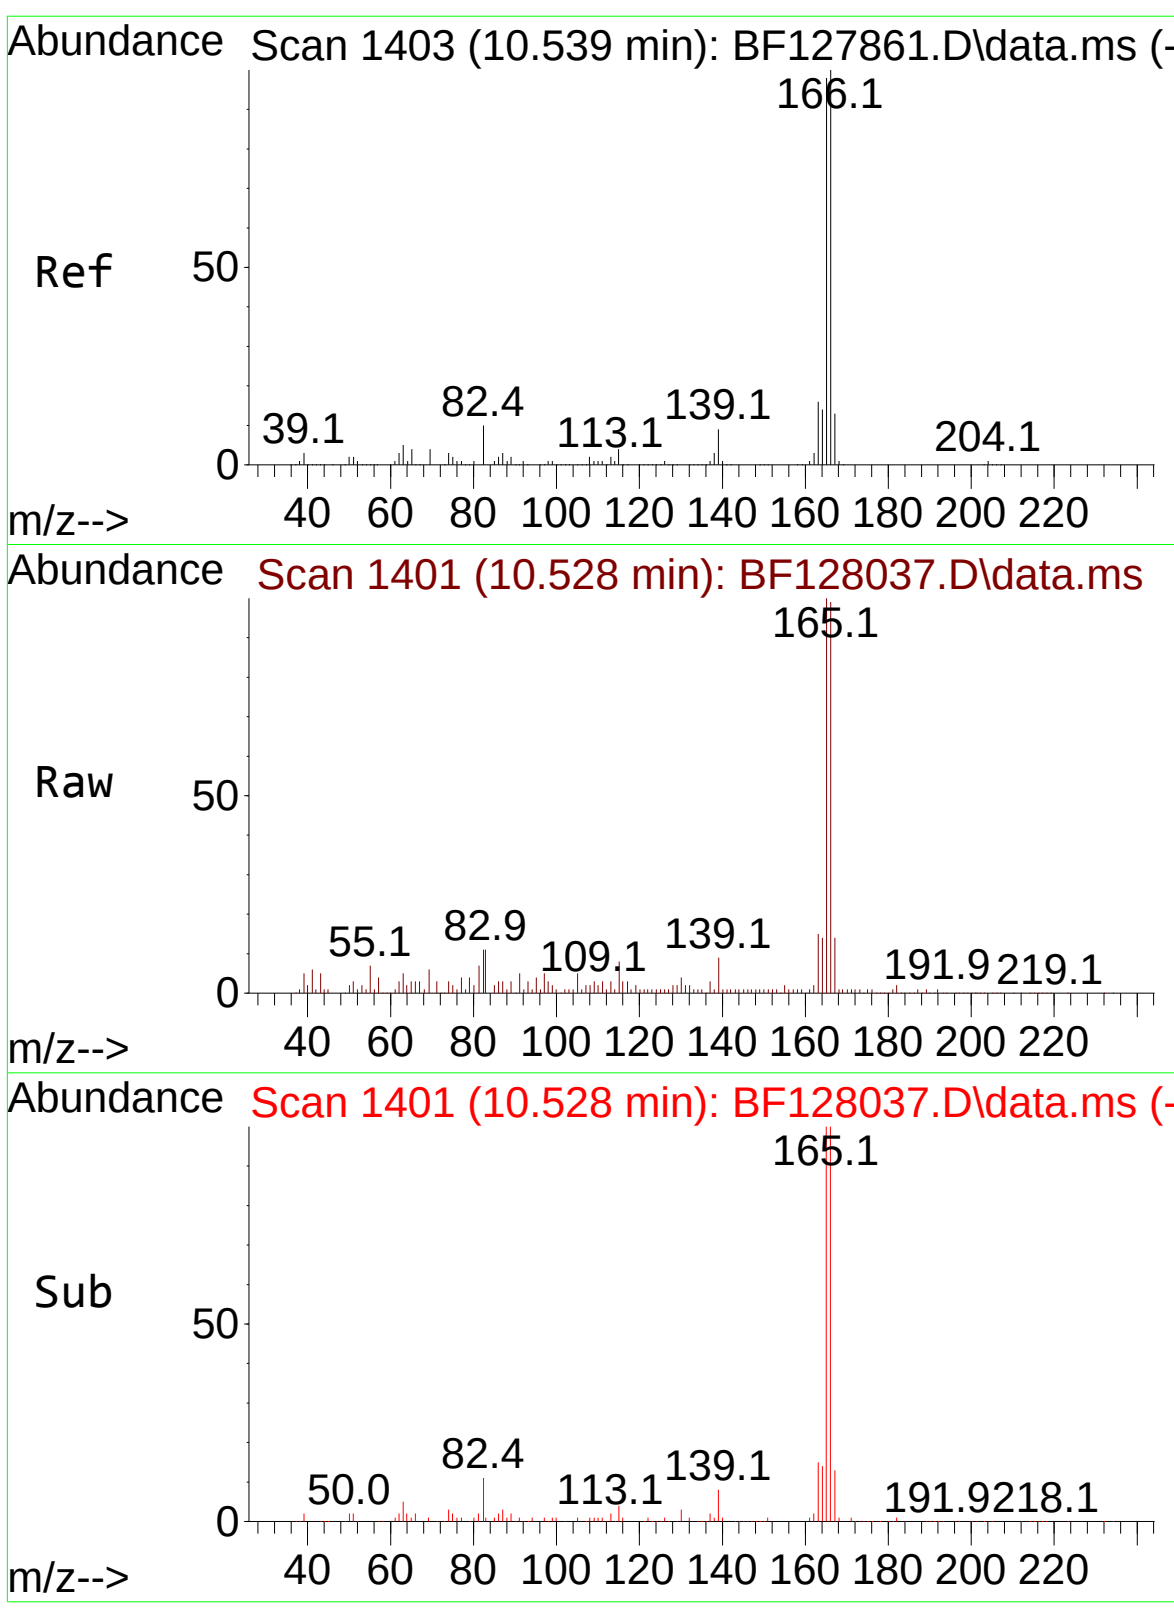

#58
Fluorene
Concen: 8.712 ng
RT: 10.528 min Scan# 1401
Delta R.T. 0.000 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:166 Resp: 82161

Ion	Ratio	Lower	Upper
166	100		
165	100.7	78.6	117.8
167	14.6	10.5	15.7



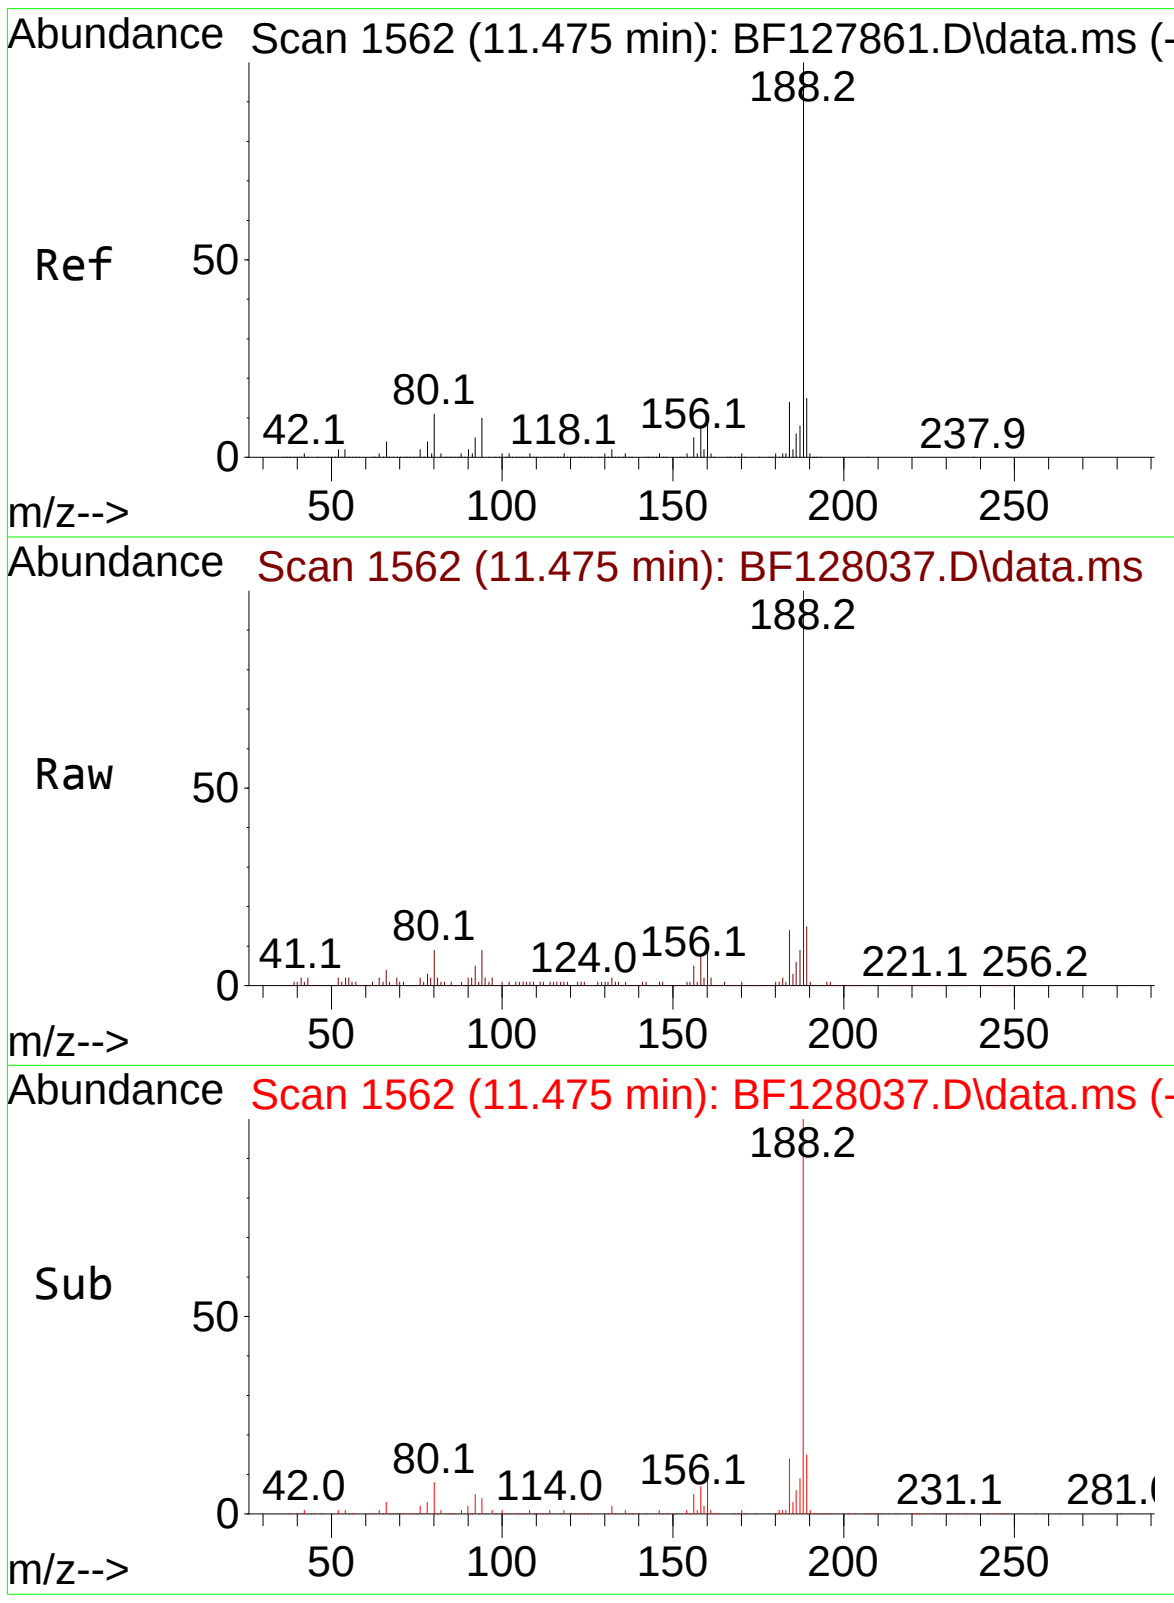

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.475 min Scan# 1
Delta R.T. 0.006 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Tgt Ion:188 Resp: 253903

Ion	Ratio	Lower	Upper
188	100		
94	9.0	8.0	12.0
80	9.0	8.9	13.3



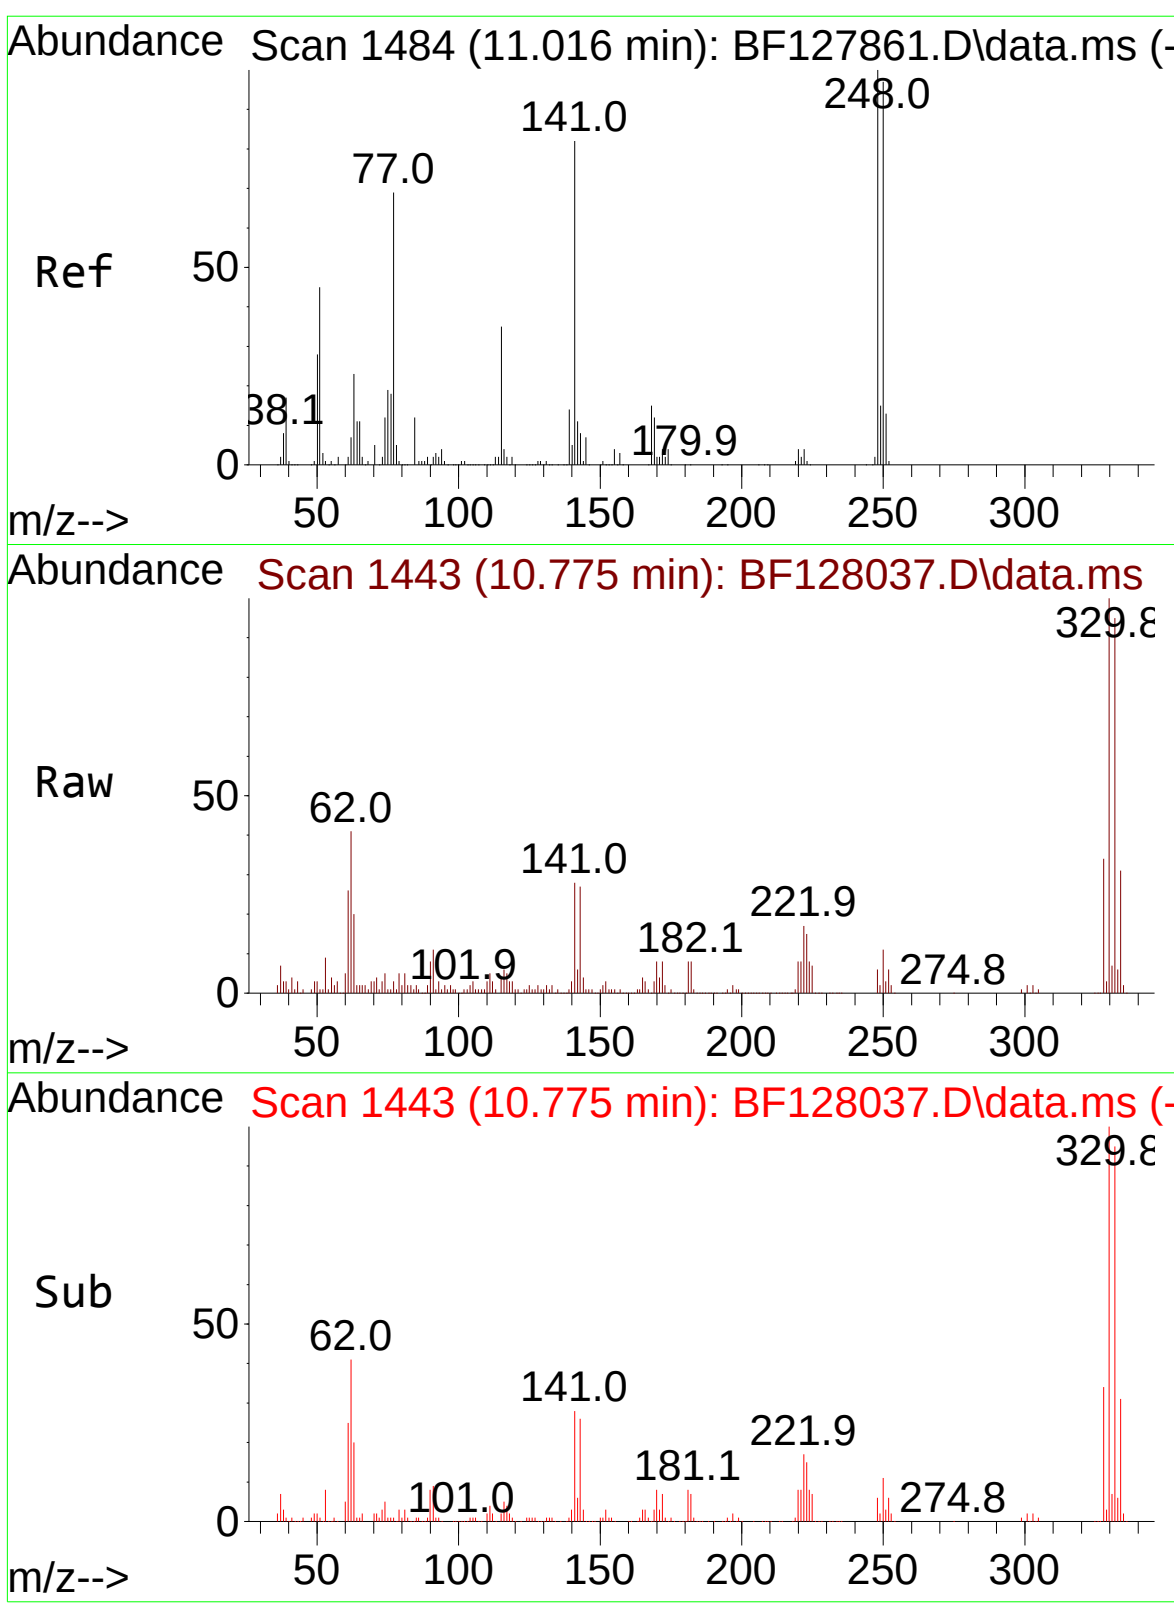

#67
4-Bromophenyl-phenylether
Concen: 3.350 ng
RT: 10.775 min Scan# 1443
Delta R.T. -0.235 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:248 Resp: 9430

Ion	Ratio	Lower	Upper
248	100		
250	193.4	77.7	116.5#
141	484.4	65.6	98.4#



Instrument :
BNA_F
ClientSampleId :
JC-01-042822

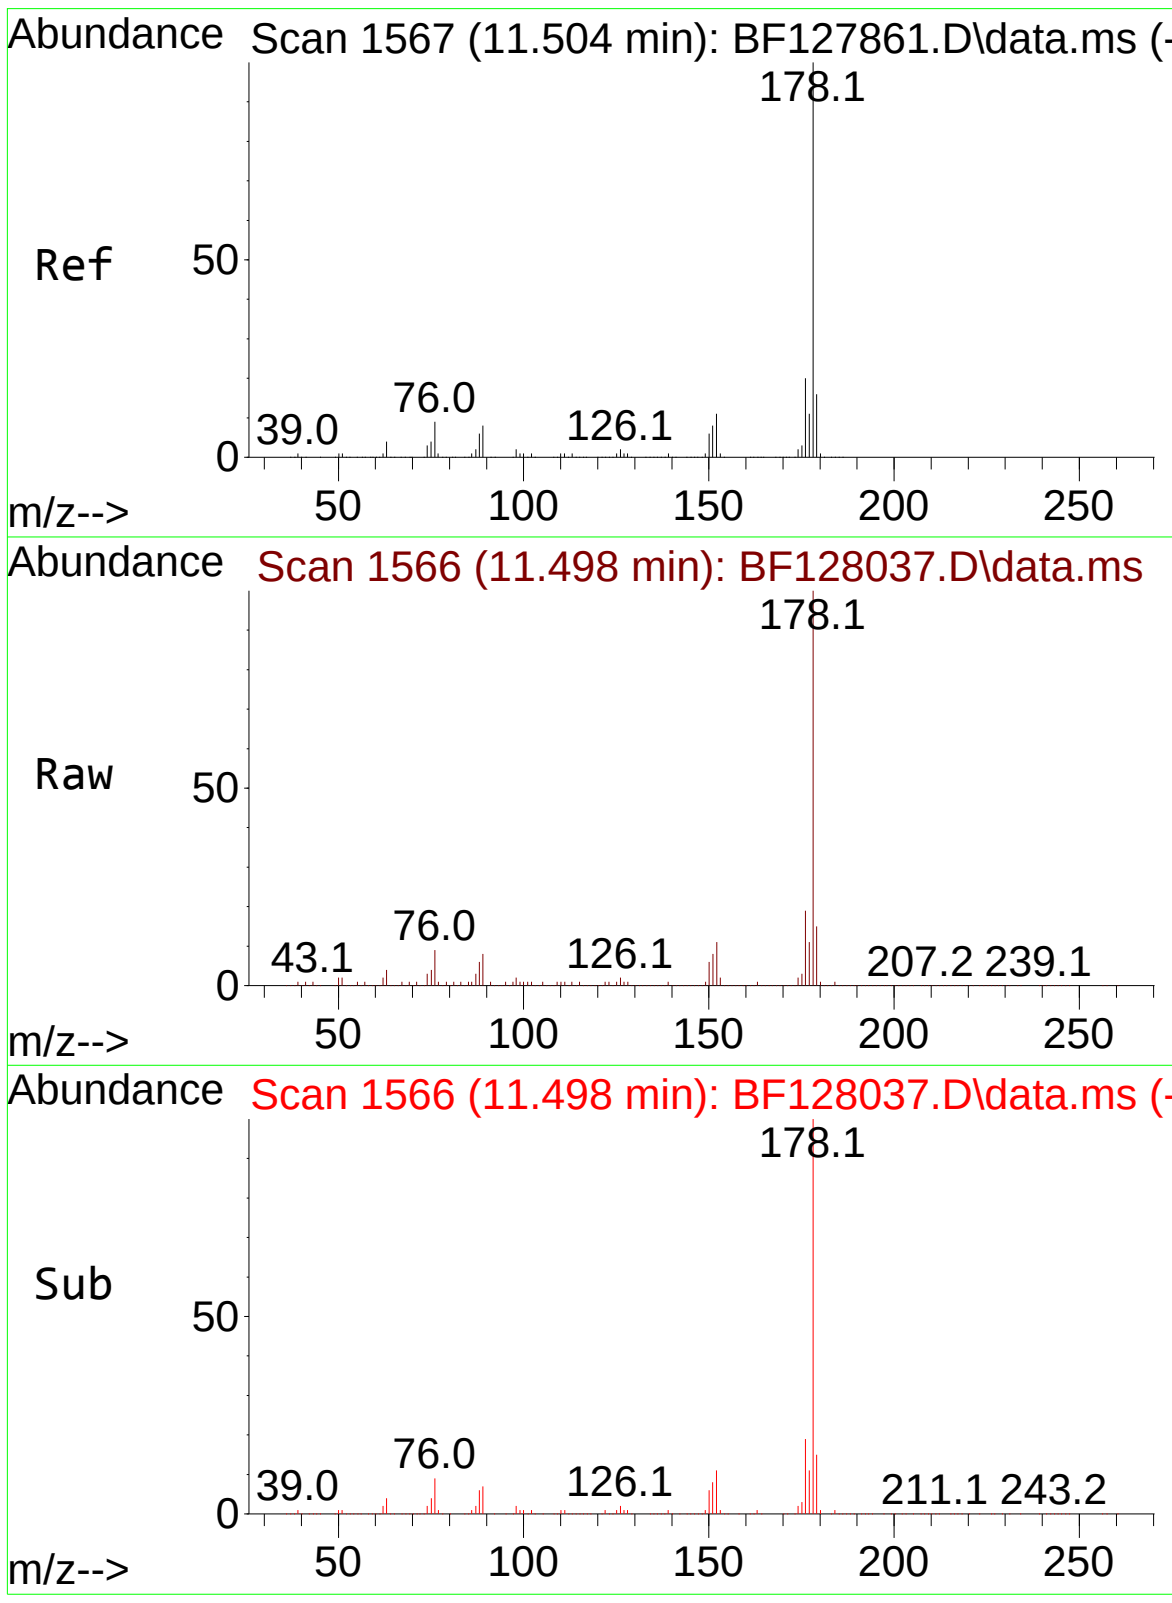

#71
Phenanthrene
Concen: 38.497 ng
RT: 11.498 min Scan# 1
Delta R.T. 0.006 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:178 Resp: 511648

Ion	Ratio	Lower	Upper
178	100		
176	19.3	15.7	23.5
179	15.5	12.6	19.0



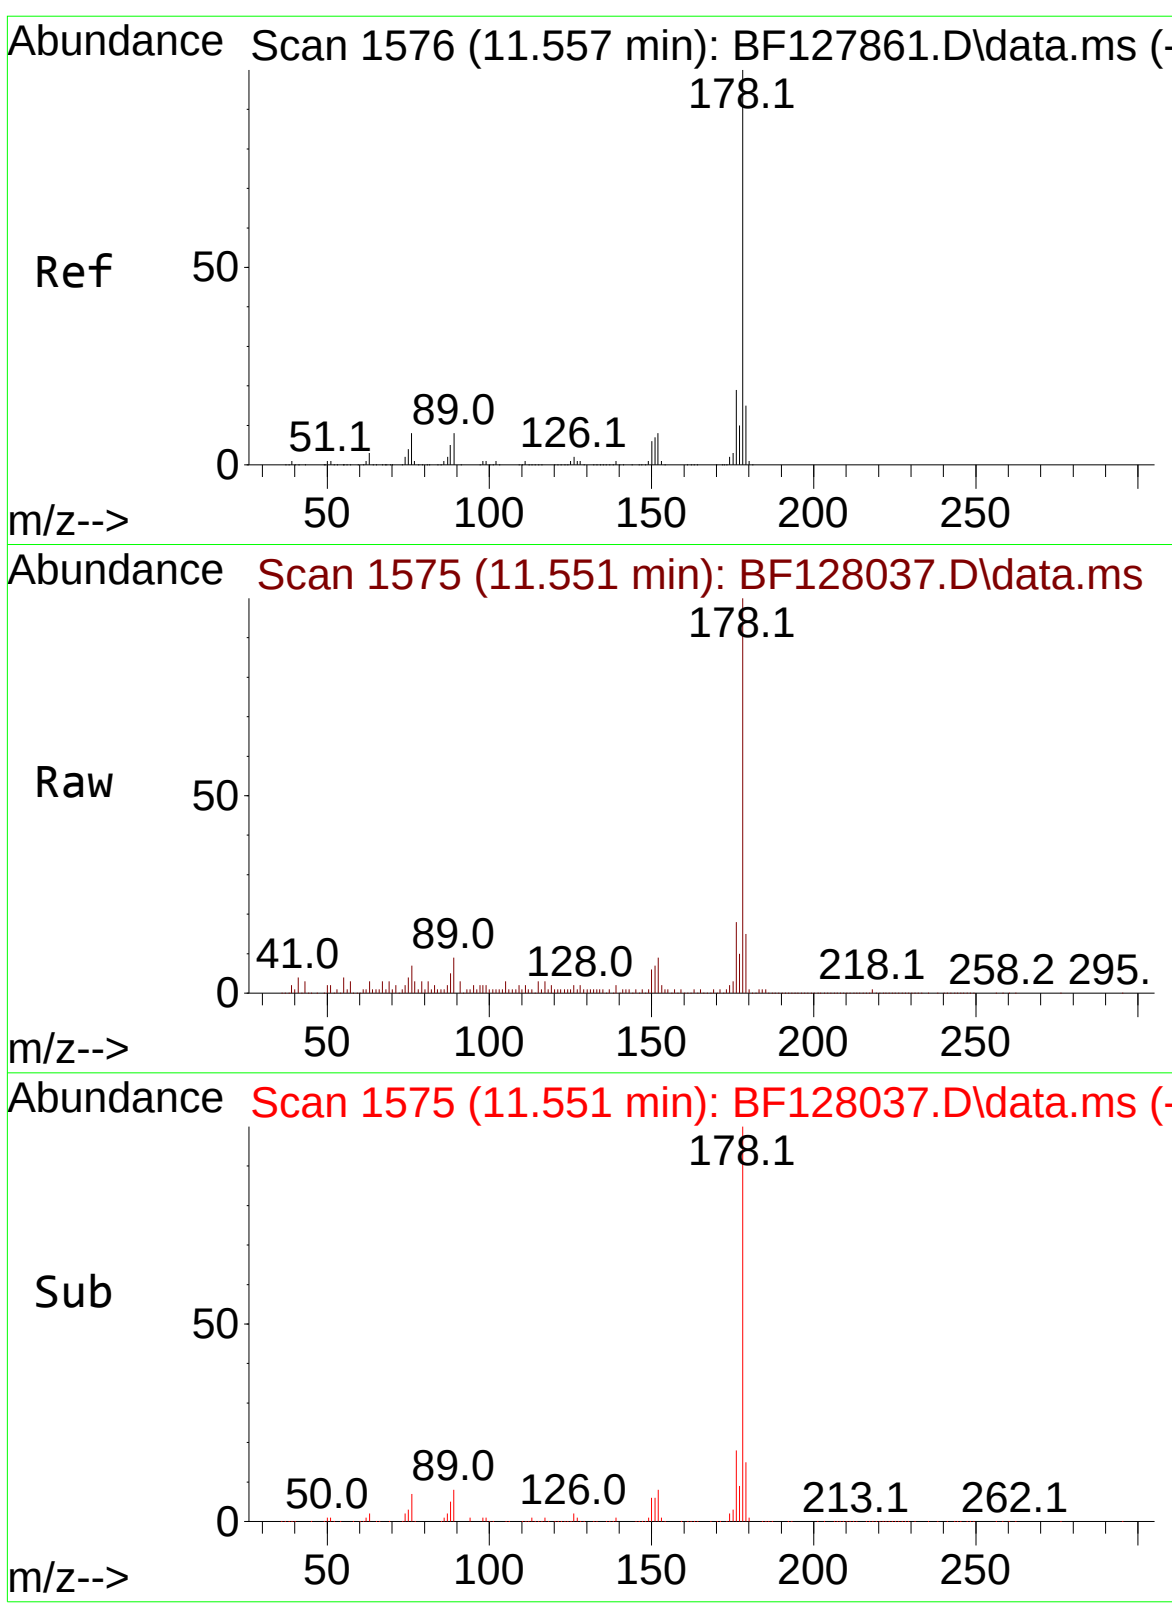

#72
Anthracene
Concen: 10.697 ng
RT: 11.551 min Scan# 1575
Delta R.T. 0.006 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:178 Resp: 141624

Ion	Ratio	Lower	Upper
178	100		
176	17.7	15.0	22.6
179	15.5	12.4	18.6



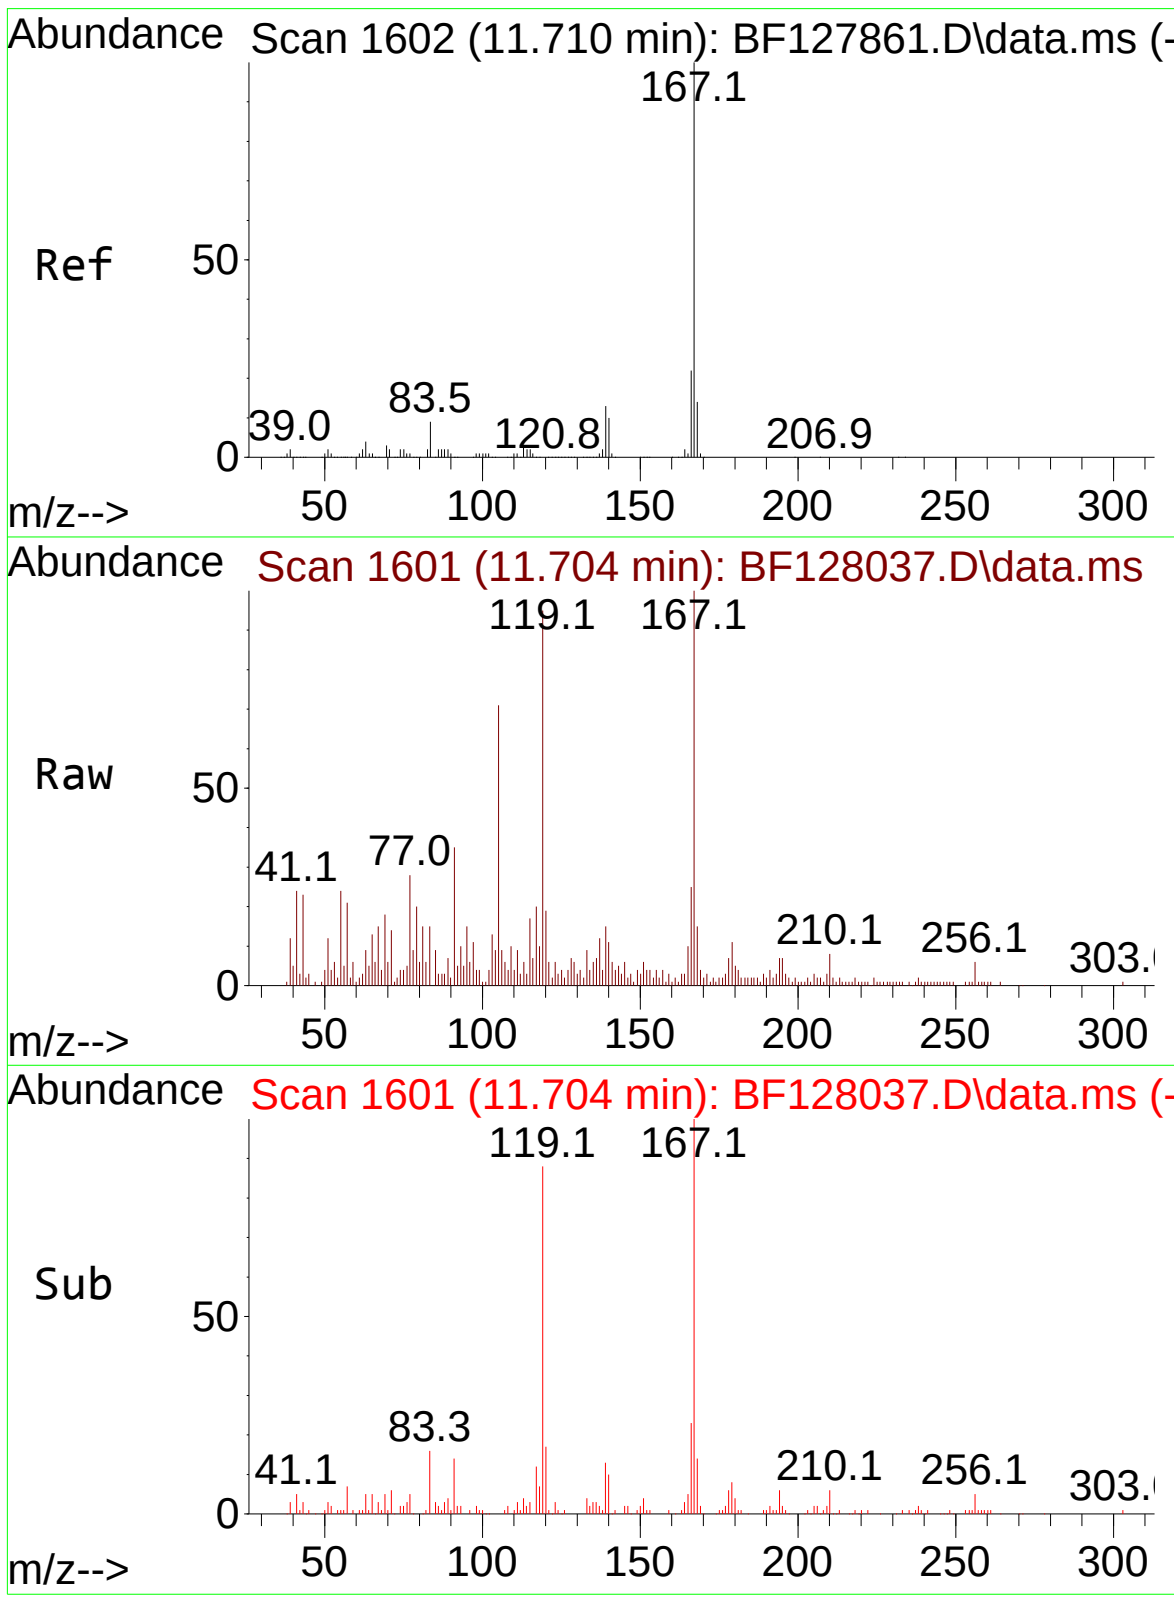

#73
Carbazole
Concen: 2.298 ng
RT: 11.704 min Scan# 1(
Delta R.T. 0.006 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Tgt Ion:167 Resp: 29318

Ion	Ratio	Lower	Upper
167	100		
166	24.9	17.6	26.4
139	15.2	10.7	16.1

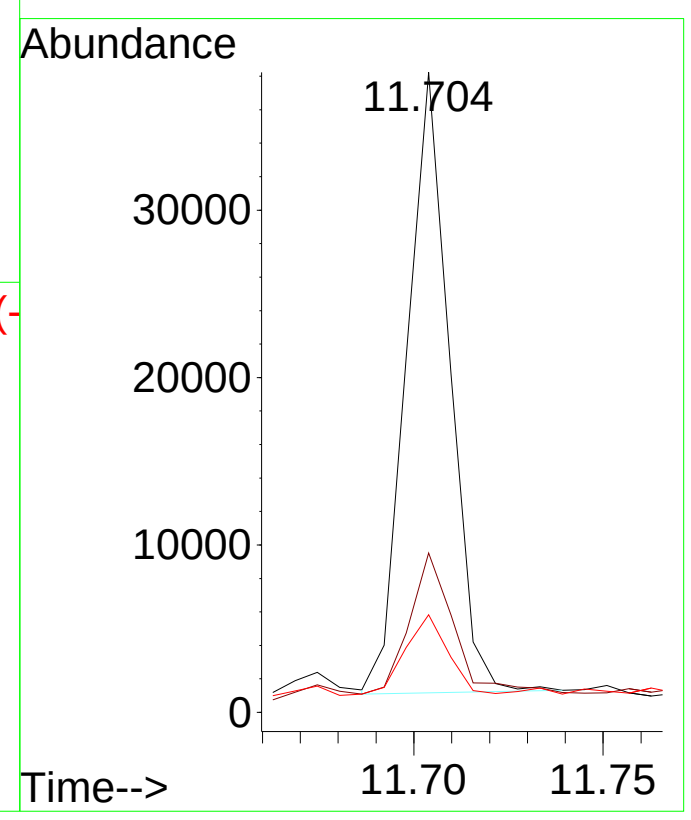

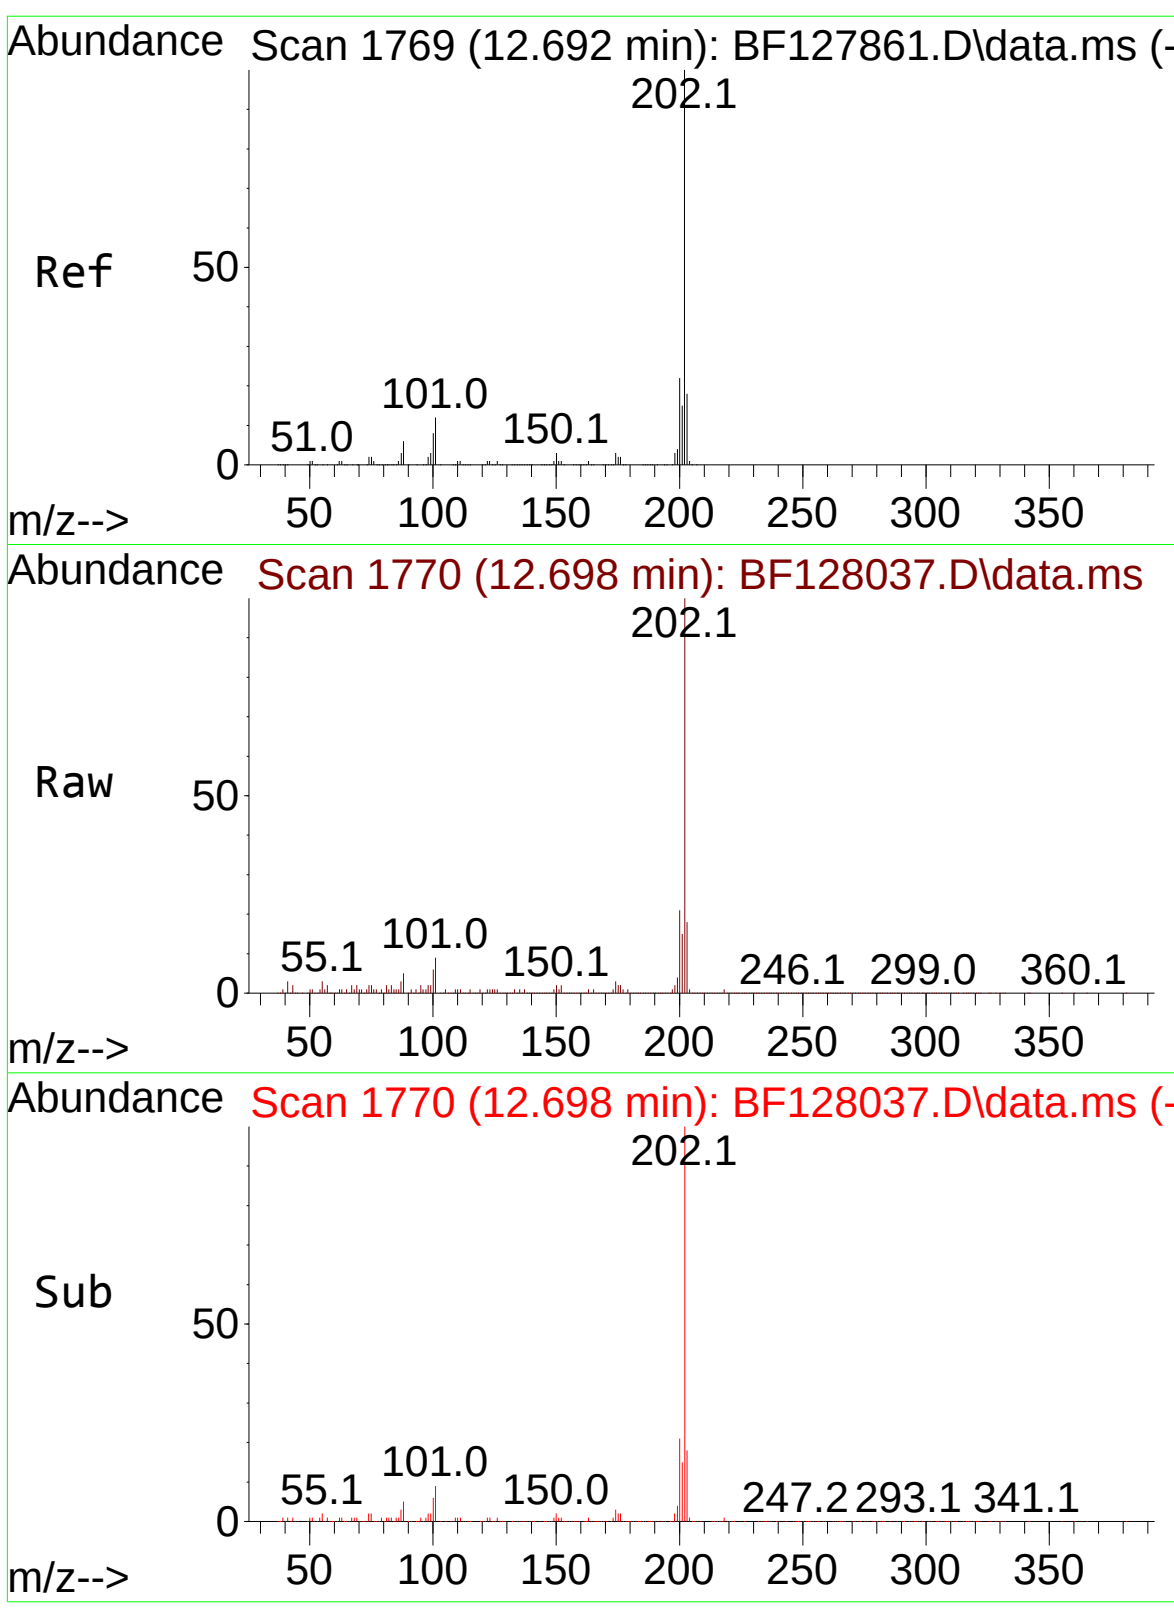

#75
Fluoranthene
Concen: 48.984 ng
RT: 12.698 min Scan# 1770
Delta R.T. 0.012 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:202 Resp: 685190

Ion	Ratio	Lower	Upper
202	100		
101	9.3	0.0	31.6
203	17.8	0.0	38.1

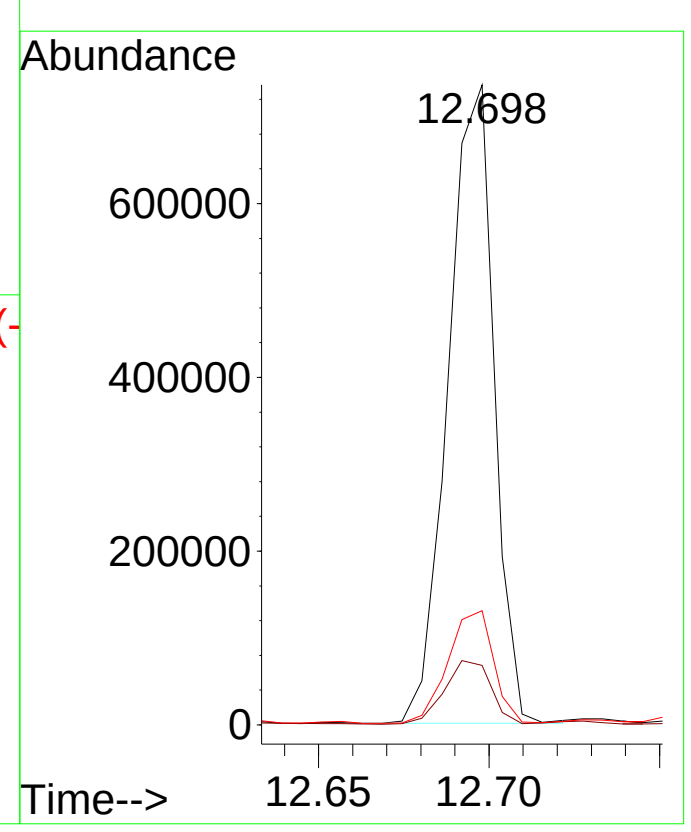

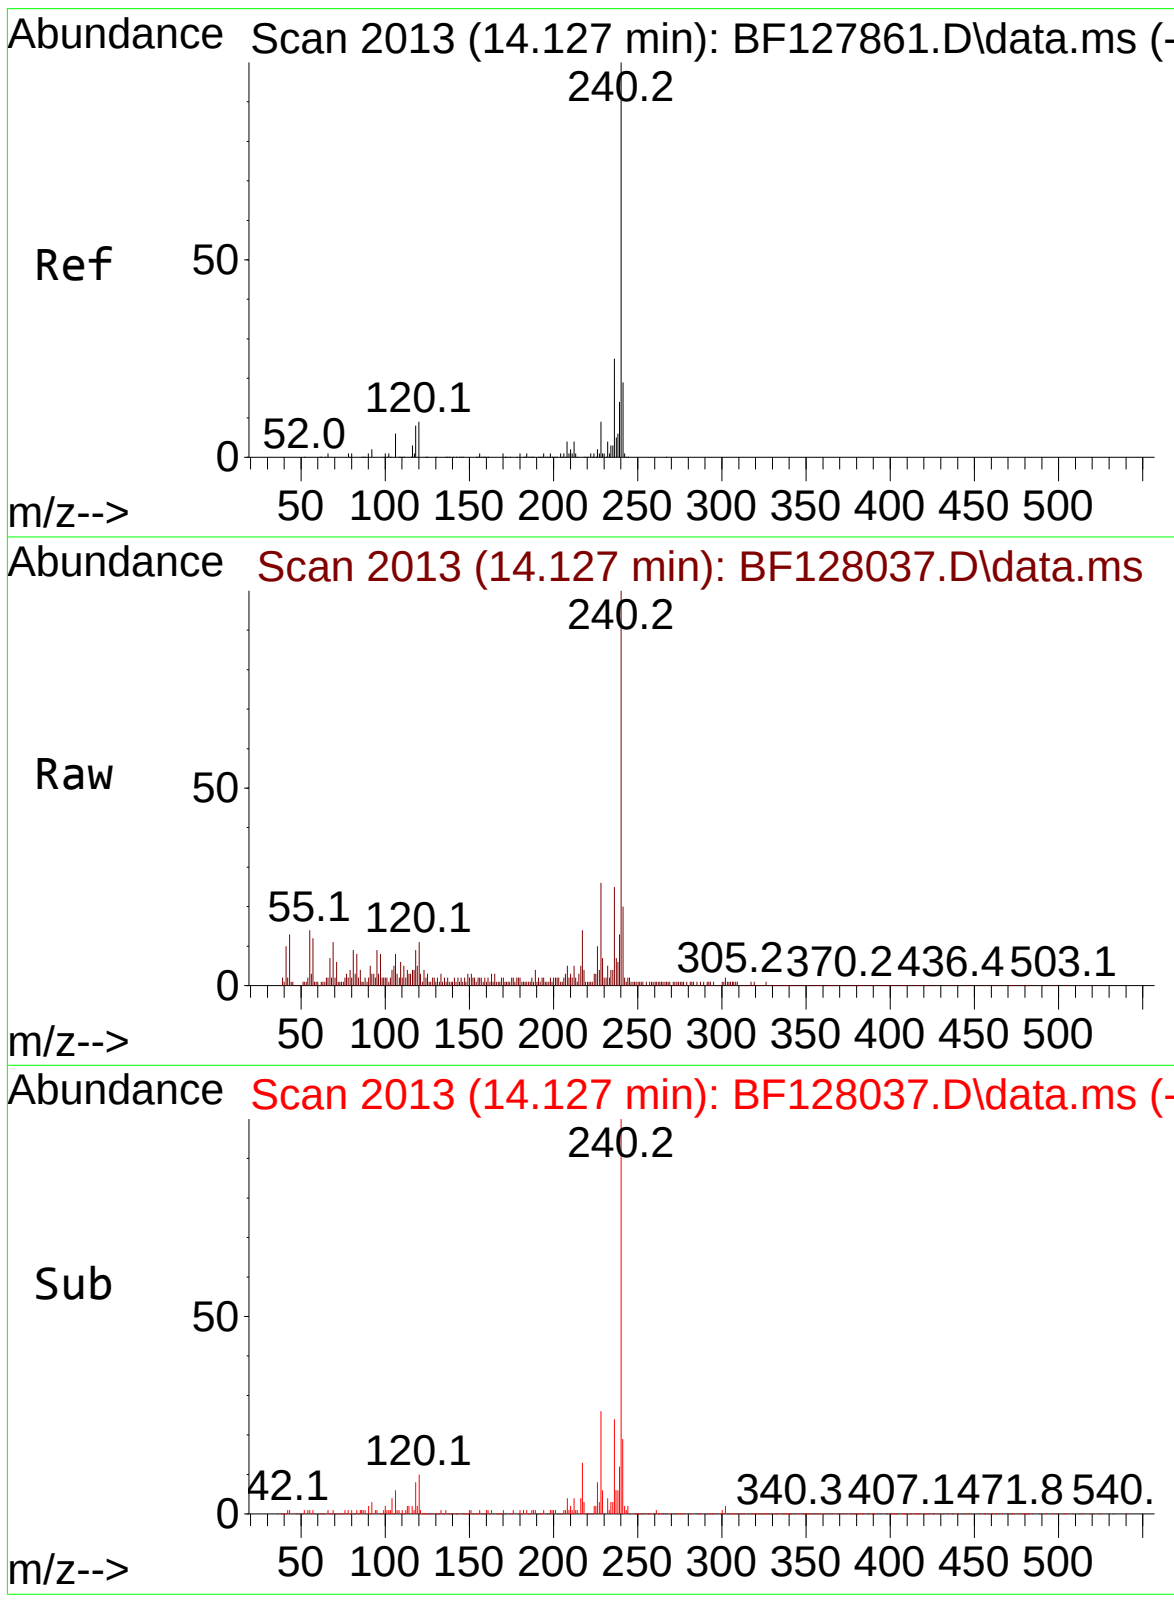

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.127 min   Scan# 20
Delta R.T. 0.012 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Tgt Ion:240 Resp: 142873

Ion	Ratio	Lower	Upper
240	100		
120	10.7	7.0	10.6#
236	24.9	20.3	30.5

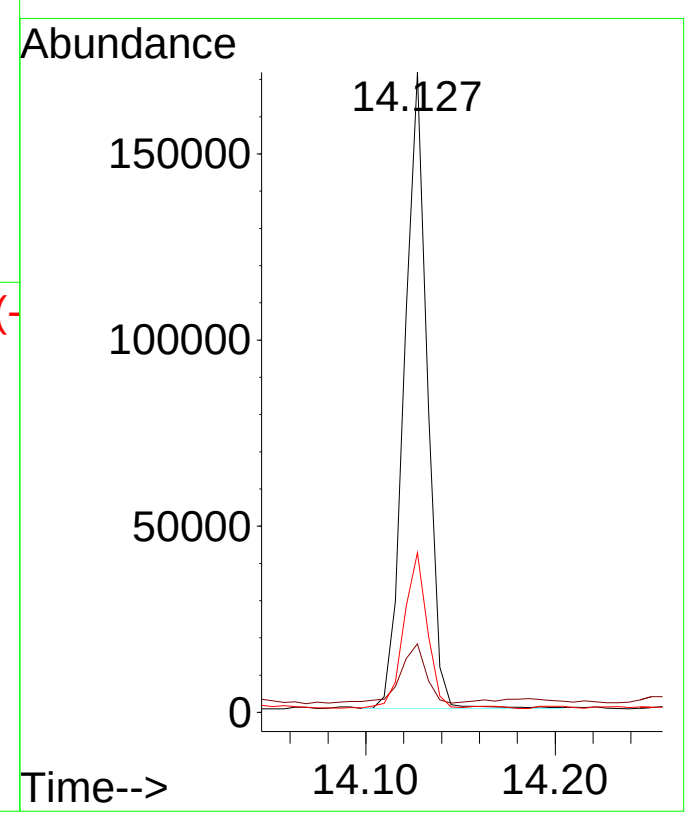

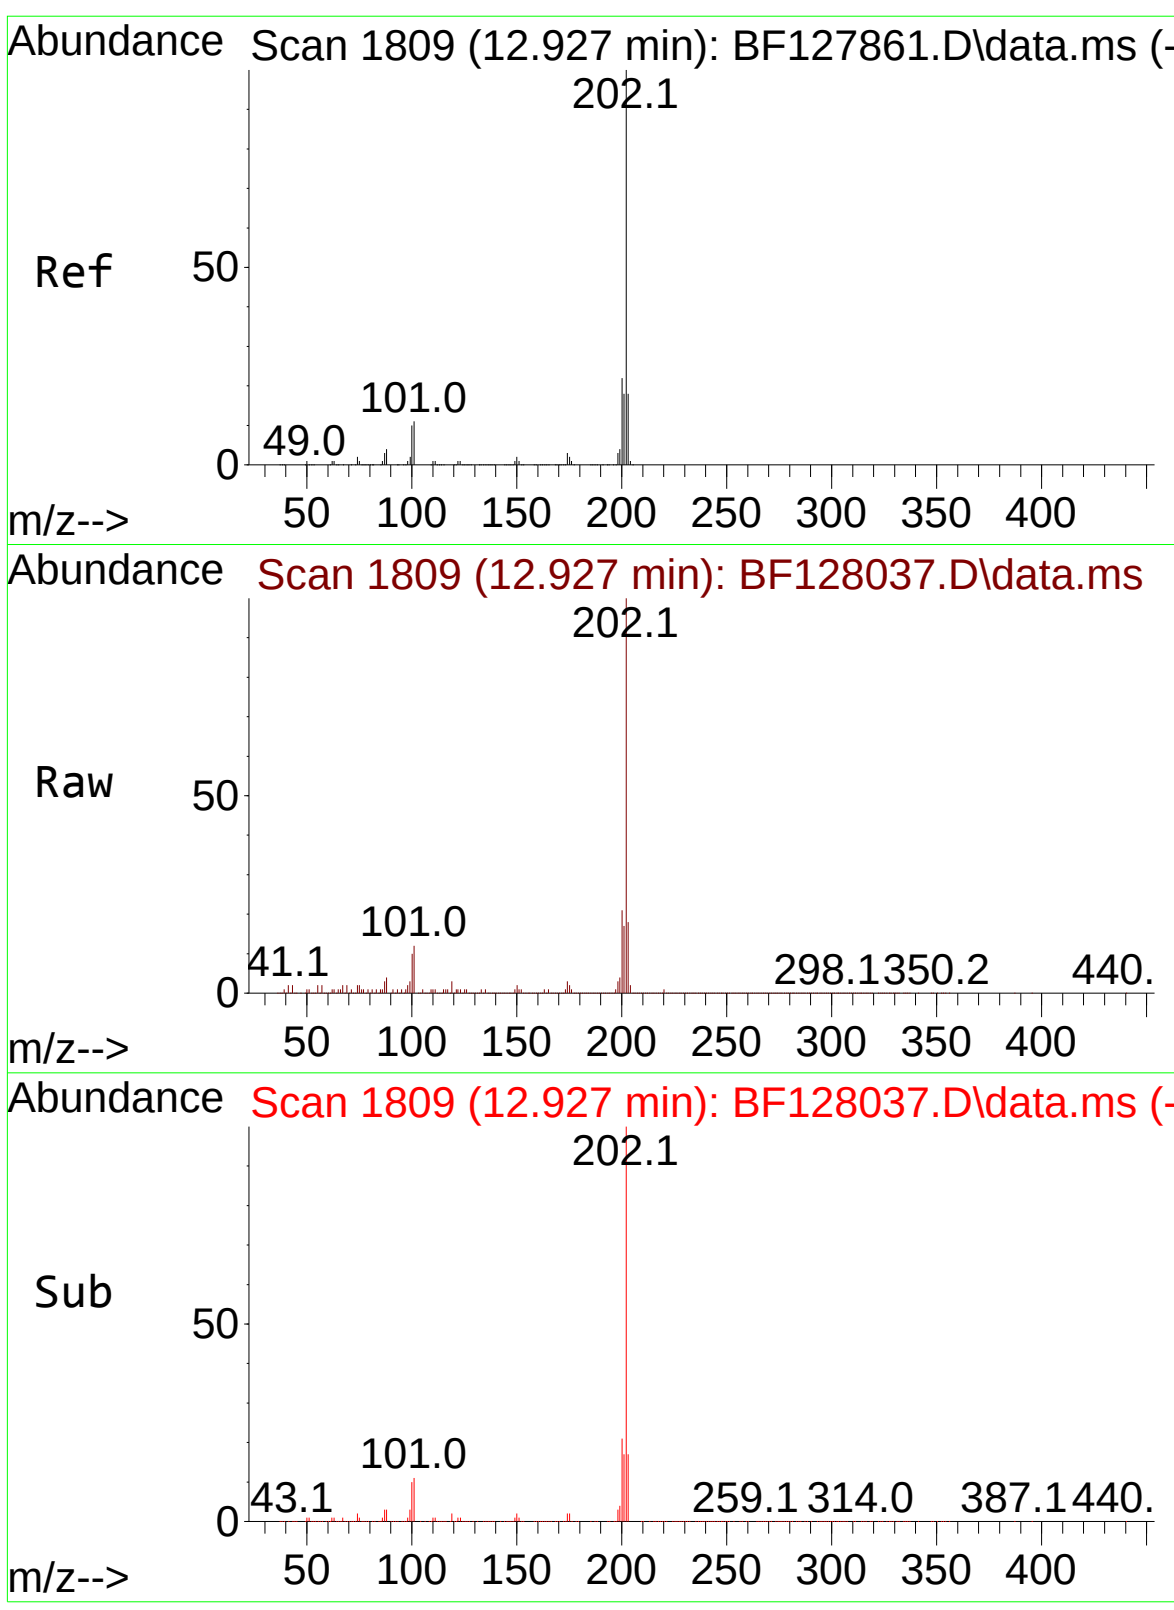

#78
Pyrene
Concen: 56.676 ng
RT: 12.927 min   Scan# 1809
Delta R.T. 0.012 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:202 Resp: 653664

Ion	Ratio	Lower	Upper
202	100		
200	20.9	17.4	26.2
203	17.7	14.0	21.0

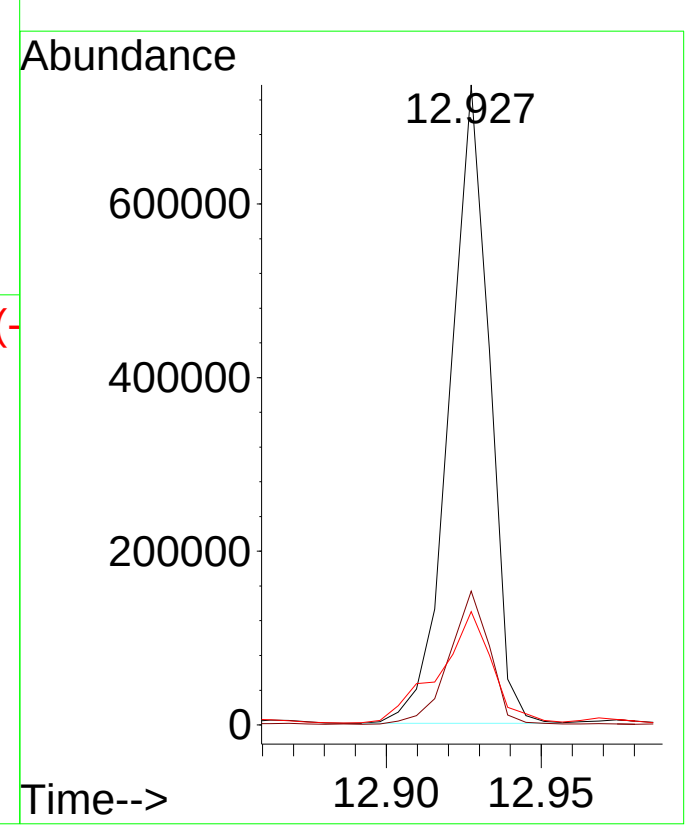

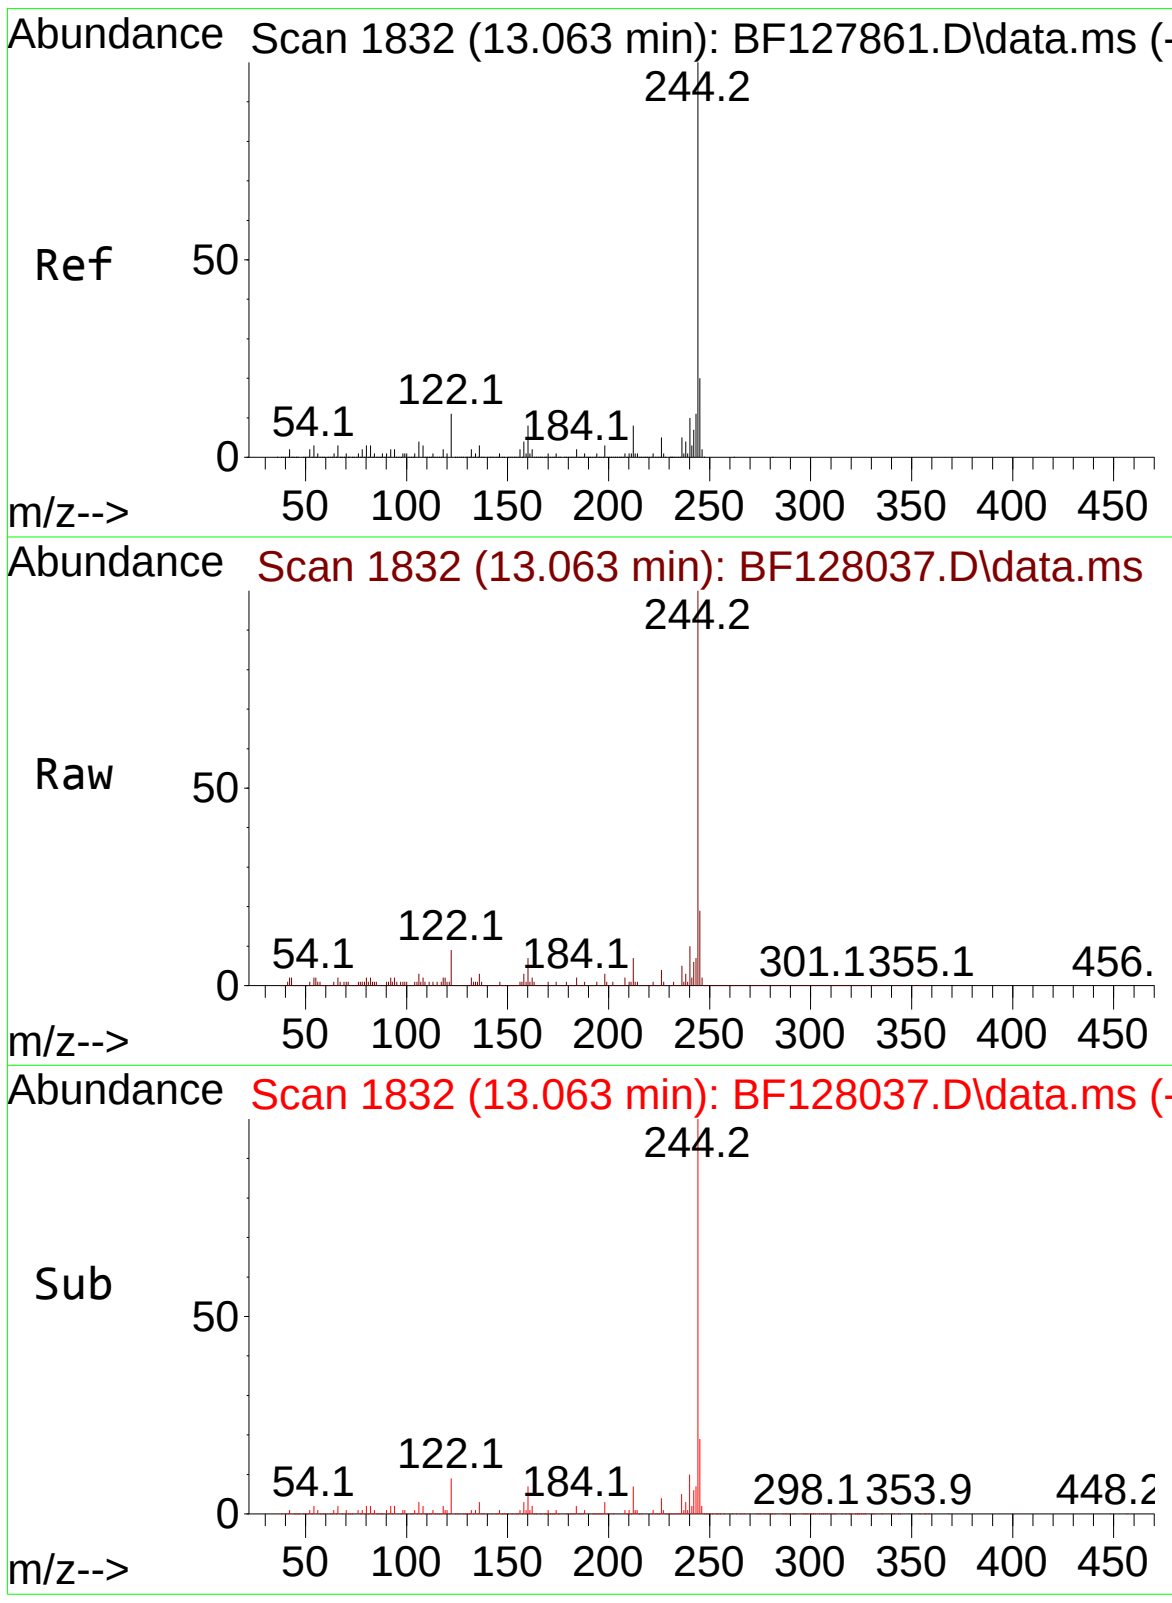

#79
Terphenyl-d14
Concen: 95.239 ng
RT: 13.063 min Scan# 1

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Delta R.T. 0.006 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:244 Resp: 744145

Ion	Ratio	Lower	Upper
244	100		
212	7.5	6.2	9.4
122	9.0	8.6	12.8



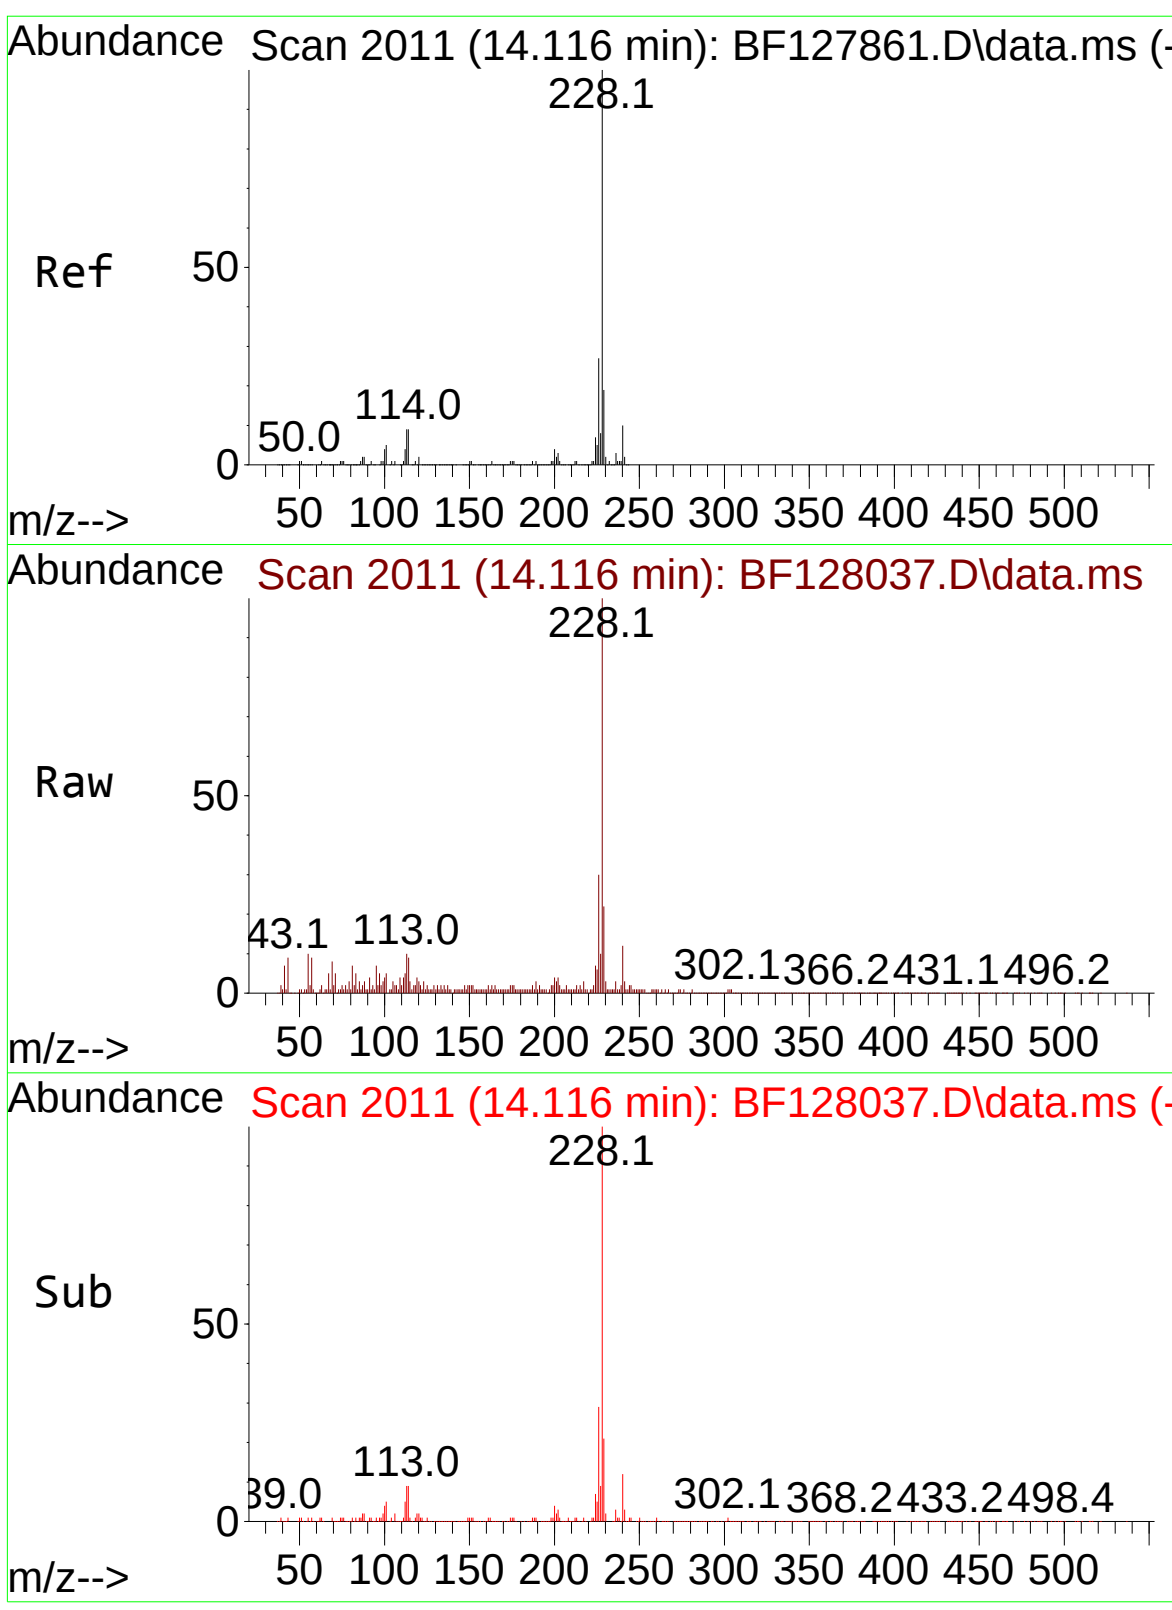

#81
Benzo(a)anthracene
Concen: 26.071 ng
RT: 14.116 min Scan# 2011
Delta R.T. 0.012 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:228 Resp: 248273

Ion	Ratio	Lower	Upper
228	100		
226	29.7	21.7	32.5
229	22.0	15.4	23.2



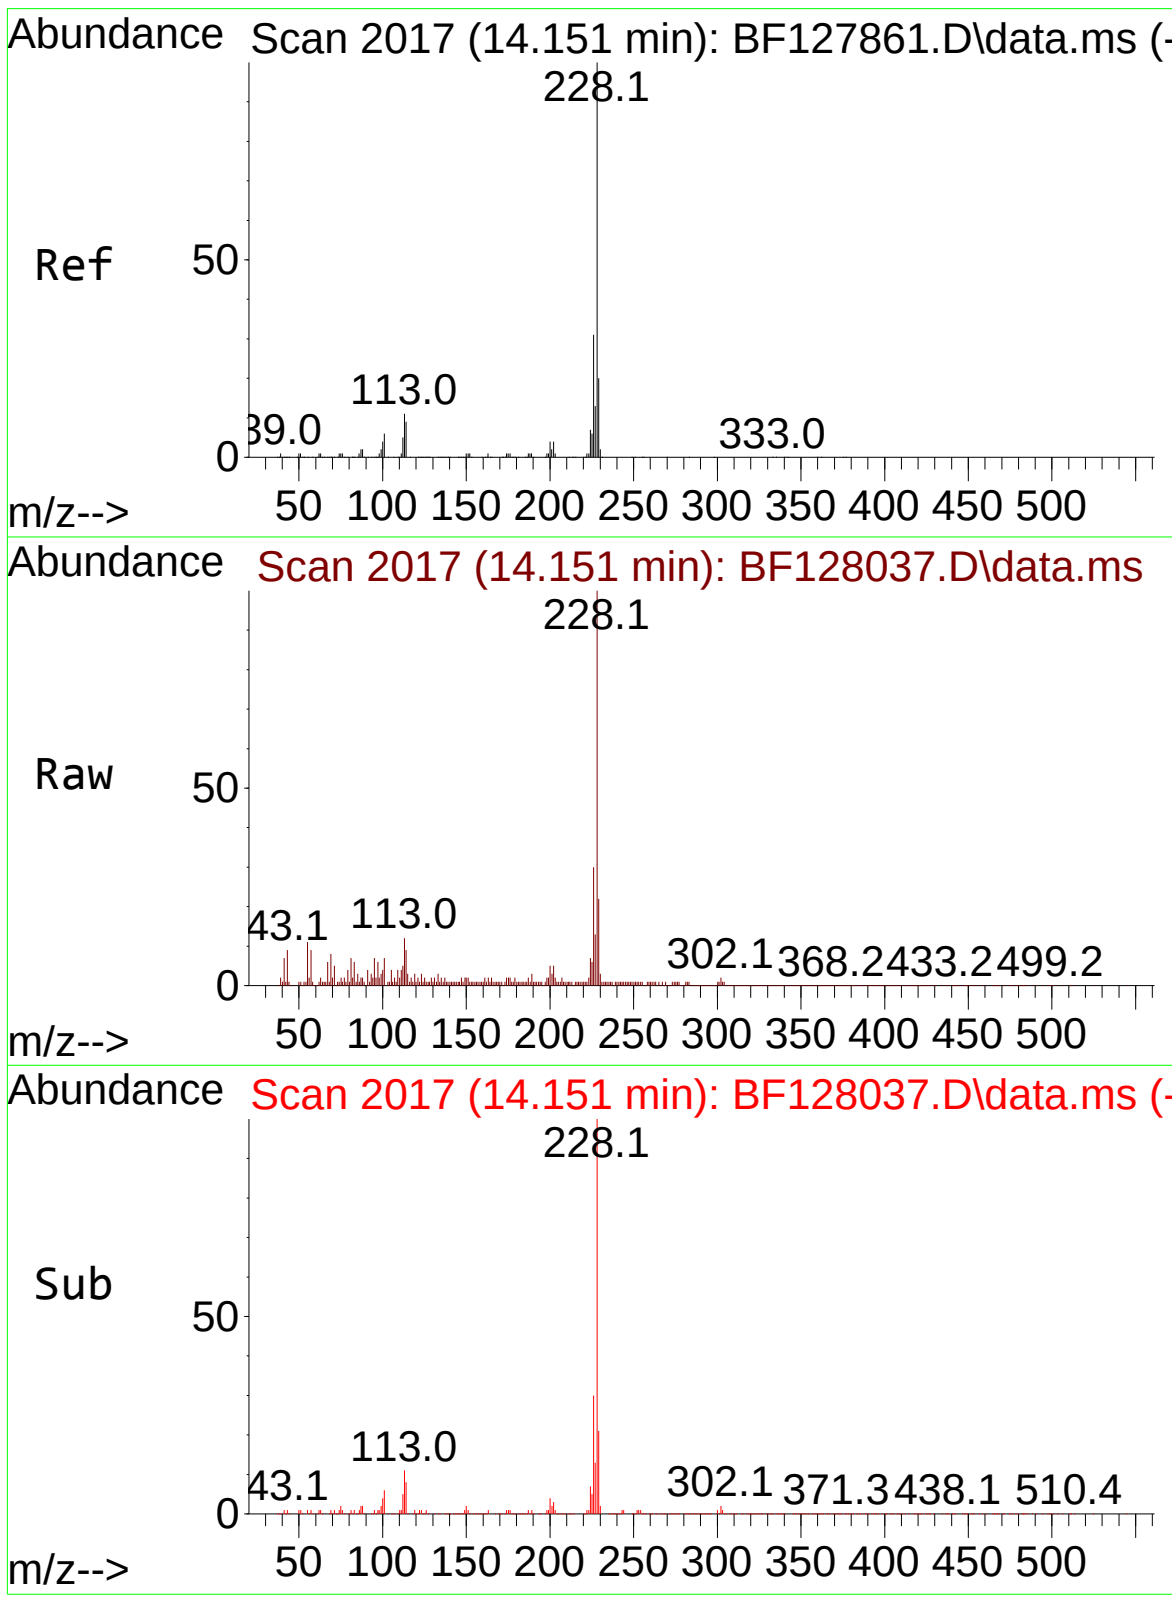

#83
Chrysene
Concen: 23.575 ng
RT: 14.151 min Scan# 2(
Delta R.T. 0.012 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Tgt Ion:228 Resp: 214405

Ion	Ratio	Lower	Upper
228	100		
226	30.4	24.4	36.6
229	21.9	15.8	23.8

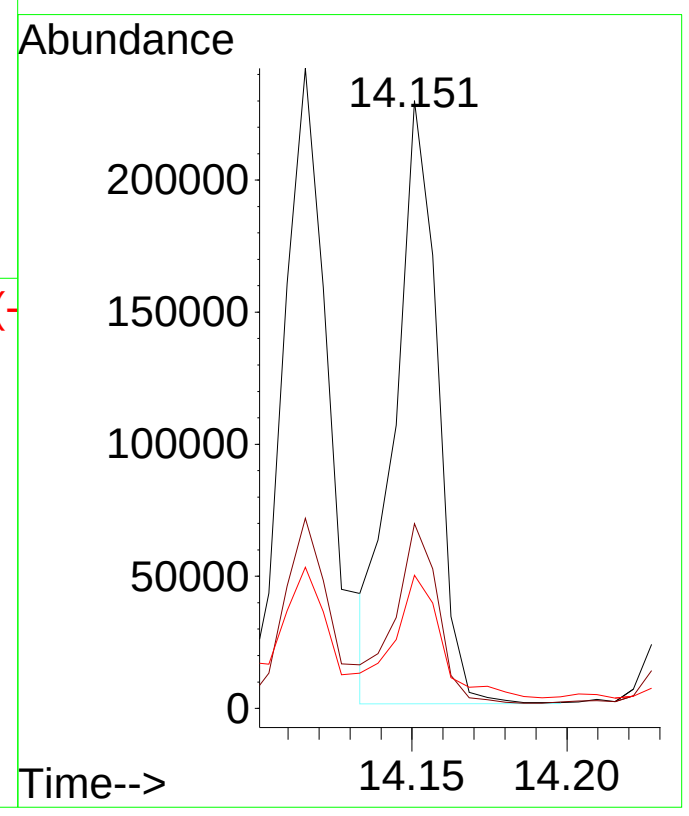

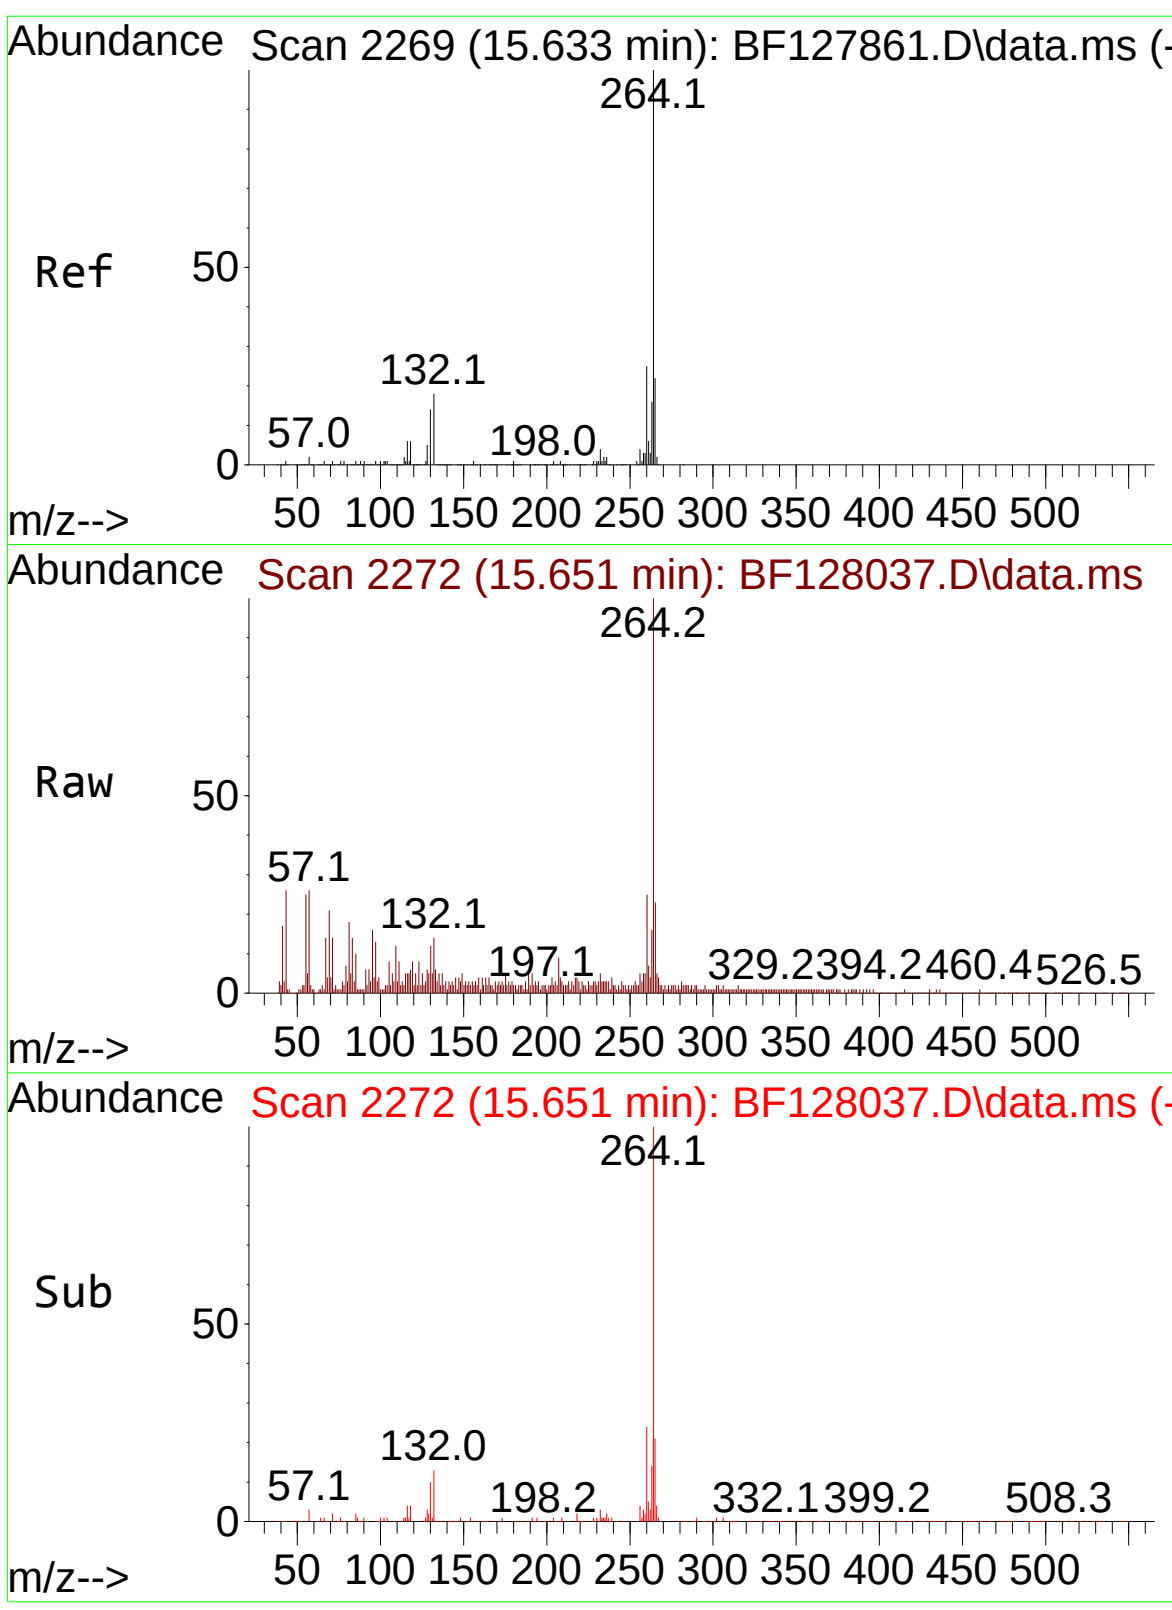

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.651 min Scan# 2272
Delta R.T. 0.029 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:264 Resp: 110797

Ion	Ratio	Lower	Upper
264	100		
260	24.8	20.1	30.1
265	22.8	17.5	26.3

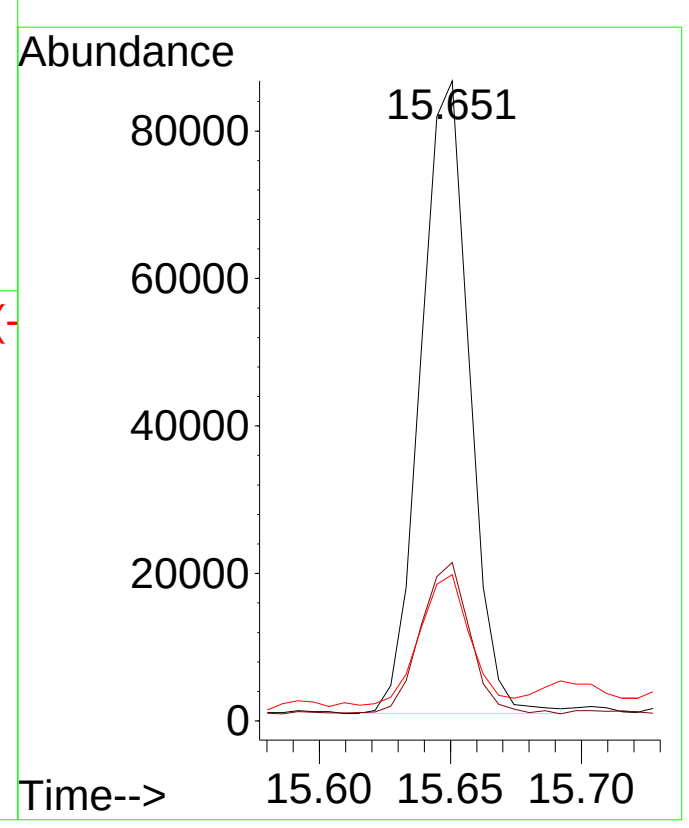

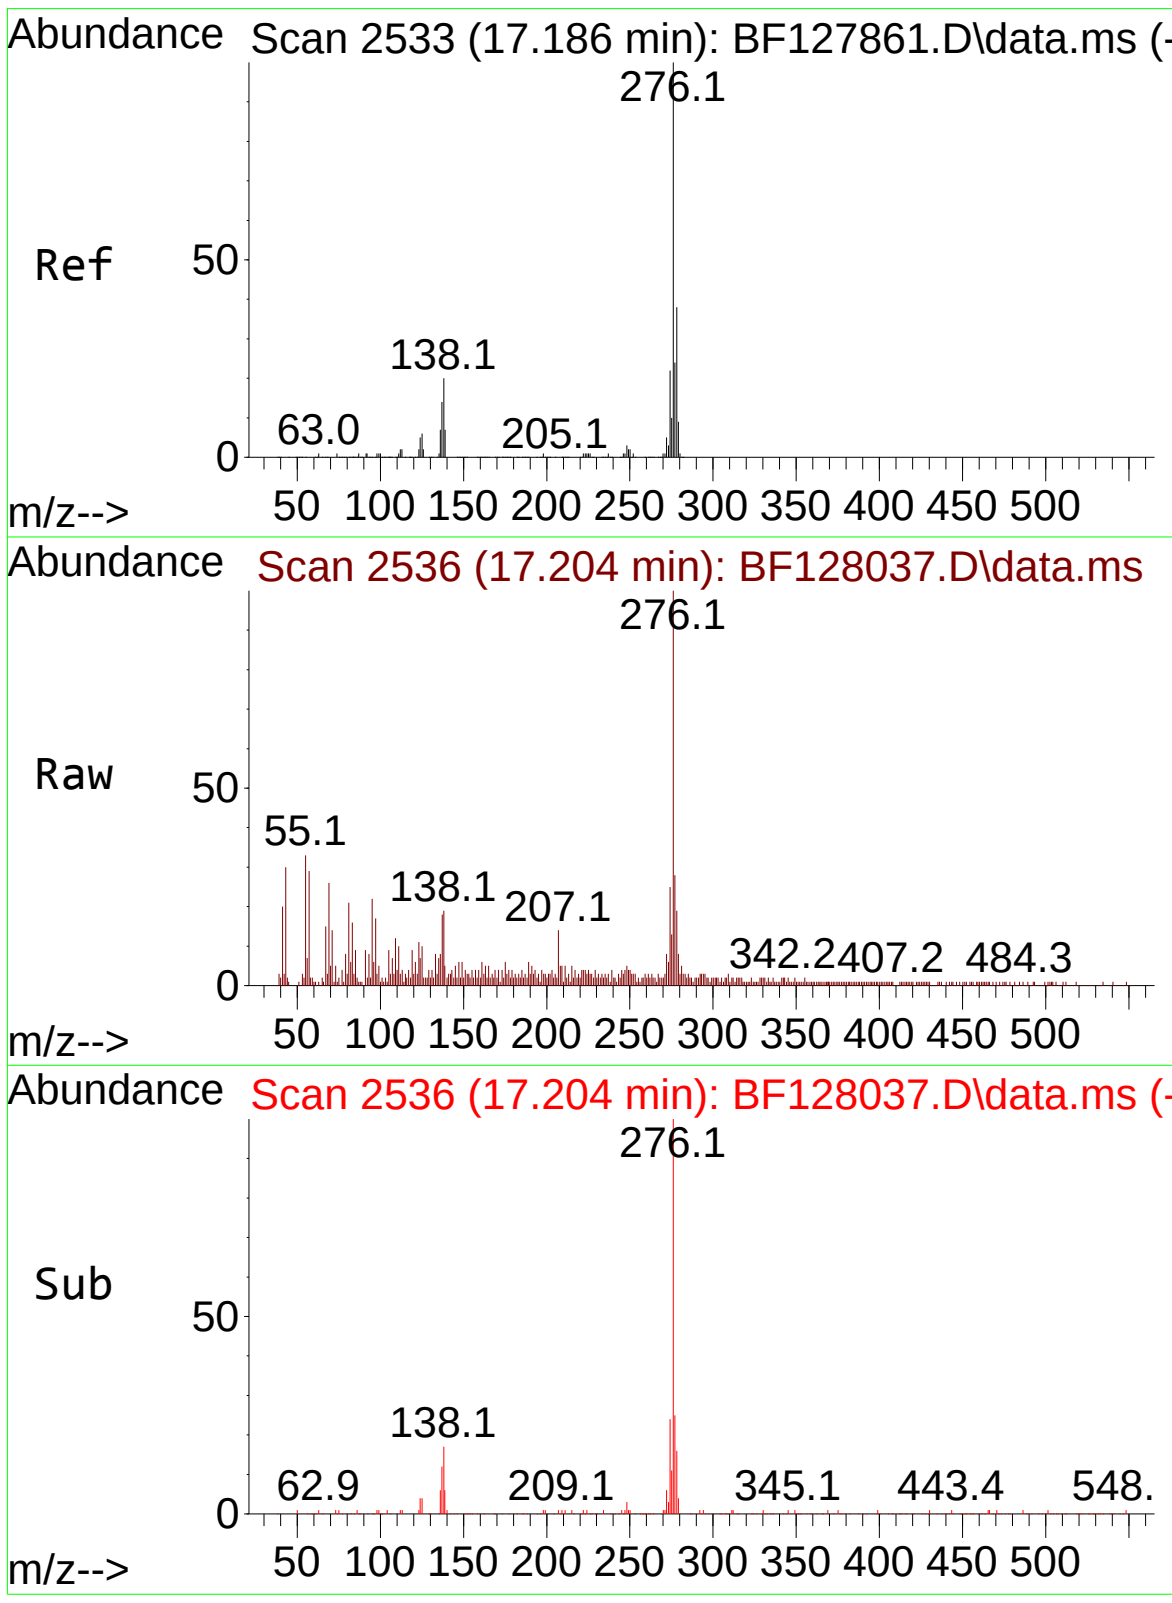

#87
Indeno(1,2,3-cd)pyrene
Concen: 13.268 ng
RT: 17.204 min Scan# 2
Delta R.T. 0.035 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Tgt Ion:276 Resp: 98125

Ion	Ratio	Lower	Upper
276	100		
138	18.4	19.0	28.4#
277	25.9	20.1	30.1



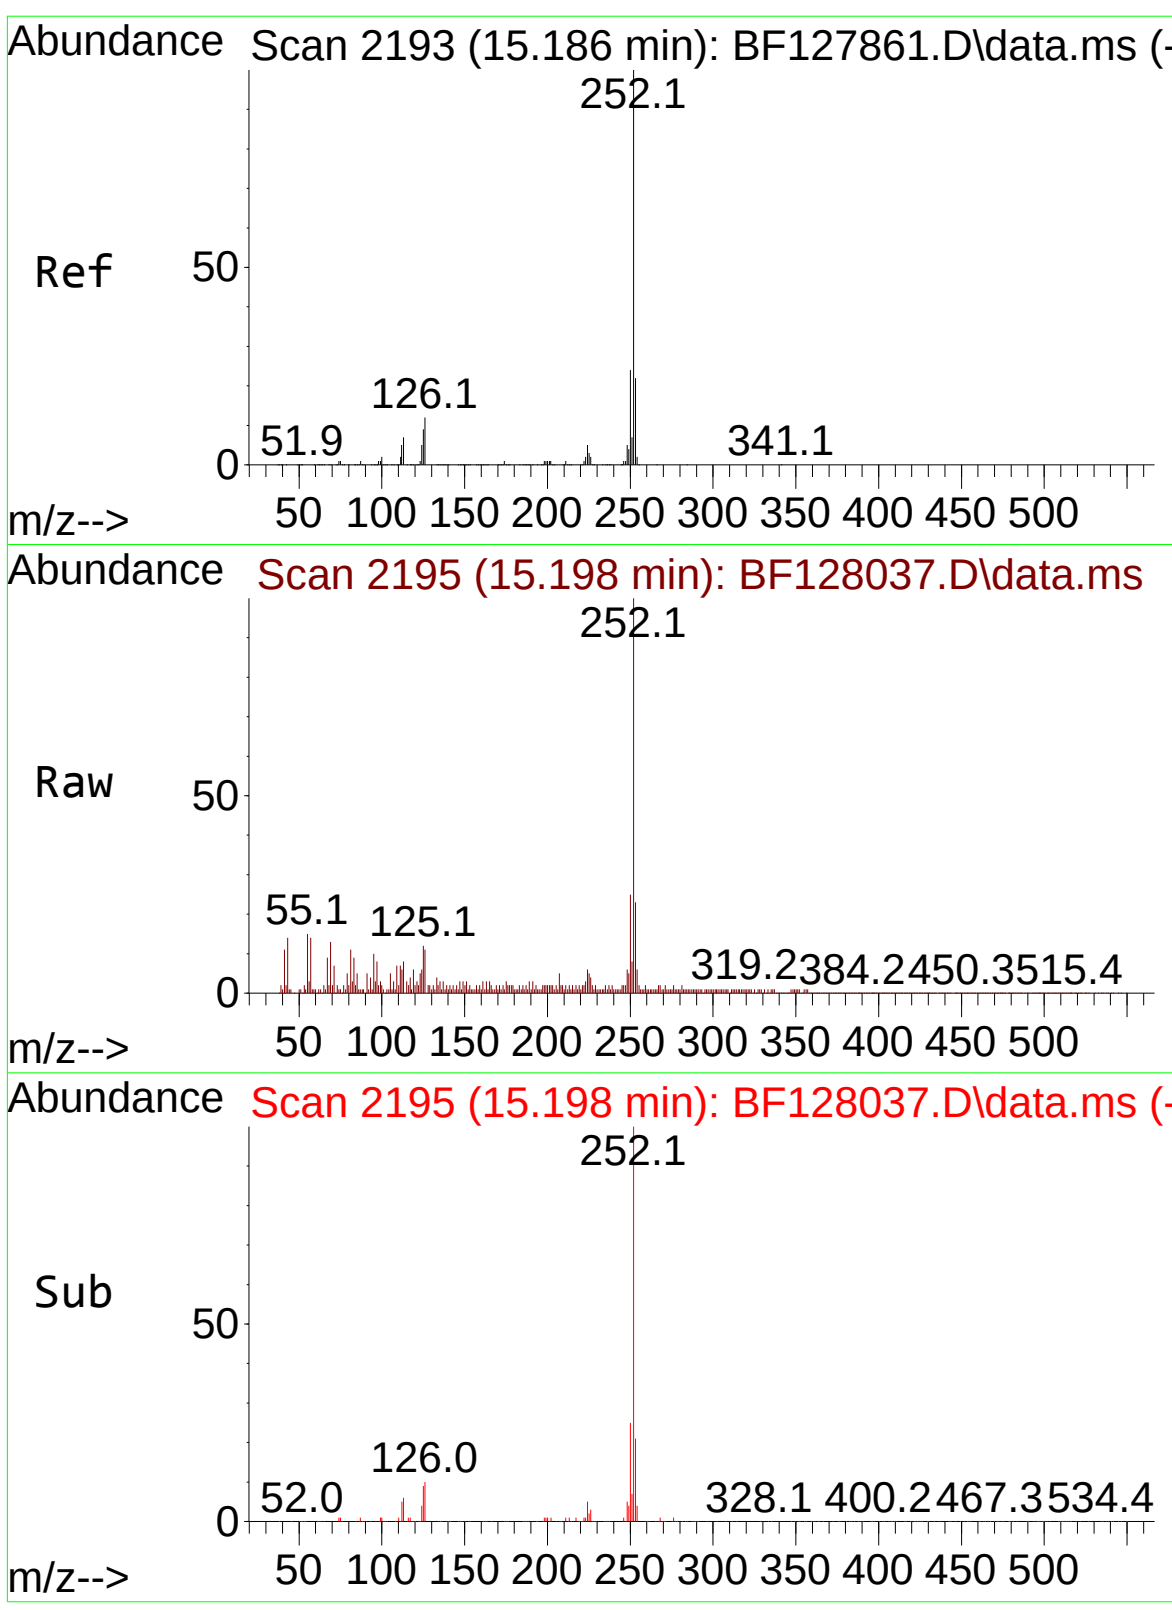

#88
Benzo(b)fluoranthene
Concen: 42.618 ng
RT: 15.198 min Scan# 2195
Delta R.T. 0.024 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:252 Resp: 296577

Ion	Ratio	Lower	Upper
252	100		
253	22.7	17.4	26.2
125	11.8	7.4	11.2#



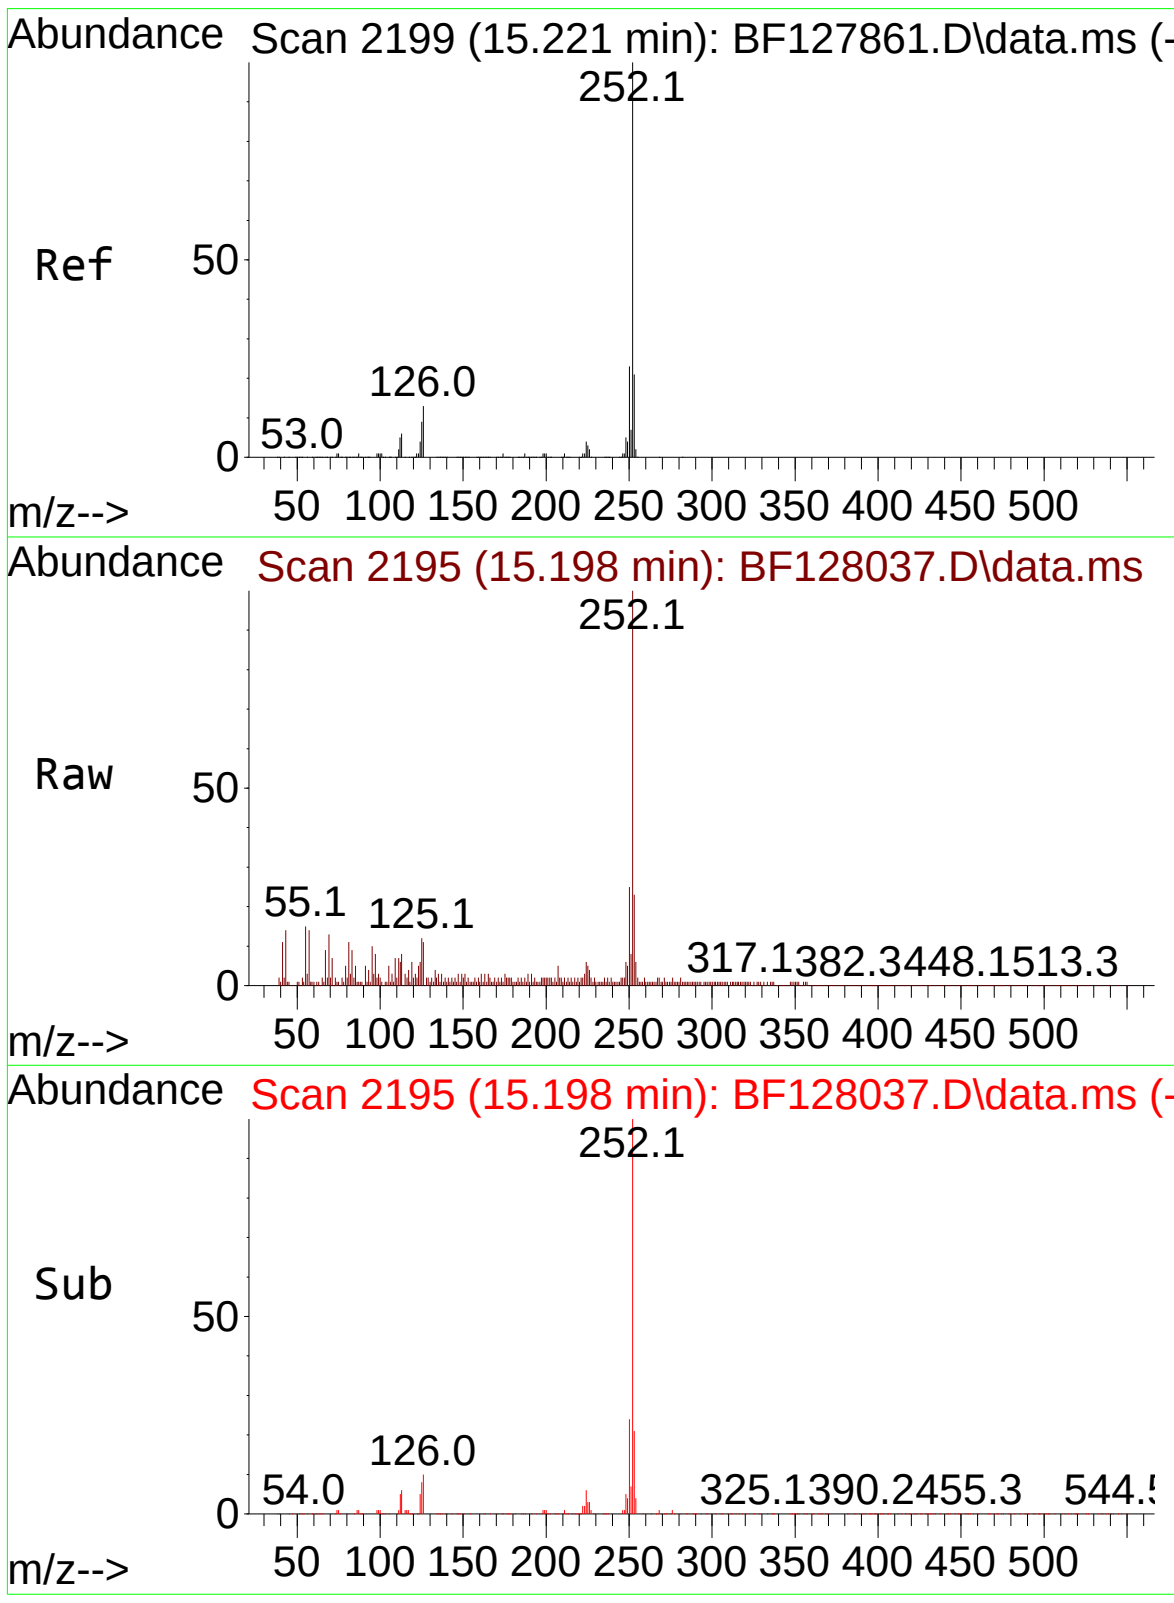

#89
Benzo(k)fluoranthene
Concen: 42.301 ng
RT: 15.198 min Scan# 2

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Delta R.T. -0.012 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:252 Resp: 296577

Ion	Ratio	Lower	Upper
252	100		
253	22.7	17.0	25.4
125	11.8	6.8	10.2#



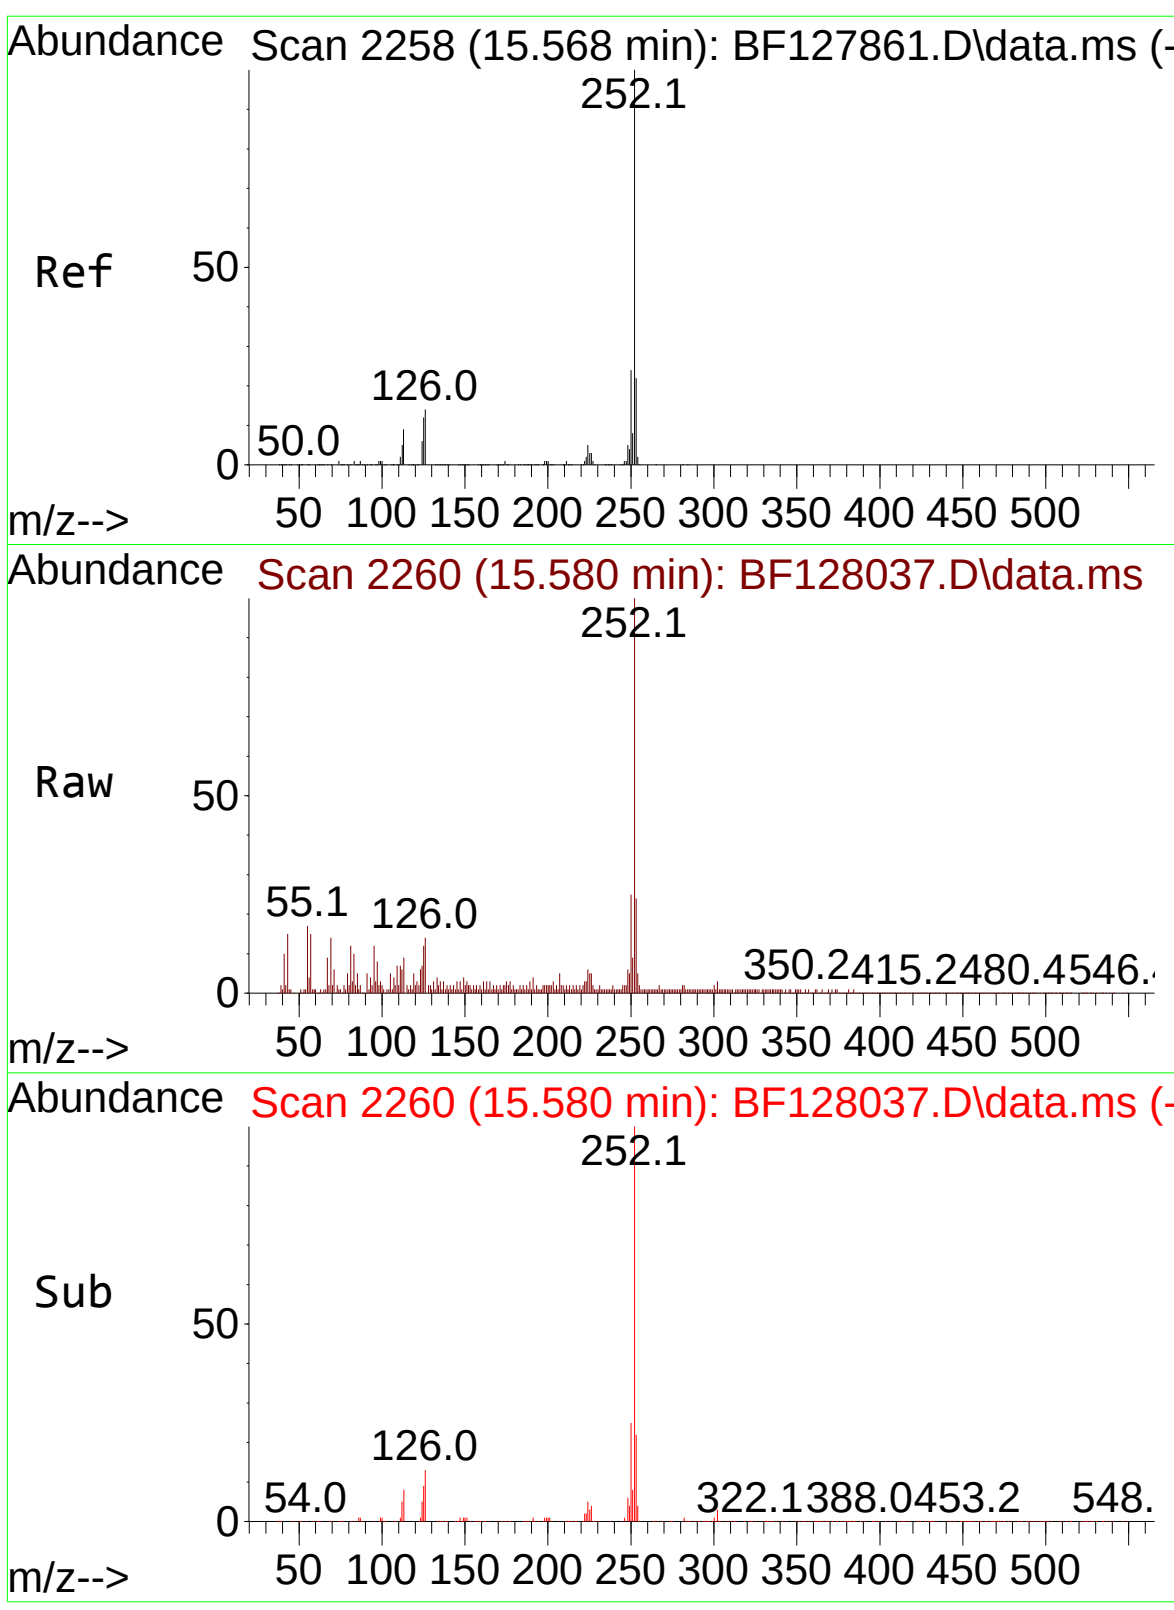

#90
Benzo(a)pyrene
Concen: 28.071 ng
RT: 15.580 min Scan# 2260
Delta R.T. 0.024 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:252 Resp: 162037

Ion	Ratio	Lower	Upper
252	100		
253	23.7	17.8	26.6
125	12.5	9.2	13.8



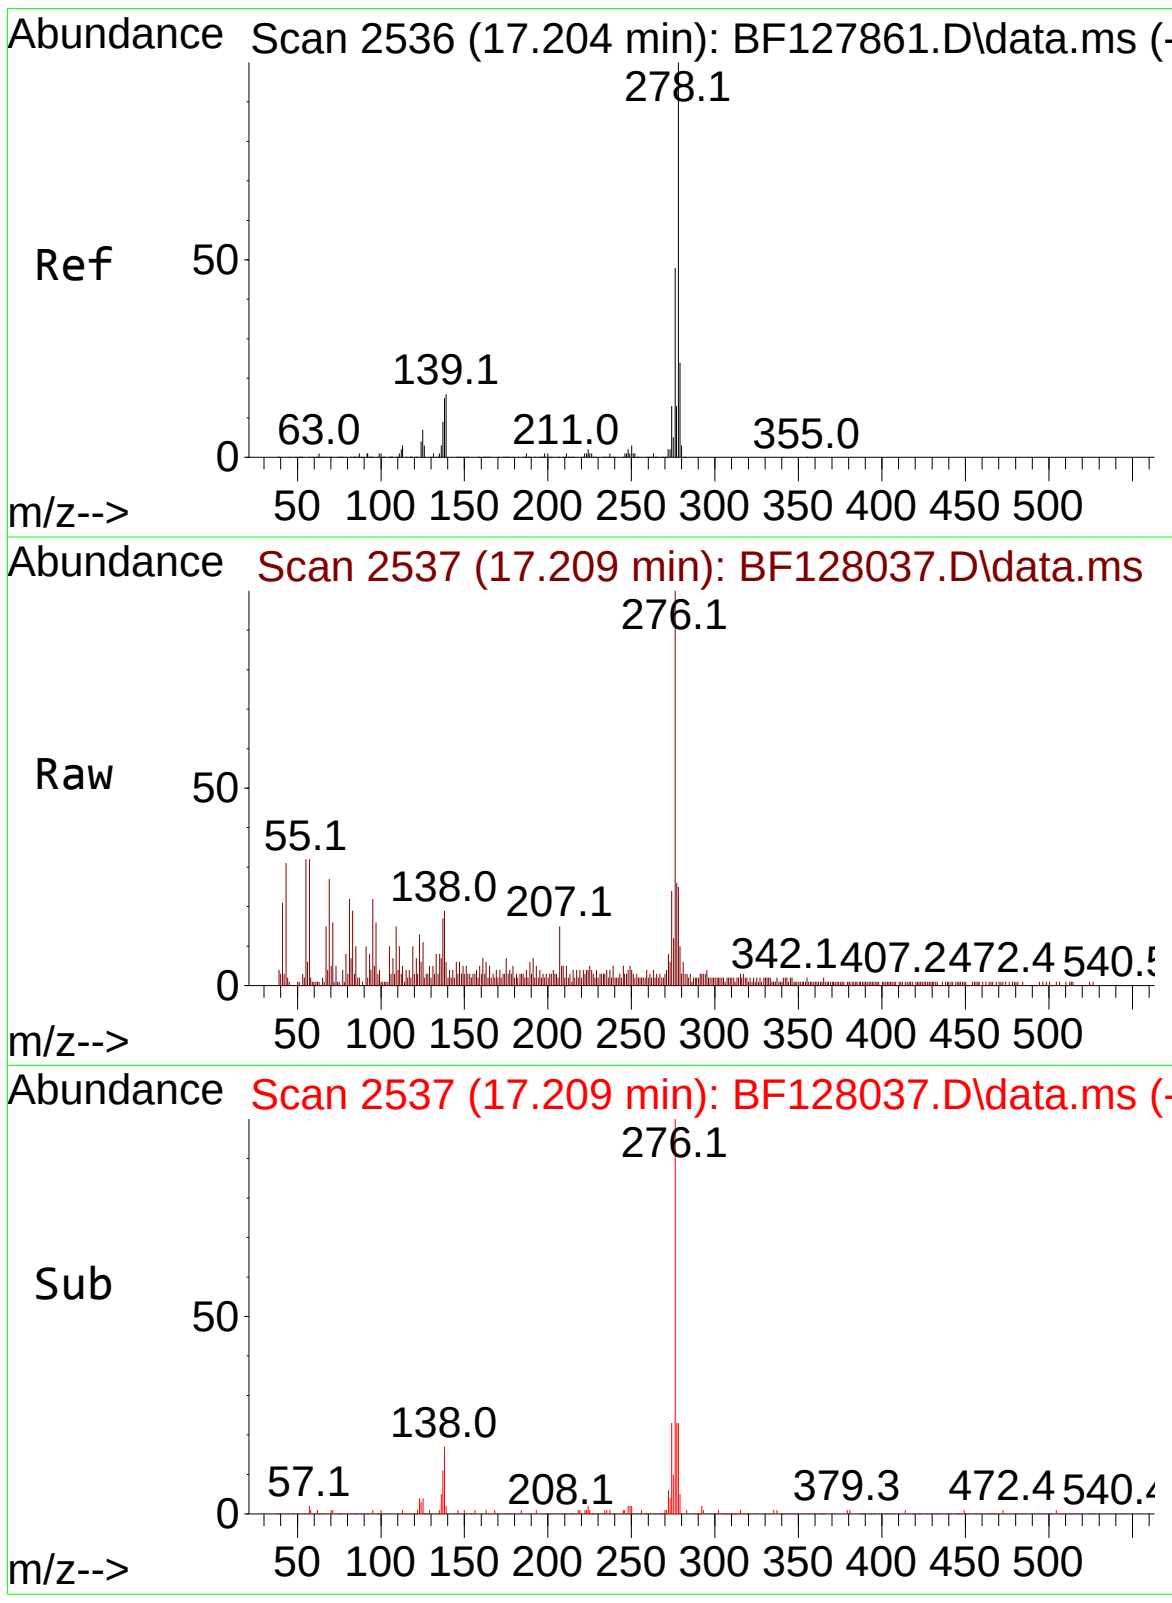

#91
Dibenzo(a,h)anthracene
Concen: 4.105 ng
RT: 17.209 min Scan# 2
Delta R.T. 0.024 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Instrument :
BNA_F
ClientSampleId :
JC-01-042822

Tgt Ion:278 Resp: 24345

Ion	Ratio	Lower	Upper
278	100		
139	25.4	12.6	19.0#
279	41.5	18.9	28.3#



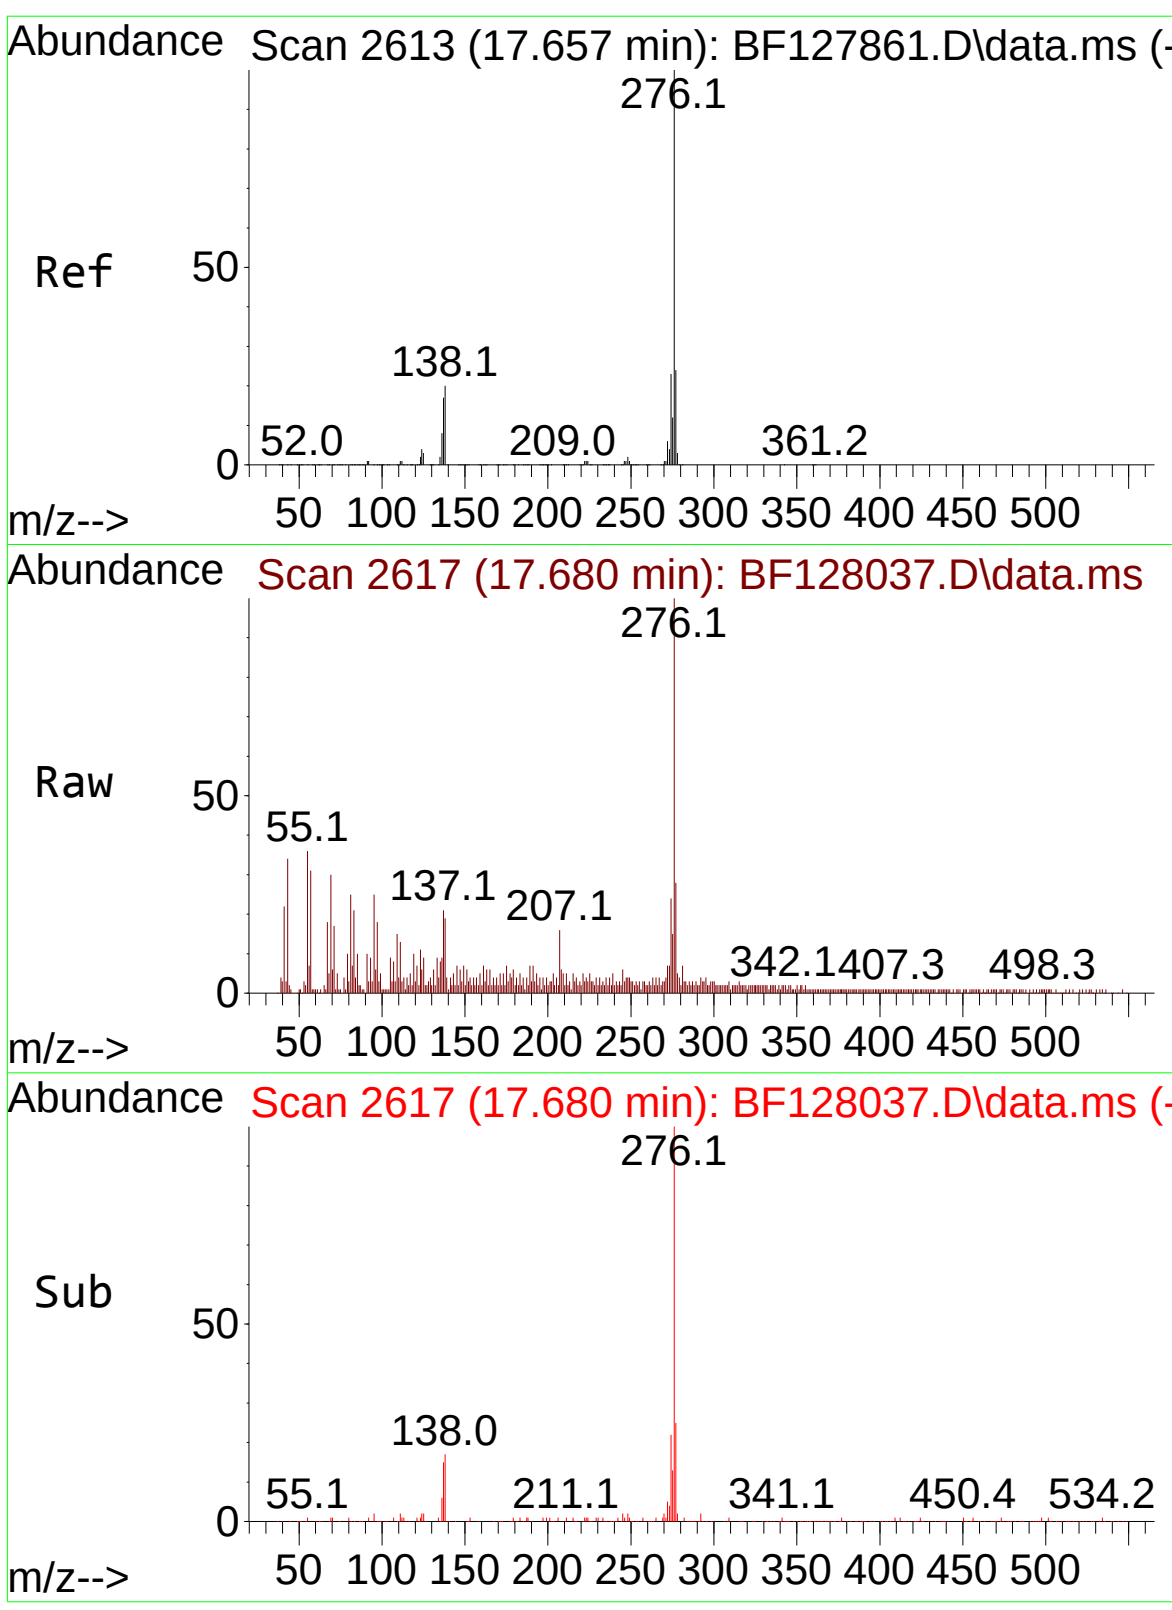

#92
Benzo(g,h,i)perylene
Concen: 16.304 ng
RT: 17.680 min Scan# 2617
Delta R.T. 0.041 min
Lab File: BF128037.D
Acq: 02 May 2022 20:34

Tgt Ion:276 Resp: 101911

Ion	Ratio	Lower	Upper
276	100		
277	28.5	18.8	28.2#
138	19.2	16.2	24.2