

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050222\
 Data File : BF128016.D
 Acq On : 02 May 2022 10:24
 Operator : CG\JU
 Sample : PB144493BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144493BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128016.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.569	553	558	561	rBV	3707141	4266165	74.71%	12.840%
2	6.563	720	727	730	rBV	3505099	4409350	77.22%	13.271%
3	6.928	785	789	792	rBV	1064677	875530	15.33%	2.635%
4	7.498	879	886	889	rBV	2374801	3082142	53.98%	9.277%
5	8.210	1001	1007	1011	rBV	1117450	1154239	20.21%	3.474%
6	9.292	1183	1191	1194	rBV	4707993	5330800	93.36%	16.044%
7	9.974	1300	1307	1310	rBV	1340397	1341627	23.50%	4.038%
8	10.769	1434	1442	1445	rBV	3302036	3401959	59.58%	10.239%
9	11.469	1554	1561	1564	rBV	1494492	1424012	24.94%	4.286%
10	13.063	1823	1832	1835	rBV	4889975	5710183	100.00%	17.186%
11	14.115	2007	2011	2014	rBV	1379286	1211293	21.21%	3.646%
12	15.627	2263	2268	2277	rBV	746019	1017876	17.83%	3.064%


Sum of corrected areas: 33225176

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050222\
Data File : BF128016.D
Acq On : 02 May 2022 10:24
Operator : CG\JU
Sample : PB144493BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144493BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

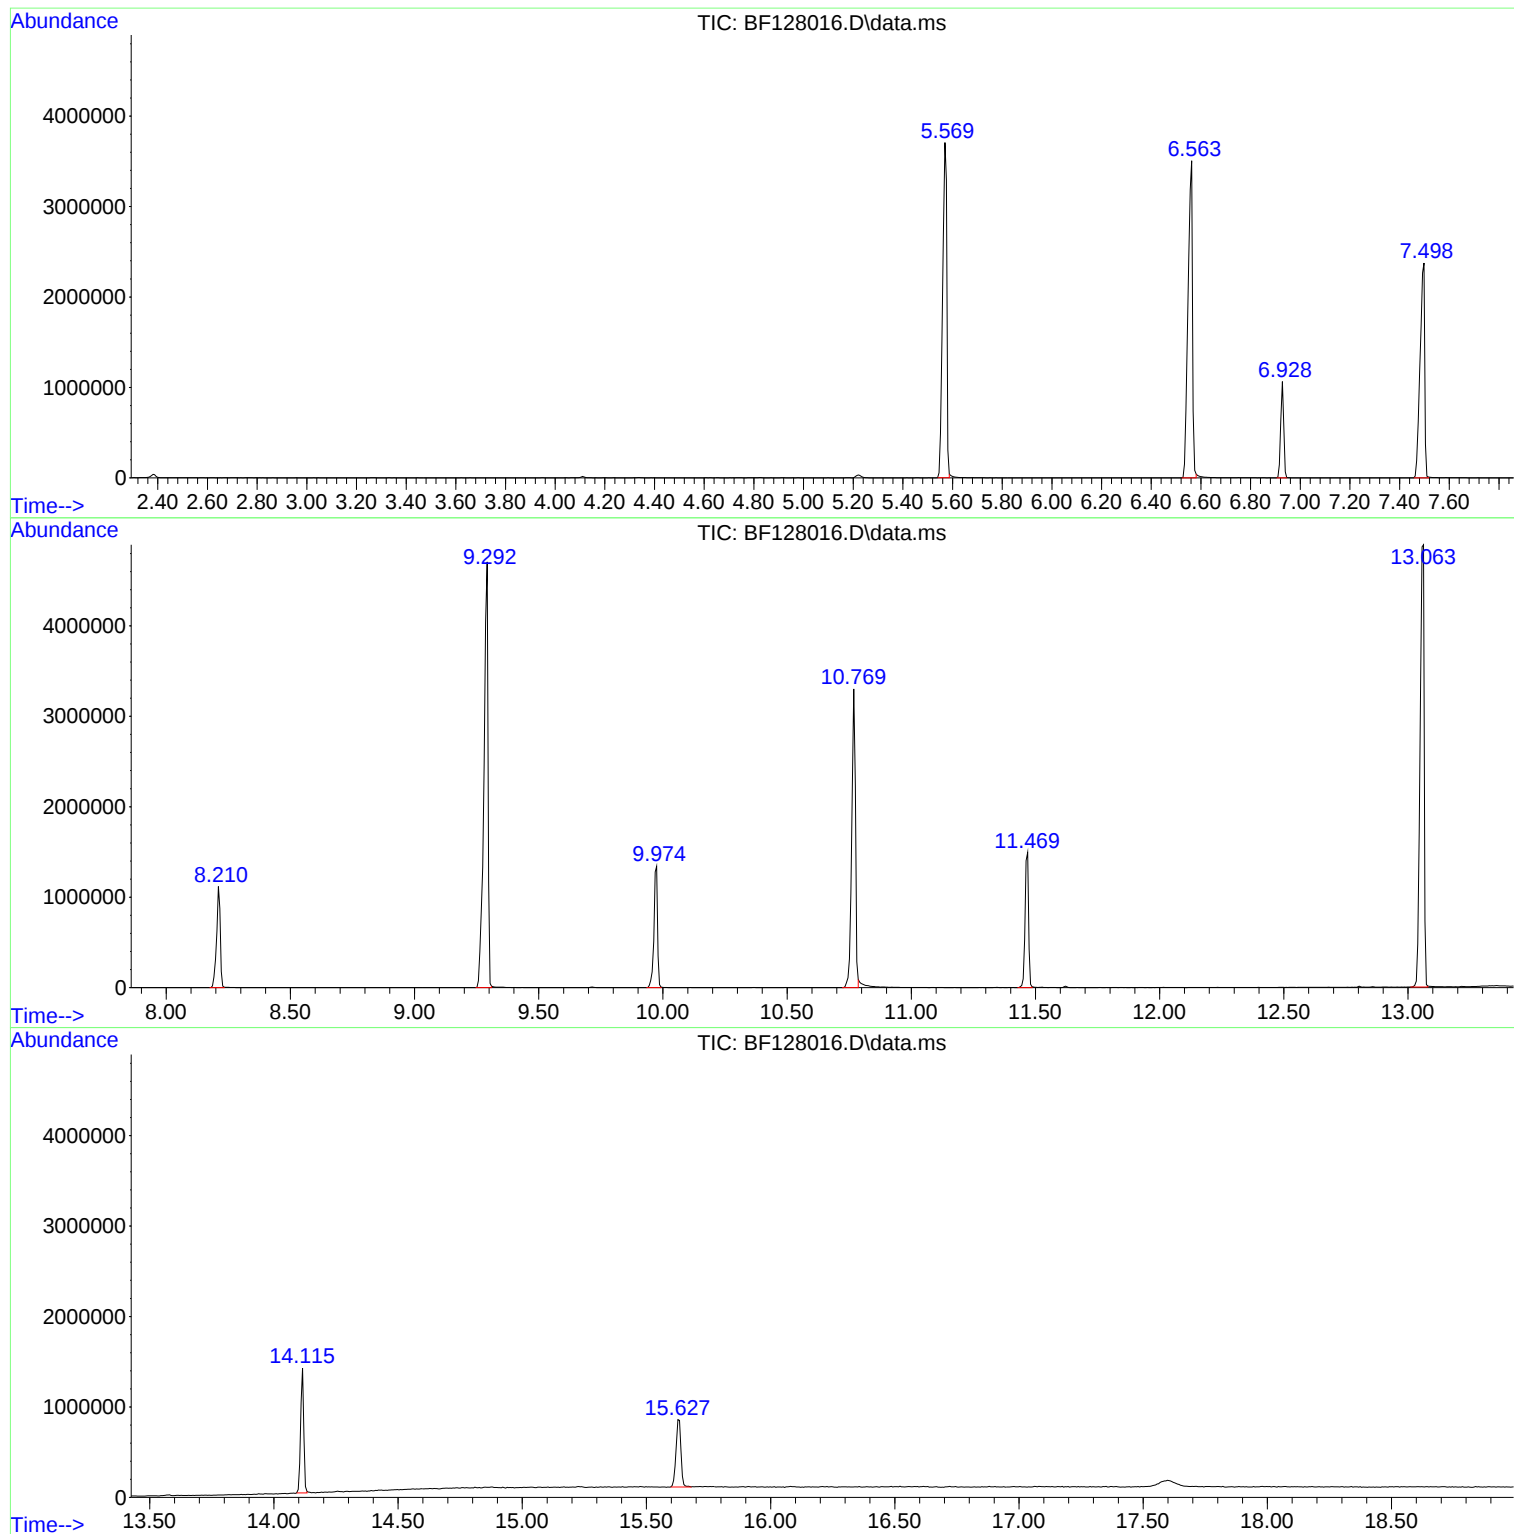

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050222\
Data File : BF128016.D
Acq On : 02 May 2022 10:24
Operator : CG\JU
Sample : PB144493BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144493BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050222\
Data File : BF128016.D
Acq On : 02 May 2022 10:24
Operator : CG\JU
Sample : PB144493BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144493BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------