
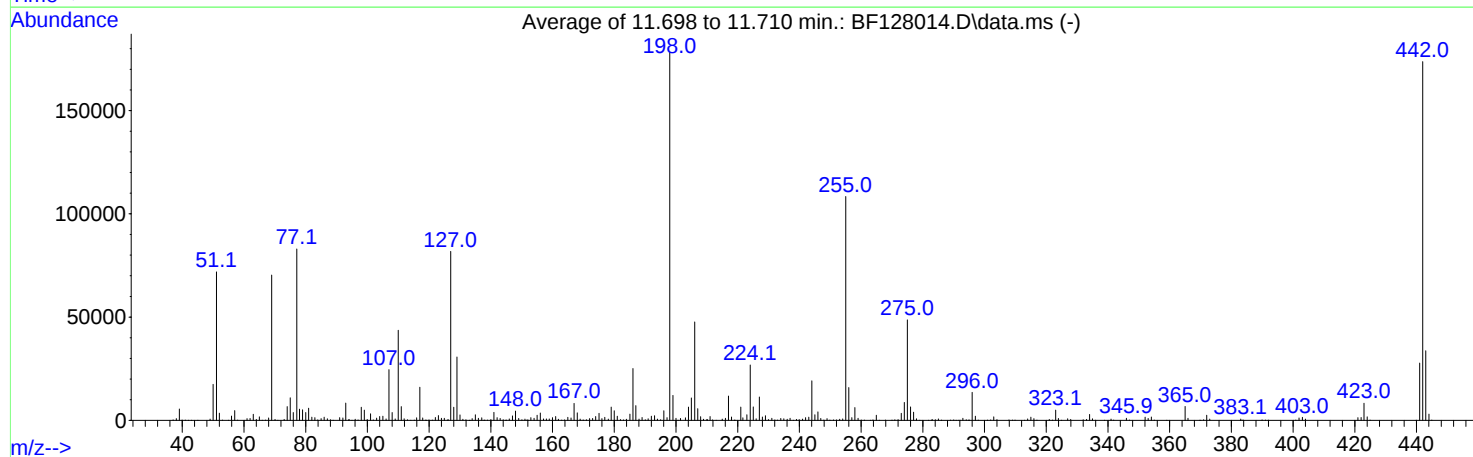


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050222\
 Data File : BF128014.D
 Acq On : 02 May 2022 09:27
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 04 04:23:29 2022

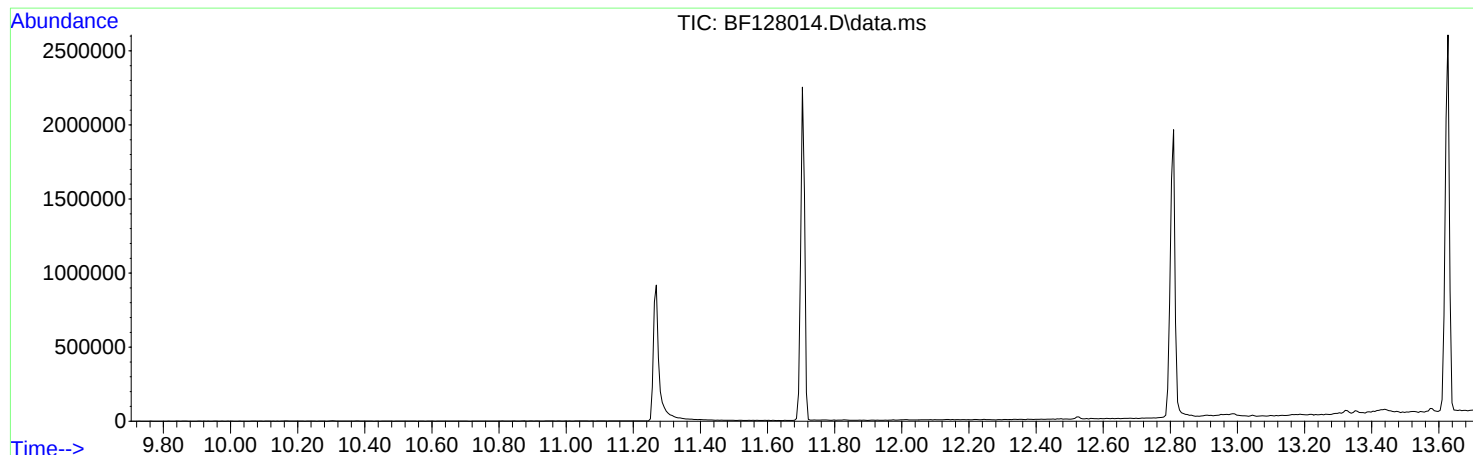

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	71901	PASS
68	69	0.00	2	1.6	1144	PASS
69	198	0.00	100	39.5	70372	PASS
70	69	0.00	2	0.6	442	PASS
127	198	10	80	45.9	81797	PASS
197	198	0.00	2	0.8	1341	PASS
198	198	100	100	100.0	178117	PASS
199	198	5	9	6.8	12095	PASS
275	198	10	60	27.3	48656	PASS
365	198	1	100	3.8	6718	PASS
441	198	0.01	100	15.6	27746	PASS
442	442	50	100	100.0	173717	PASS
443	442	15	24	19.4	33691	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
5/2/2022	BNA_F	<u>BF128014.D</u>
Compound Name	Response	Retention Time
DDT	420276	13.62
DDD	4182	13.32
DDE	1502	12.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5684	425960	1.33

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050222\
Data File : BF128014.D
Acq On : 02 May 2022 09:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 02 14:50:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 05:13:03 2022
Response via : Initial Calibration

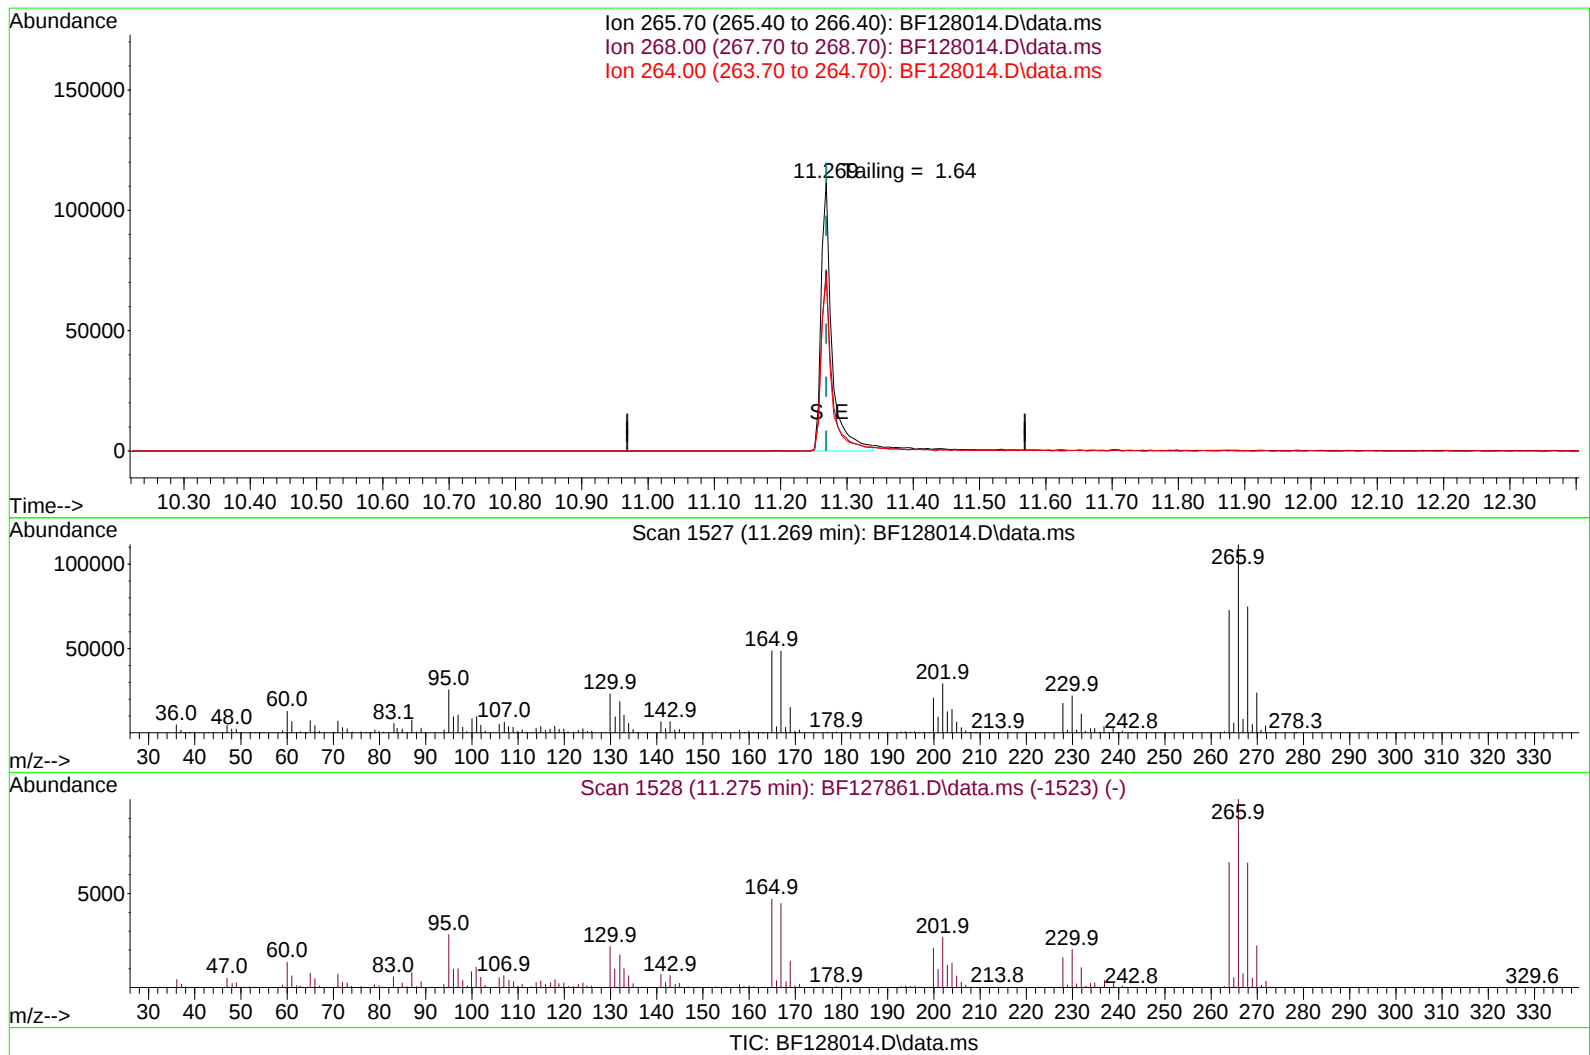

(70) Pentachlorophenol (C)

11.269min (+ 0.000) 28075.29 ng




response 132336

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	67.01
264.00	66.40	65.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050222\
Data File : BF128014.D
Acq On : 02 May 2022 09:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 02 14:50:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 05:13:03 2022
Response via : Initial Calibration

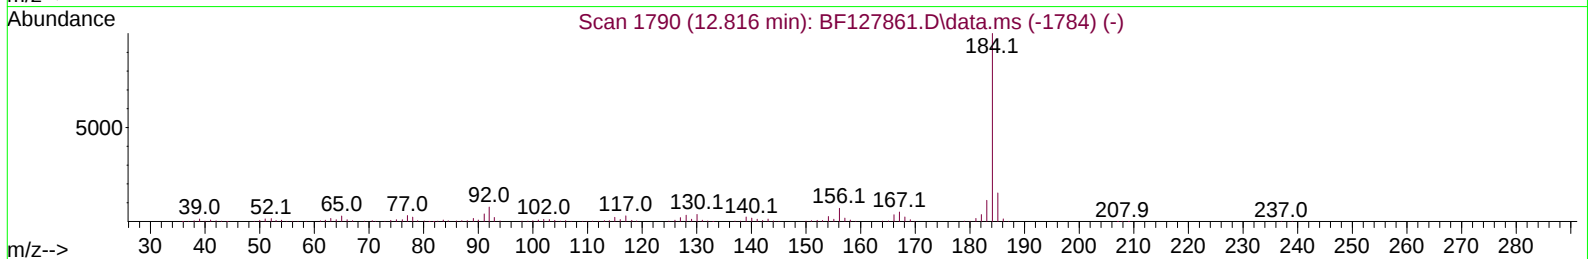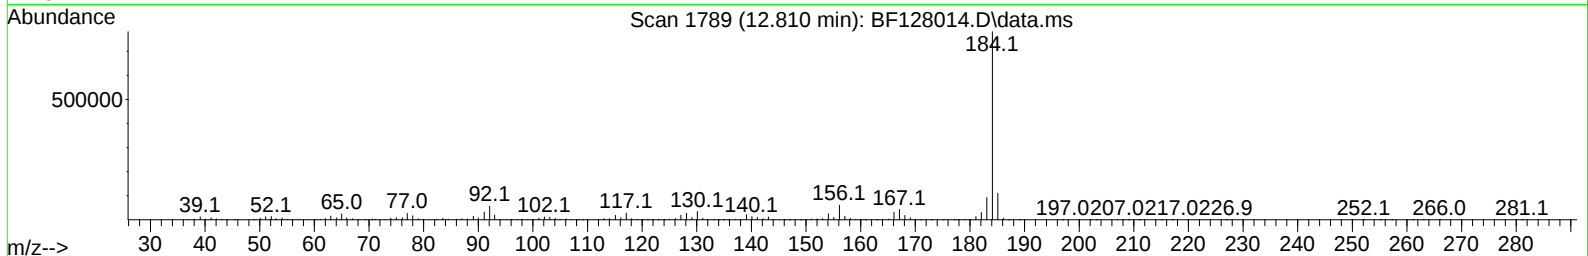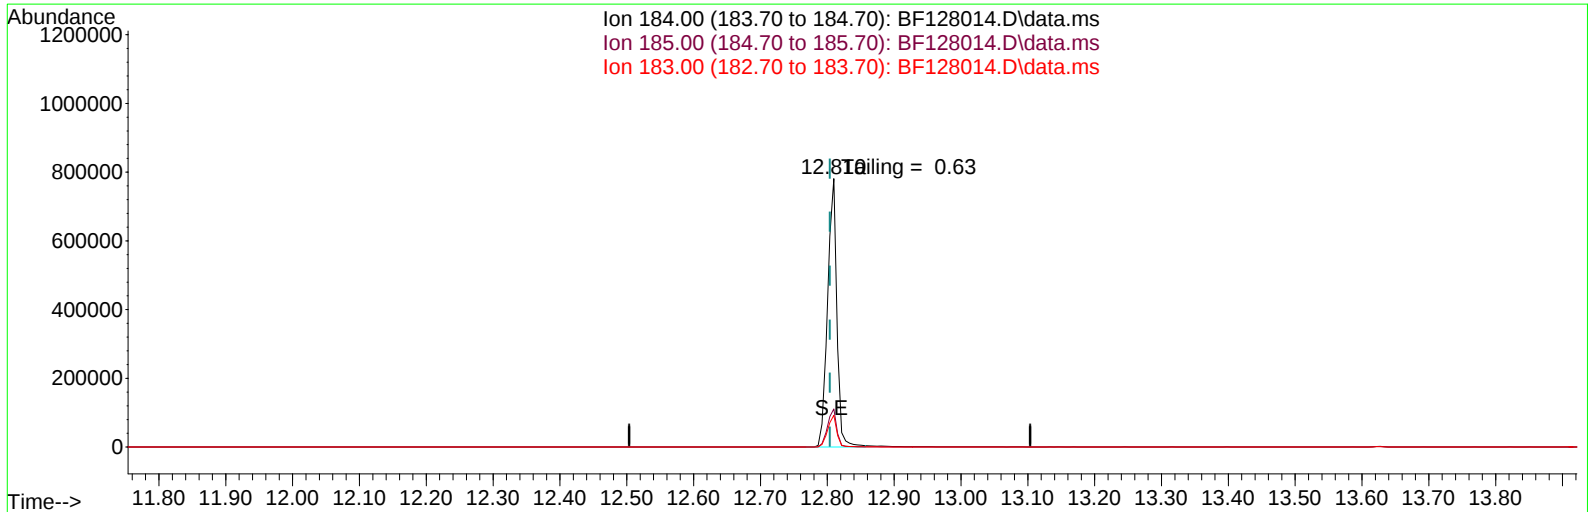

TIC: BF128014.D\data.ms

(77) Benzidine

12.810min (+ 0.006) 65261.99 ng

response 761903

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.19
183.00	11.20	11.83
0.00	0.00	0.00