
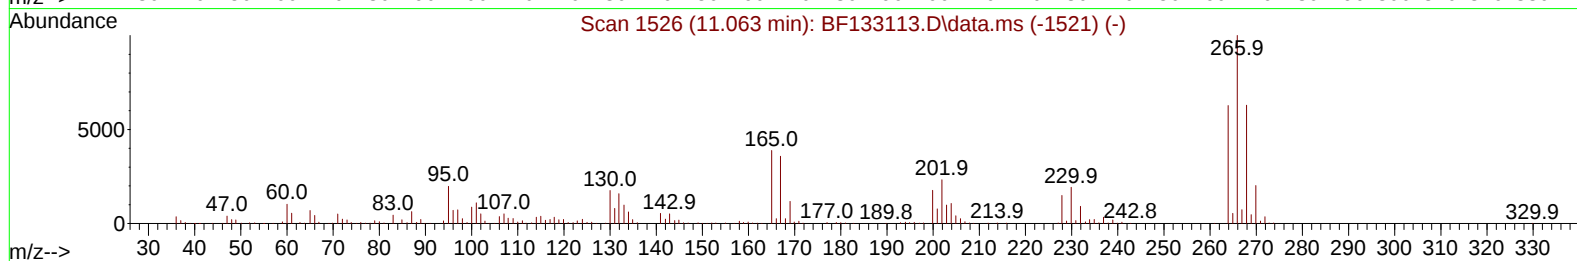
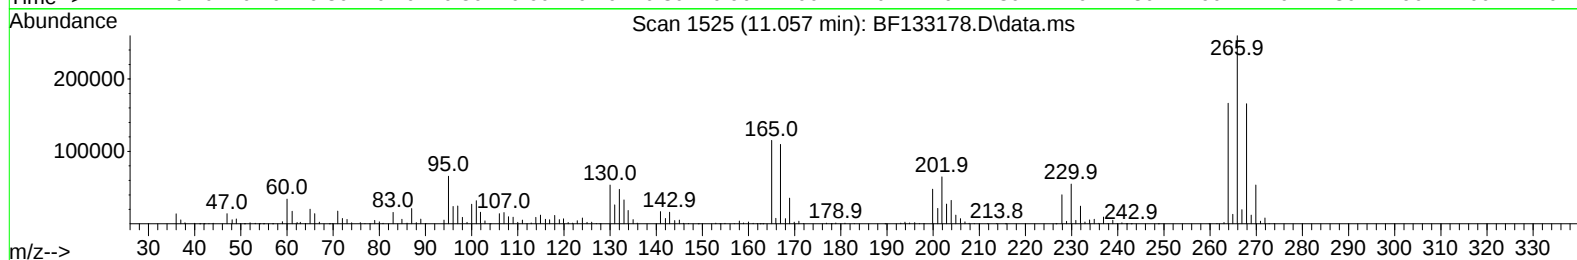


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050223\
Data File : BF133178.D
Acq On : 02 May 2023 09:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 11:10:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 02 10:52:52 2023
Response via : Initial Calibration

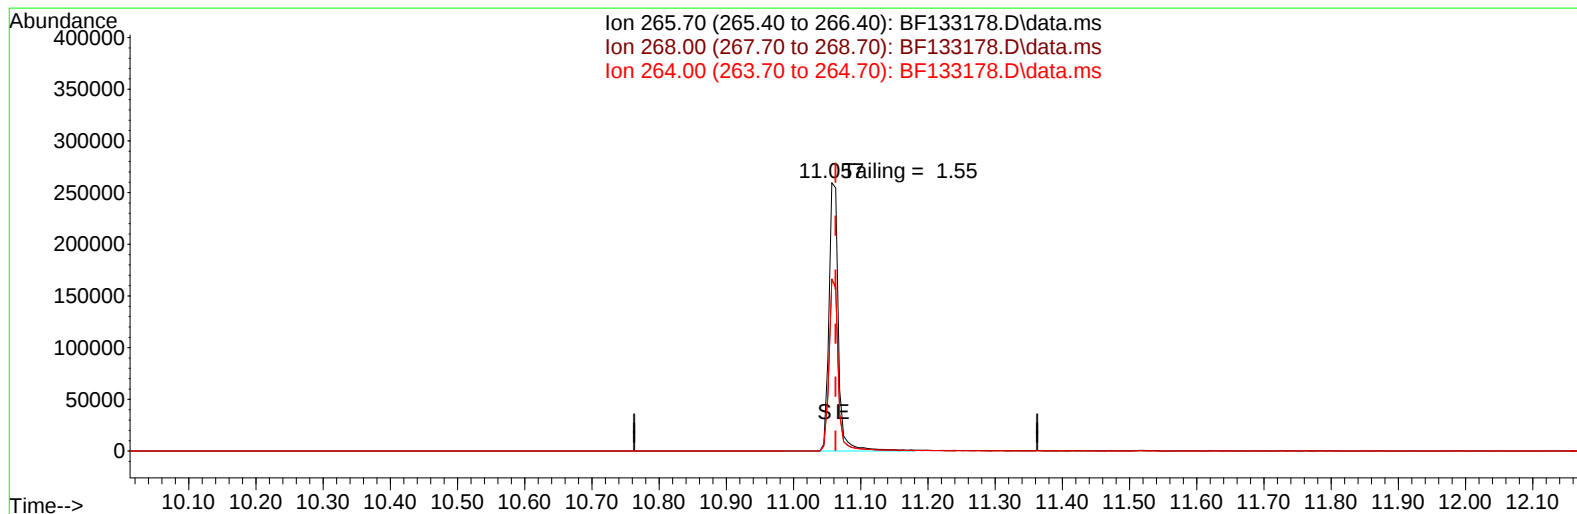

TIC: BF133178.D\data.ms

(70) Pentachlorophenol (C)




11.057min (-0.006) 90911.68 ng

response 255441

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.84
264.00	63.30	64.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050223\
Data File : BF133178.D
Acq On : 02 May 2023 09:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 04:59:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 04:52:44 2023
Response via : Initial Calibration

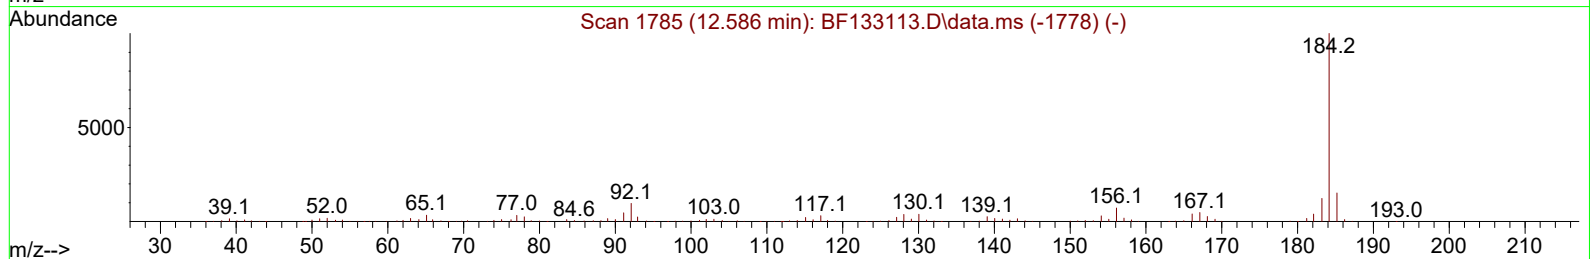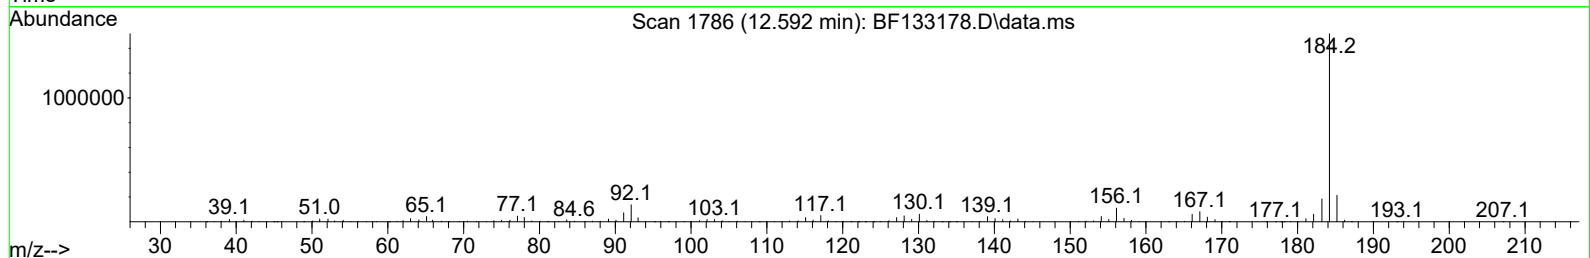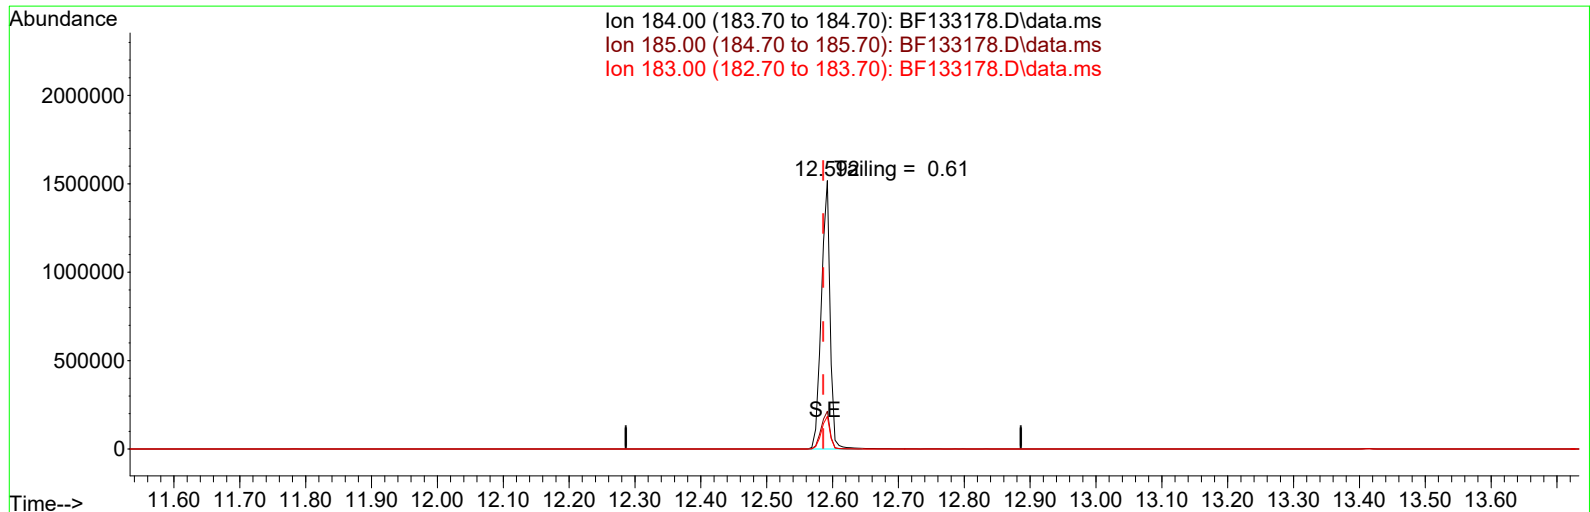

TIC: BF133178.D\data.ms

(77) Benzidine

12.592min (+ 0.006) 174450.67 ng

response 1401275

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.07#
183.00	11.70	12.19
0.00	0.00	0.00