

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050223\
 Data File : BF133180.D
 Acq On : 02 May 2023 10:24
 Operator : CG\JU
 Sample : PB152505BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB152505BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133180.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.957	484	488	494	rVB	77304	110096	1.52%	0.242%
2	5.357	550	556	559	rBV	5745949	6268253	86.81%	13.762%
3	6.375	723	729	732	rBV	5038098	6466429	89.55%	14.197%
4	6.734	786	790	793	rBV	1471979	1284134	17.78%	2.819%
5	7.298	880	886	889	rBV	4184418	4245102	58.79%	9.320%
6	8.016	1003	1008	1011	rBV	2283145	1751281	24.25%	3.845%
7	9.092	1185	1191	1194	rBV	6594024	6861627	95.02%	15.065%
8	9.769	1302	1306	1309	rBV	2294336	1962993	27.18%	4.310%
9	10.557	1435	1440	1443	rBV	4175538	4216743	58.40%	9.258%
10	11.251	1554	1558	1561	rBV	2424219	1993262	27.60%	4.376%
11	12.845	1823	1829	1832	rBV	6419200	7220982	100.00%	15.854%
12	13.886	2001	2006	2009	rBV	1847109	1704347	23.60%	3.742%
13	15.304	2242	2247	2252	rBV	1250768	1462371	20.25%	3.211%




Sum of corrected areas: 45547620

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050223\
Data File : BF133180.D
Acq On : 02 May 2023 10:24
Operator : CG\JU
Sample : PB152505BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB152505BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

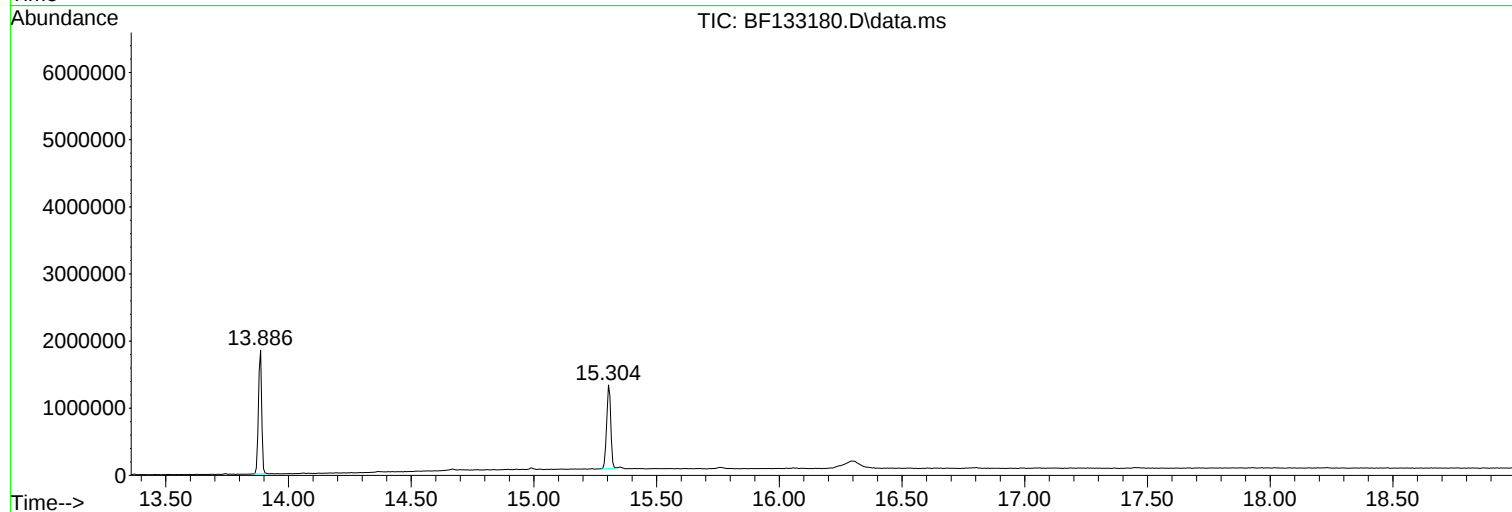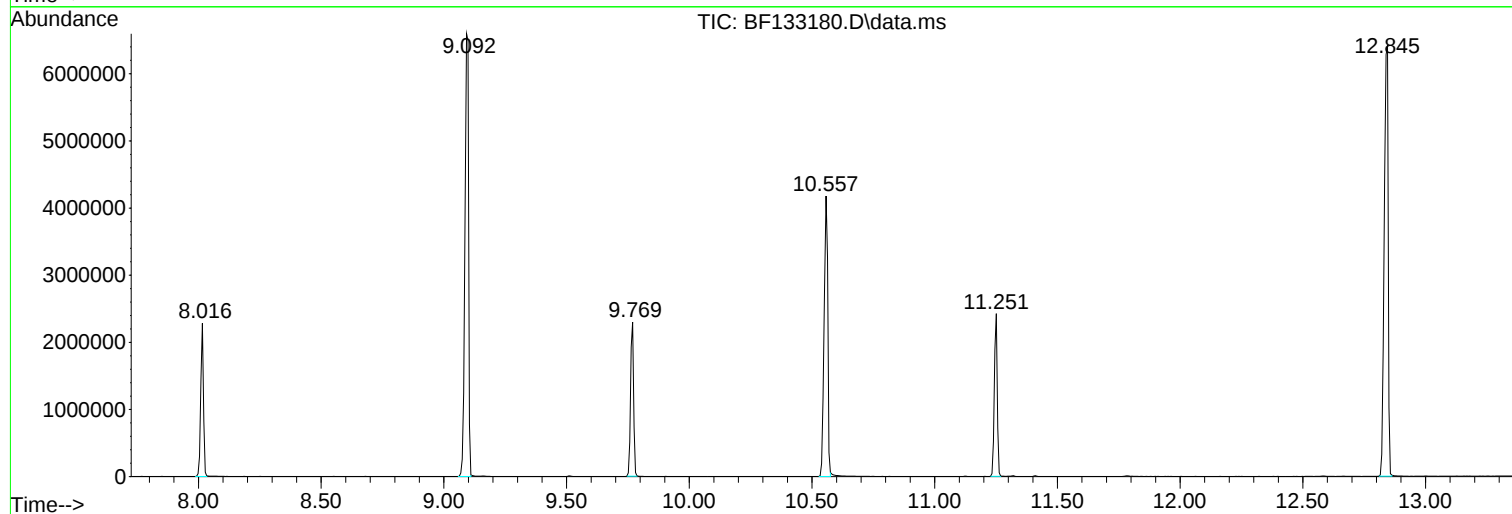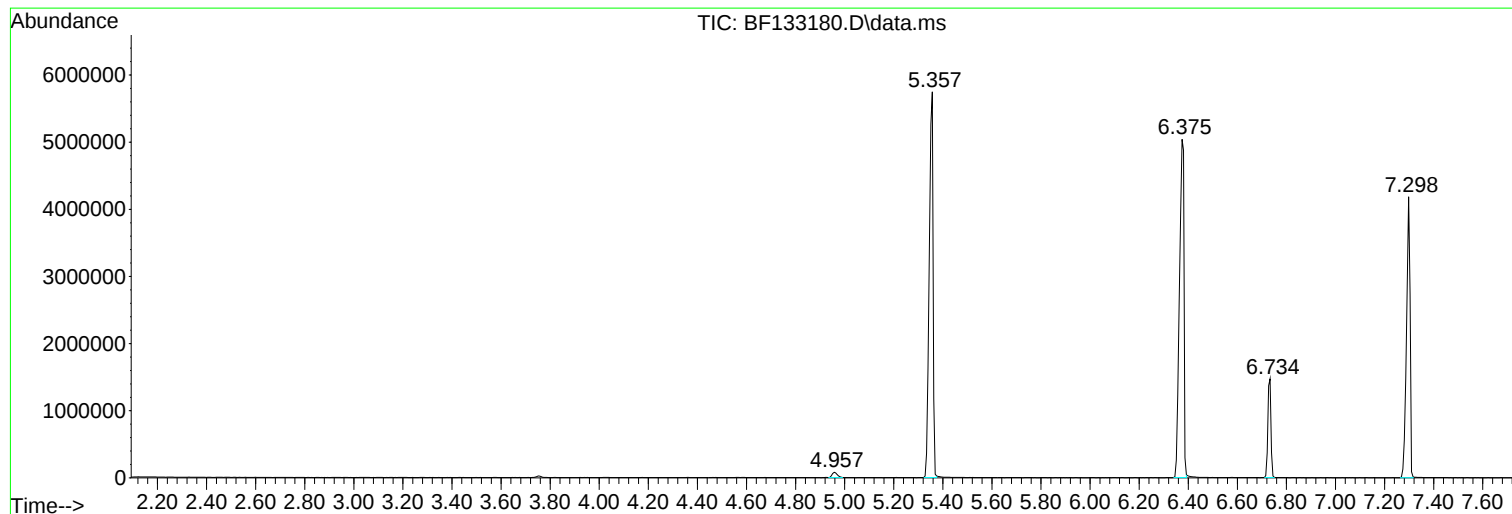

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050223\
Data File : BF133180.D
Acq On : 02 May 2023 10:24
Operator : CG\JU
Sample : PB152505BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB152505BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050223\
Data File : BF133180.D
Acq On : 02 May 2023 10:24
Operator : CG\JU
Sample : PB152505BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB152505BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------