
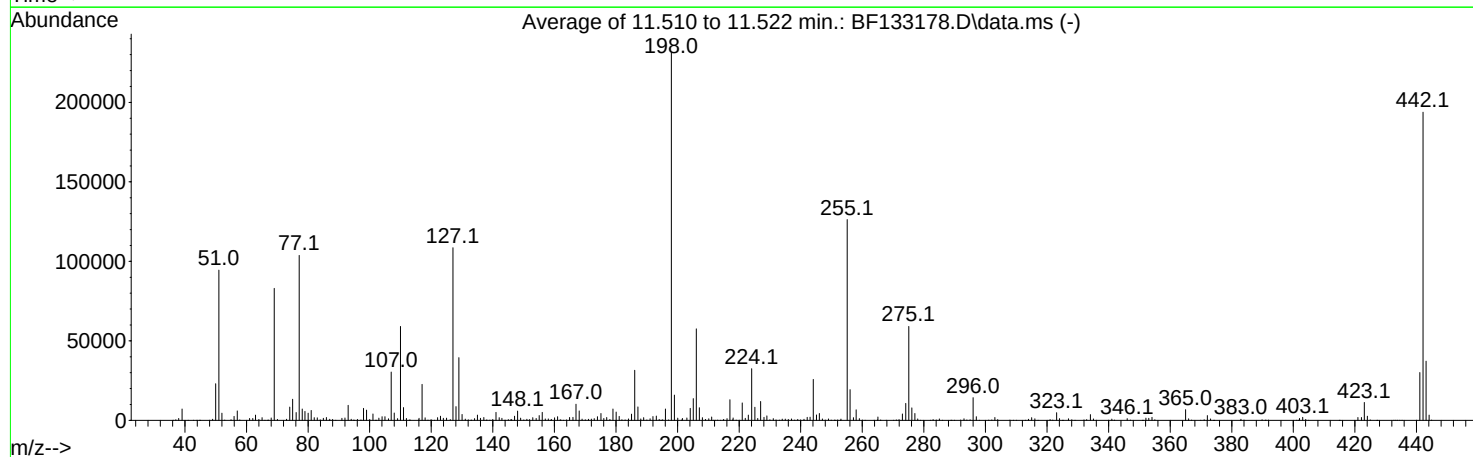


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050223\
Data File : BF133178.D
Acq On : 02 May 2023 09:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 03 04:52:44 2023

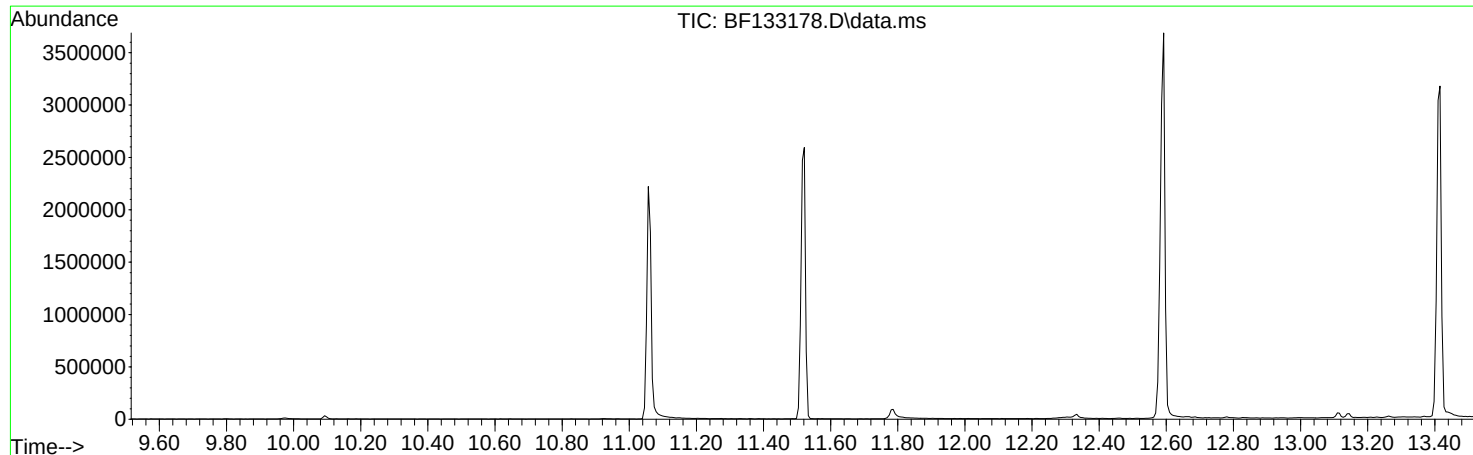




AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	40.8	94493	PASS
68	69	0.00	2	1.9	1566	PASS
69	198	0.00	100	35.9	83027	PASS
70	69	0.00	2	0.7	612	PASS
127	198	10	80	46.9	108589	PASS
197	198	0.00	2	0.1	317	PASS
198	198	100	100	100.0	231365	PASS
199	198	5	9	6.9	15897	PASS
275	198	10	60	25.6	59120	PASS
365	198	1	100	2.9	6743	PASS
441	198	0.01	100	13.0	30061	PASS
442	442	50	100	100.0	193859	PASS
443	442	15	24	19.2	37215	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050223\
Data File : BF133178.D
Acq On : 02 May 2023 09:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 02 11:10:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 02 10:52:52 2023
Response via : Initial Calibration

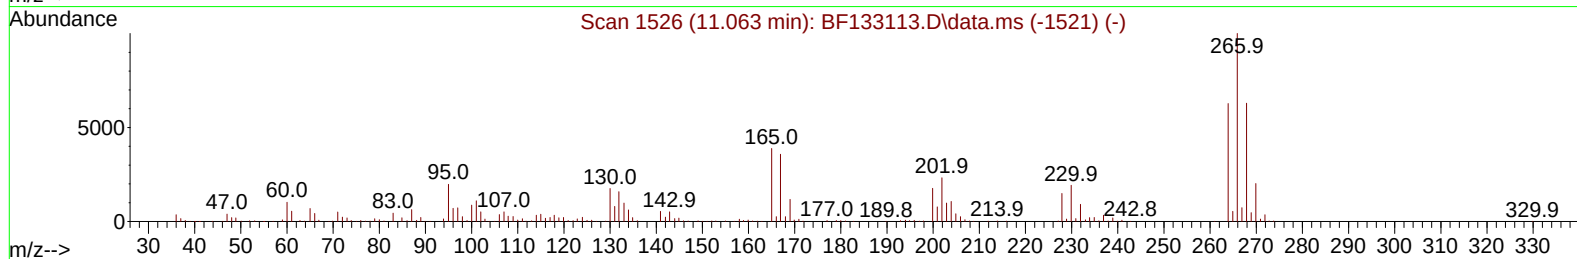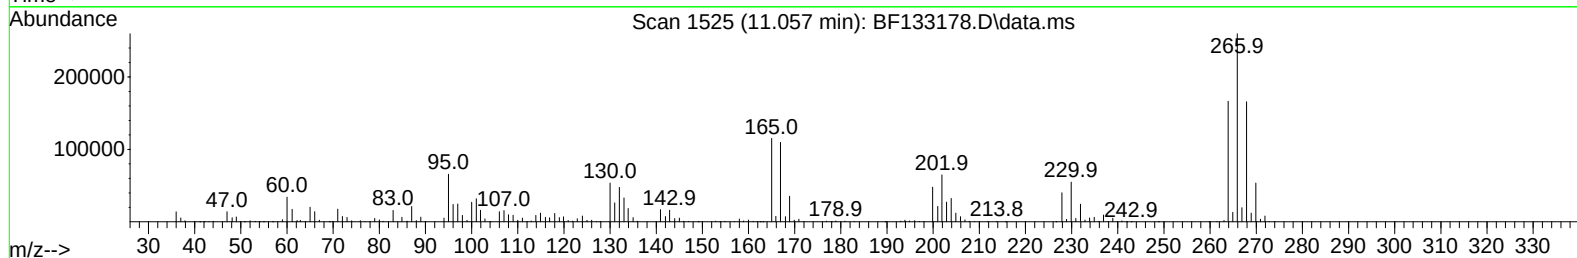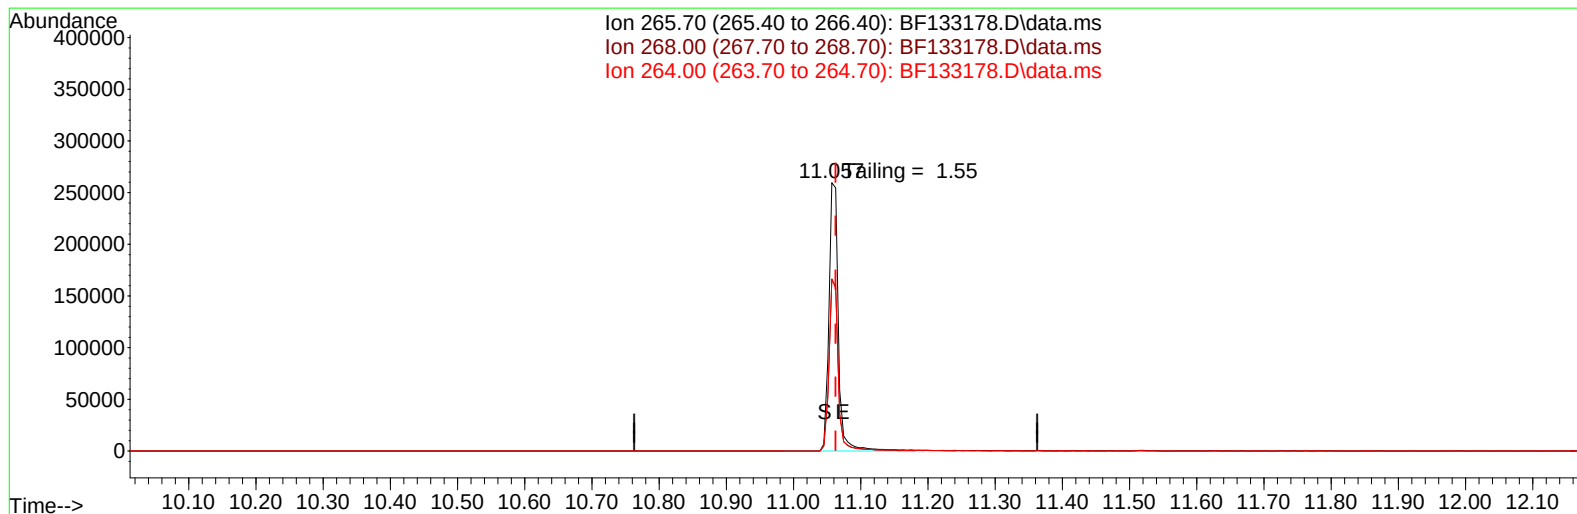

TIC: BF133178.D\data.ms

(70) Pentachlorophenol (C)

11.057min (-0.006) 90911.68 ng




response 255441

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.84
264.00	63.30	64.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050223\
 Data File : BF133178.D
 Acq On : 02 May 2023 09:23
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 03 04:59:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 04:52:44 2023
 Response via : Initial Calibration

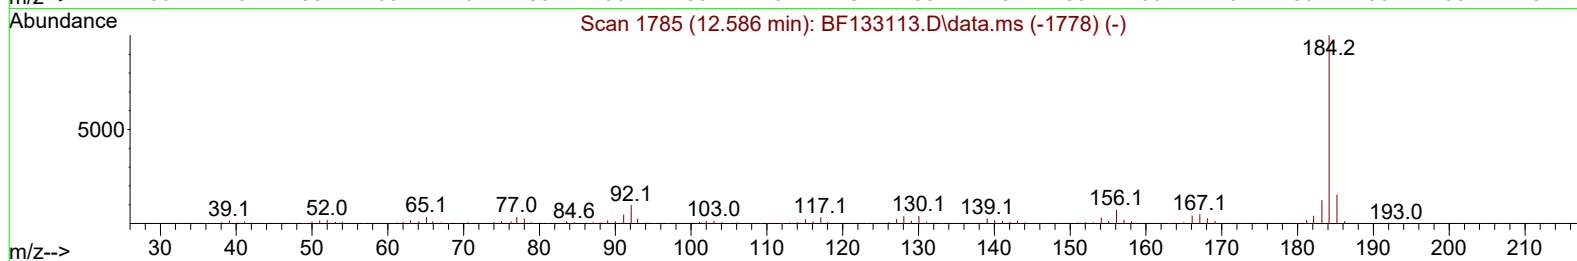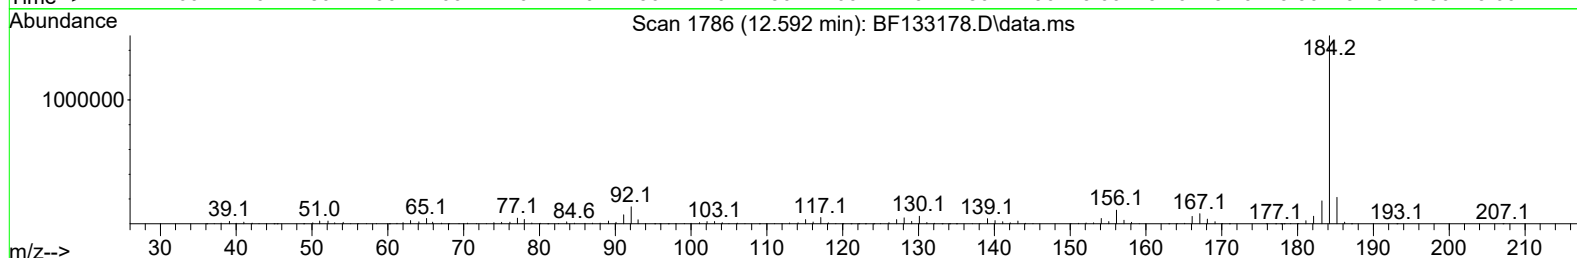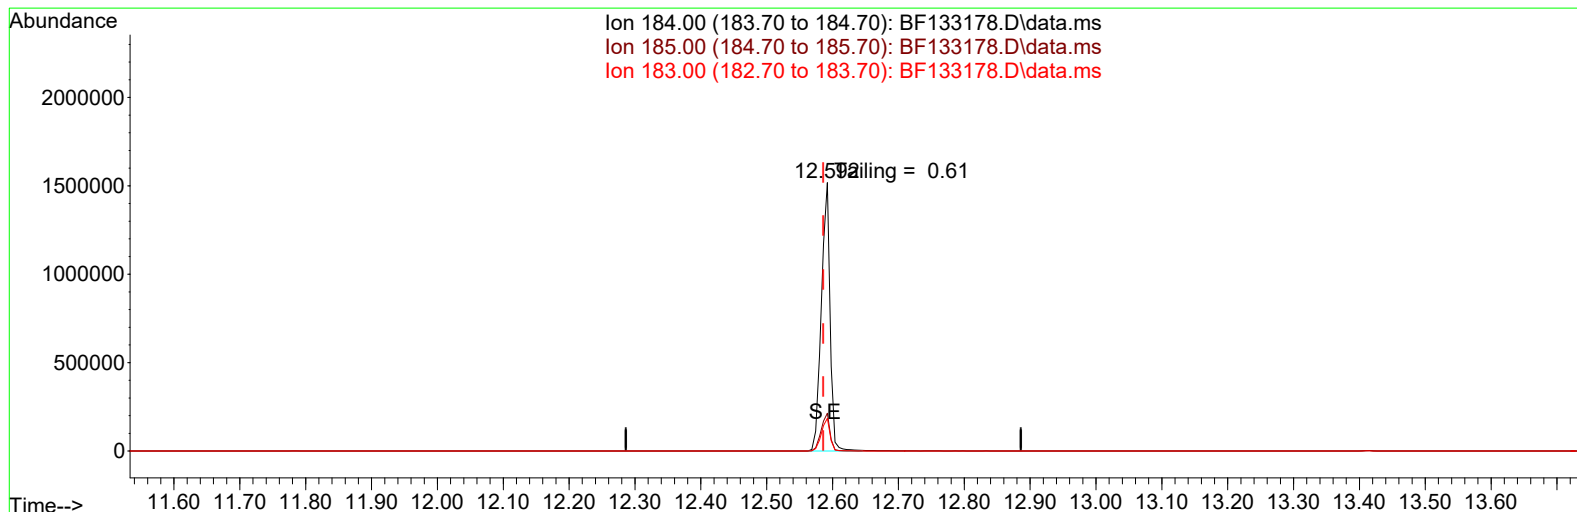

TIC: BF133178.D\data.ms

(77) Benzidine

12.592min (+ 0.006) 174450.67 ng

response 1401275

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.07#
183.00	11.70	12.19
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/2/2023	BNA_F	<u>BF133178.D</u>
Compound Name	Response	Retention Time
DDT	593794	13.416
DDD	14055	13.116
DDE	1343	12.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15398	609192	2.53

Instrument :
BNA_F
ClientSampleId :
DFTPP