
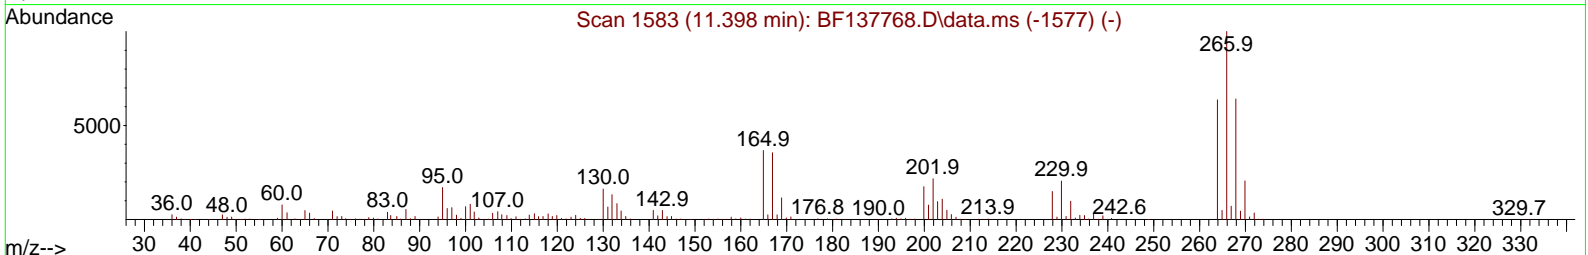
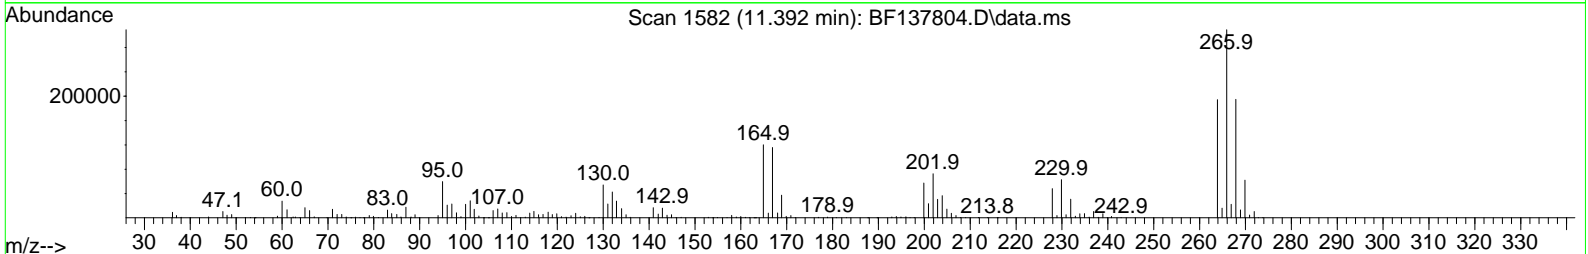


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050224\
 Data File : BF137804.D
 Acq On : 02 May 2024 09:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 20:48:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 01 03:25:08 2024
 Response via : Initial Calibration

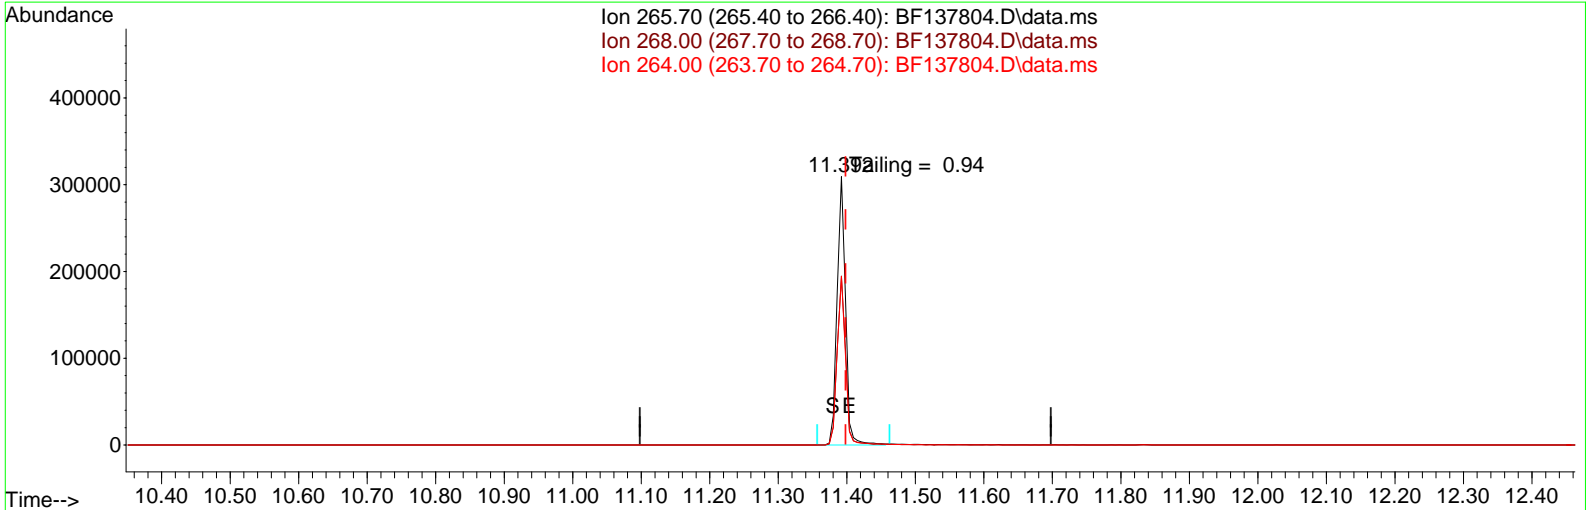

TIC: BF137804.D\data.ms

(70) Pentachlorophenol (C)




11.392min (-0.006) 549220.01 ng

response 264595

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	62.98
264.00	63.70	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050224\
 Data File : BF137804.D
 Acq On : 02 May 2024 09:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 20:48:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 01 03:25:08 2024
 Response via : Initial Calibration

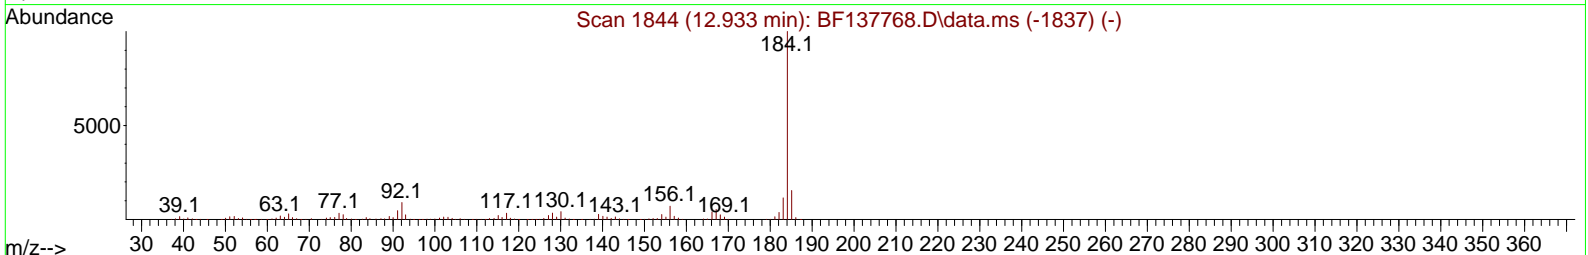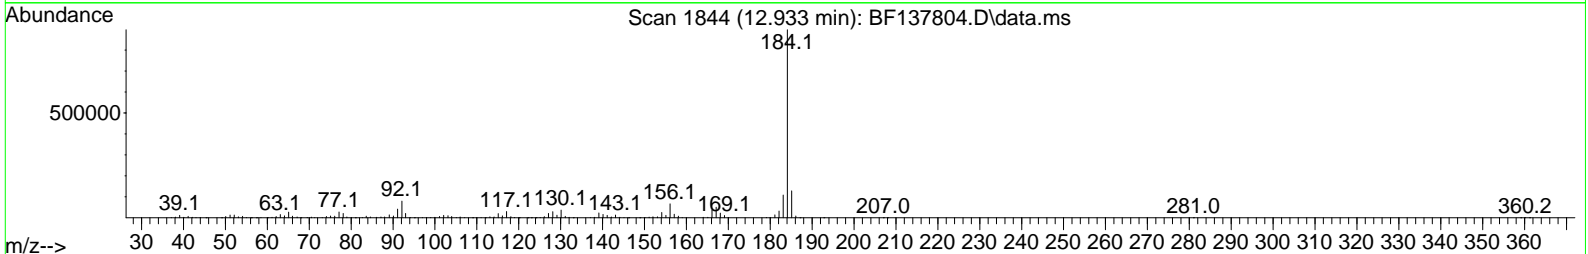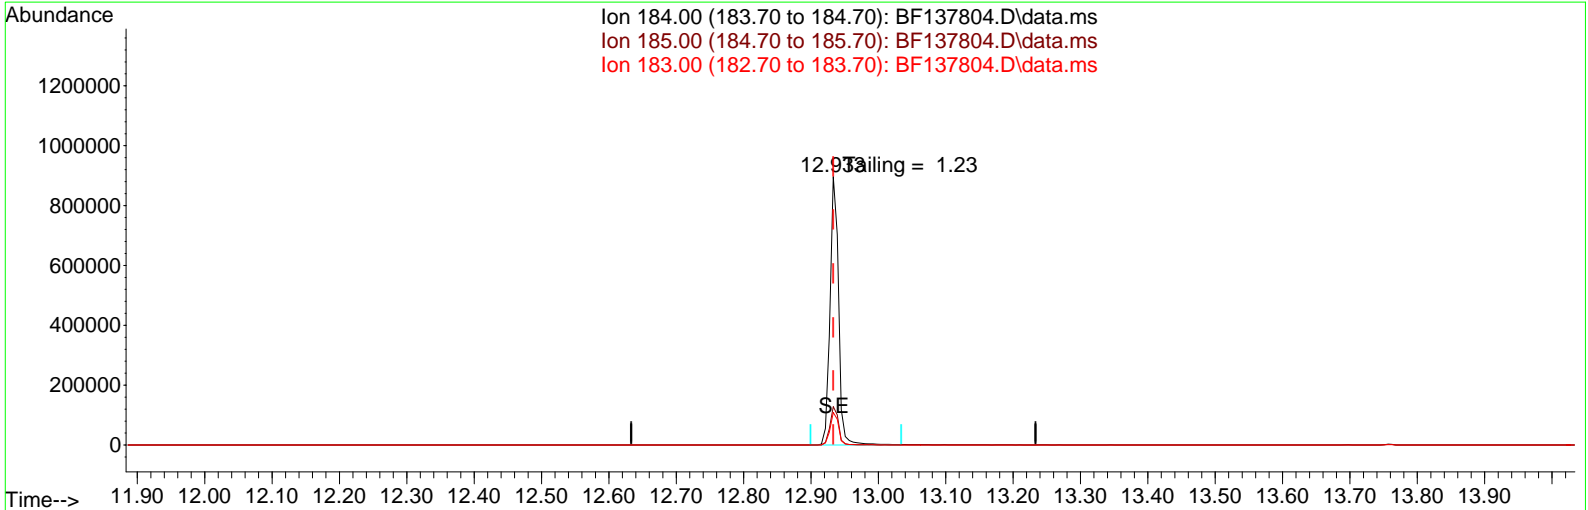

TIC: BF137804.D\data.ms

(77) Benzidine

12.933min (-0.000) 3919.25 ng m

response 787237

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.32
183.00	11.50	12.10
0.00	0.00	0.00