


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050224\
Data File : BF137804.D
Acq On : 02 May 2024 09:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 03:25:08 2024

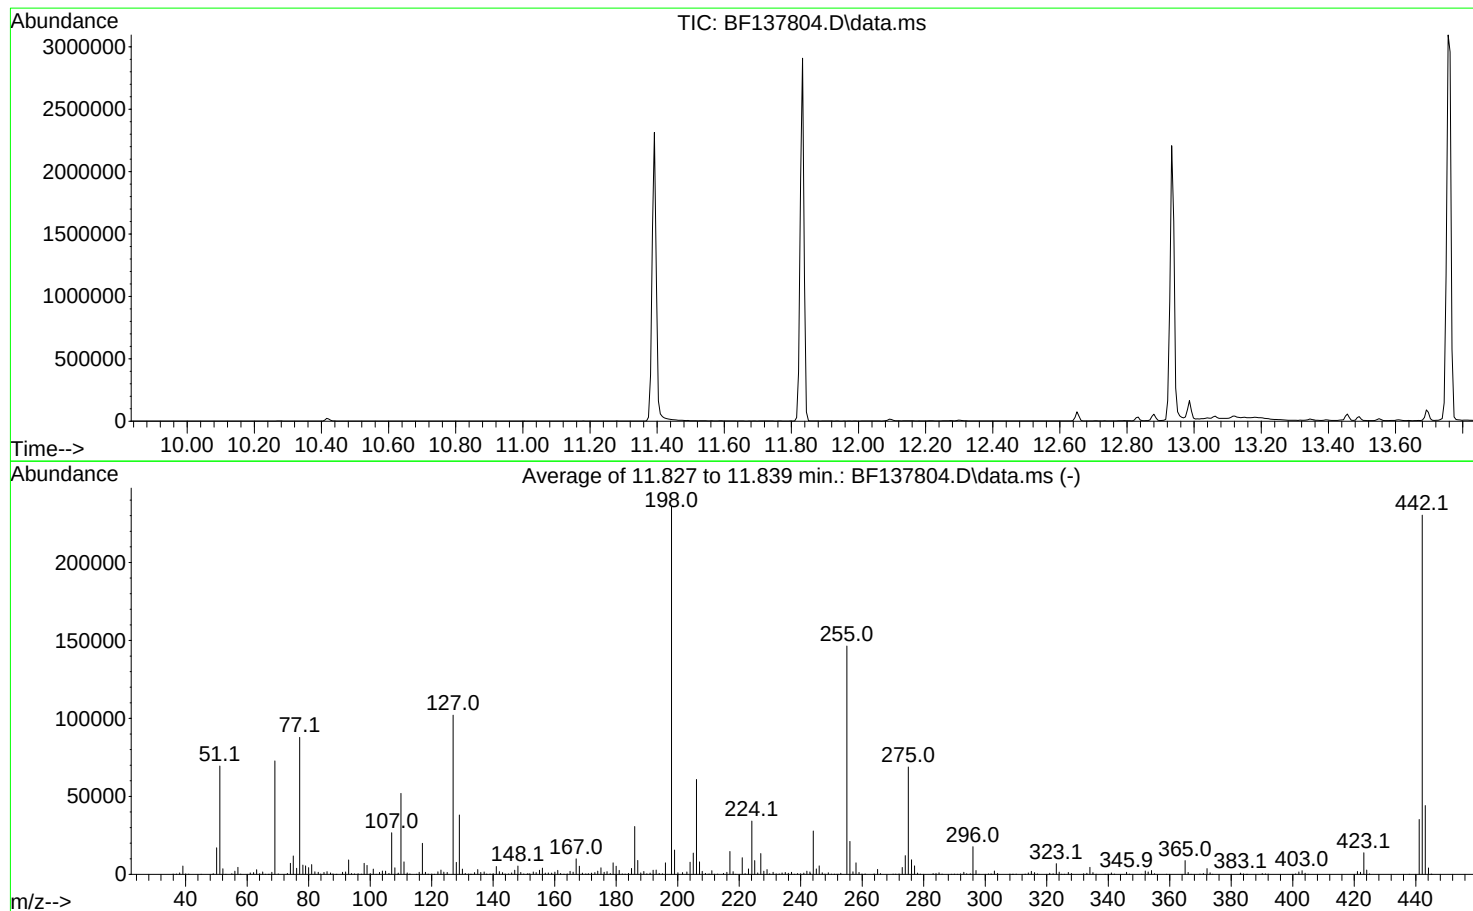

AutoFind: Scans 1656, 1657, 1658; Background Corrected with Scan 1650

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	29.5	69512	PASS
68	69	0.00	2	1.9	1378	PASS
69	198	0.00	100	30.8	72752	PASS
70	69	0.00	2	0.5	351	PASS
127	198	10	80	43.3	102048	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	235893	PASS
199	198	5	9	6.6	15618	PASS
275	198	10	60	29.2	68875	PASS
365	198	1	100	3.8	8865	PASS
441	198	0.01	100	14.9	35224	PASS
442	442	50	100	100.0	230328	PASS
443	442	15	24	19.1	44085	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/2/2024	BNA_F	<u>BF137804.D</u>
Compound Name	Response	Retention Time
DDT	578956	13.762
DDD	14435	13.457
DDE	1934	13.121
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16369	595325	2.75

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050224\
Data File : BF137804.D
Acq On : 02 May 2024 09:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 02 20:48:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

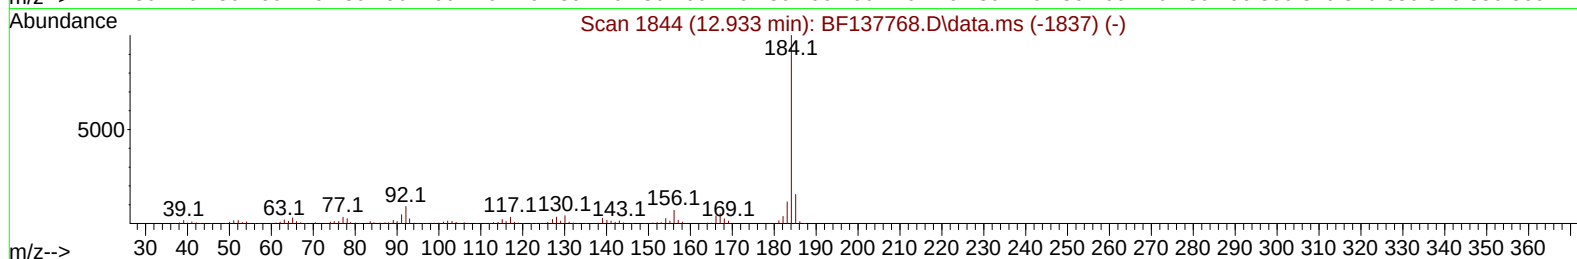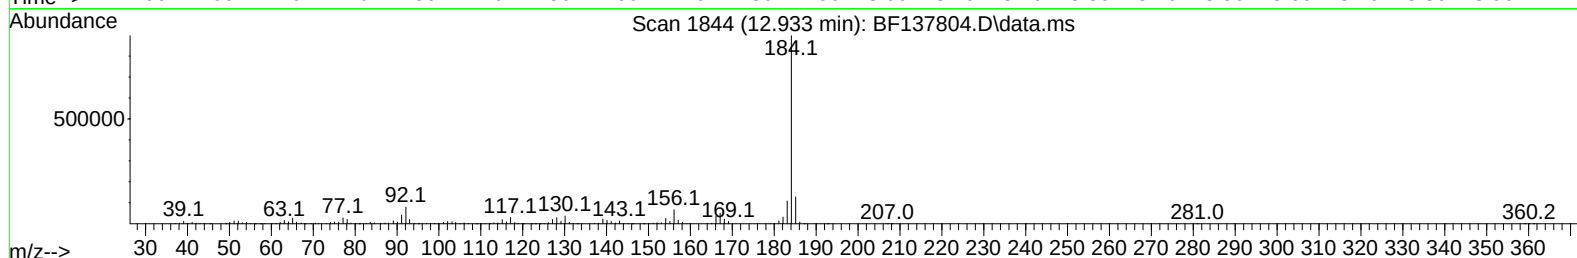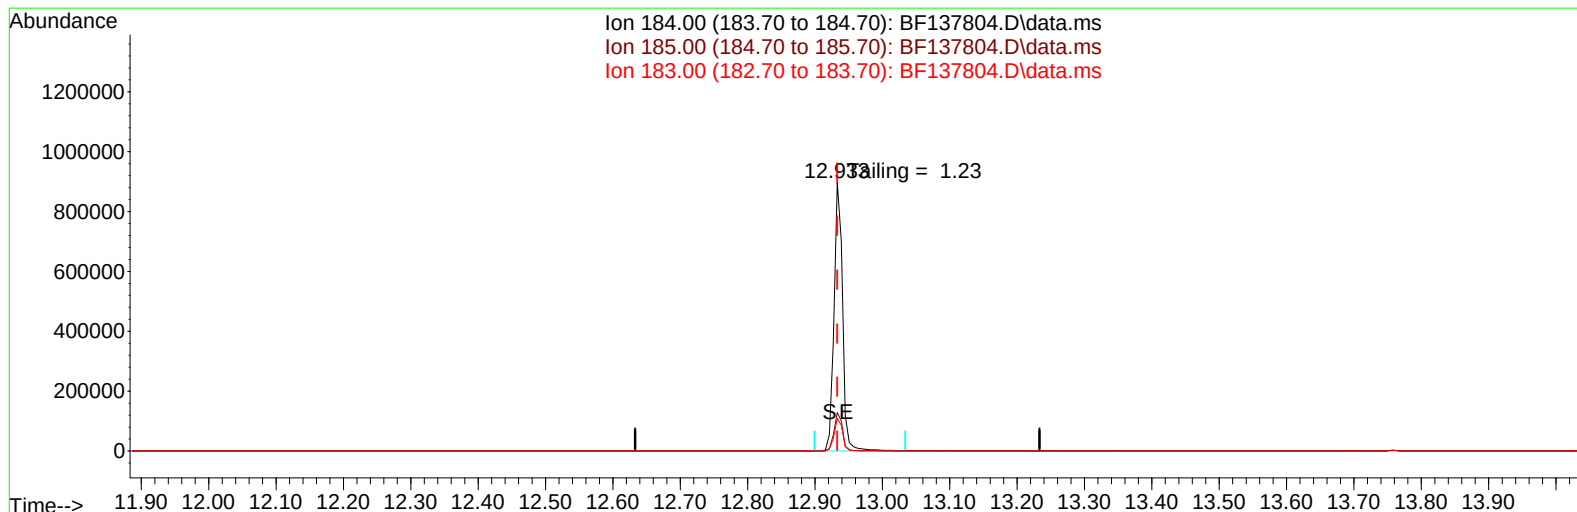

TIC: BF137804.D\data.ms

(77) Benzidine

12.933min (-0.000) 3919.25 ng m

response 787237

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.32
183.00	11.50	12.10
0.00	0.00	0.00