
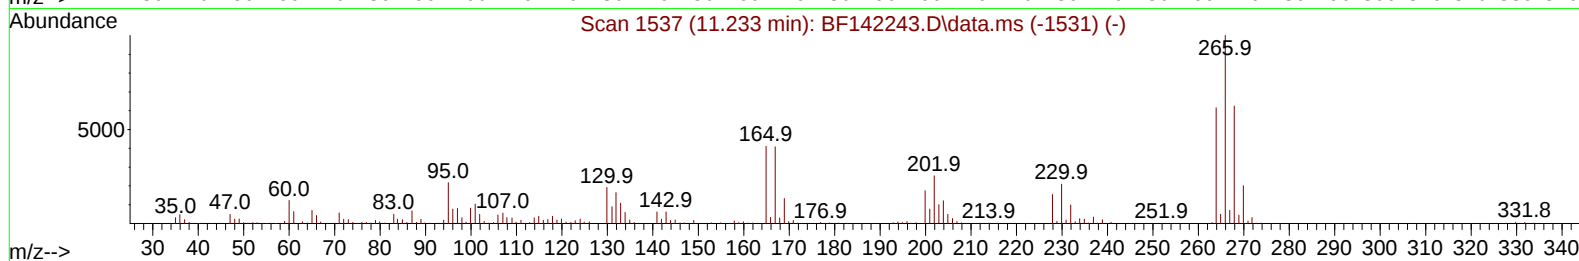
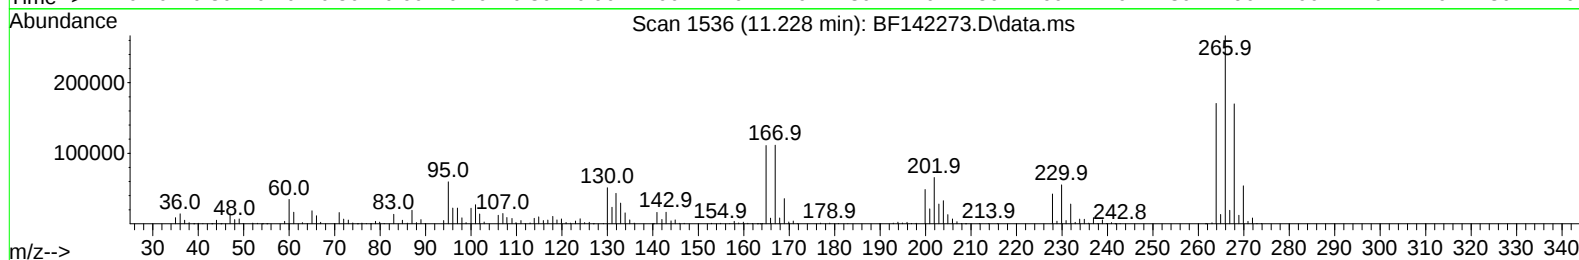


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050225\
Data File : BF142273.D
Acq On : 02 May 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 11:49:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 30 16:00:01 2025
Response via : Initial Calibration

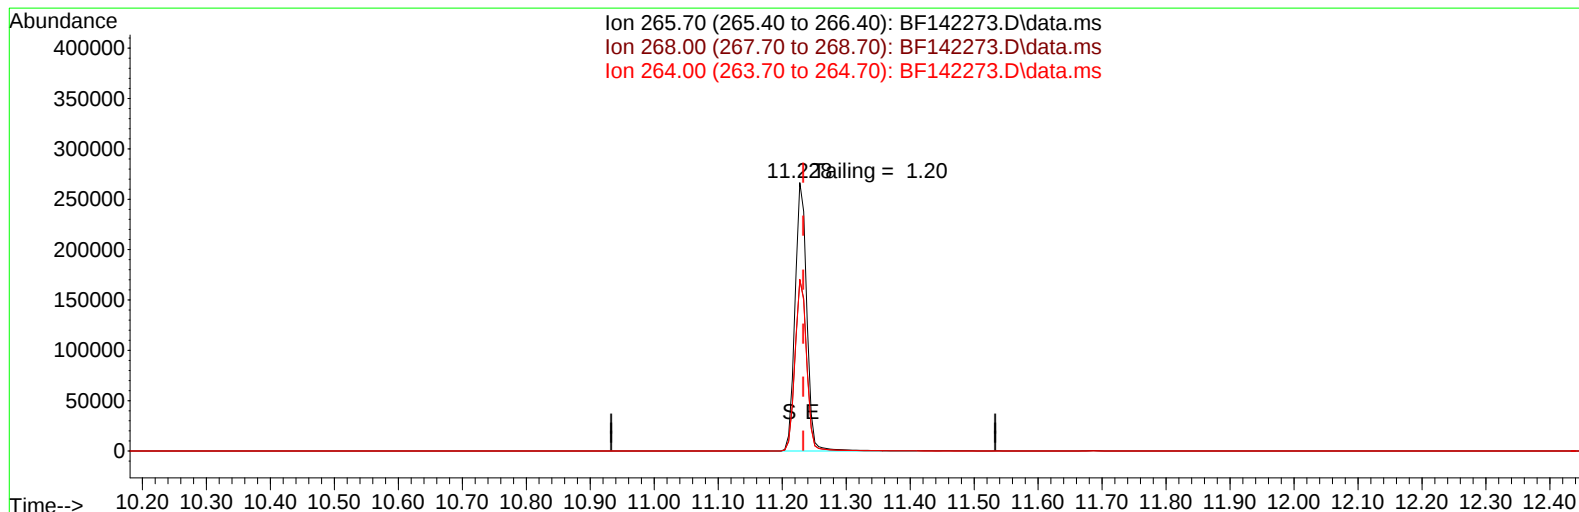

TIC: BF142273.D\data.ms

(70) Pentachlorophenol (C)




11.228min (-0.005) 200113.05 ng

response 342837

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	63.76
264.00	61.60	64.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050225\
Data File : BF142273.D
Acq On : 02 May 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 11:49:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 30 16:00:01 2025
Response via : Initial Calibration

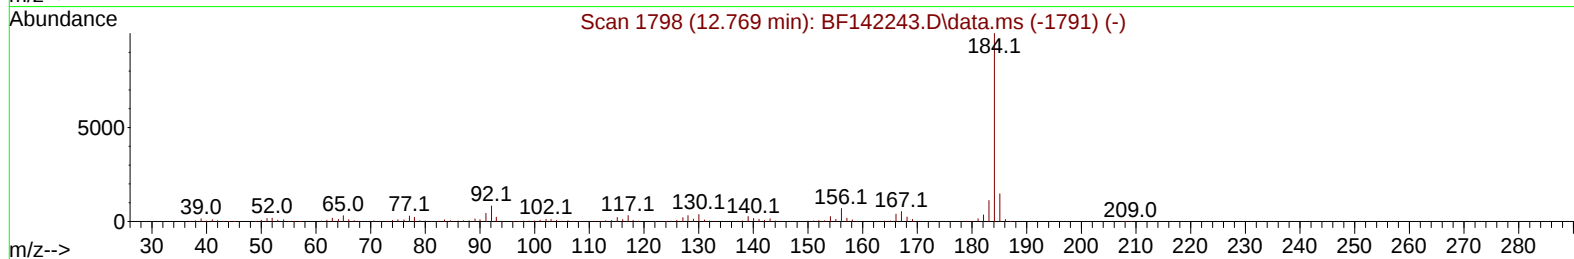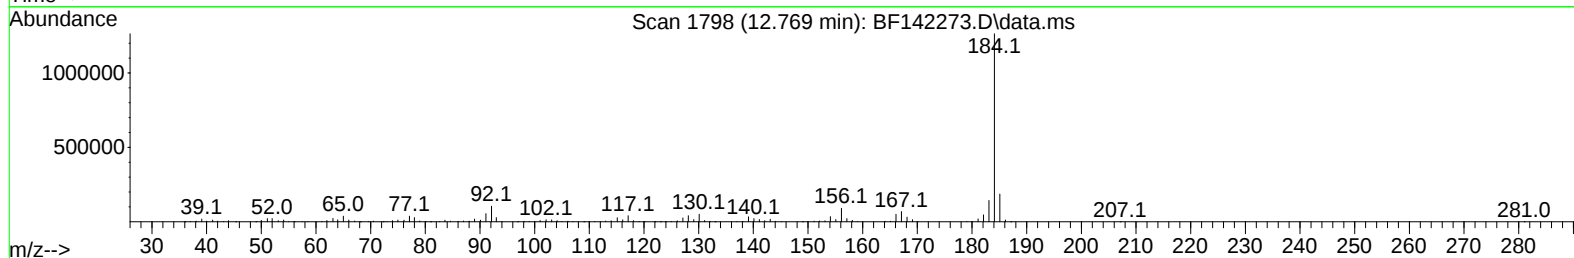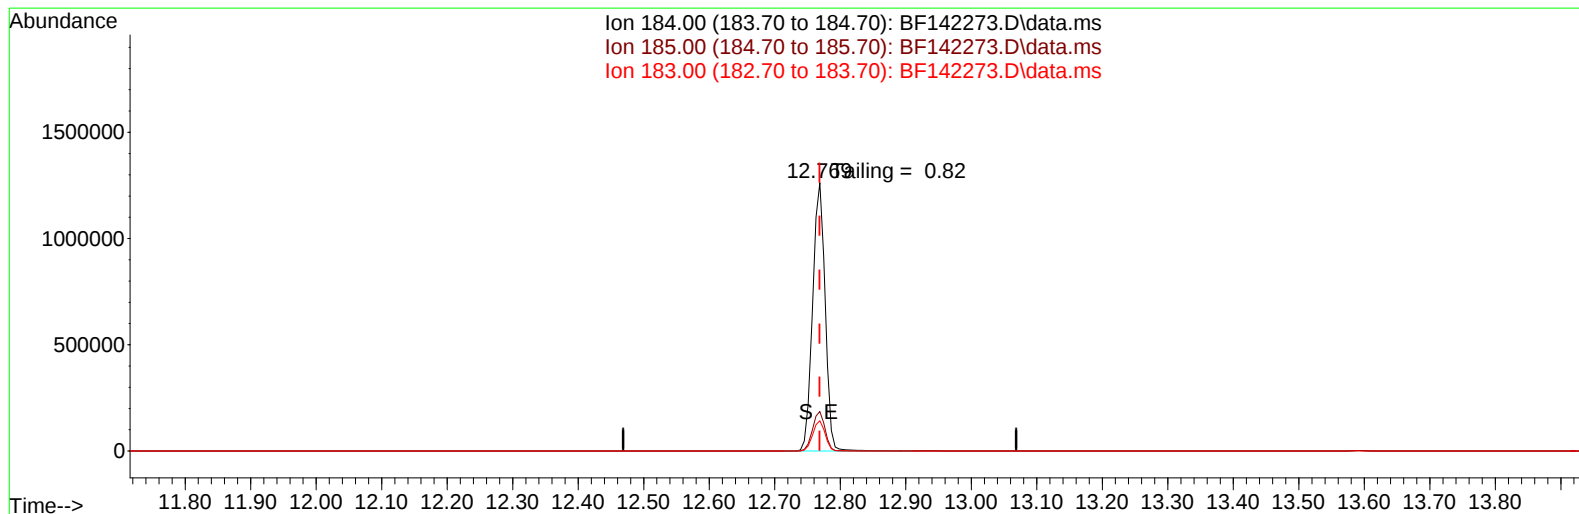

TIC: BF142273.D\data.ms

(77) Benzidine

12.769min (-0.000) 120826.54 ng

response 1673715

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.73
183.00	11.10	11.31
0.00	0.00	0.00