
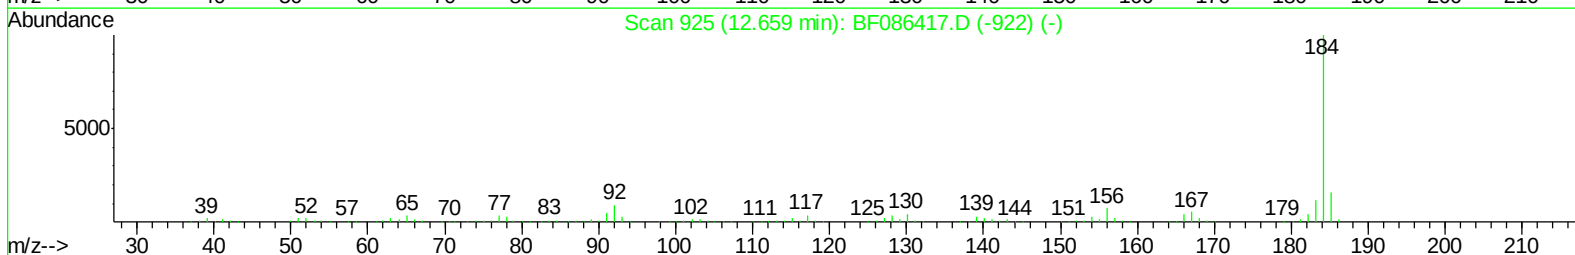
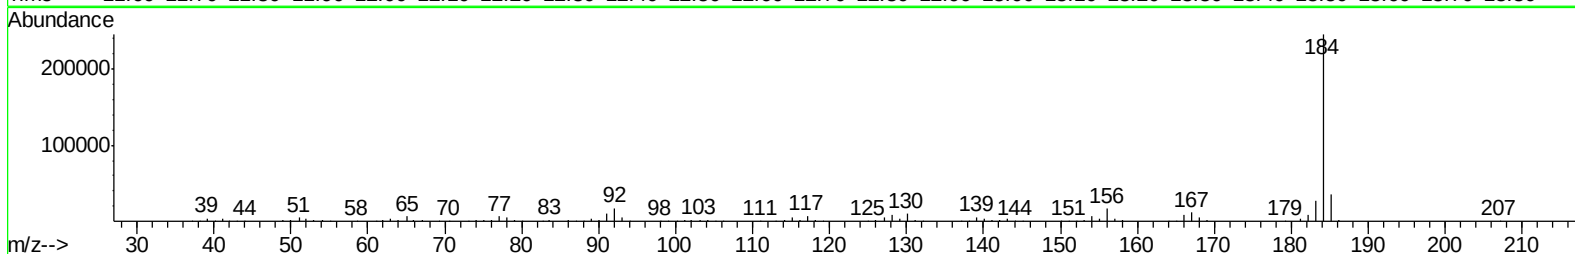


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050316\
Data File : BF086658.D
Acq On : 3 May 2016 22:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 05:56:15 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 14:20:52 2016
Response via : Initial Calibration

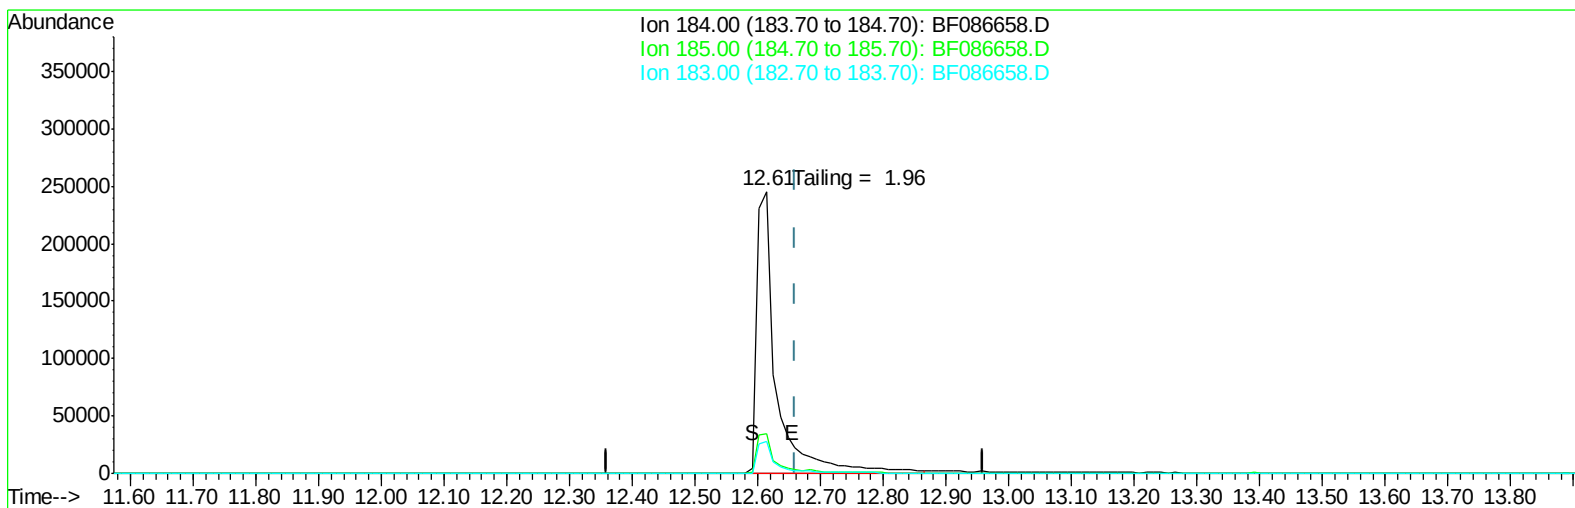

TIC: BF086658.D

(76) Benzidine




12.614min (-0.045) 0.00ng

response 546647

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.20
183.00	12.20	11.27
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050316\
Data File : BF086658.D
Acq On : 3 May 2016 22:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 05:56:15 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 14:20:52 2016
Response via : Initial Calibration

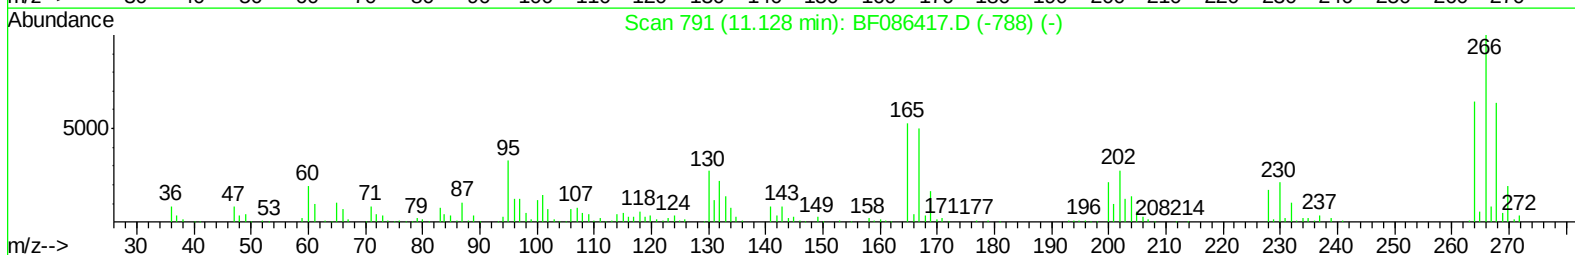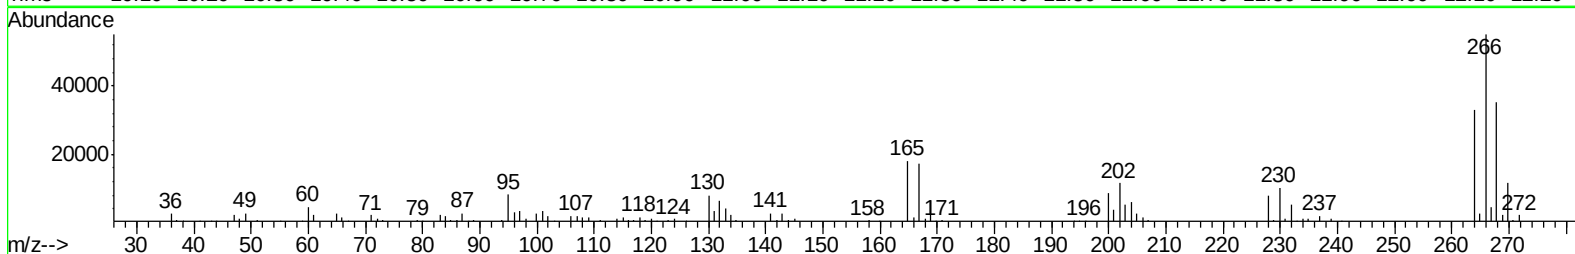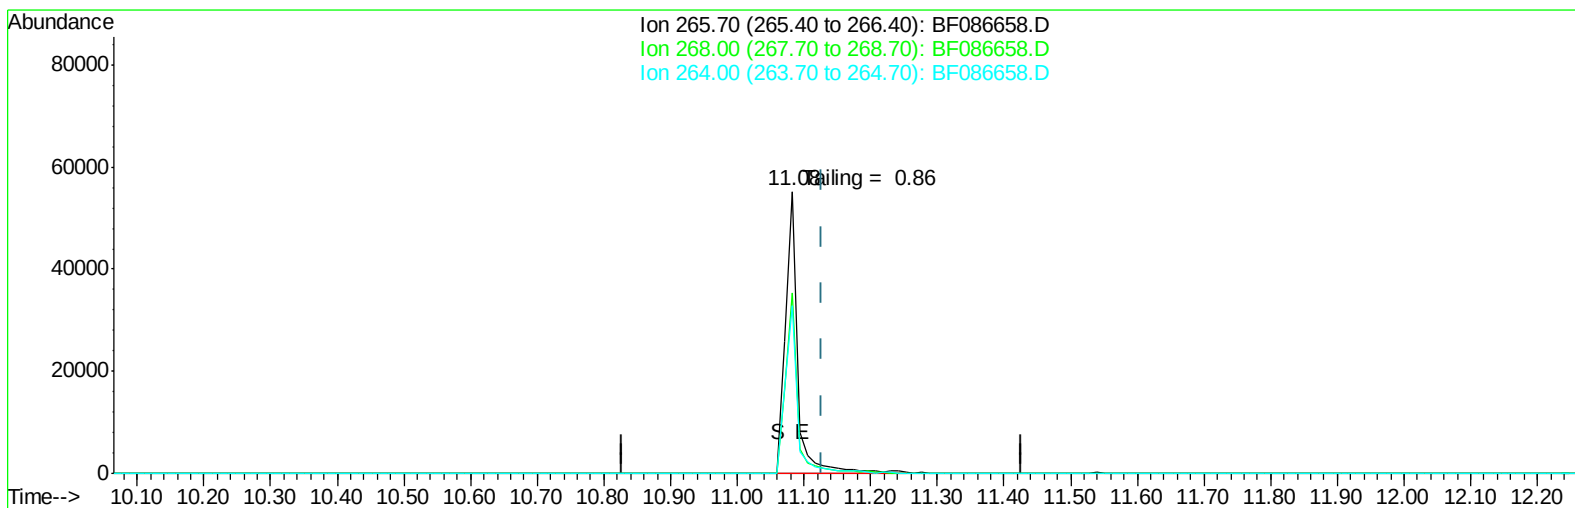

TIC: BF086658.D

(69) Pentachlorophenol (C)

11.082min (-0.045) 26516.74ng

response 70868

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.10
264.00	66.10	59.71
0.00	0.00	0.00