

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050316\
 Data File : BF086653.D
 Acq On : 3 May 2016 19:19
 Operator : UM/SJ
 Sample : H2685-11 4X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 26WARD-2B-CS-5(10-20FTBGS)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.898	244	246	253	rBV	26676	48403	3.46%	0.345%
2	5.333	281	284	301	rBV	958812	1004537	71.72%	7.161%
3	6.384	374	376	383	rBV	1007081	1045221	74.63%	7.451%
4	6.510	385	387	390	rBV	776990	1004980	71.75%	7.164%
5	6.750	406	408	419	rBV	1179428	1128547	80.58%	8.045%
6	6.910	419	422	424	rBV	593119	756366	54.00%	5.392%
7	7.310	455	457	473	rBV	415551	628646	44.88%	4.481%
8	7.527	474	476	483	rVB2	12840	28096	2.01%	0.200%
9	8.042	518	521	523	rBV	1341538	1369704	97.79%	9.764%
10	9.116	612	615	617	rBV	1200100	1015621	72.51%	7.240%
11	9.516	647	650	652	rBV	88857	104488	7.46%	0.745%
12	9.733	667	669	671	rBV	25638	20969	1.50%	0.149%
13	9.790	671	674	676	rBV	1619041	1400613	100.00%	9.984%
14	10.225	711	712	714	rVB	25788	34196	2.44%	0.244%
15	10.453	729	732	735	rBV	18350	32367	2.31%	0.231%
16	10.568	740	742	745	rBV2	307500	456668	32.60%	3.255%
17	10.705	752	754	760	rVB	49294	67809	4.84%	0.483%
18	11.150	791	793	794	rBV	27750	23053	1.65%	0.164%
19	11.265	801	803	806	rBV2	851639	1028961	73.47%	7.335%
20	11.802	848	850	853	rBV3	16657	21886	1.56%	0.156%
21	12.065	871	873	874	rBV	13592	16000	1.14%	0.114%
22	12.316	894	895	897	rBV2	11843	21275	1.52%	0.152%
23	12.476	907	909	912	rBV	54384	54012	3.86%	0.385%
24	12.522	912	913	917	rVV4	13634	20355	1.45%	0.145%
25	12.705	926	929	930	rBV2	52485	85802	6.13%	0.612%
26	12.854	940	942	947	rBV	674406	717821	51.25%	5.117%
27	13.391	987	989	990	rBV	38167	44792	3.20%	0.319%
28	13.905	1031	1034	1036	rBV	753738	983462	70.22%	7.011%
29	15.299	1153	1156	1165	rVB	597346	863757	61.67%	6.157%


Sum of corrected areas: 14028407

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050316\
Data File : BF086653.D
Acq On : 3 May 2016 19:19
Operator : UM/SJ
Sample : H2685-11 4X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
26WARD-2B-CS-5(10-20FTBGS)

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

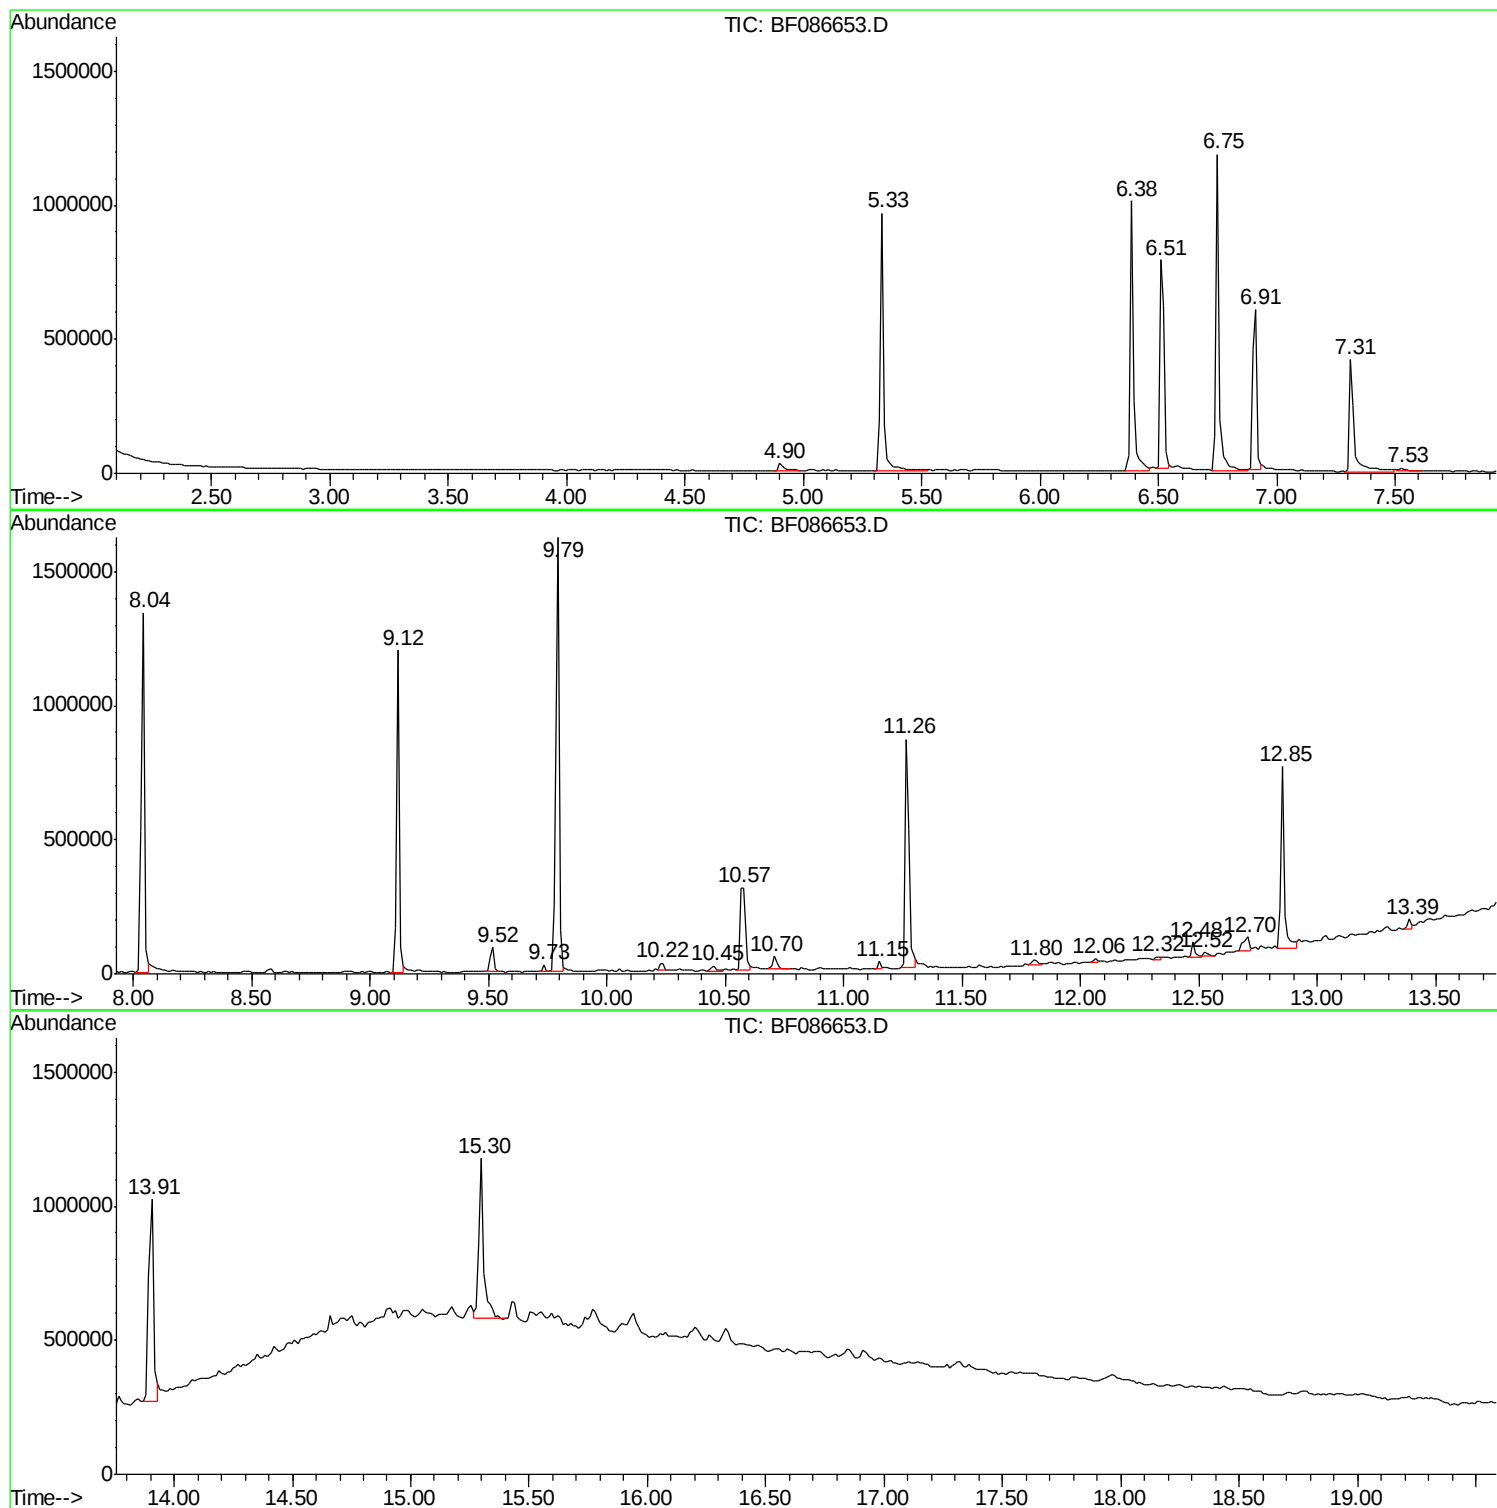

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050316\
Data File : BF086653.D
Acq On : 3 May 2016 19:19
Operator : UM/SJ
Sample : H2685-11 4X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
26WARD-2B-CS-5(10-20FTBGS)










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.51 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.51	17.81 ng	1004980	1,4-Dichlorobenzene-d4	6.75

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	14
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	10
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

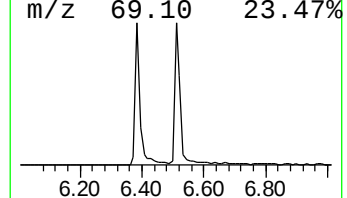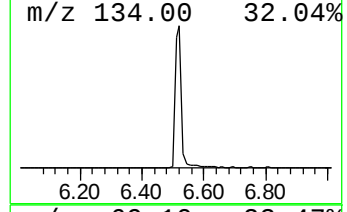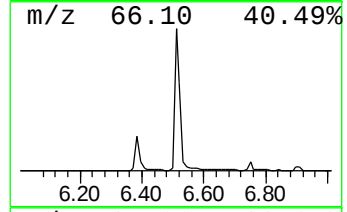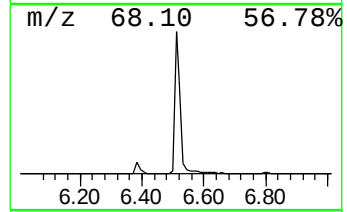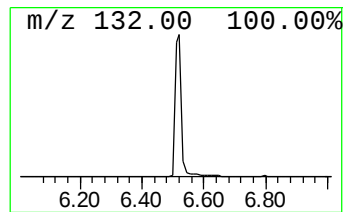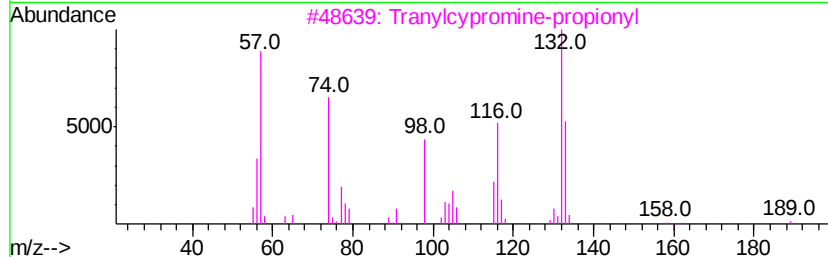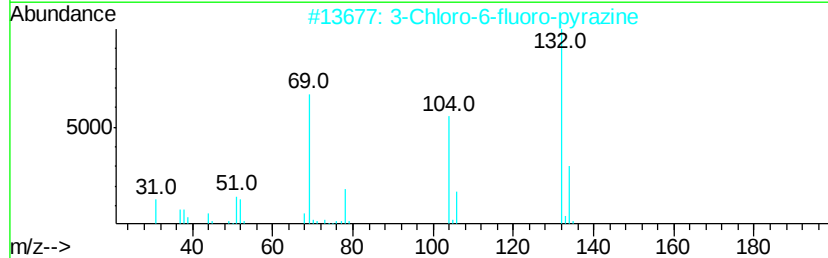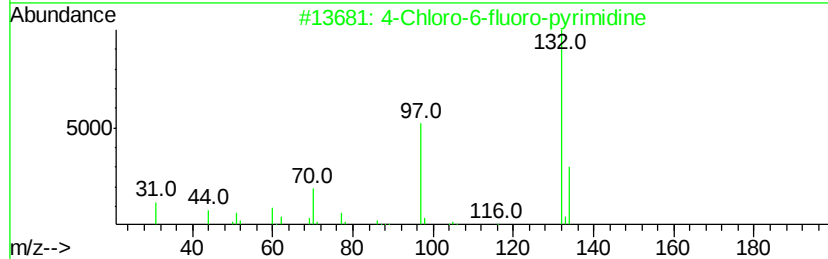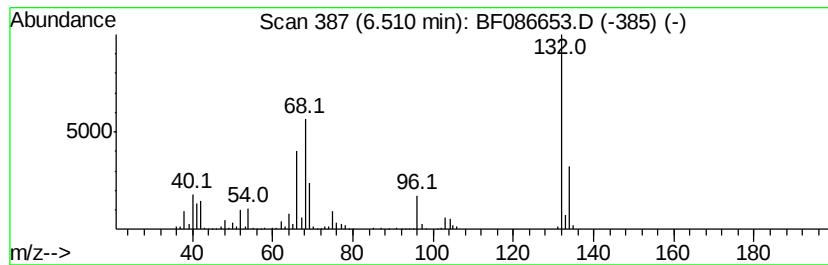

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF050316\
Data File : BF086653.D
Acq On : 3 May 2016 19:19
Operator : UM/SJ
Sample : H2685-11 4X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
26WARD-2B-CS-5(10-20FTBGS)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.51	6.51	17.8	ng	1004980	1	6.75	1128550	20.0