


Data Path : Z:\HPCHEM1\BNA F\DATA\BF050316\
 Data File : BF086658.D
 Acq On : 3 May 2016 22:59
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 27 14:20:52 2016

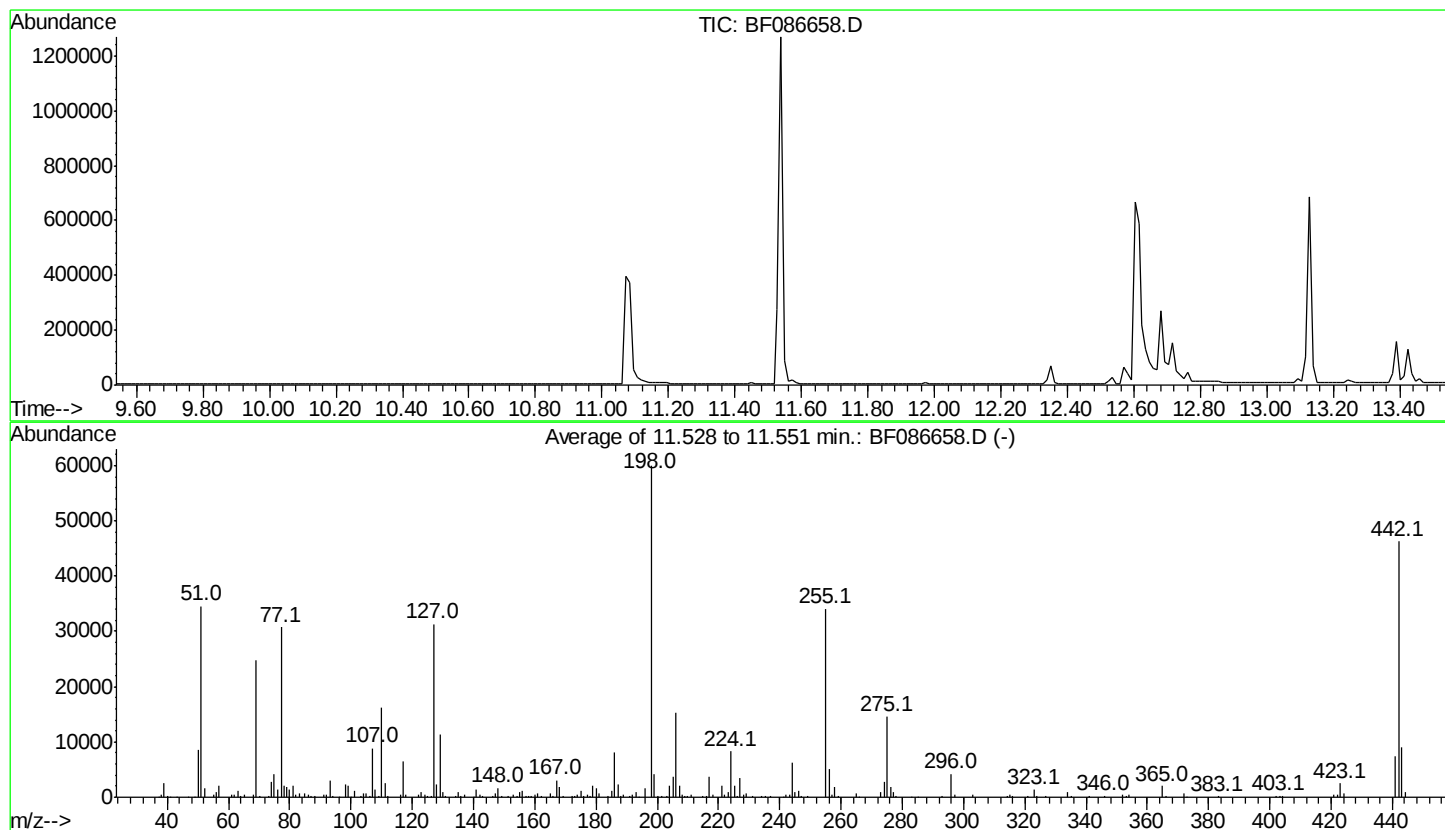

AutoFind: Scans 826, 827, 828; Background Corrected with Scan 823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.6	34541	PASS
68	69	0.00	2	1.8	457	PASS
69	198	0.00	100	41.2	24705	PASS
70	69	0.00	2	0.5	134	PASS
127	198	10	80	52.3	31369	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59988	PASS
199	198	5	9	7.0	4177	PASS
275	198	10	60	24.2	14546	PASS
365	198	1	100	3.4	2030	PASS
441	442	0.01	24	16.1	7445	PASS
442	198	50	100	77.2	46292	PASS
443	442	15	24	19.3	8940	PASS