
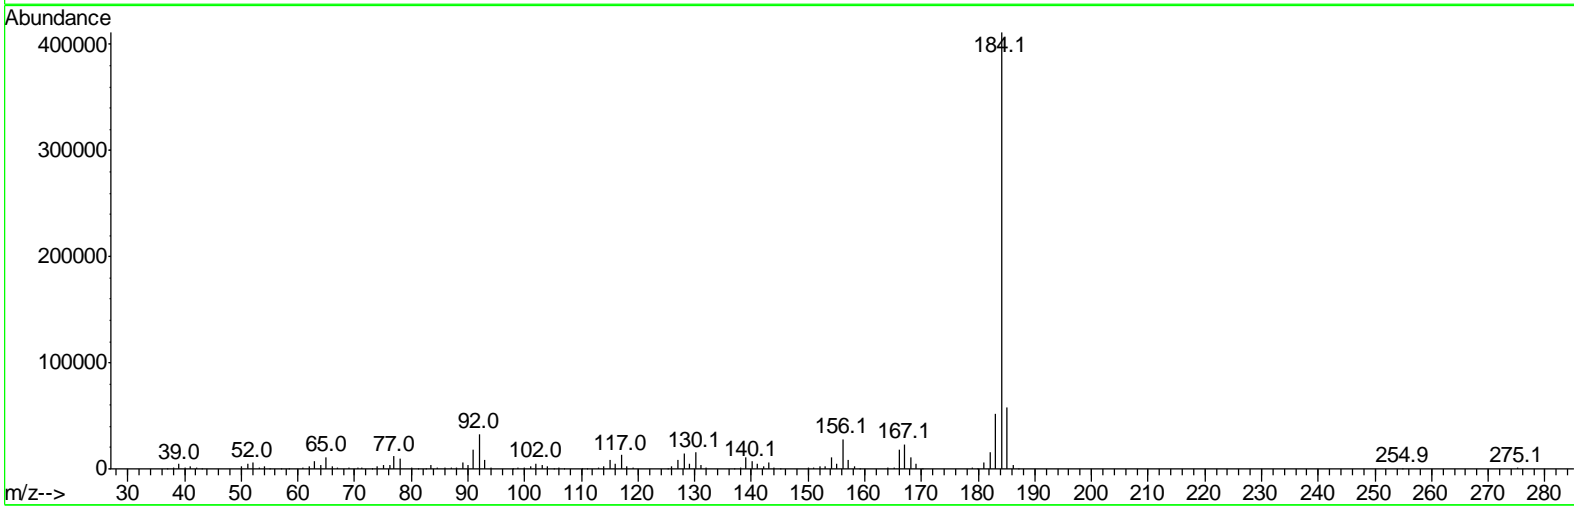


Data Path : Z:\HPCHEM1\BNA F\DATA\BF050317\  
 Data File : BF094838.D  
 Acq On : 3 May 2017 17:10  
 Operator : SJ/MA  
 Sample : DF7PP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 07:26:14 2017  
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed May 03 17:24:51 2017  
 Response via : Initial Calibration

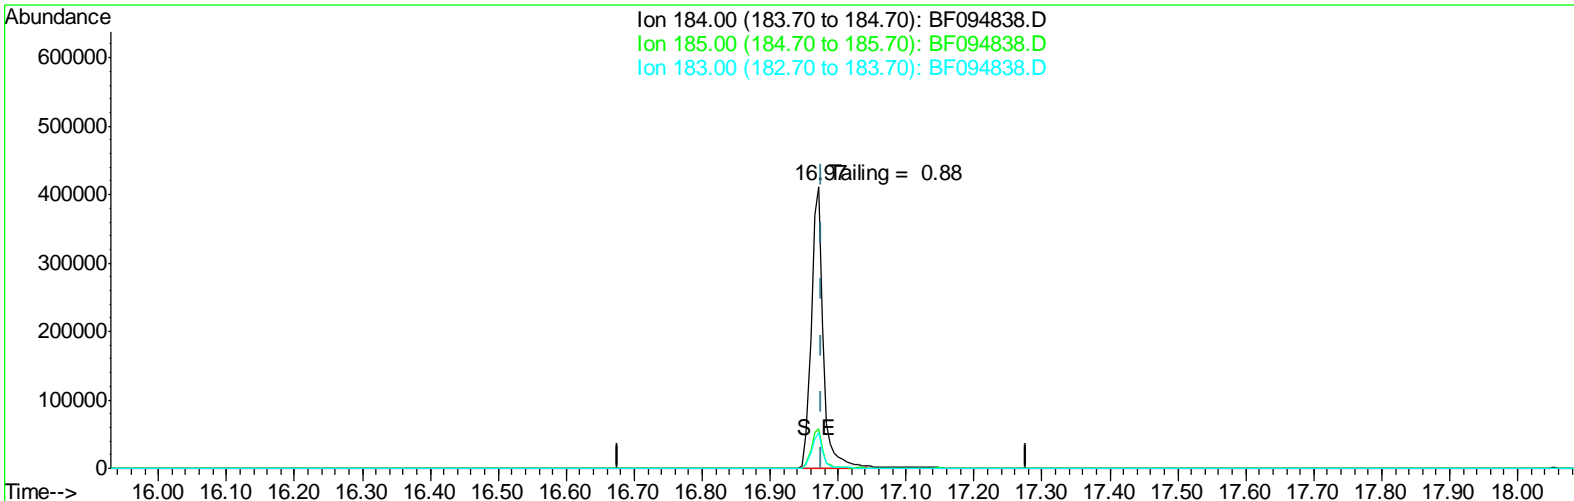

TIC: BF094838.D

(76) Benzidine



16.971min (-0.006) 0.00ng

response 508725

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.07#
183.00	12.20	12.58
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050317\  
 Data File : BF094838.D  
 Acq On : 3 May 2017 17:10  
 Operator : SJ/MA  
 Sample : DF7TPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 07:26:14 2017  
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed May 03 17:24:51 2017  
 Response via : Initial Calibration

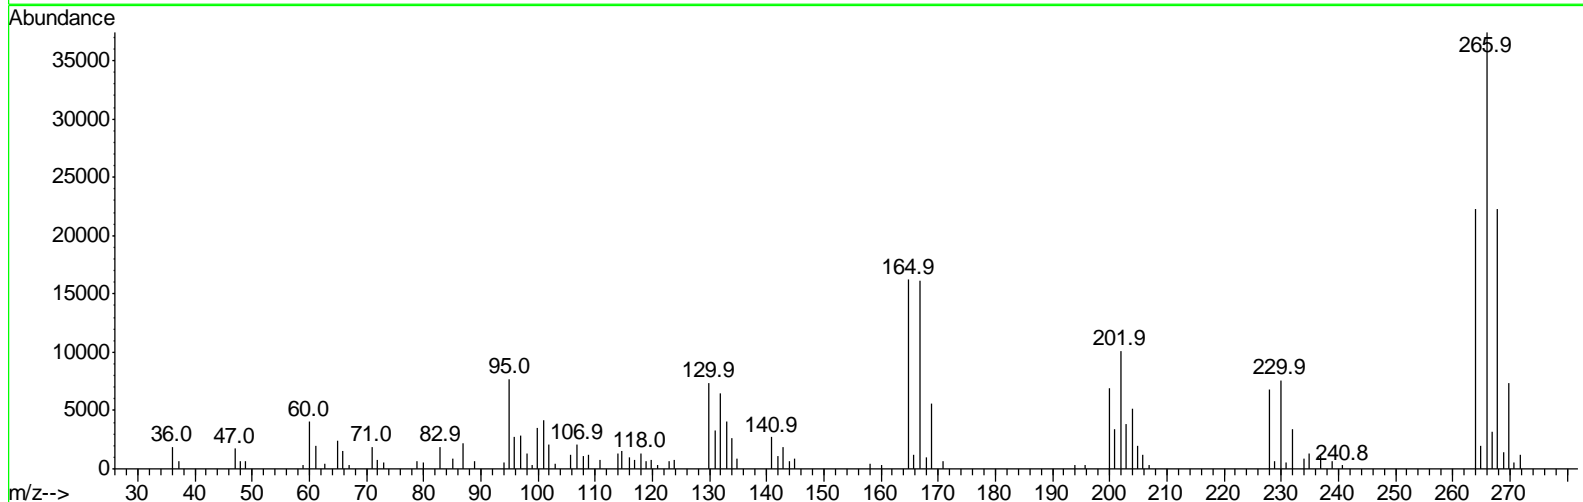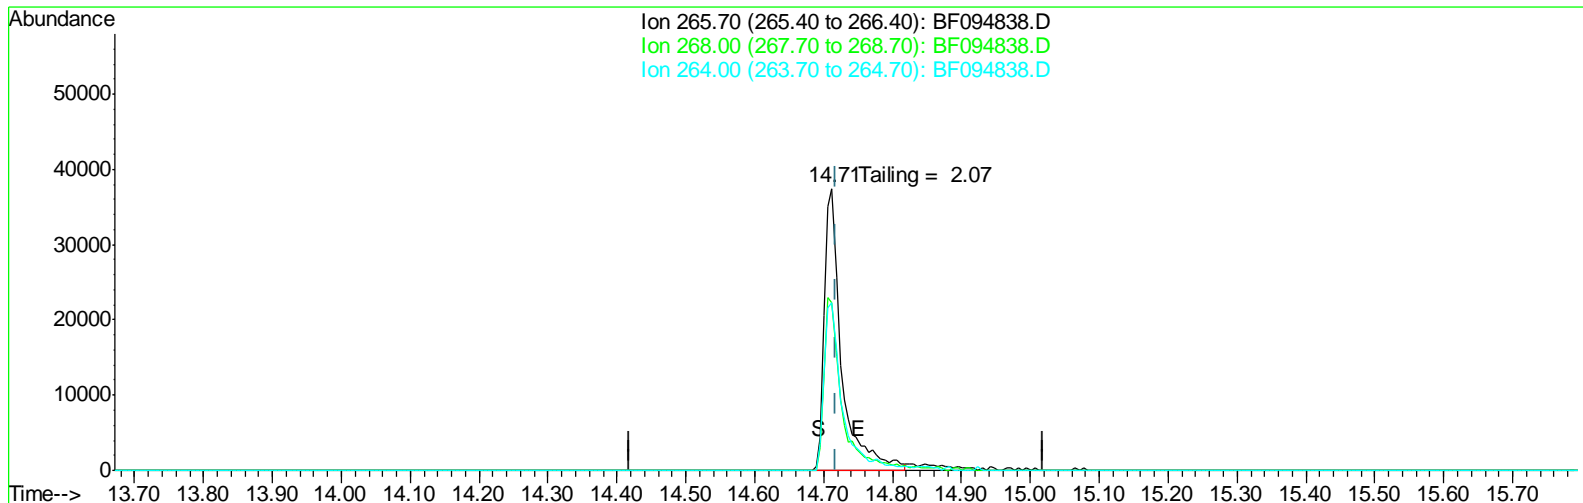

TIC: BF094838.D

(69) Pentachlorophenol (C)

14.712min (-0.006) 0.00ng

response 63796

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.59
264.00	64.60	59.42
0.00	0.00	0.00