
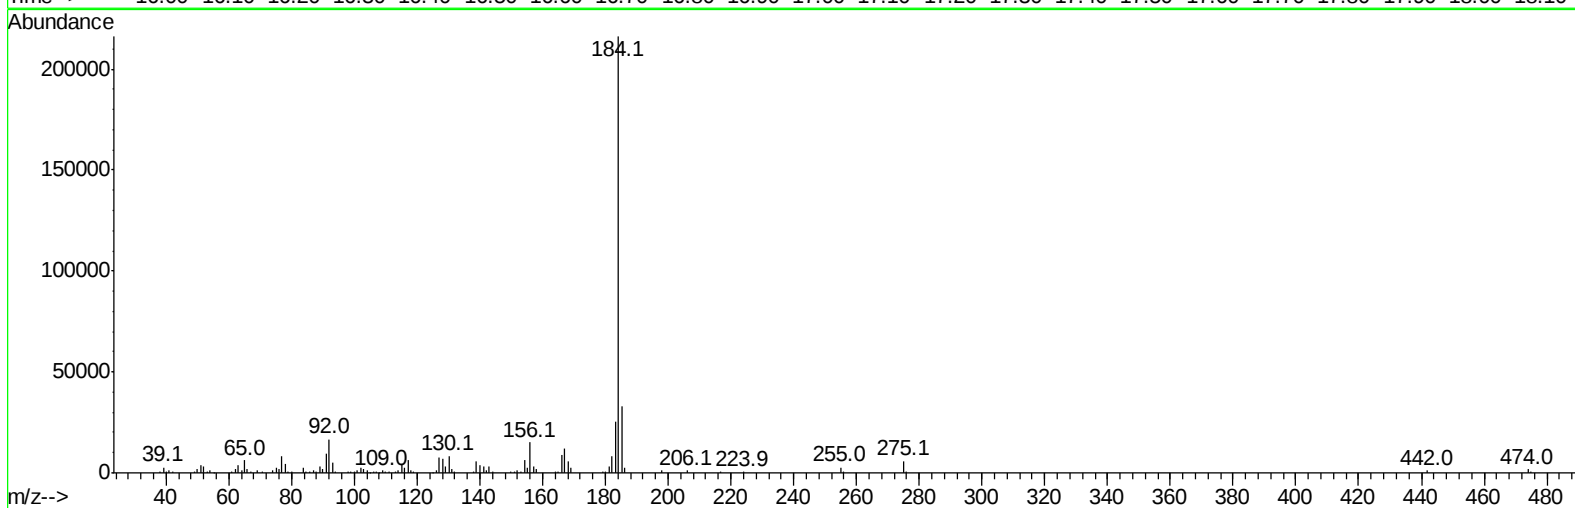


Data Path : Z:\HPCHEM1\BNA F\DATA\BF050317\  
Data File : BF094861.D  
Acq On : 4 May 2017 6:42  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 09:04:00 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 03 17:24:51 2017  
Response via : Initial Calibration

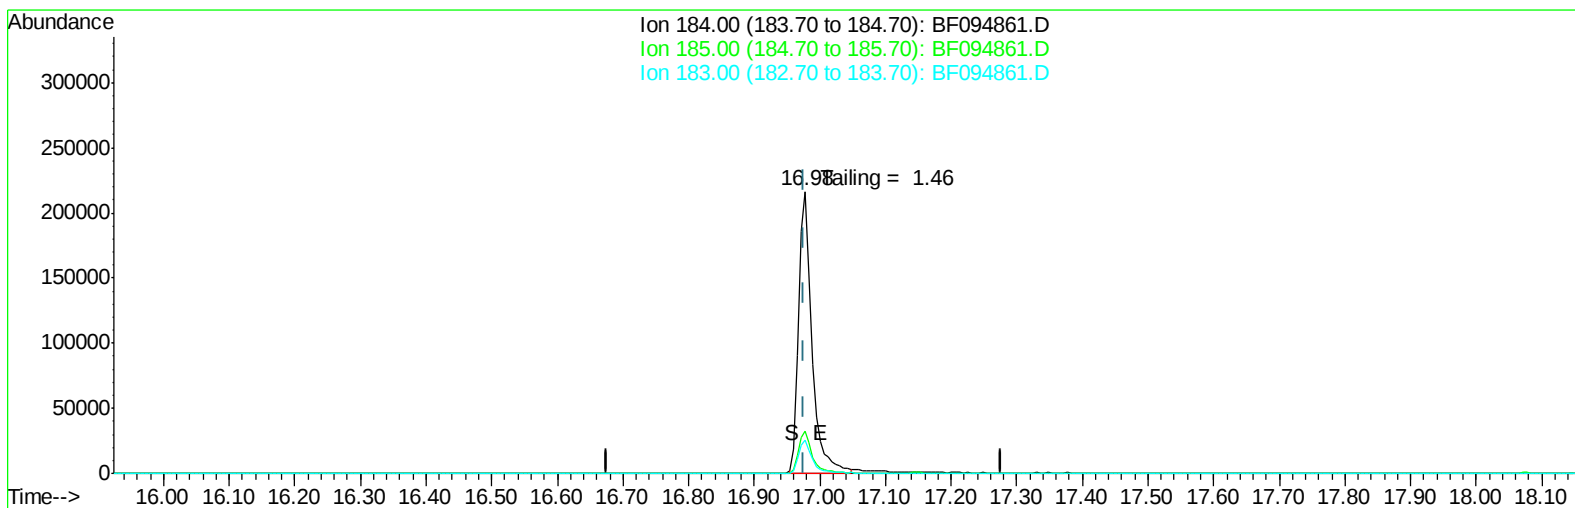

TIC: BF094861.D

(76) Benzidine



16.977min (+0.000) 0.00ng

response 319227

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 19.40 | 15.20# |
| 183.00 | 12.20 | 11.71  |
| 0.00   | 0.00  | 0.00   |

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050317\  
Data File : BF094861.D  
Acq On : 4 May 2017 6:42  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 09:04:00 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 03 17:24:51 2017  
Response via : Initial Calibration

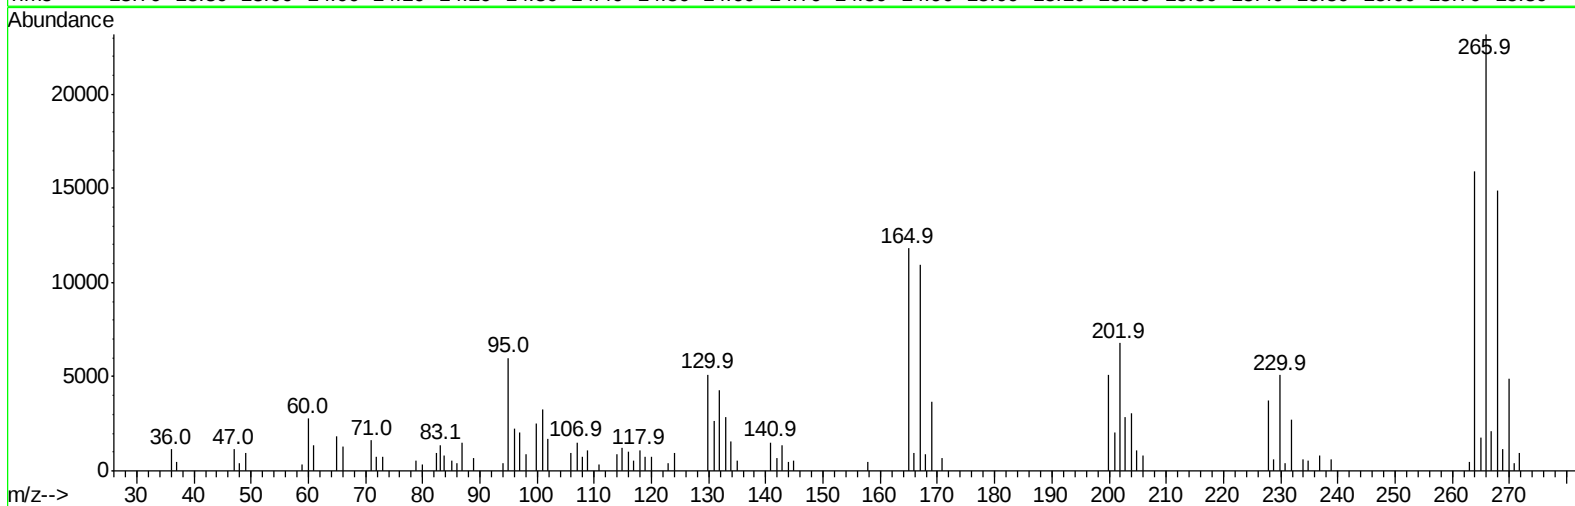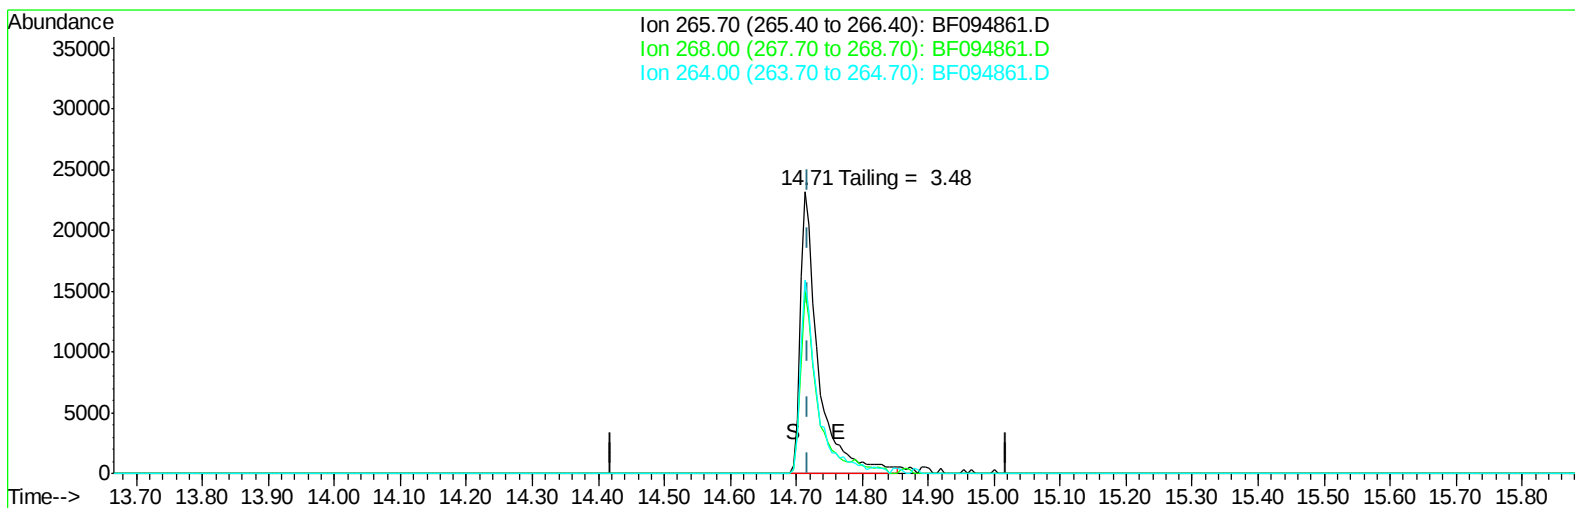

TIC: BF094861.D

(69) Pentachlorophenol (C)

14.713min (-0.006) 0.00ng

response 45177

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 64.35 |
| 264.00 | 64.60 | 68.61 |
| 0.00   | 0.00  | 0.00  |