


Data Path : Z:\HPCHEM1\BNA_F\Data\BF050317\
 Data File : BF094838.D
 Acq On : 3 May 2017 17:10
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 03 17:24:51 2017

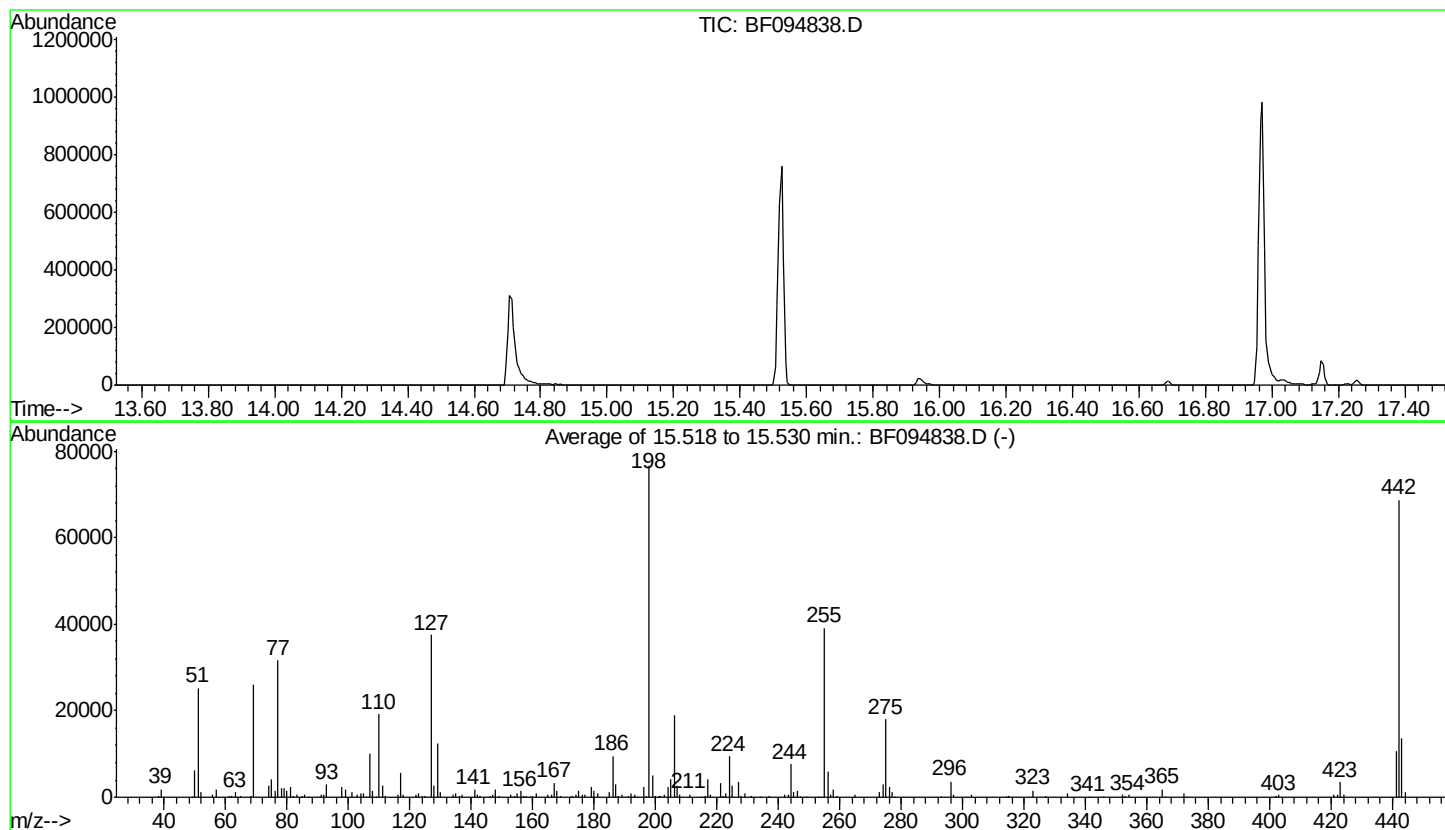

AutoFind: Scans 2309, 2310, 2311; Background Corrected with Scan 2303

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	25188	PASS
68	69	0.00	2	1.6	429	PASS
69	198	0.00	100	34.0	26040	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.9	37474	PASS
197	198	0.00	2	0.3	208	PASS
198	198	100	100	100.0	76661	PASS
199	198	5	9	6.6	5081	PASS
275	198	10	60	23.5	18042	PASS
365	198	1	100	2.5	1899	PASS
441	442	0.01	24	15.6	10745	PASS
442	198	50	100	89.6	68669	PASS
443	442	15	24	19.9	13641	PASS