


Data Path : Z:\HPCHEM1\BNA_F\Data\BF050317\
 Data File : BF094861.D
 Acq On : 4 May 2017 6:42
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 03 17:24:51 2017

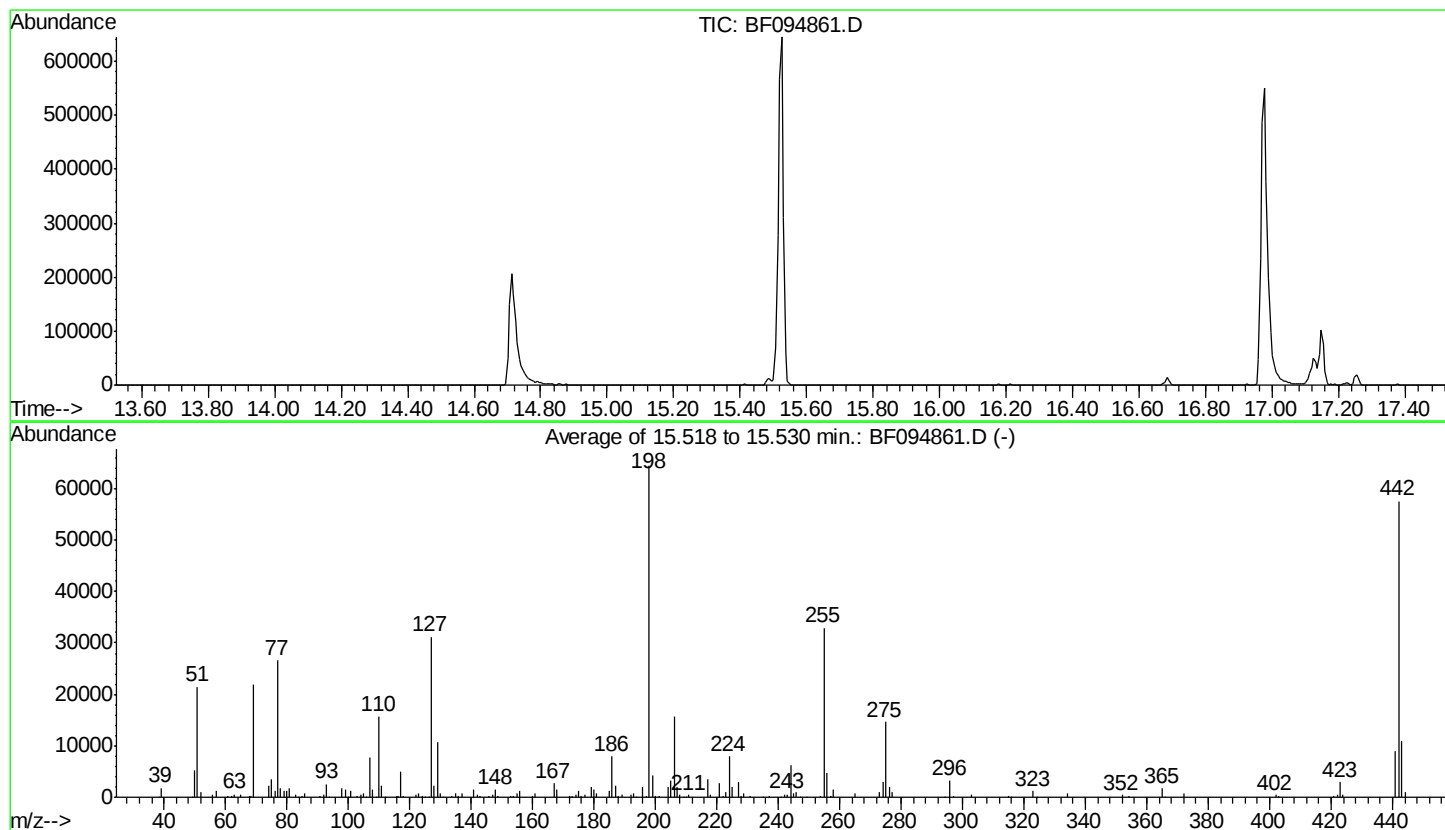

AutoFind: Scans 2309, 2310, 2311; Background Corrected with Scan 2303

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	21532	PASS
68	69	0.00	2	1.0	213	PASS
69	198	0.00	100	34.1	21972	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.4	31187	PASS
197	198	0.00	2	0.3	171	PASS
198	198	100	100	100.0	64464	PASS
199	198	5	9	6.7	4346	PASS
275	198	10	60	22.6	14578	PASS
365	198	1	100	2.6	1649	PASS
441	442	0.01	24	15.6	8988	PASS
442	198	50	100	89.3	57565	PASS
443	442	15	24	19.1	11003	PASS