

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050318\
 Data File : BF105079.D
 Acq On : 3 May 2018 18:16
 Operator : JU/SJ
 Sample : PB108708BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: May 04 01:56:53 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 02 17:25:18 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.78	152	104910	20.00	ng	0.00
21) Naphthalene-d8	8.06	136	447033	20.00	ng	-0.01
38) Acenaphthene-d10	9.82	164	221324	20.00	ng	-0.01
63) Phenanthrene-d10	11.31	188	439363	20.00	ng	-0.01
75) Chrysene-d12	14.00	240	343449	20.00	ng	-0.03
86) Perylene-d12	15.55	264	256468	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	787856	114.83	ng	0.01
7) Phenol-d6	6.43	99	940546	111.57	ng	0.00
23) Nitrobenzene-d5	7.35	82	560475	81.87	ng	-0.02
41) 2,4,6-Tribromophenol	10.62	330	276613	120.48	ng	-0.01
44) 2-Fluorobiphenyl	9.14	172	1119556	79.91	ng	-0.02
78) Terphenyl-d14	12.90	244	1229752	81.63	ng	-0.01
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.35	70	73055	13.26	ng	# 71
25) Isophorone	7.35	82	560470	38.71	ng	# 64
50) 2,6-Dinitrotoluene	9.82	165	27925	8.65	ng	# 25
56) 2,4-Dinitrotoluene	9.82	165	27925	6.59	ng	# 23
64) 4,6-Dinitro-2-methylphenol	10.62	198	384	7.50	ng	# 11
66) 4-Bromophenyl-phenylether	10.62	248	17116	3.66	ng	# 1
76) Benizidine	12.90	184	16307	Below Cal		98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF050318\
Data File : BF105079.D
Acq On : 3 May 2018 18:16
Operator : JU/SJ
Sample : PB108708BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: May 04 01:56:53 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 02 17:25:18 2018
Response via : Initial Calibration

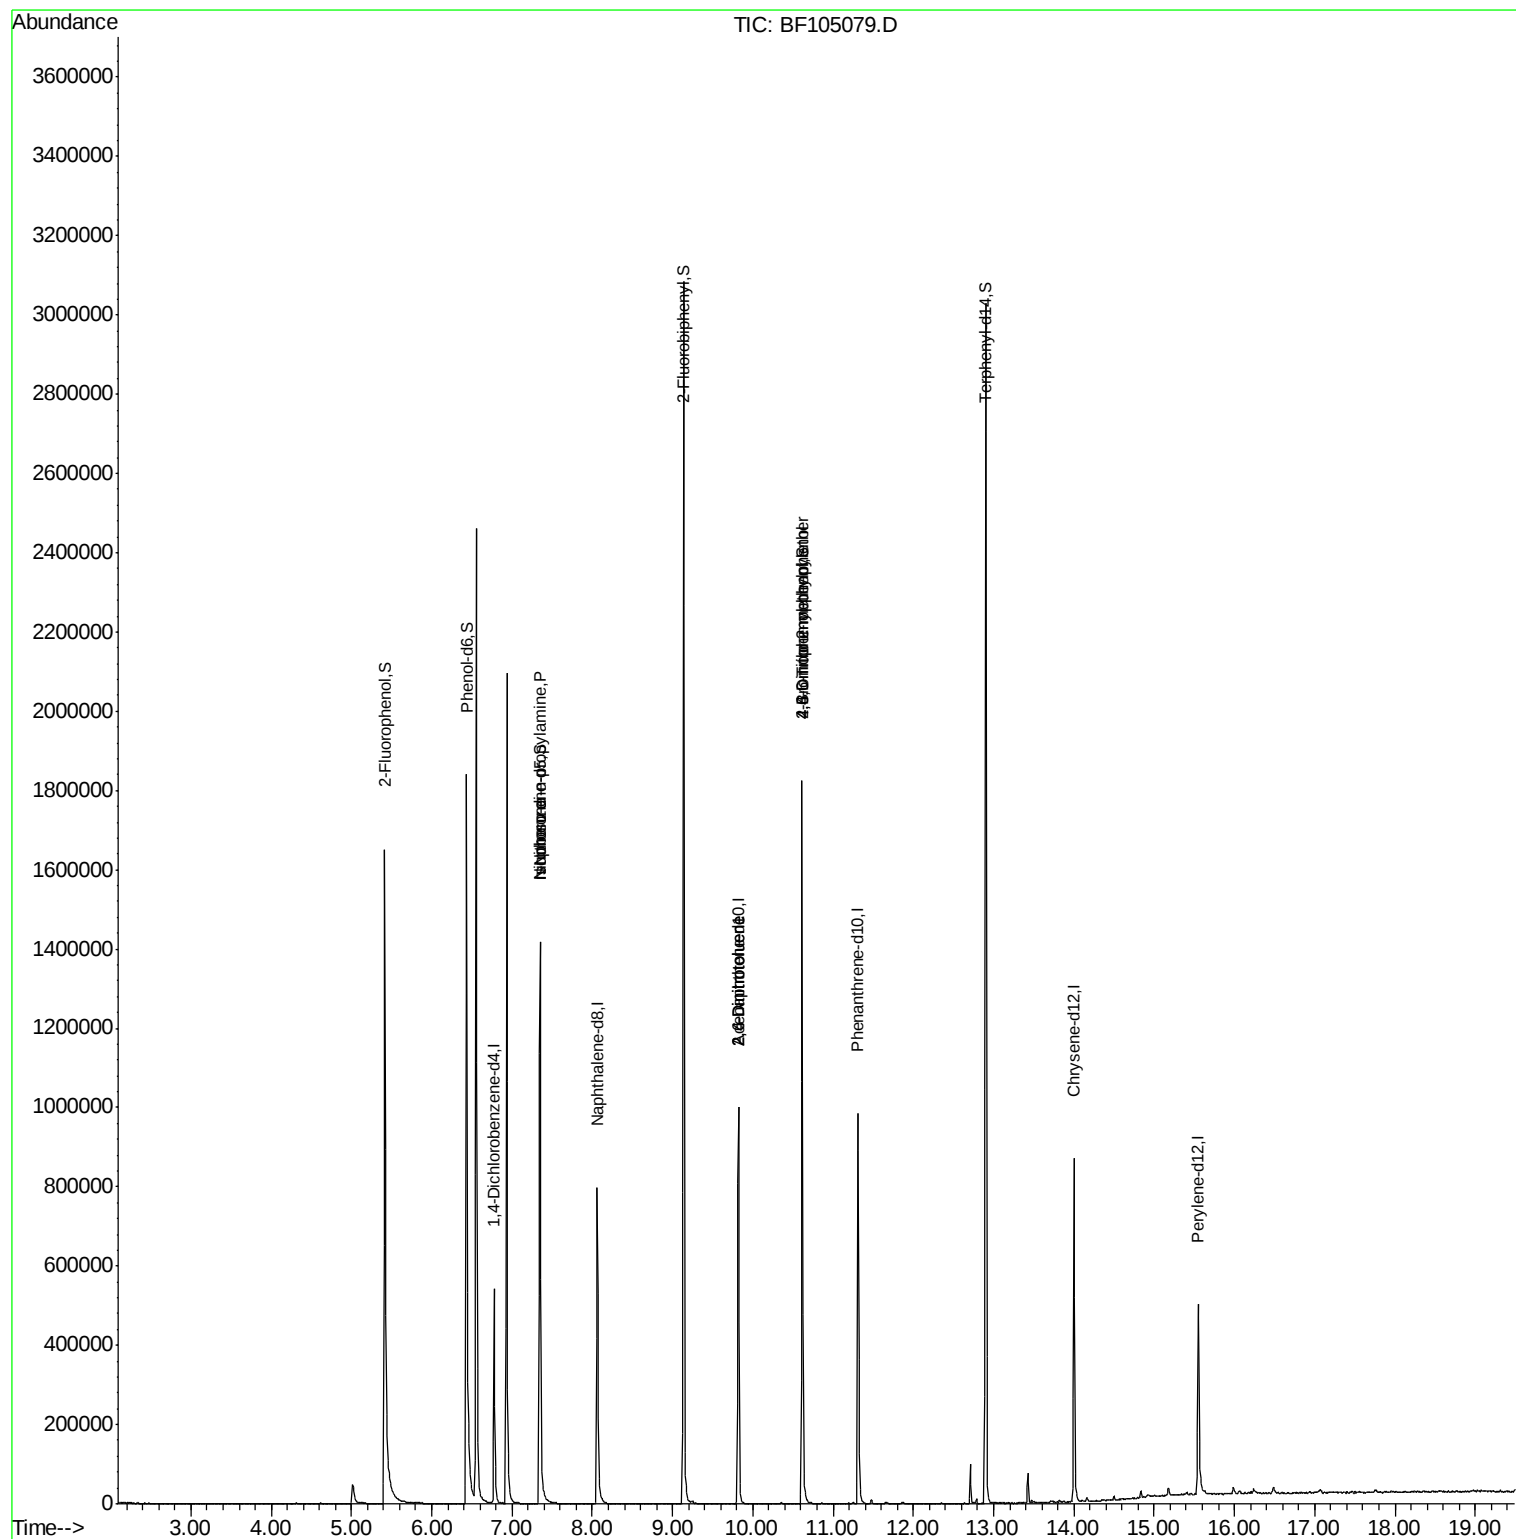

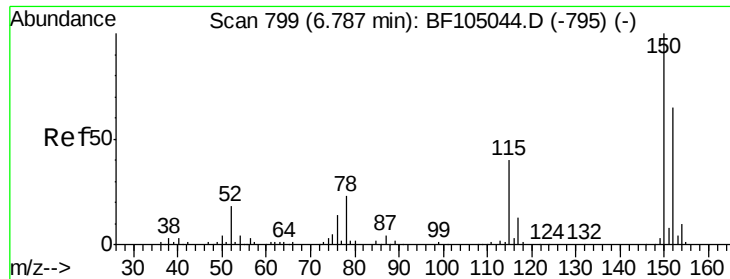


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.78 min Scan# 798
Delta R.T. -0.01 min
Lab File: BF105079.D
Acq: 3 May 2018 18:16

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 104910
Ion Ratio Lower Upper
152 100
150 158.6 124.6 186.8
115 60.0 50.1 75.1

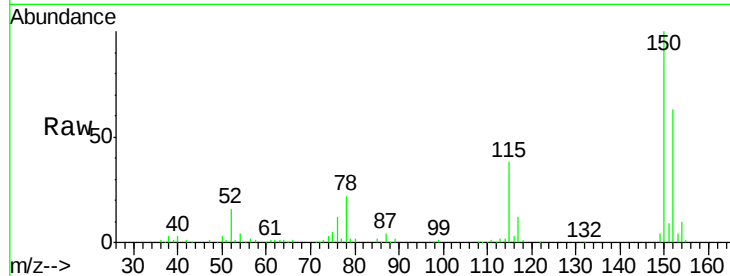


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

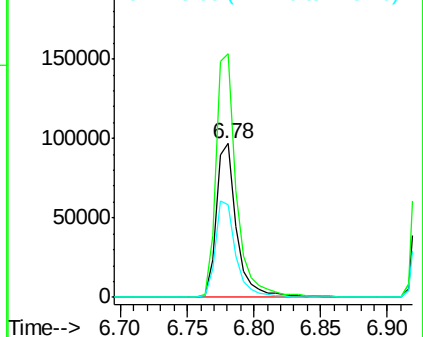



#5


2-Fluorophenol
Concen: 114.83 ng
RT: 5.42 min Scan# 566
Delta R.T. 0.01 min
Lab File: BF105079.D
Acq: 3 May 2018 18:16

Tgt Ion:112 Resp: 787856
Ion Ratio Lower Upper
112 100
64 51.7 47.9 71.9
63 26.3 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

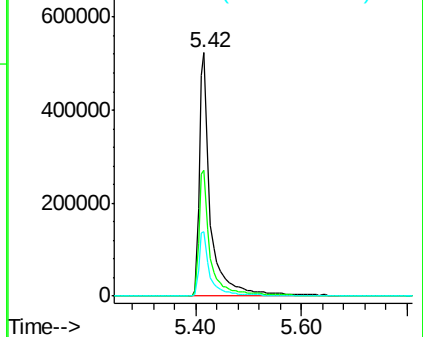

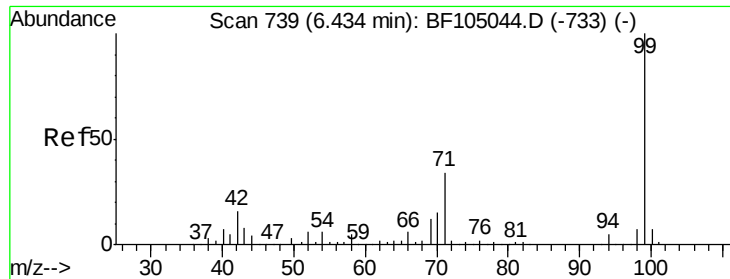

#7

Phenol-d6

Concen: 111.57 ng

RT: 6.43 min Scan# 739

Delta R.T. -0.01 min

Lab File: BF105079.D

Acq: 3 May 2018 18:16

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 940546

Ion Ratio Lower Upper

99 100

42 15.5 14.5 21.7




71 34.4 25.4 38.0



Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

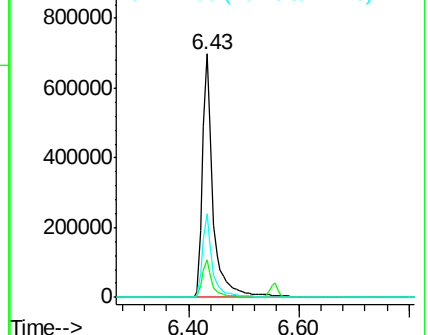

#19

n-Nitroso-di-n-propylamine

Concen: 13.26 ng

RT: 7.35 min Scan# 895

Delta R.T. 0.14 min

Lab File: BF105079.D

Acq: 3 May 2018 18:16

Tgt Ion: 70 Resp: 73055


Ion Ratio Lower Upper

70 100

42 39.5 47.5 71.3#

101 0.0 7.4 11.2#

130 2.6 16.6 25.0#






Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

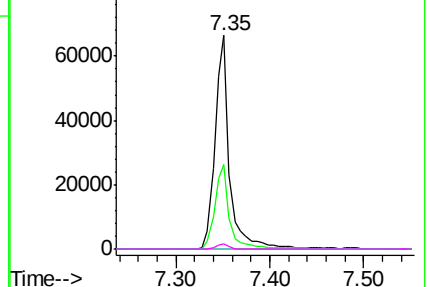


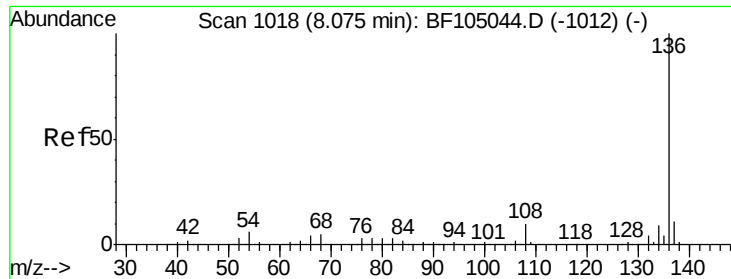




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.06 min Scan# 1016
Delta R.T. -0.01 min
Lab File: BF105079.D
Acq: 3 May 2018 18:16

Instrument :
BNA_F
ClientSampleId :

Tot Ion:136	Resp:	447033
Ion Ratio	Lower	Upper
136	100	
137	11.3	8.9 13.3
54	6.1	6.6 9.8#
68	5.4	5.0 7.4

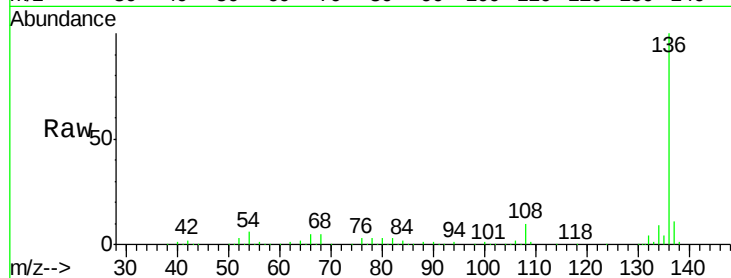


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

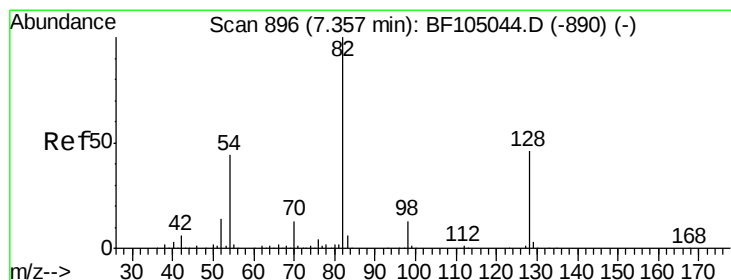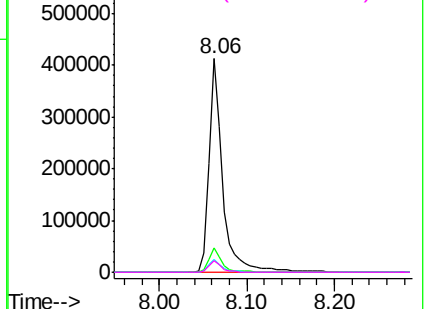
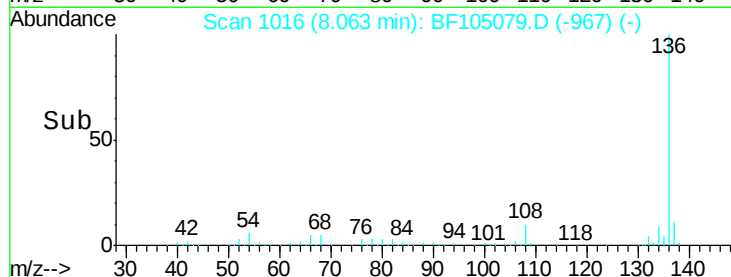



#23
Nitrobenzene-d5
Concen: 81.87 ng
RT: 7.35 min Scan# 895
Delta R.T. -0.02 min
Lab File: BF105079.D
Acq: 3 May 2018 18:16

Tgt Ion: 82	Resp:	560475
Ion Ratio	Lower	Upper
82	100	
128	48.5	36.1 54.1
54	43.9	41.4 62.2

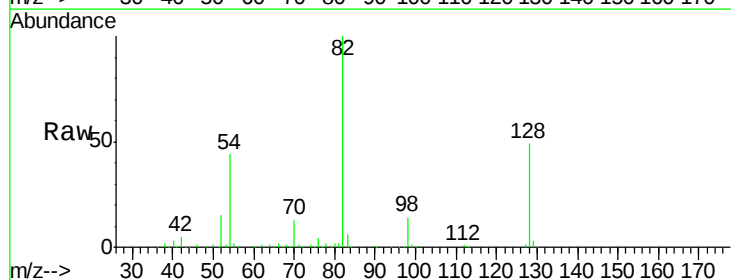

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

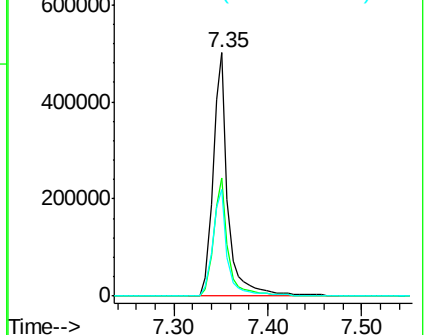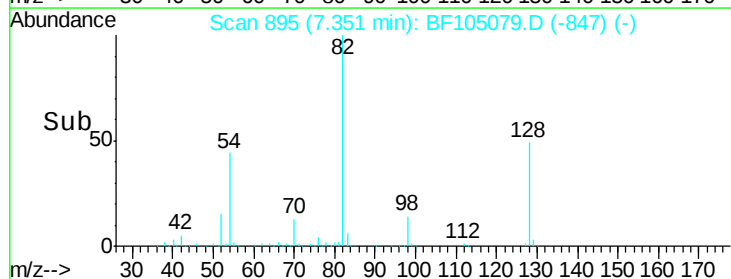

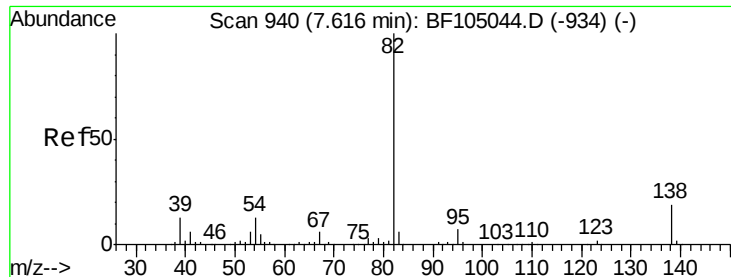

#25

Isophorone

Concen: 38.71 ng

RT: 7.35 min Scan# 895

Delta R.T. -0.27 min

Lab File: BF105079.D

Acq: 3 May 2018 18:16

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 560470

Ion Ratio Lower Upper

82 100

95 0.0 5.2 7.8#




138 0.0 14.9 22.3#

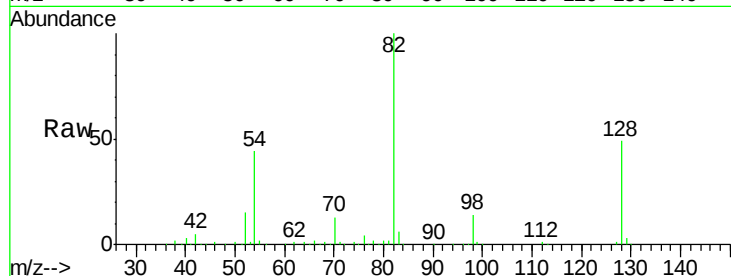

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

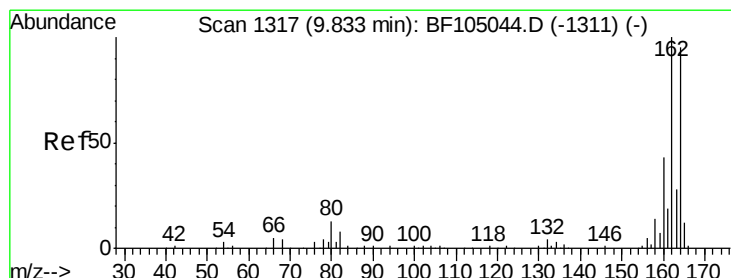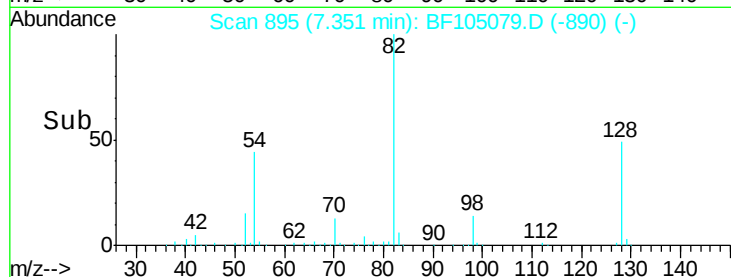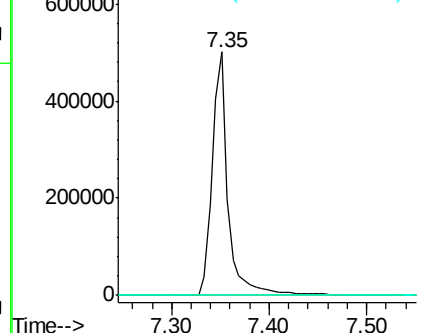

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.82 min Scan# 1315

Delta R.T. -0.01 min

Lab File: BF105079.D

Acq: 3 May 2018 18:16


Tgt Ion:164 Resp: 221324

Ion Ratio Lower Upper

164 100

162 104.4 86.1 129.1



160 46.7 38.3 57.5

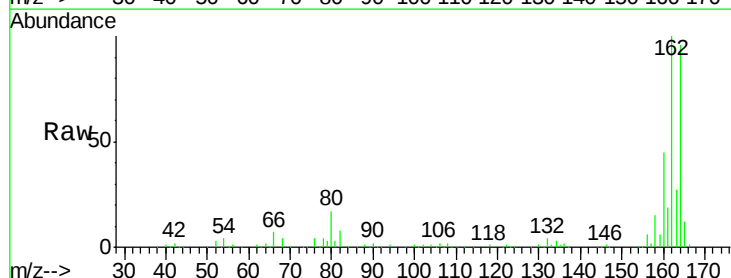


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

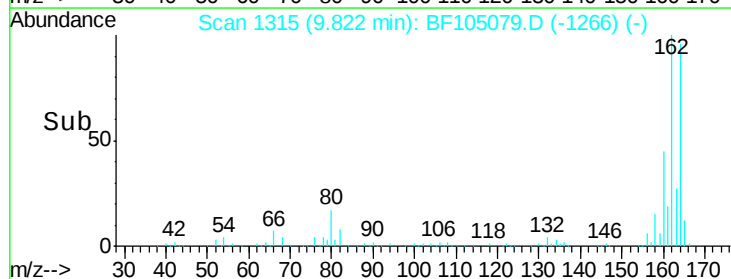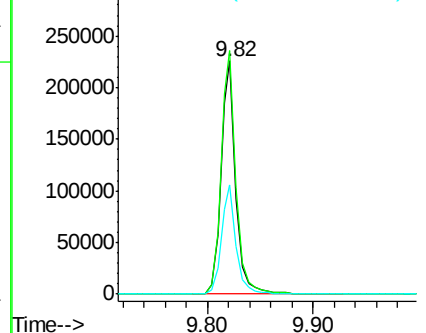







#41
 2,4,6-Tribromophenol
 Concen: 120.48 ng
 RT: 10.62 min Scan# 1451
 Delta R.T. -0.01 min
 Lab File: BF105079.D
 Acq: 3 May 2018 18:16

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.6	77.0	115.6
141	33.3	29.9	44.9

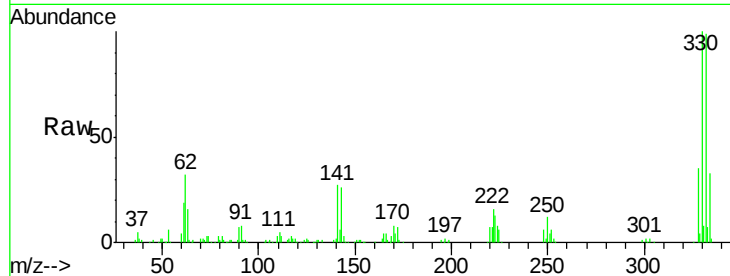


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

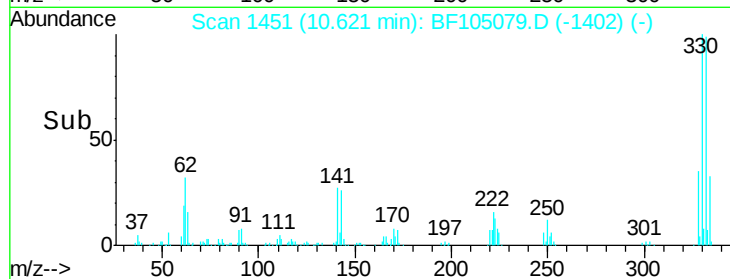
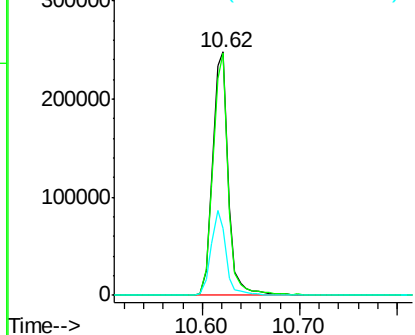



#44
 2-Fluorobiphenyl
 Concen: 79.91 ng
 RT: 9.14 min Scan# 1199
 Delta R.T. -0.02 min
 Lab File: BF105079.D
 Acq: 3 May 2018 18:16

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.0	29.7	44.5
170	23.7	19.6	29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

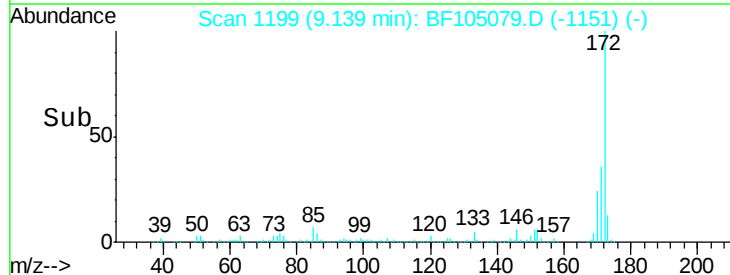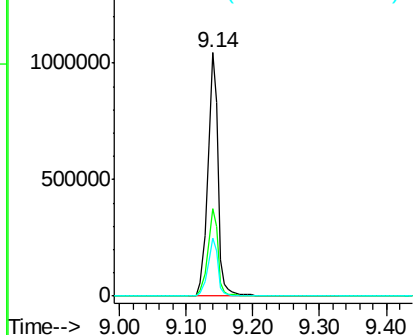


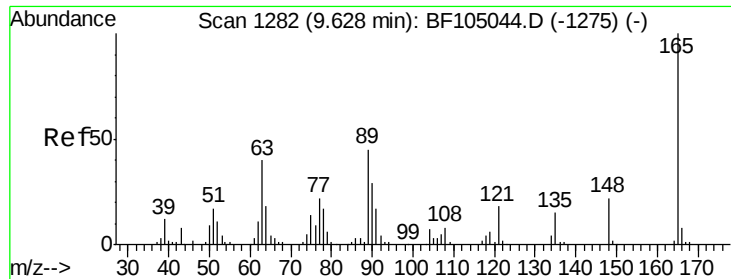

#50
 2,6-Dinitrotoluene
 Concen: 8.65 ng
 RT: 9.82 min Scan# 1315
 Delta R.T. 0.19 min
 Lab File: BF105079.D
 Acq: 3 May 2018 18:16

Instrument :
 BNA_F
 ClientSampleId :




Tot Ion	Ratio	Lower	Upper
165	100		
63	1.2	44.7	67.1#
89	1.4	44.0	66.0#

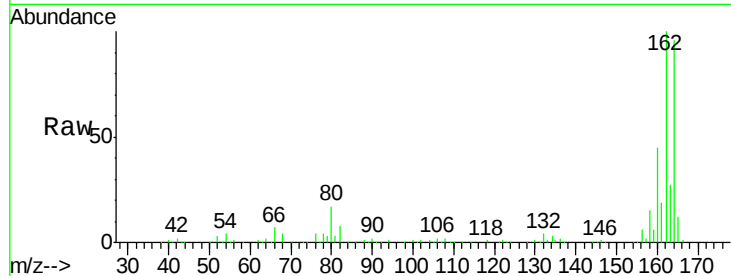

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

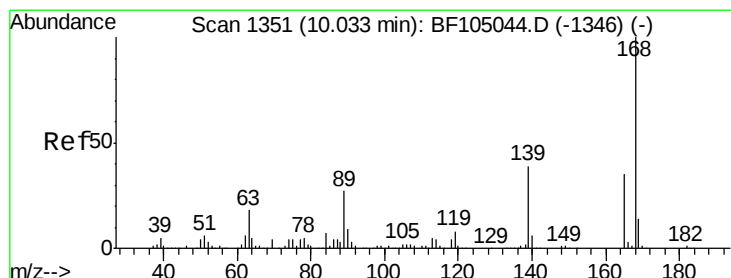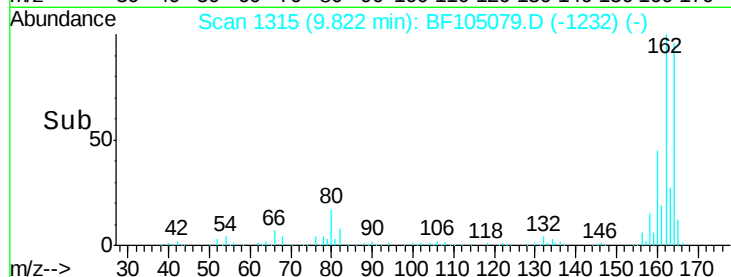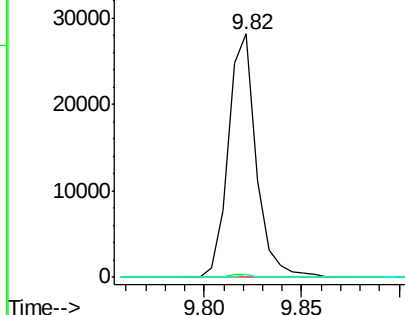

#56
 2,4-Dinitrotoluene
 Concen: 6.59 ng
 RT: 9.82 min Scan# 1315
 Delta R.T. -0.22 min
 Lab File: BF105079.D
 Acq: 3 May 2018 18:16




Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.2	36.4	54.6#
89	1.4	57.8	86.6#
182	0.0	1.6	2.4#


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

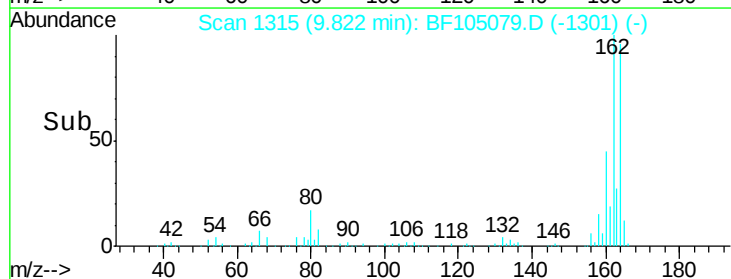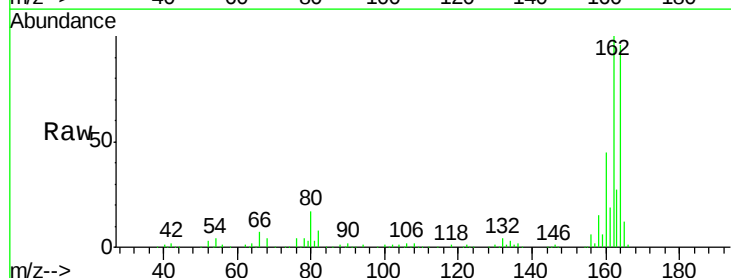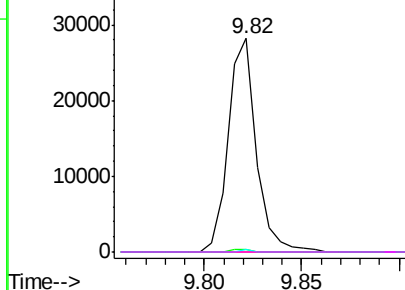







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.31 min Scan# 1568
Delta R.T. -0.01 min
Lab File: BF105079.D
Acq: 3 May 2018 18:16

Instrument :
BNA_F
ClientSampleId :

Tot Ion:188 Resp: 439363
Ion Ratio Lower Upper
188 100
94 10.1 8.5 12.7
80 10.8 9.2 13.8

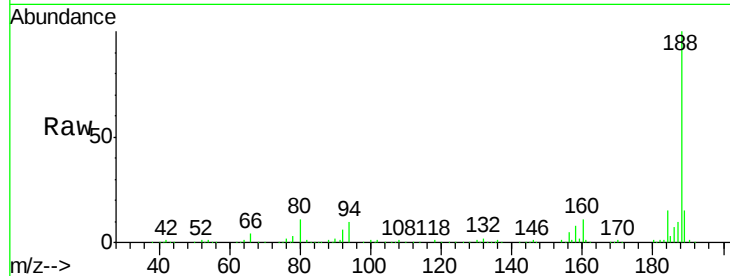


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1


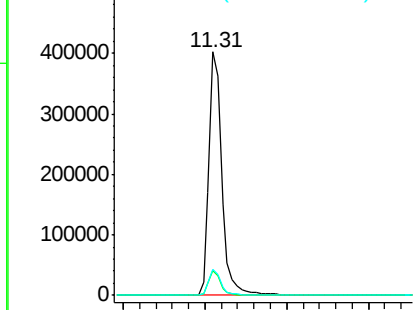



#64
4,6-Dinitro-2-methylphenol
Concen: 7.50 ng
RT: 10.62 min Scan# 1451
Delta R.T. 0.17 min
Lab File: BF105079.D
Acq: 3 May 2018 18:16

Tgt Ion:198 Resp: 384
Ion Ratio Lower Upper
198 100
51 116.5 37.7 77.7#
105 128.4 36.3 76.3#

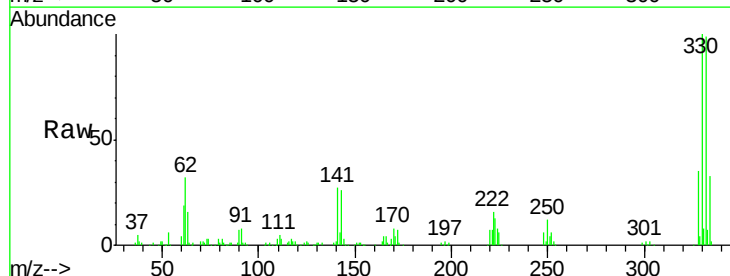

Abundance Ion 198.00 (197.70 to 198.70): E
Ion 51.00 (50.70 to 51.70): BF1
Ion 105.00 (104.70 to 105.70): E

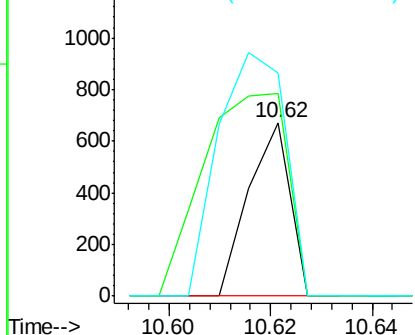


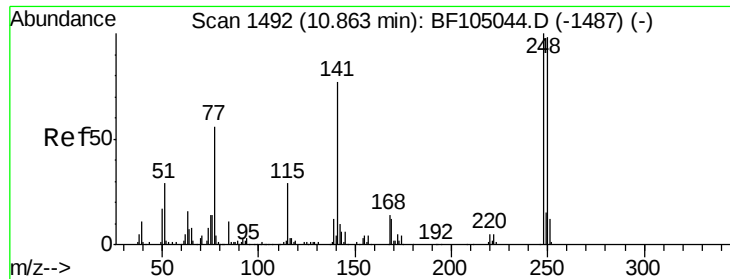




#66
4-Bromophenyl-phenylether
Concen: 3.66 ng
RT: 10.62 min Scan# 1450
Delta R.T. -0.25 min
Lab File: BF105079.D
Acq: 3 May 2018 18:16

Instrument :
BNA_F
ClientSampled :

Tot Ion:248 Resp: 17116
Ion Ratio Lower Upper
248 100
250 188.4 76.9 115.3#
141 557.8 74.4 111.6#

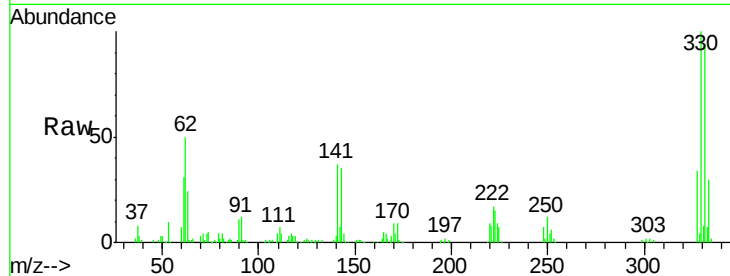


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

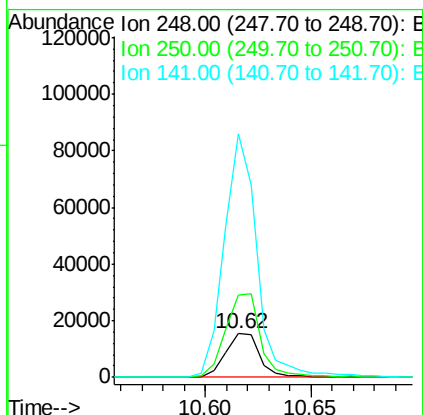




#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.00 min Scan# 2026
Delta R.T. -0.03 min
Lab File: BF105079.D
Acq: 3 May 2018 18:16

Tgt Ion:240 Resp: 343449
Ion Ratio Lower Upper
240 100
120 12.3 9.5 14.3
236 26.2 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

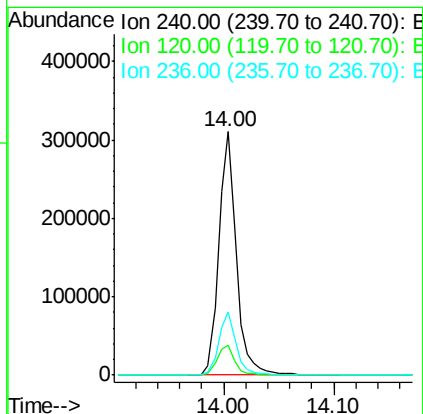

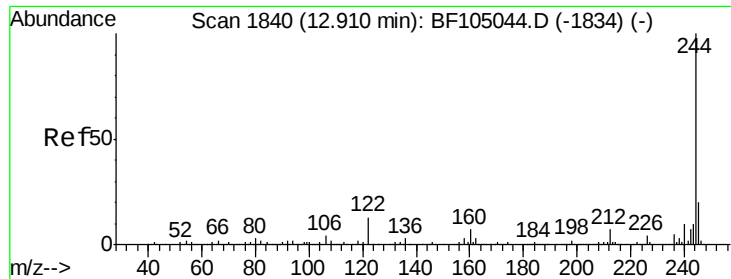

#78

Terphenyl-d14

Concen: 81.63 ng

RT: 12.90 min Scan# 1839

Delta R.T. -0.01 min

Lab File: BF105079.D

Acq: 3 May 2018 18:16

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 1229752

Ion Ratio Lower Upper

244 100

212 7.0 5.4 8.0




122 12.9 11.0 16.4

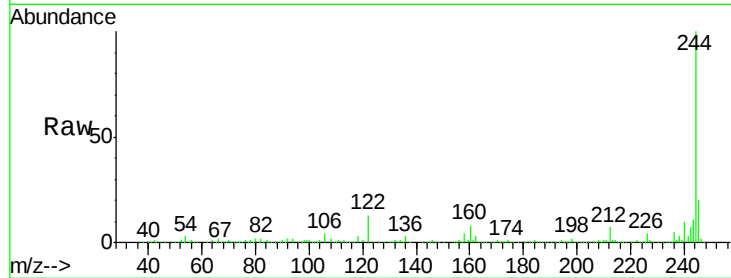

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

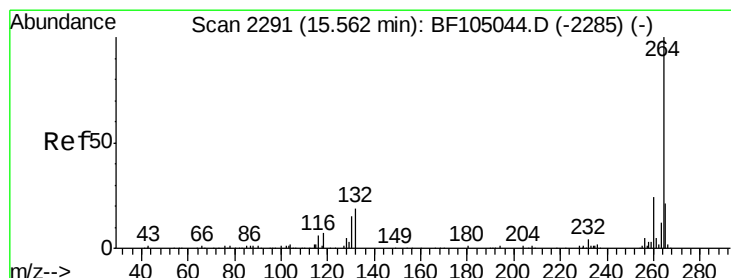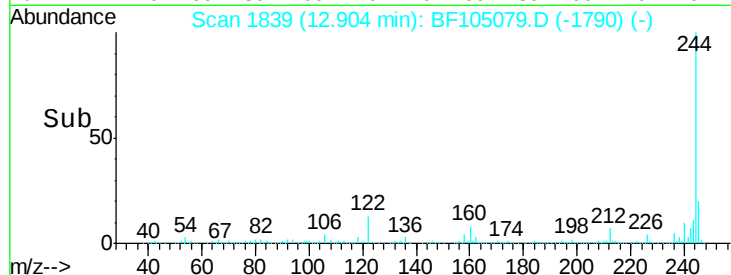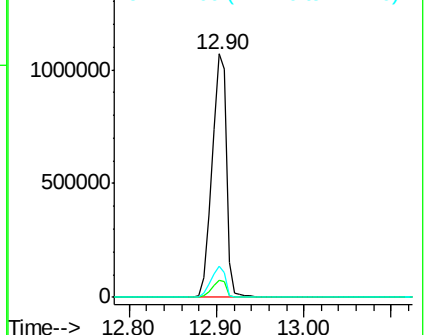

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.55 min Scan# 2289

Delta R.T. -0.04 min

Lab File: BF105079.D

Acq: 3 May 2018 18:16


Tgt Ion:264 Resp: 256468

Ion Ratio Lower Upper

264 100

260 24.2 19.2 28.8

265 21.4 17.5 26.3

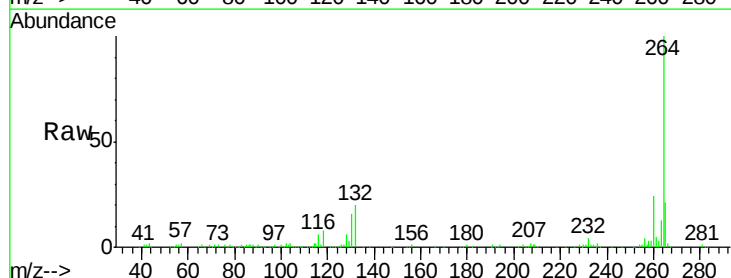

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

