


Data Path : Z:\HPCHEM1\BNA F\Data\BF050318\
 Data File : BF105072.D
 Acq On : 3 May 2018 14:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 02 17:25:18 2018

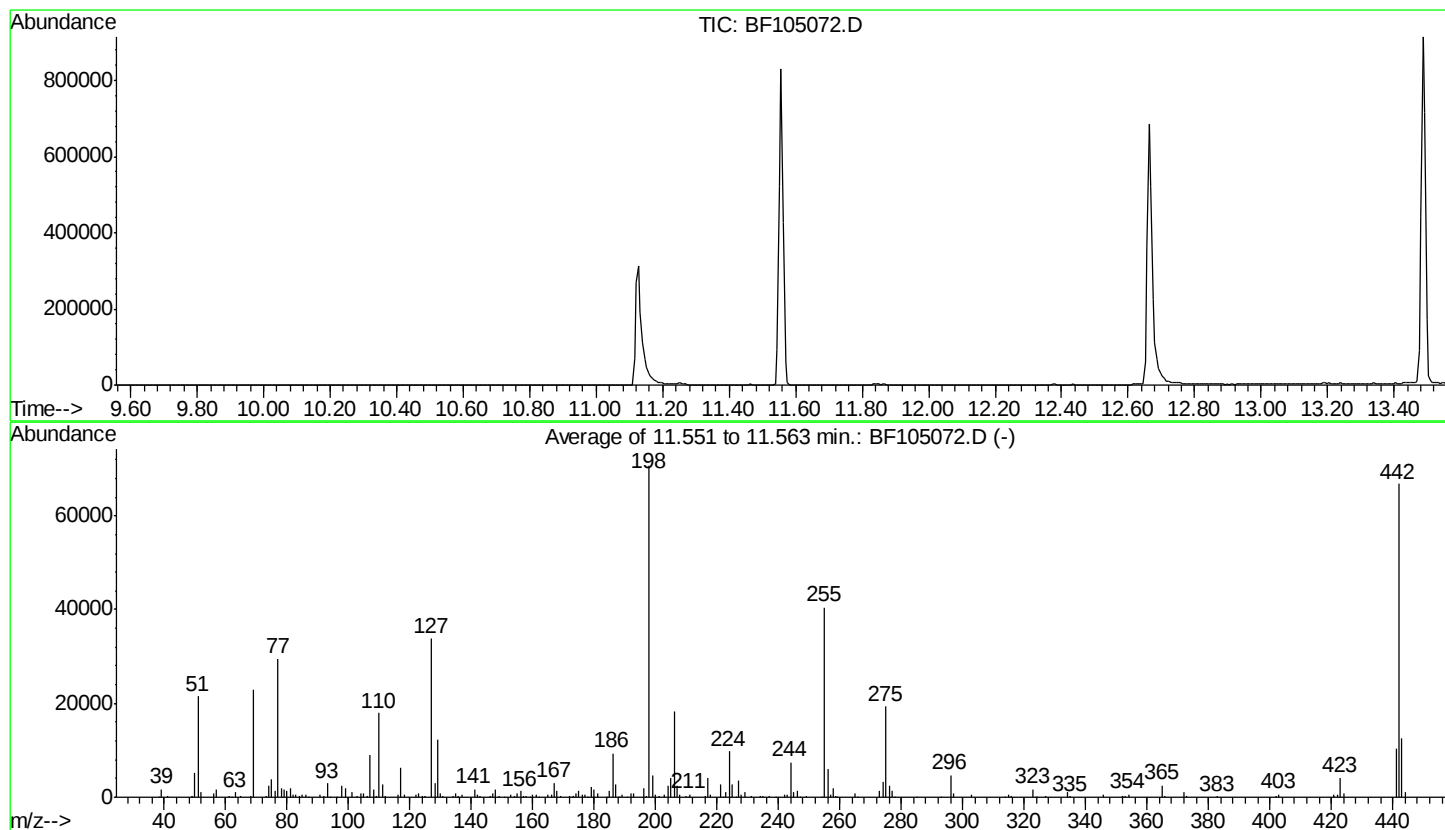

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	21555	PASS
68	69	0.00	2	1.5	339	PASS
69	198	0.00	100	32.5	22977	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	33842	PASS
197	198	0.00	2	0.3	222	PASS
198	198	100	100	100.0	70714	PASS
199	198	5	9	6.8	4787	PASS
275	198	10	60	27.3	19283	PASS
365	198	1	100	3.5	2481	PASS
441	443	0.01	100	83.5	10427	PASS
442	198	50	100	94.4	66754	PASS
443	442	15	24	18.7	12486	PASS