
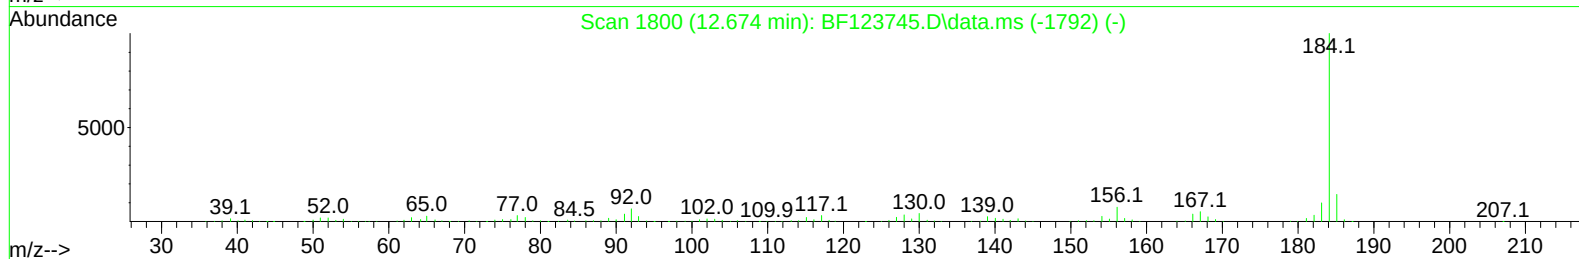
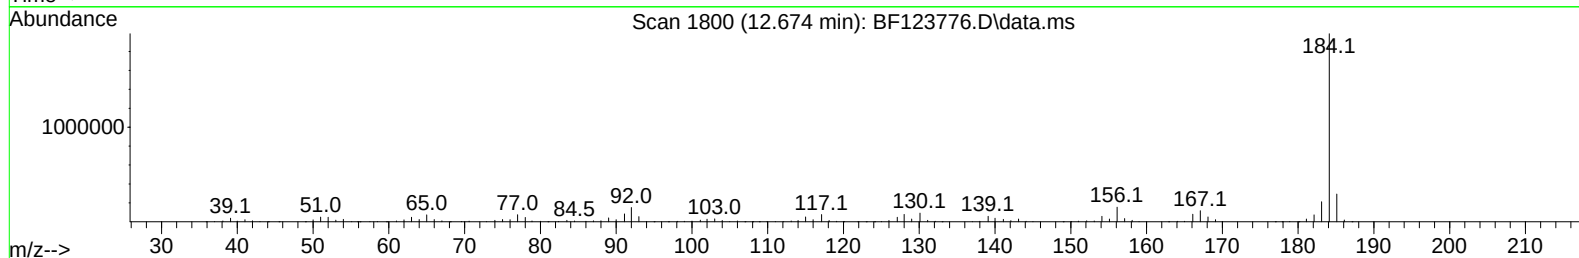


Quant Time: May 03 13:20:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

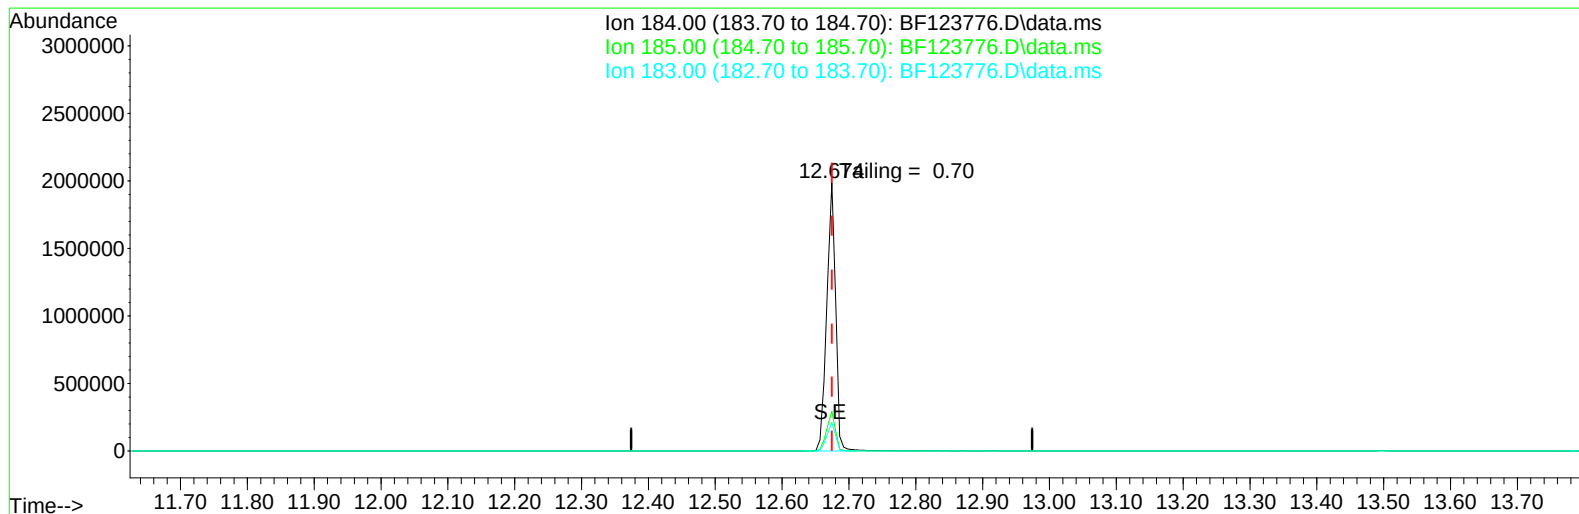

TIC: BF123776.D\data.ms

(77) Benzidine




12.674min (-0.000) 25678.05 ng

response 1841278

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.72
183.00	9.80	10.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050321\
 Data File : BF123776.D
 Acq On : 3 May 2021 12:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 13:20:52 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 27 16:30:39 2021
 Response via : Initial Calibration

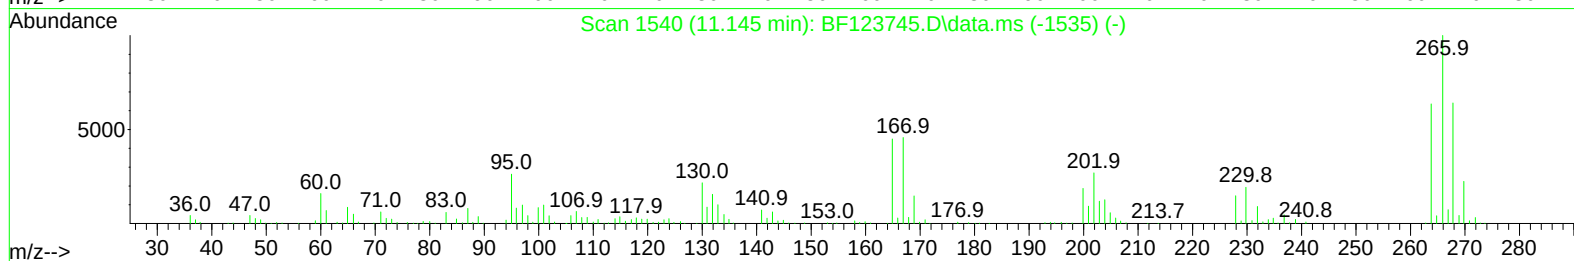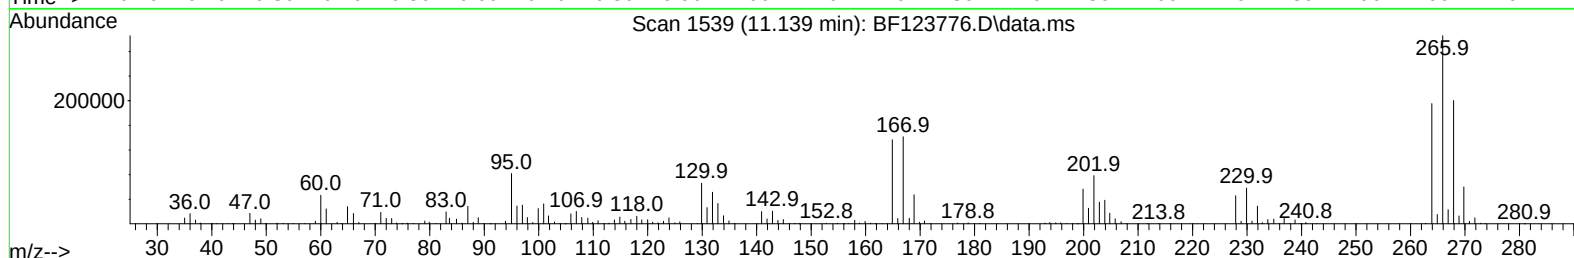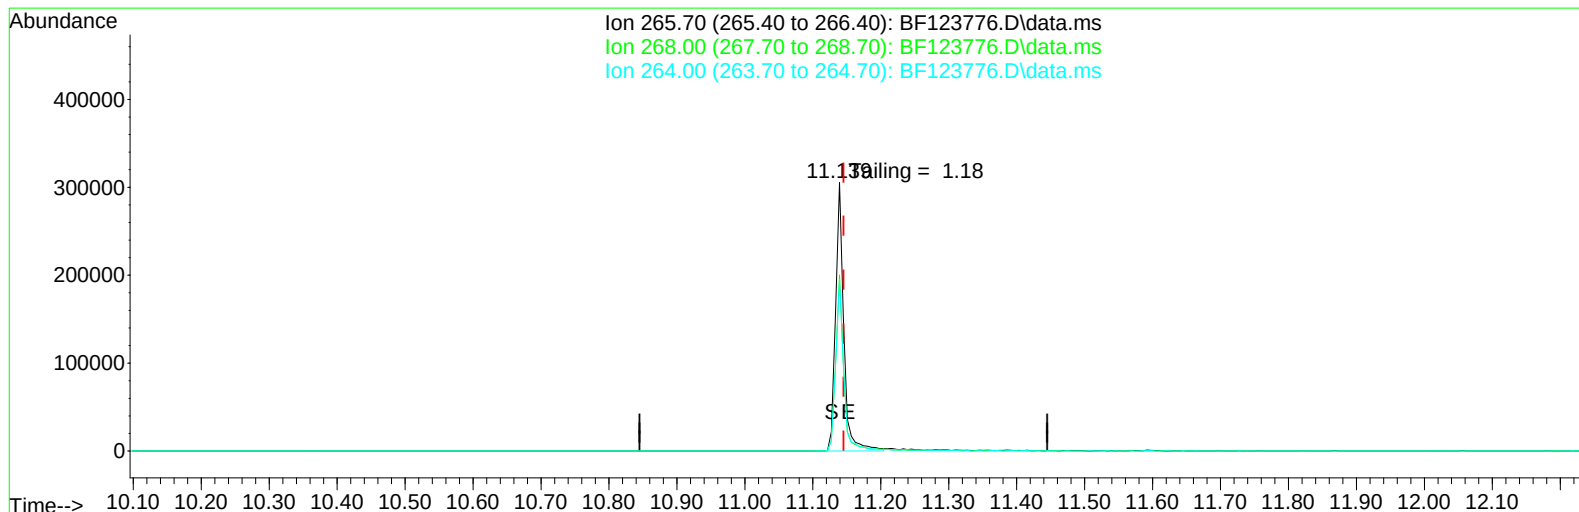

TIC: BF123776.D\data.ms

(70) Pentachlorophenol (C)

11.139min (-0.006) 184737.79 ng

response 259568

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	65.56
264.00	65.70	63.99
0.00	0.00	0.00