




abundance

2500000

Ion 184.00 (183.70 to 184.70): BF123783.D\data.ms

Ion 185.00 (184.70 to 185.70): BF123783.D\data.ms

Ion 183.00 (182.70 to 183.70): BF123783.D\data.ms

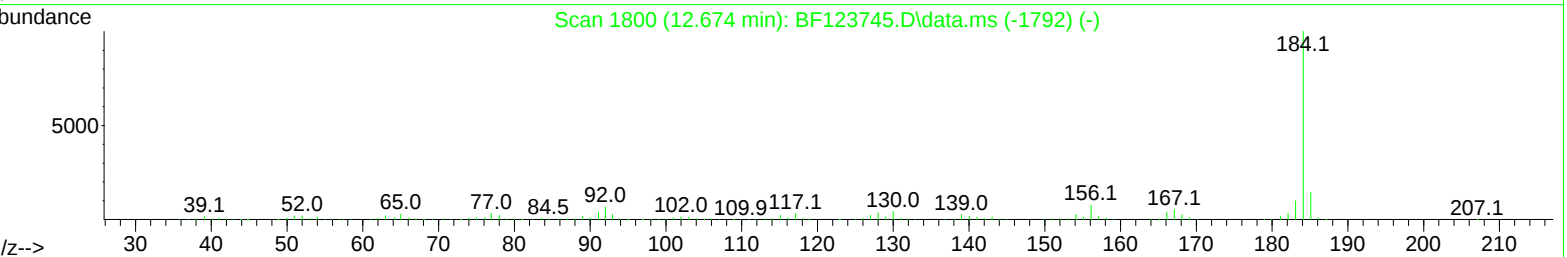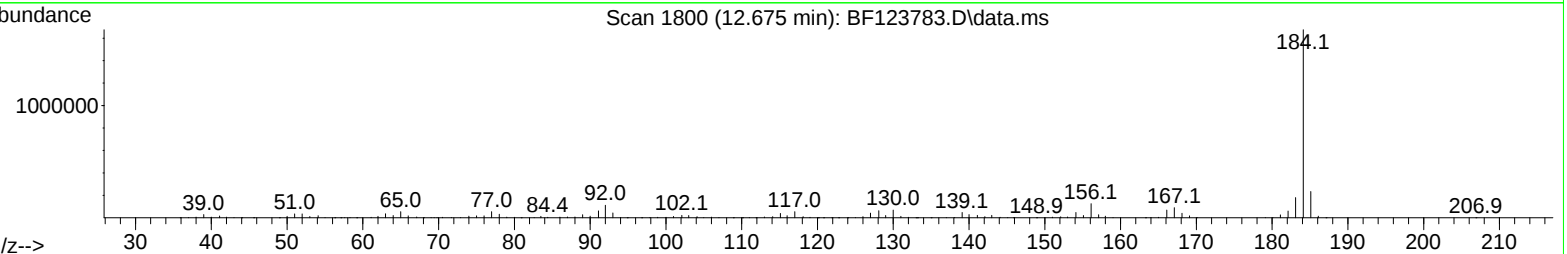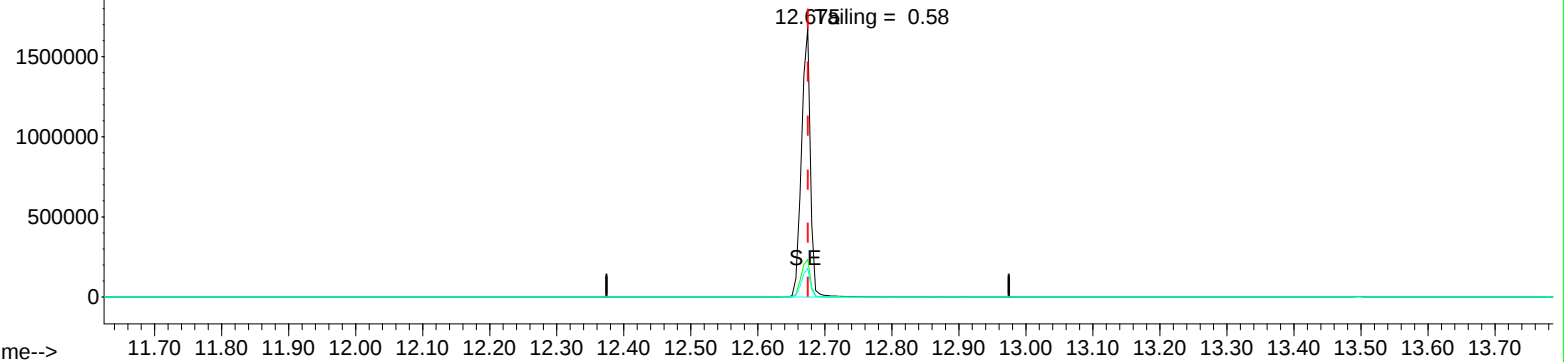

TIC: BF123783.D\data.ms

(77) Benzidine




12.675min (+ 0.000) 0.00 ng

response **1547382**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.98
183.00	9.80	10.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050321\
Data File : BF123783.D
Acq On : 3 May 2021 17:02
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 17:45:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

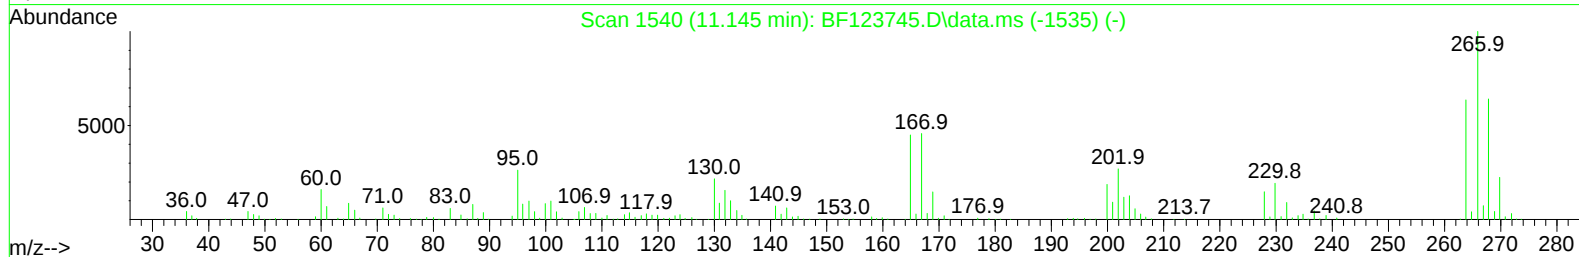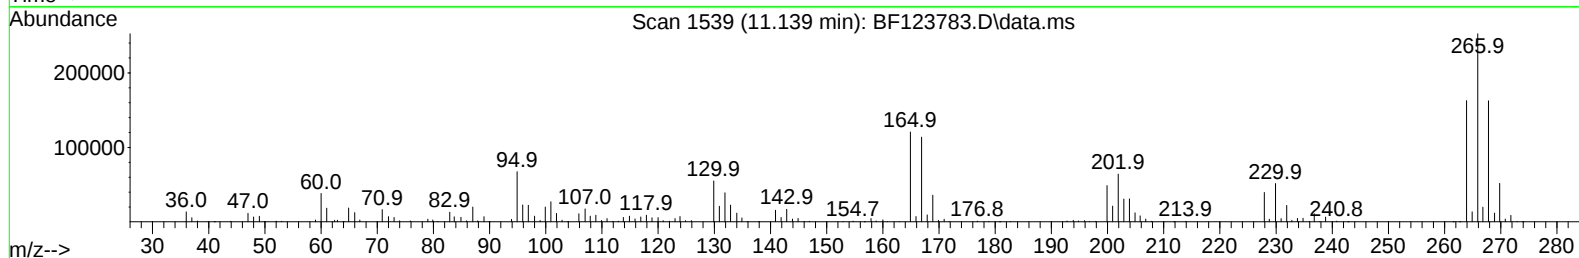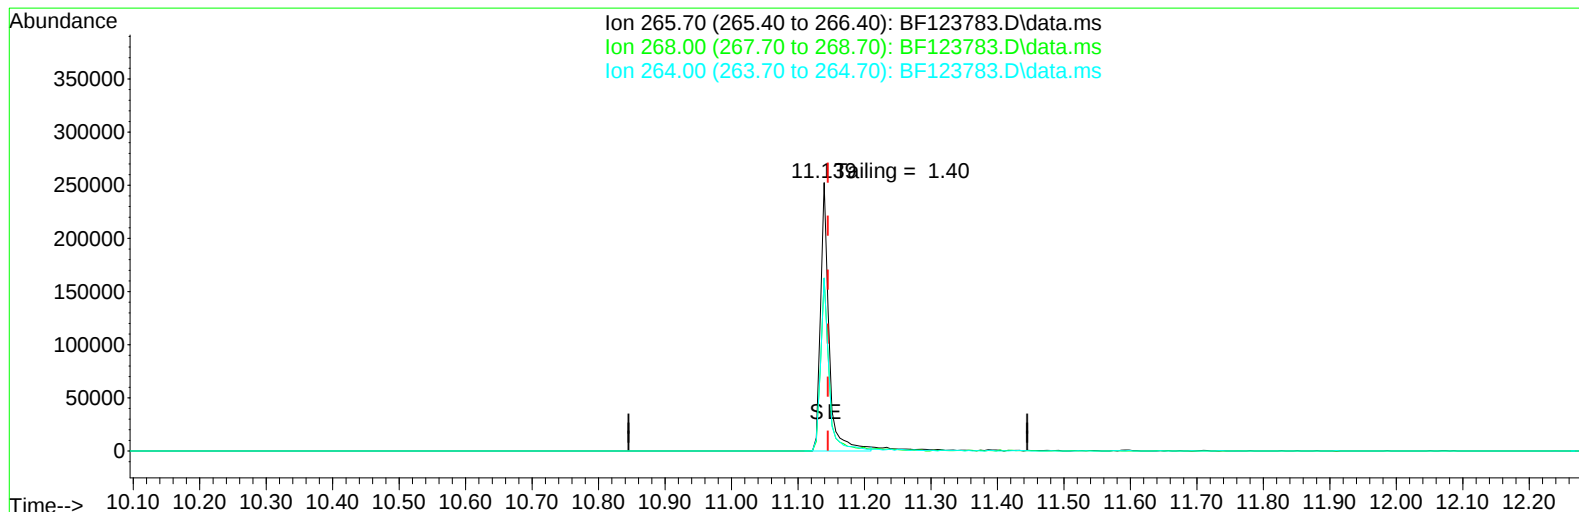

TIC: BF123783.D\data.ms

(70) Pentachlorophenol (C)

11.139min (-0.006) 42028.54 ng

response 233900

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.41
264.00	65.70	64.46
0.00	0.00	0.00