


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050321\
 Data File : BF123776.D
 Acq On : 3 May 2021 12:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 04 12:58:27 2021

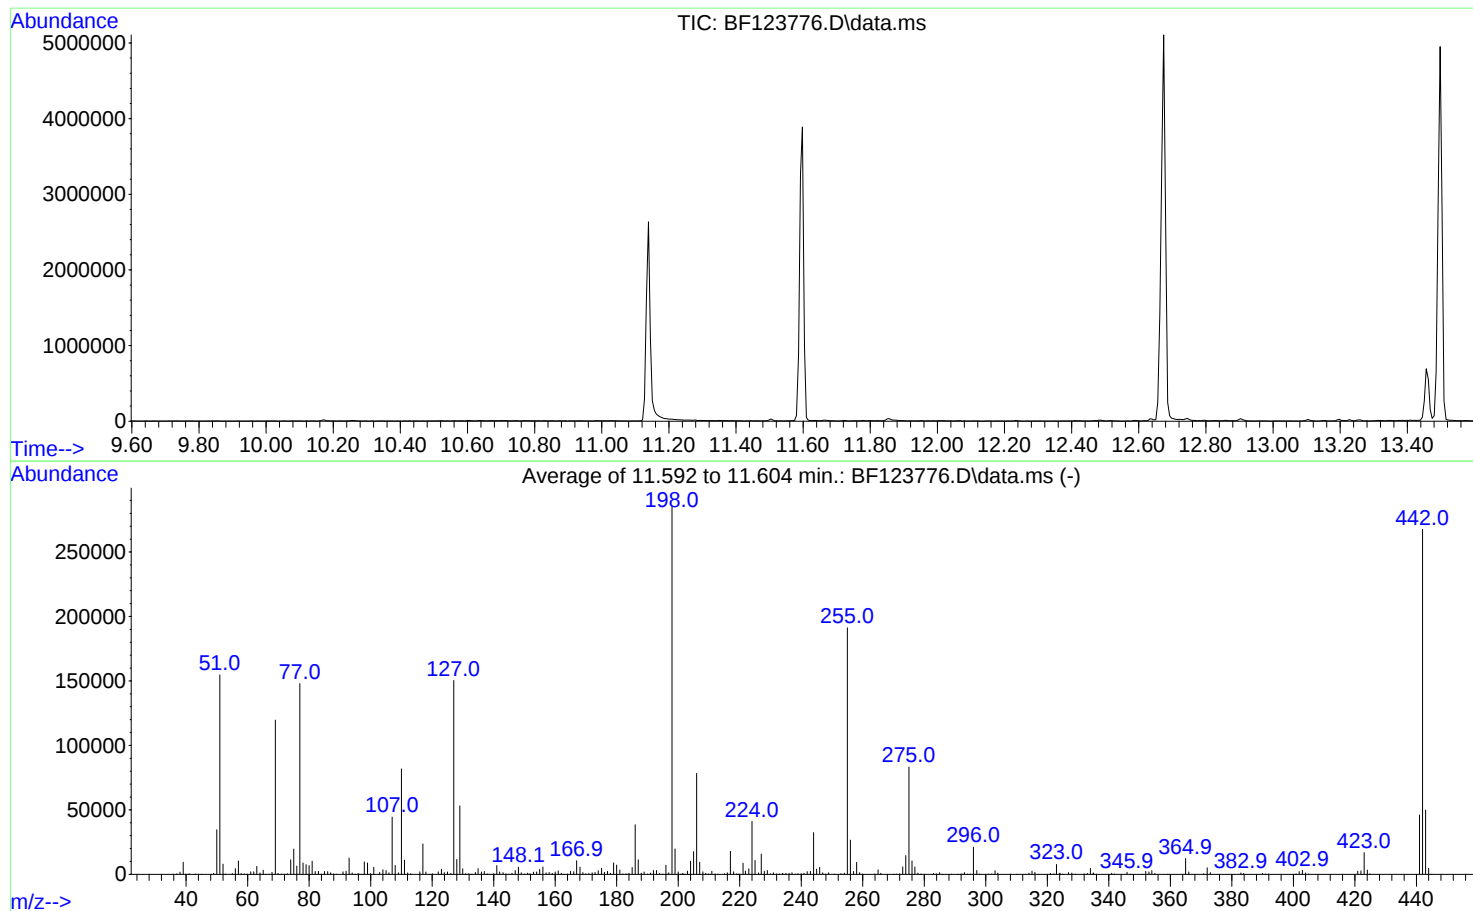

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.2	154688	PASS
68	69	0.00	2	1.3	1580	PASS
69	198	0.00	100	41.9	119603	PASS
70	69	0.00	2	0.6	735	PASS
127	198	10	80	52.7	150389	PASS
197	198	0.00	2	0.4	1244	PASS
198	198	100	100	100.0	285293	PASS
199	198	5	9	6.9	19680	PASS
275	198	10	60	29.2	83256	PASS
365	198	1	100	4.3	12348	PASS
441	198	0.01	100	16.2	46093	PASS
442	442	50	100	100.0	267541	PASS
443	442	15	24	18.6	49896	PASS

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/3/2021	BNA_F	<u>BF123776.D</u>
Compound Name	Response	Retention Time
DDT	762392	13.49
DDD	3891	13.19
DDE	1248	12.85
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5139	767531	0.67

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050321\
 Data File : BF123776.D
 Acq On : 3 May 2021 12:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 03 13:20:52 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 27 16:30:39 2021
 Response via : Initial Calibration

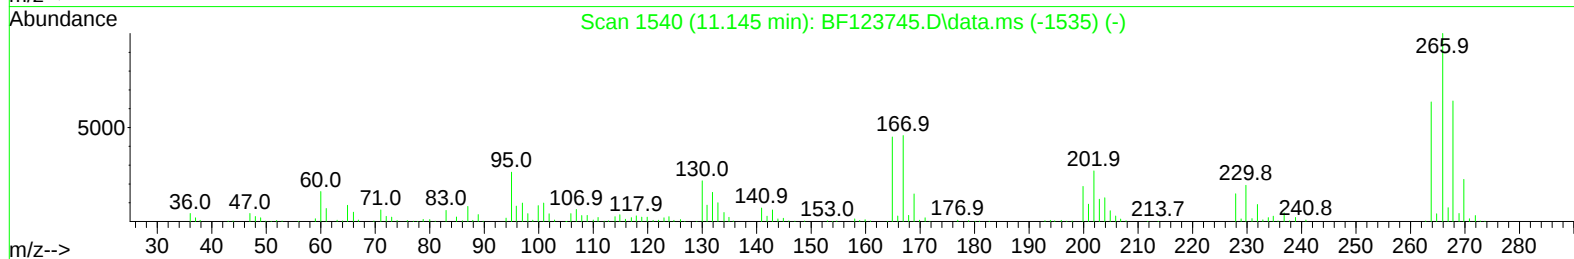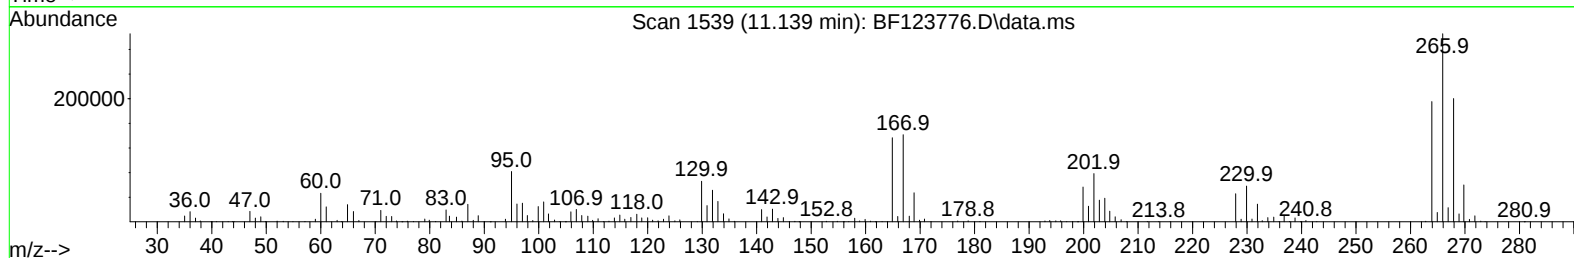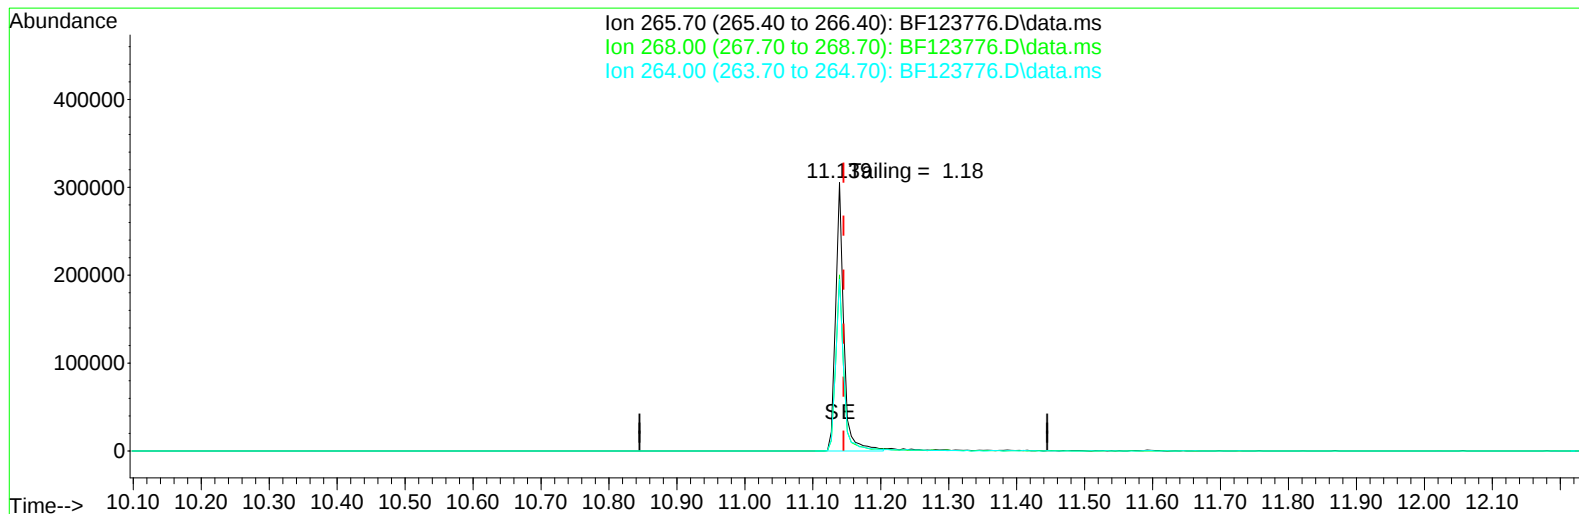

TIC: BF123776.D\data.ms

(70) Pentachlorophenol (C)

11.139min (-0.006) 184737.79 ng




response 259568

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	65.56
264.00	65.70	63.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050321\
Data File : BF123776.D
Acq On : 3 May 2021 12:44
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 03 13:20:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

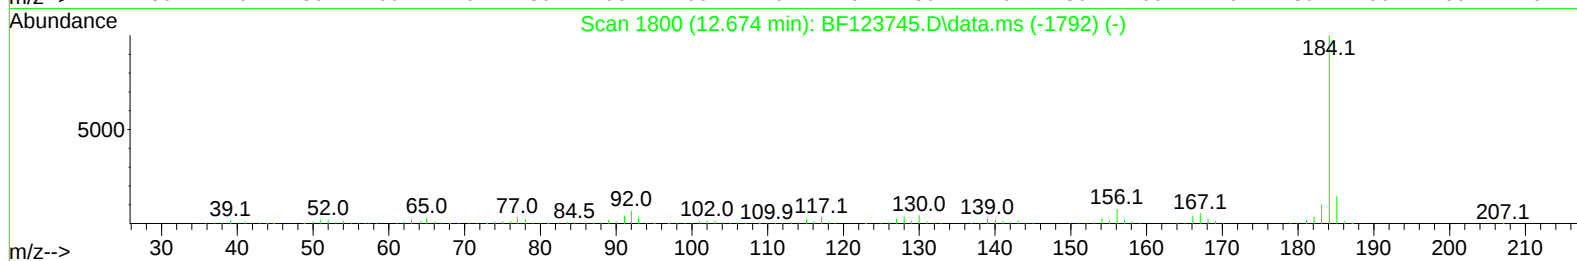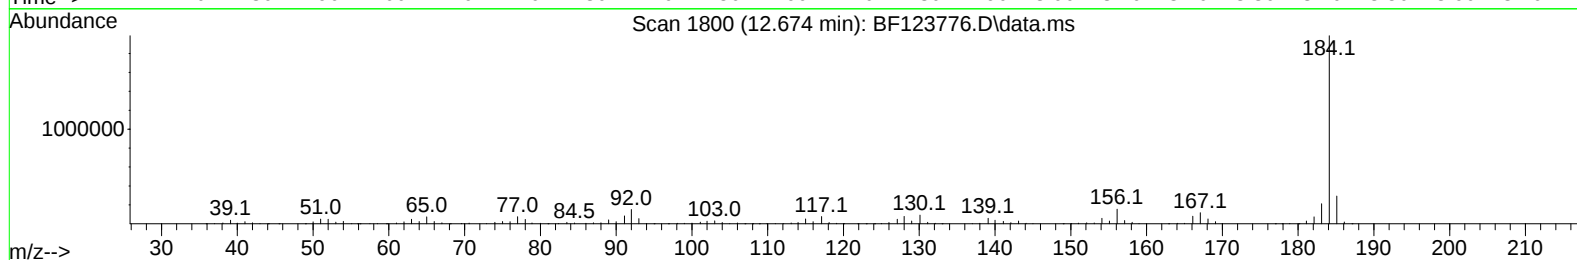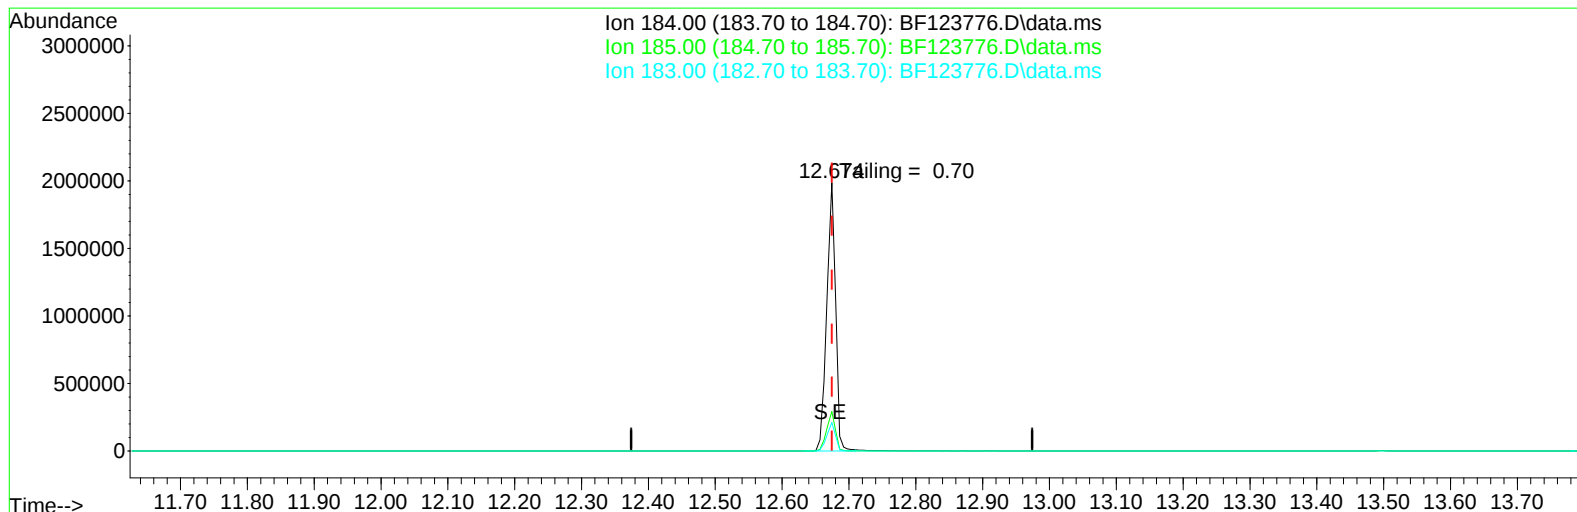

TIC: BF123776.D\data.ms

(77) Benzidine

12.674min (-0.000) 25678.05 ng

response 1841278

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.72
183.00	9.80	10.62
0.00	0.00	0.00