


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050321\
 Data File : BF123783.D
 Acq On : 3 May 2021 17:02
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 04 12:58:27 2021

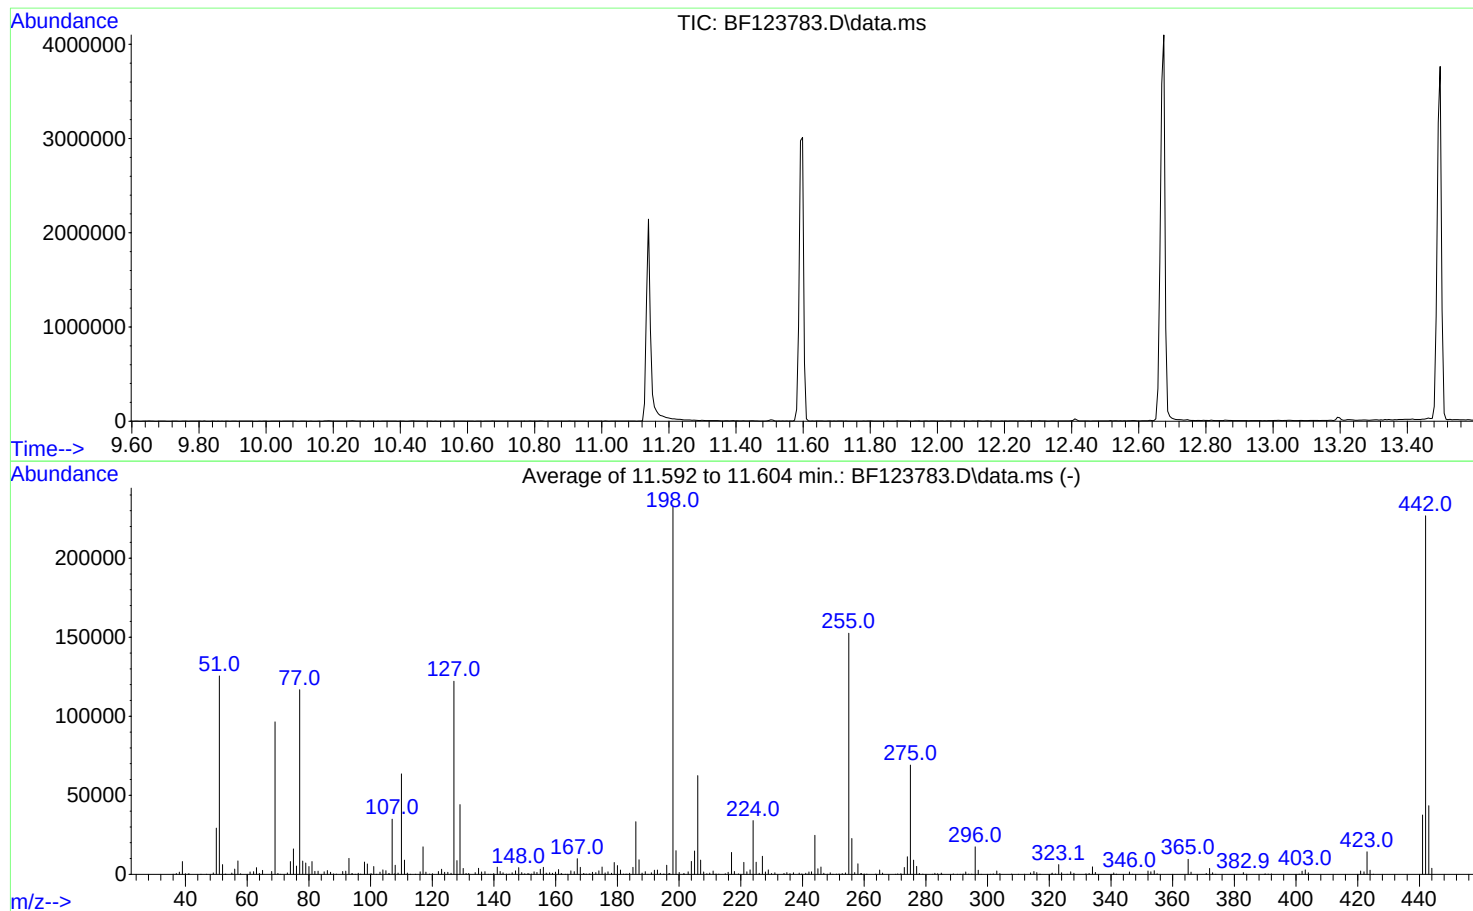

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.0	125549	PASS
68	69	0.00	2	1.9	1862	PASS
69	198	0.00	100	41.5	96484	PASS
70	69	0.00	2	0.6	618	PASS
127	198	10	80	52.5	122152	PASS
197	198	0.00	2	0.3	640	PASS
198	198	100	100	100.0	232680	PASS
199	198	5	9	6.4	15001	PASS
275	198	10	60	29.7	69152	PASS
365	198	1	100	4.1	9550	PASS
441	198	0.01	100	16.1	37528	PASS
442	442	50	100	100.0	226795	PASS
443	442	15	24	19.1	43411	PASS

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/3/2021	BNA_F	<u>BF123783.D</u>
Compound Name	Response	Retention Time
DDT	626927	13.49
DDD	5392	13.49
DDE	829	12.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6221	633148	0.98

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050321\
 Data File : BF123783.D
 Acq On : 3 May 2021 17:02
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 03 17:45:45 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 27 16:30:39 2021
 Response via : Initial Calibration

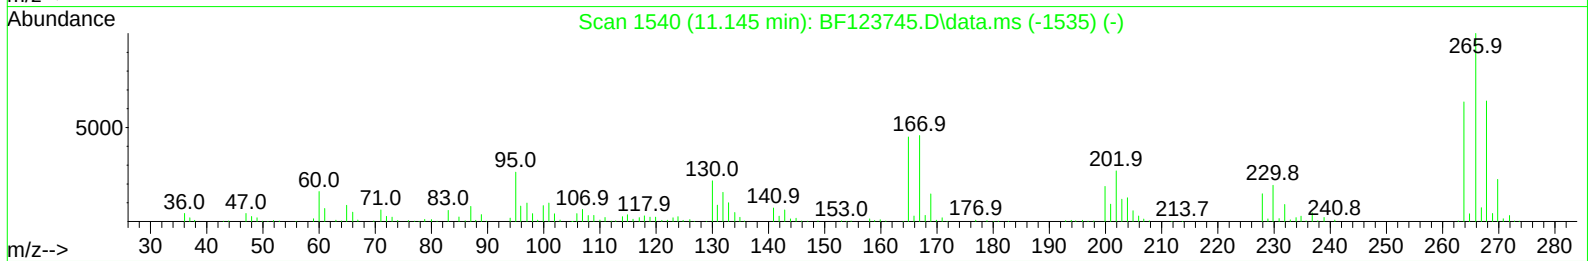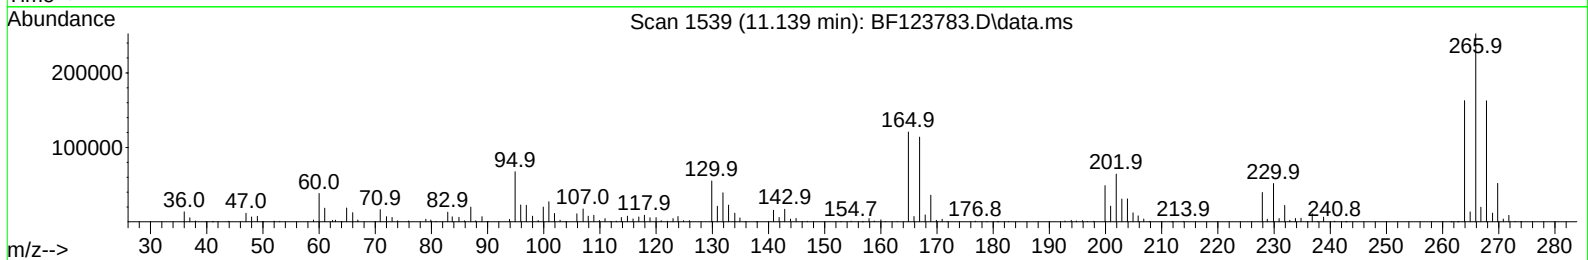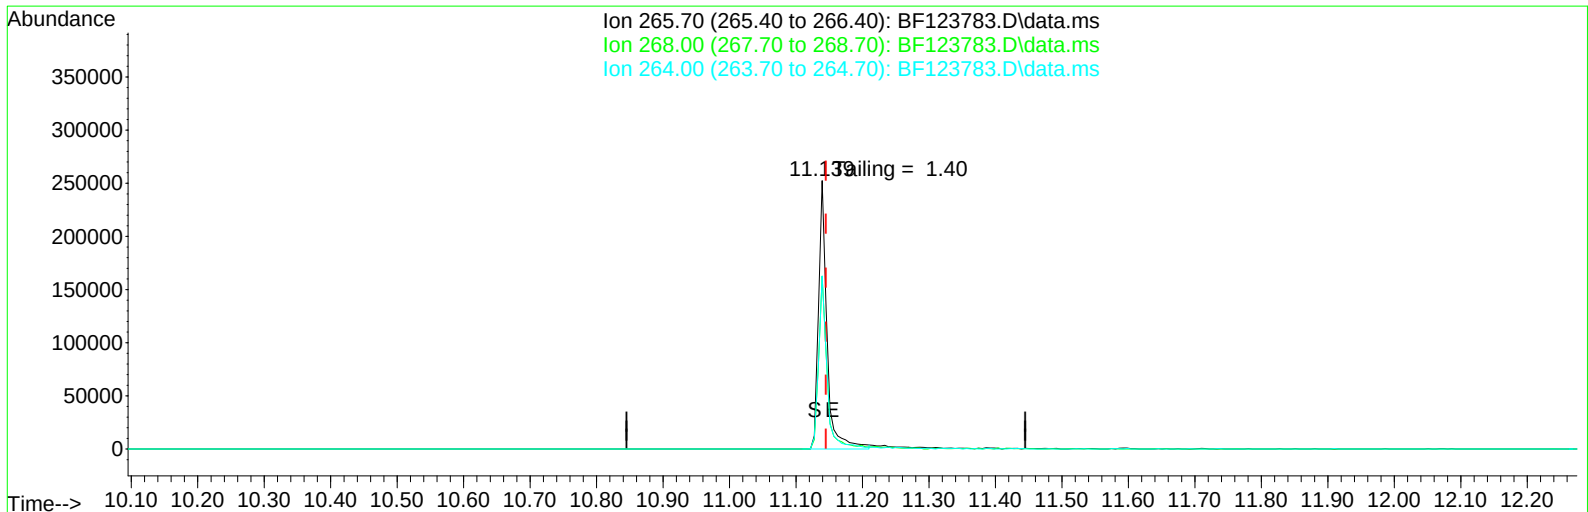

TIC: BF123783.D\data.ms

(70) Pentachlorophenol (C)

11.139min (-0.006) 42028.54 ng




response 233900

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.41
264.00	65.70	64.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050321\
Data File : BF123783.D
Acq On : 3 May 2021 17:02
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 03 17:45:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 16:30:39 2021
Response via : Initial Calibration

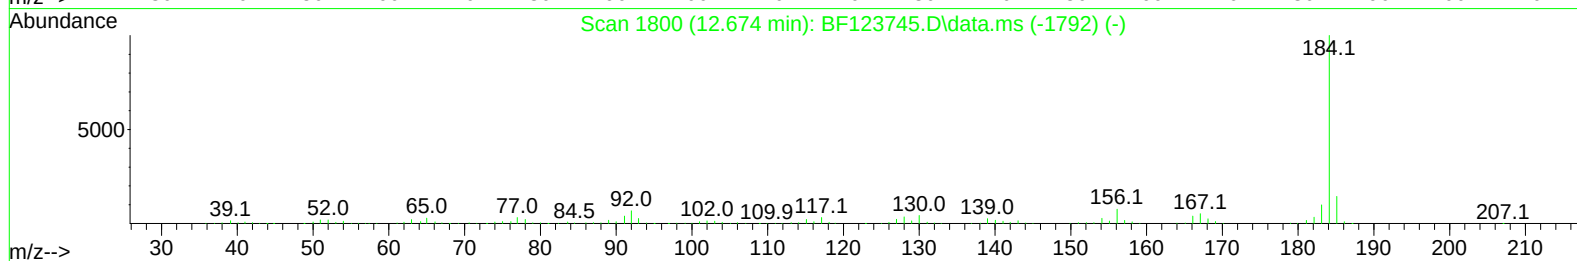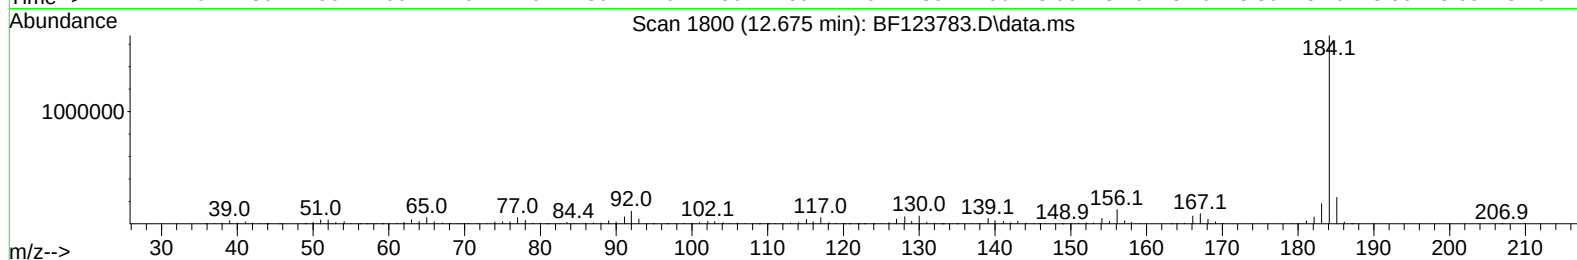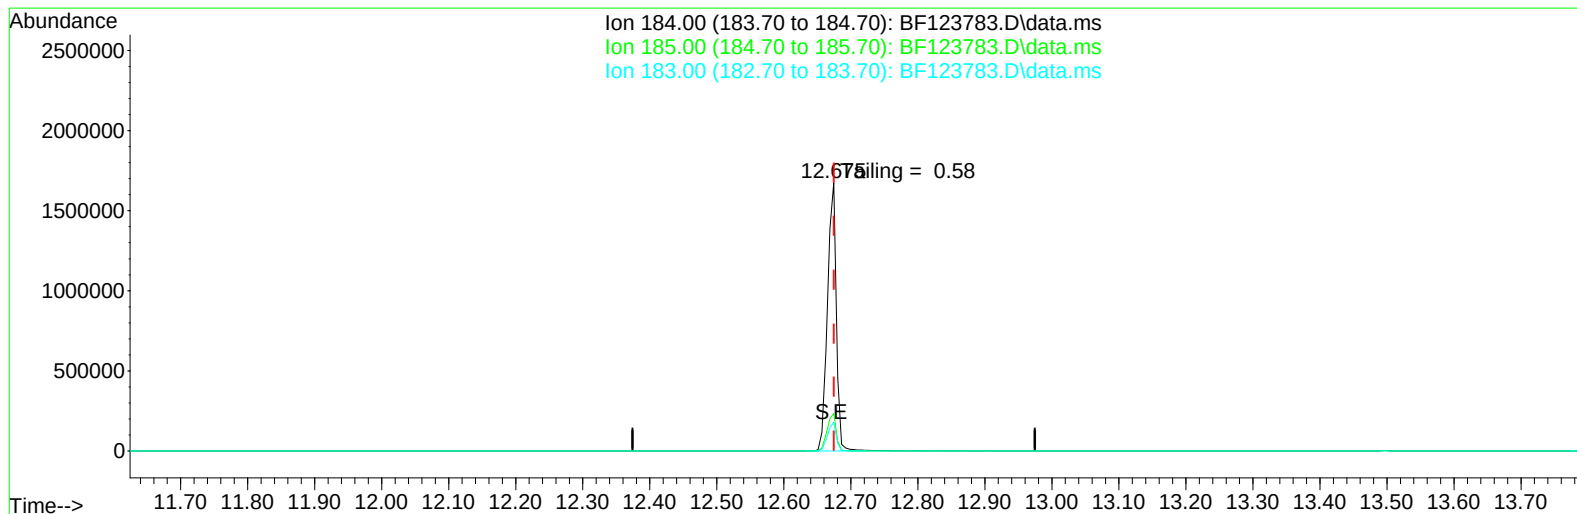

TIC: BF123783.D\data.ms

(77) Benzidine

12.675min (+ 0.000) 0.00 ng

response 1547382

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.98
183.00	9.80	10.76
0.00	0.00	0.00