
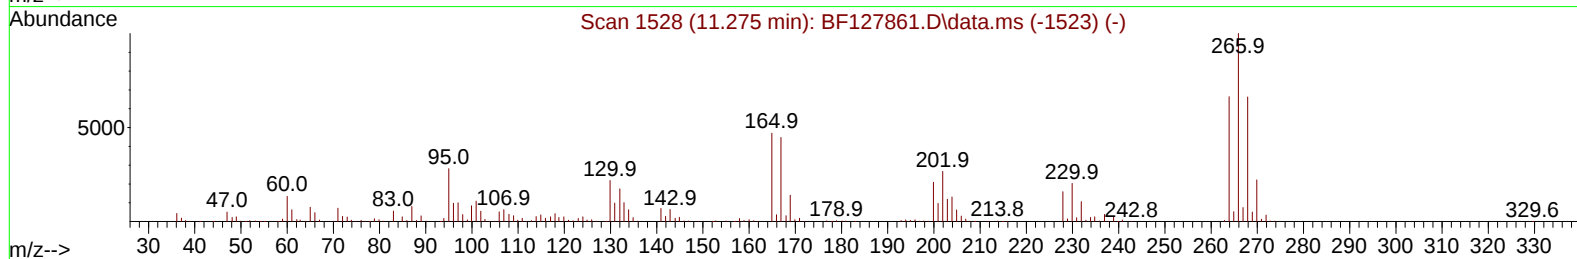
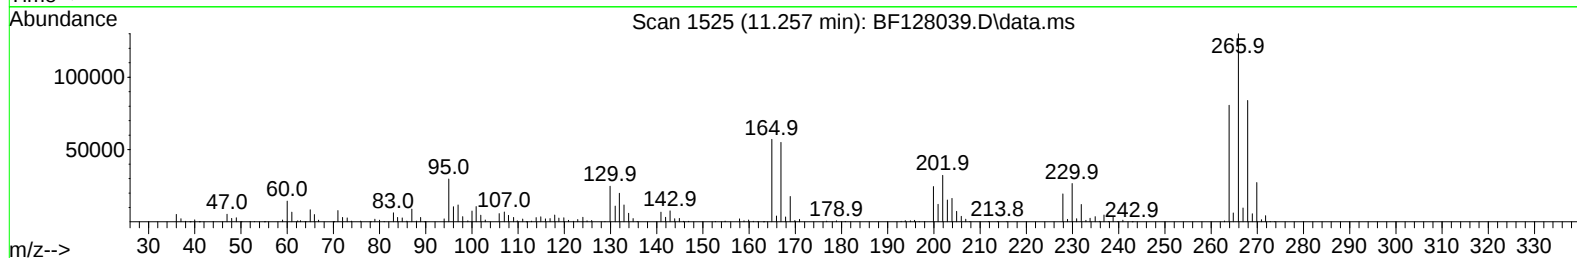


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050322\
Data File : BF128039.D
Acq On : 03 May 2022 11:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 09:02:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 04:23:29 2022
Response via : Initial Calibration

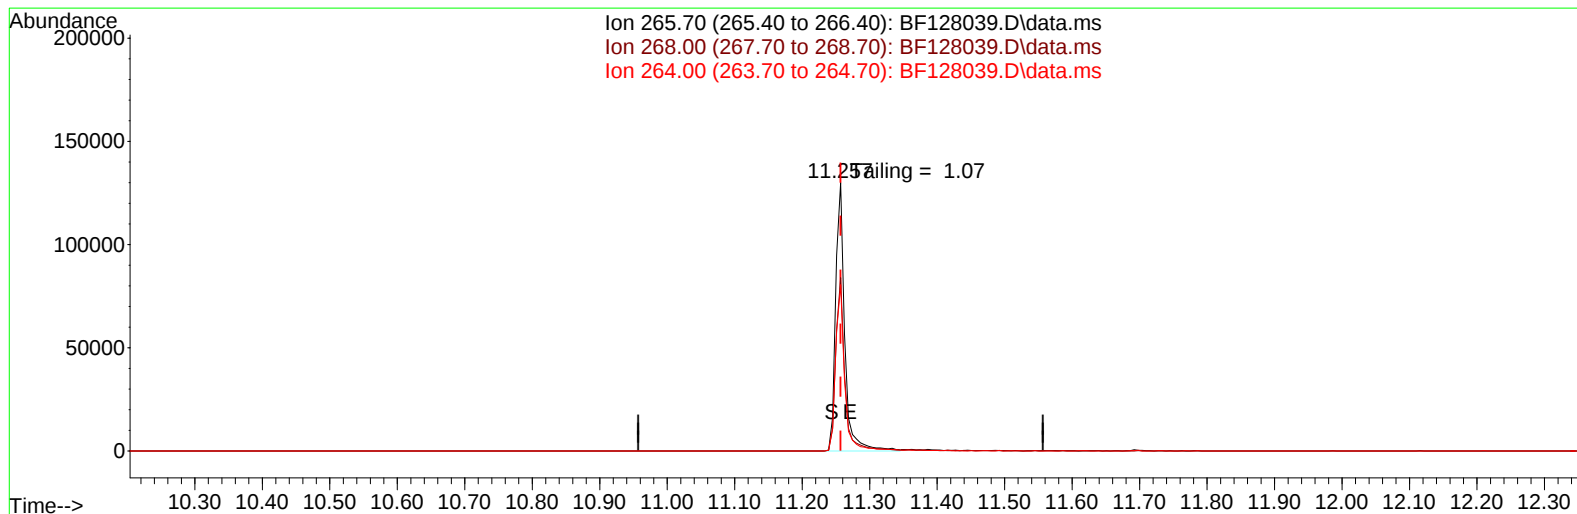

TIC: BF128039.D\data.ms

(70) Pentachlorophenol (C)




11.257min (-0.000) 22915.30 ng

response 122972

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	64.57
264.00	66.40	61.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050322\
Data File : BF128039.D
Acq On : 03 May 2022 11:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 09:02:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 04:23:29 2022
Response via : Initial Calibration

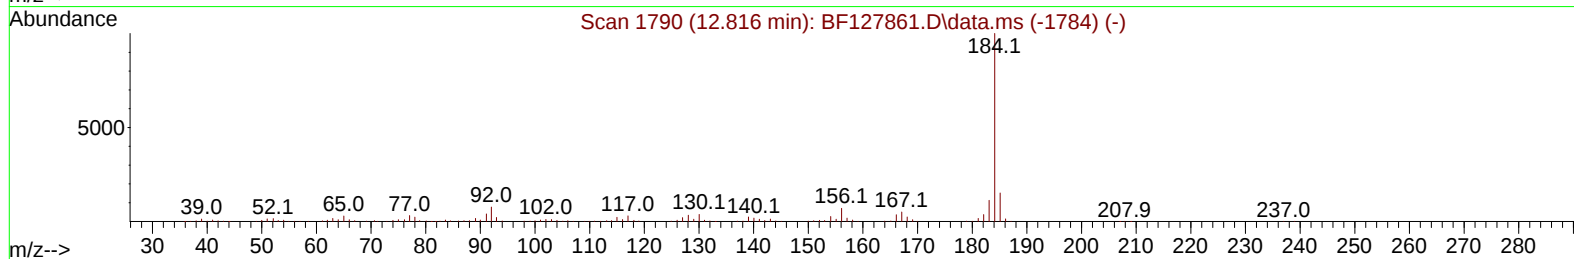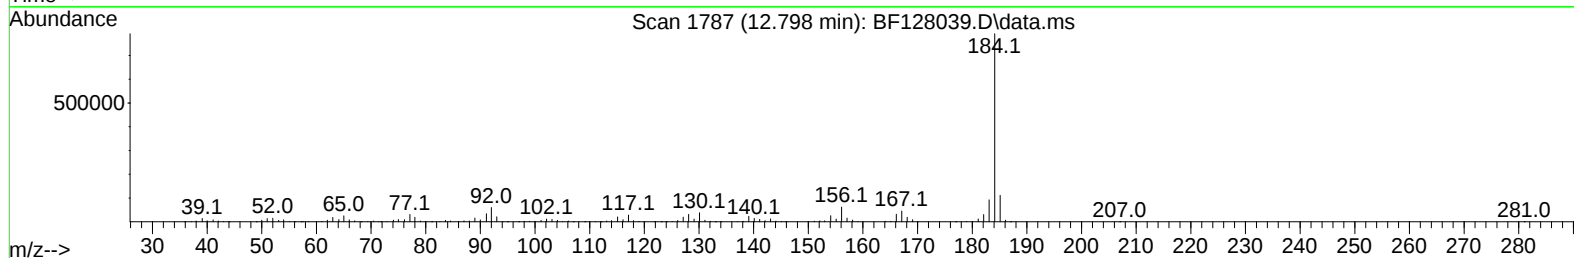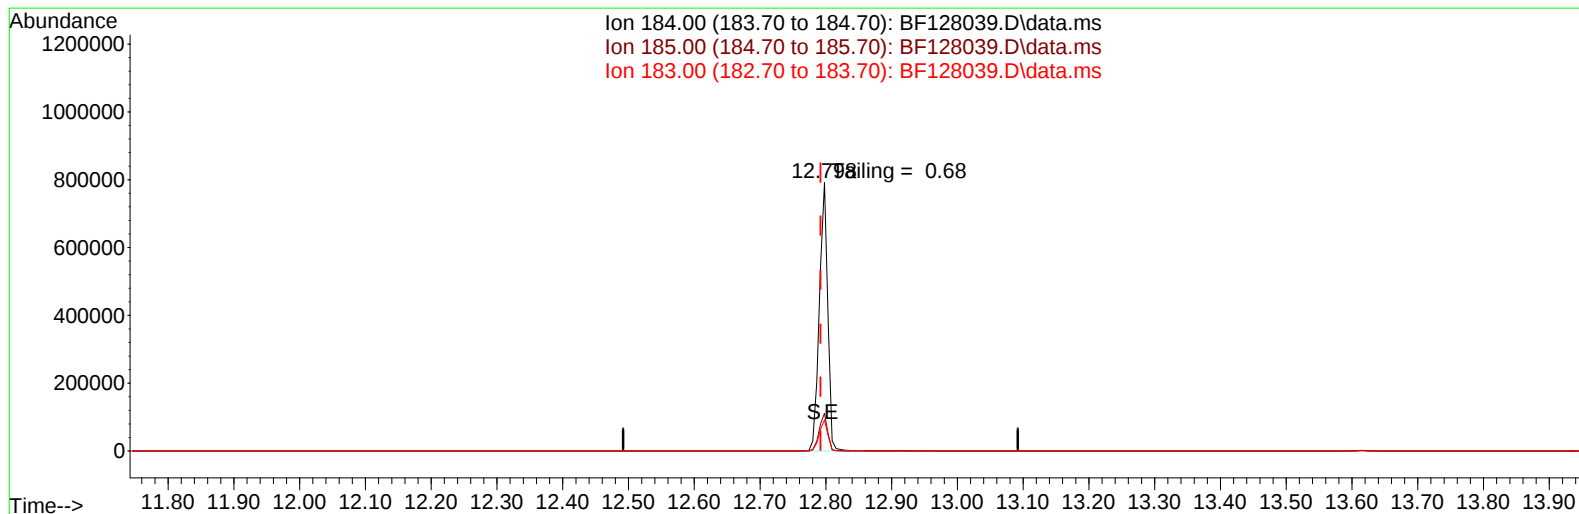

TIC: BF128039.D\data.ms

(77) Benzidine**12.798min (+ 0.006) 567654.92 ng****response 708896**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.11
183.00	11.20	11.64
0.00	0.00	0.00