

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050322\
 Data File : BF128041.D
 Acq On : 03 May 2022 12:57
 Operator : CG\JU
 Sample : PB144533BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144533BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.552	549	555	558	rBV	3338304	3313436	75.22%	12.926%
2	6.546	718	724	727	rBV	3004210	3440206	78.10%	13.420%
3	6.916	783	787	790	rBV	860153	669195	15.19%	2.611%
4	7.481	877	883	886	rBV	2154168	2374509	53.91%	9.263%
5	8.199	1000	1005	1009	rBV	983567	881381	20.01%	3.438%
6	9.281	1182	1189	1192	rBV	3756701	4180168	94.90%	16.307%
7	9.957	1299	1304	1308	rBV	1086934	1029658	23.38%	4.017%
8	10.757	1433	1440	1443	rBV	2519196	2704407	61.40%	10.550%
9	11.451	1554	1558	1562	rBV	1289757	1075645	24.42%	4.196%
10	13.045	1823	1829	1832	rBV	4420868	4404803	100.00%	17.183%
11	14.098	2004	2008	2012	rBV	875155	866720	19.68%	3.381%
12	15.610	2260	2265	2271	rBV2	535681	694269	15.76%	2.708%




Sum of corrected areas: 25634397

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050322\
Data File : BF128041.D
Acq On : 03 May 2022 12:57
Operator : CG\JU
Sample : PB144533BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144533BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

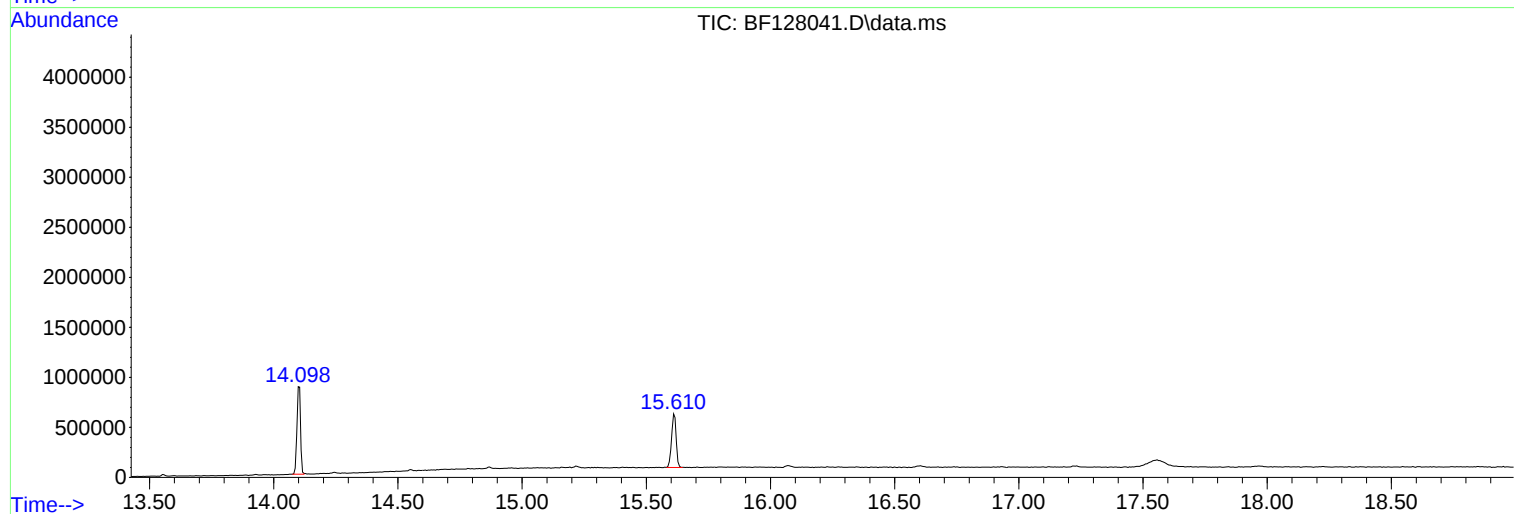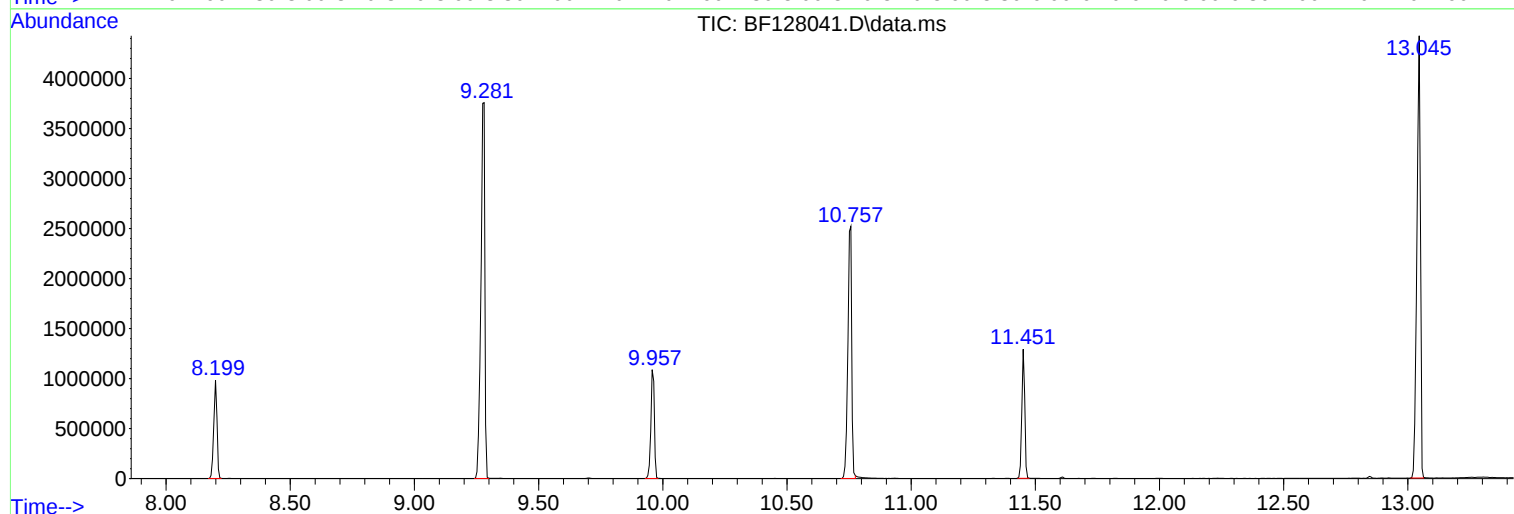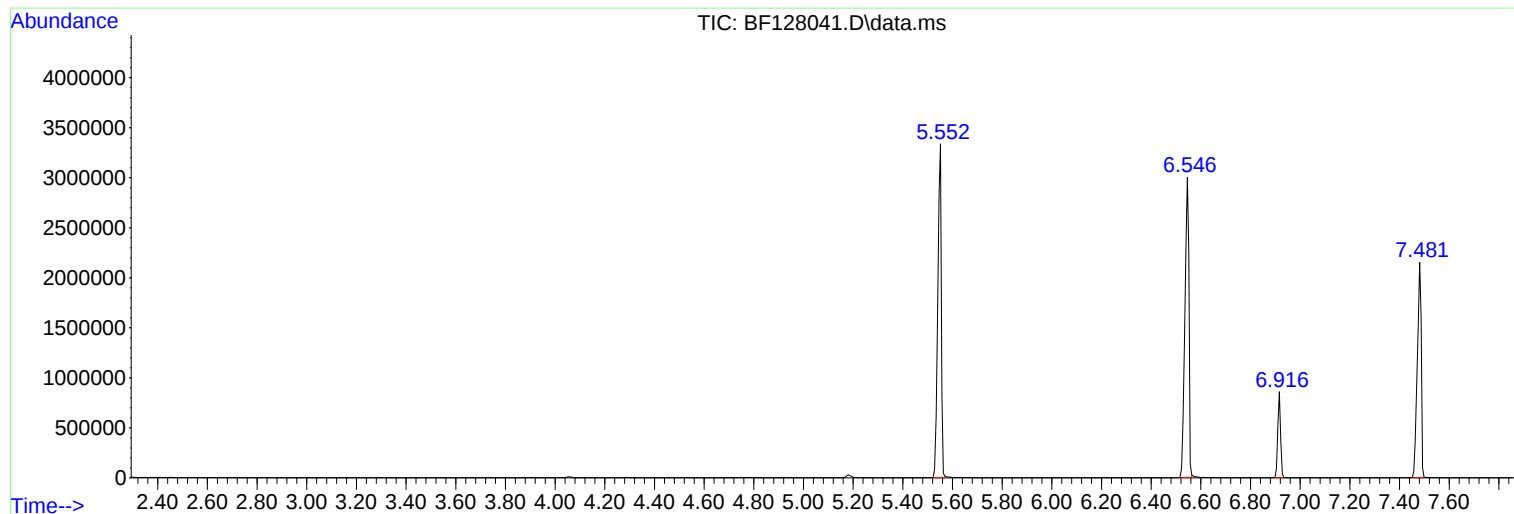

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050322\
Data File : BF128041.D
Acq On : 03 May 2022 12:57
Operator : CG\JU
Sample : PB144533BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144533BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050322\
Data File : BF128041.D
Acq On : 03 May 2022 12:57
Operator : CG\JU
Sample : PB144533BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144533BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------