
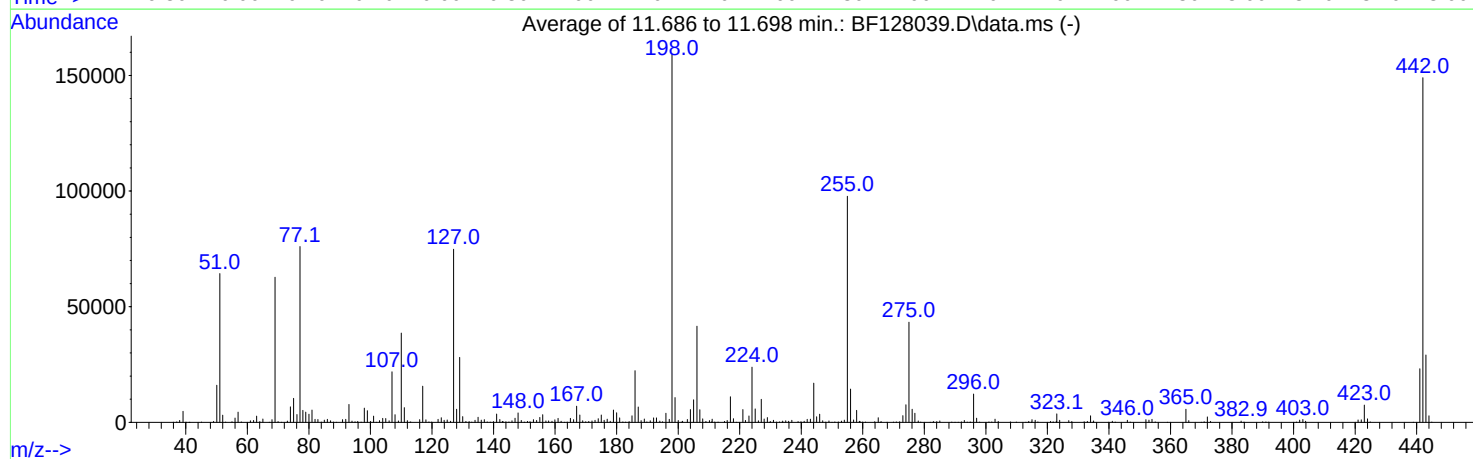


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050322\
 Data File : BF128039.D
 Acq On : 03 May 2022 11:49
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 04 04:23:29 2022

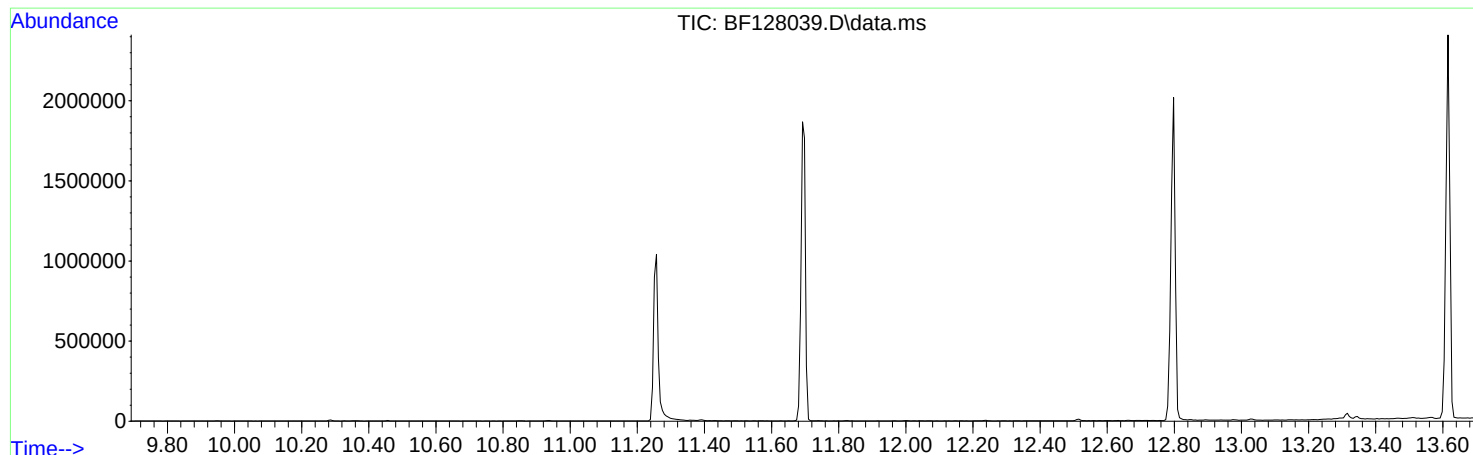




AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	64347	PASS
68	69	0.00	2	1.9	1189	PASS
69	198	0.00	100	39.5	62760	PASS
70	69	0.00	2	0.6	349	PASS
127	198	10	80	47.1	74832	PASS
197	198	0.00	2	0.8	1310	PASS
198	198	100	100	100.0	159035	PASS
199	198	5	9	6.7	10709	PASS
275	198	10	60	27.2	43272	PASS
365	198	1	100	3.5	5642	PASS
441	198	0.01	100	14.6	23173	PASS
442	442	50	100	100.0	149013	PASS
443	442	15	24	19.5	29113	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050322\
Data File : BF128039.D
Acq On : 03 May 2022 11:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 04 09:02:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 04:23:29 2022
Response via : Initial Calibration

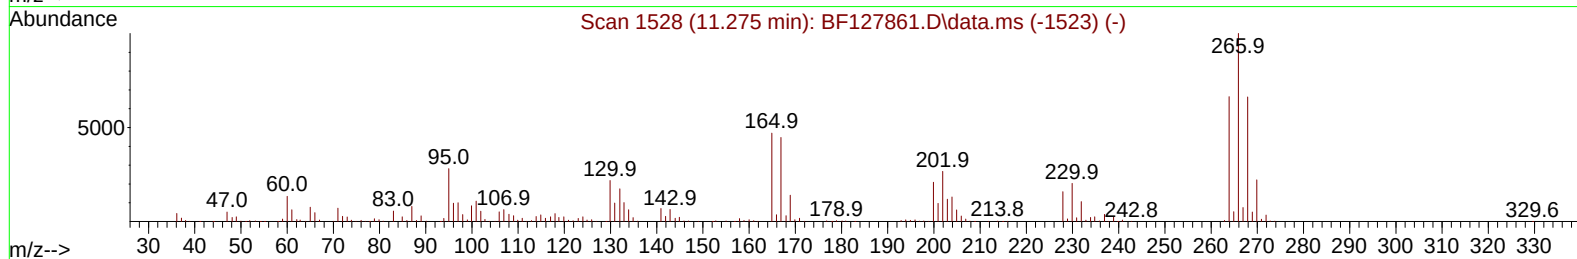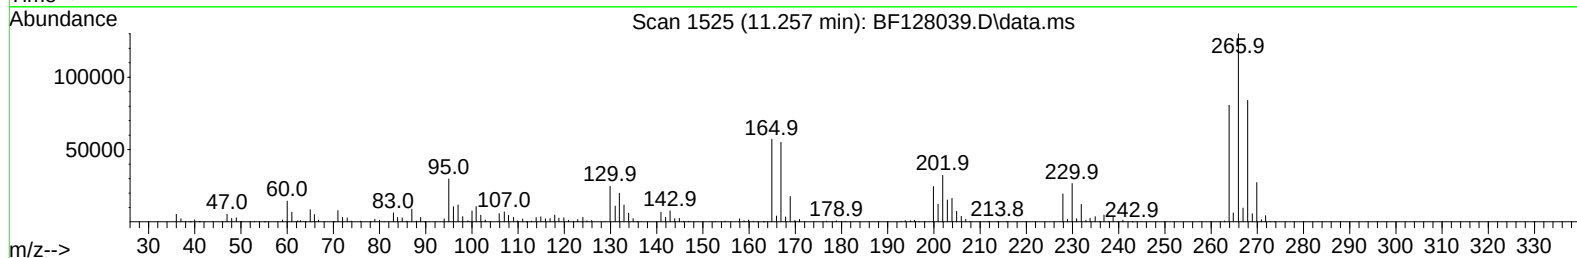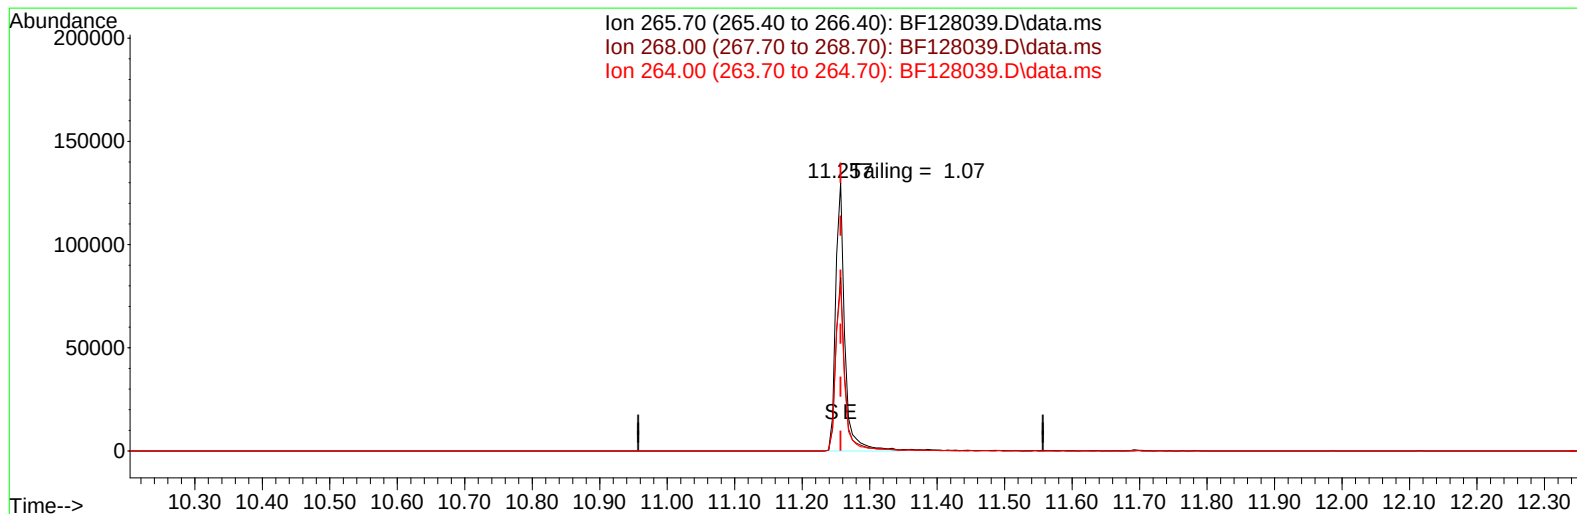

TIC: BF128039.D\data.ms

(70) Pentachlorophenol (C)

11.257min (-0.000) 22915.30 ng




response 122972

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	64.57
264.00	66.40	61.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050322\
Data File : BF128039.D
Acq On : 03 May 2022 11:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 04 09:02:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 04:23:29 2022
Response via : Initial Calibration

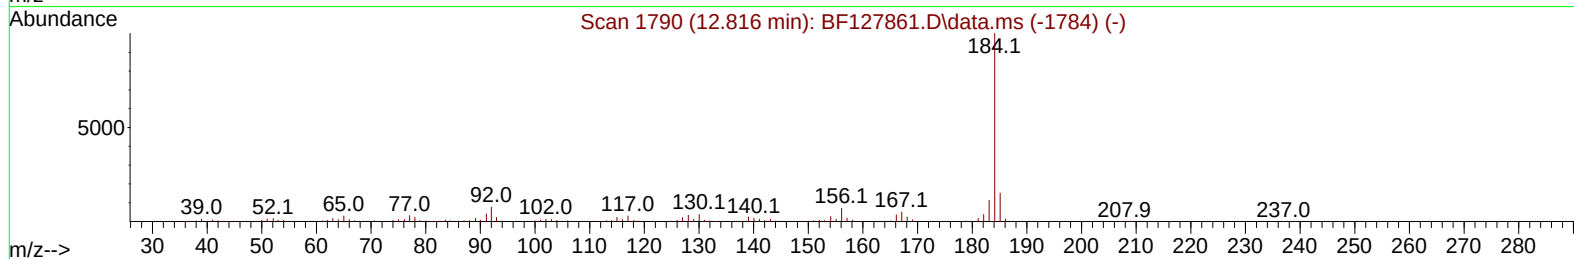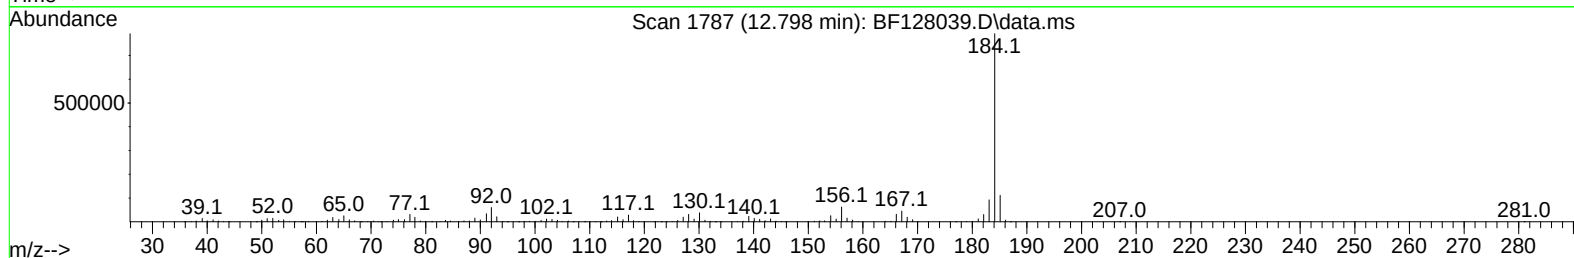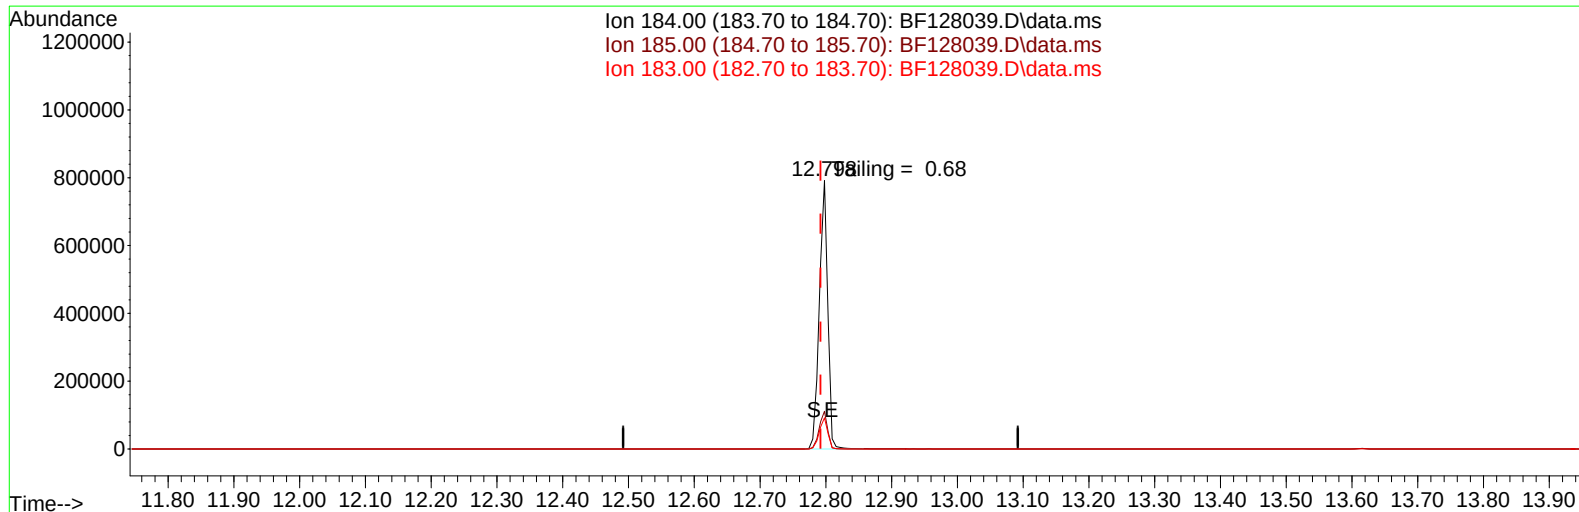

TIC: BF128039.D\data.ms

(77) Benzidine

12.798min (+ 0.006) 567654.92 ng

response 708896

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.11
183.00	11.20	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/3/2022	BNA_F	<u>BF128039.D</u>
Compound Name	Response	Retention Time
DDT	387609	13.616
DDD	7654	13.316
DDE	641	12.974
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8295	395904	2.10

Instrument :
BNA_F
ClientSampleId :
DFTPP